

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 22:31
 Operator : SM\AJ
 Sample : K4131-26
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:44:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.597	5.317	171.0E6	122.2E6	117.889	122.823
Target Compounds							
1) T	Dalapon	2.095	0.000	30619566	0	16.522	N.D. #
2) T	3,5-DICHL...	0.000	4.634	0	141.6E6	N.D.	109.162
5) T	DICAMBA	5.690	0.000	10635874	0	1.781	N.D. #
6) T	MCP	5.817	0.000	16821409	0	3.630	N.D. #
7) T	MCPA	0.000	5.650	0	121.1E6	N.D.	28.776
10) T	Pentachlo...	0.000	6.573	0	18542534	N.D.	1.428
11) T	2,4,5-TP ...	0.000	6.962	0	41172104	N.D.	7.937
12) T	2,4,5-T	7.606	0.000	95898640	0	11.489	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 22:31
Operator : SM\AJ
Sample : K4131-26
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:44:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

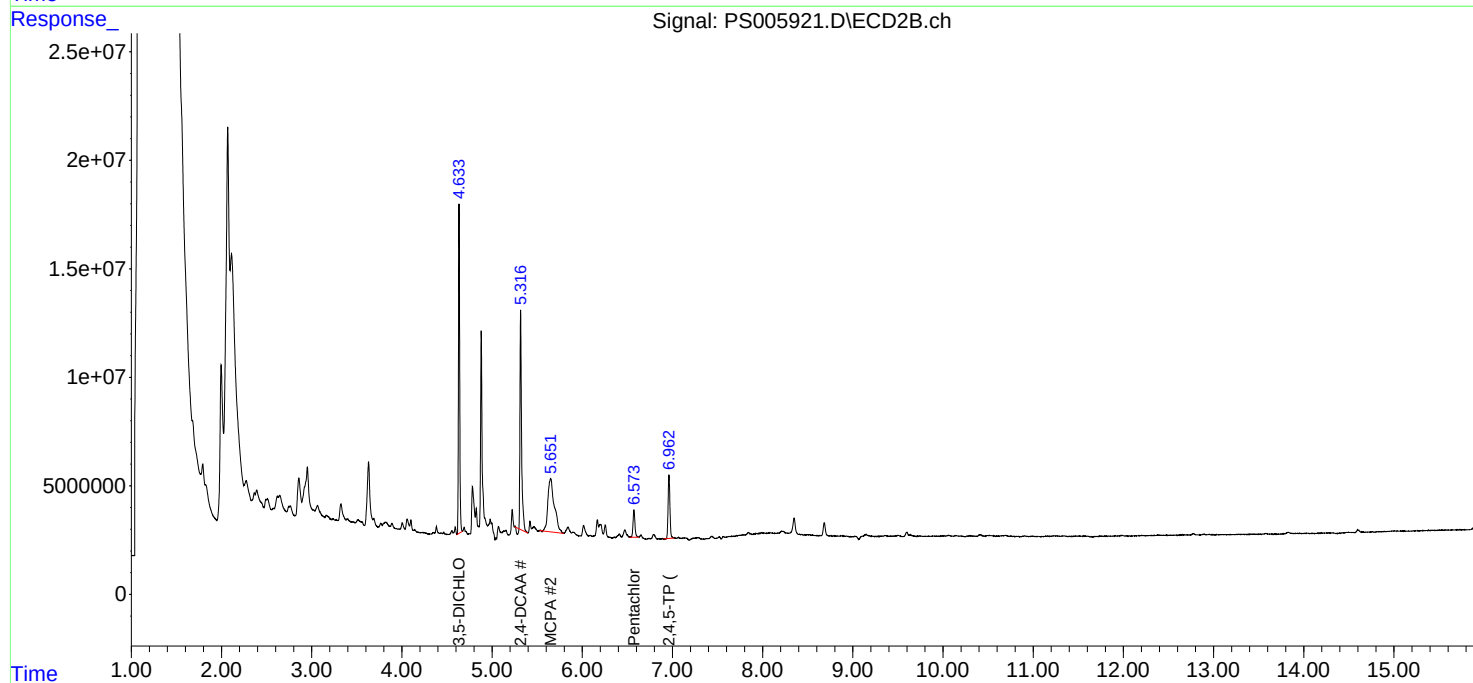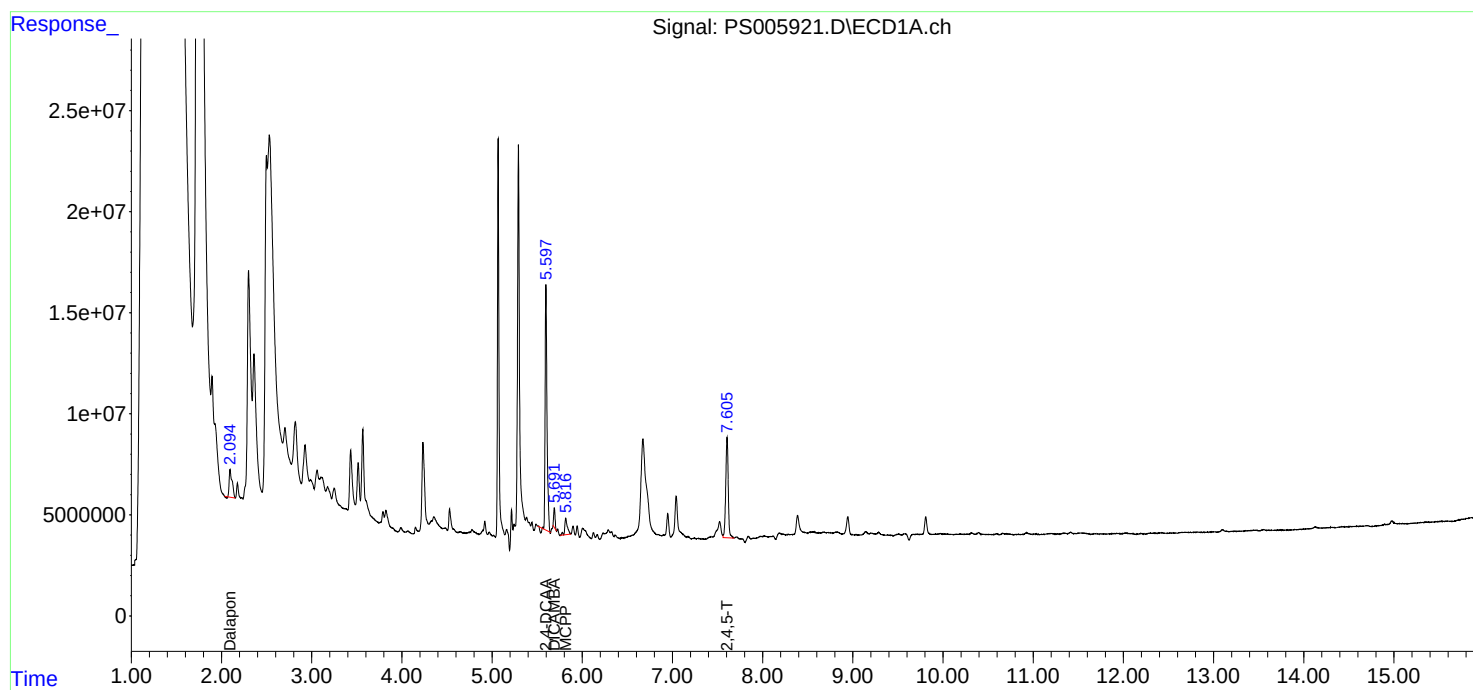


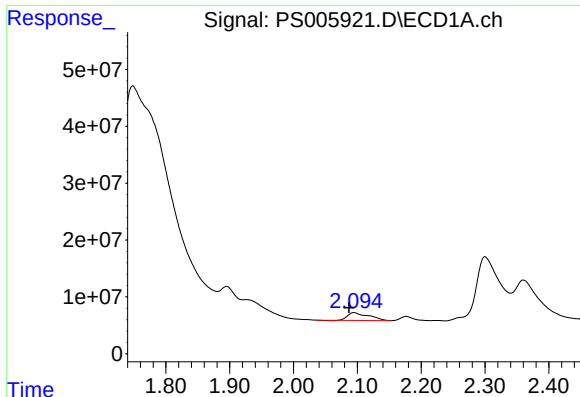

#1 Dalapon


R.T.: 2.095 min
Delta R.T.: 0.008 min
Response: 30619566
Conc: 16.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

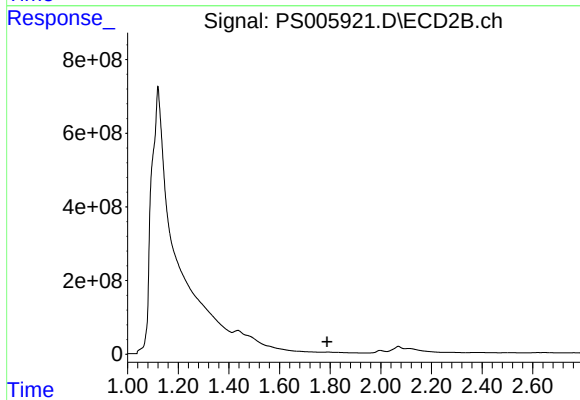


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

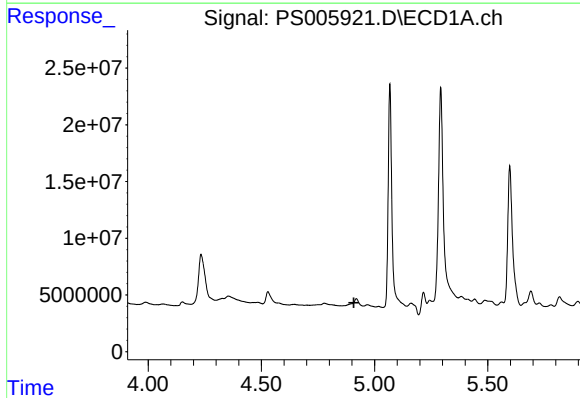


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

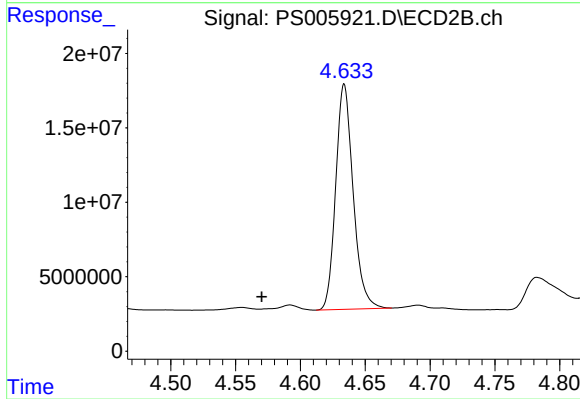

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.634 min
Delta R.T.: 0.064 min
Response: 141617678
Conc: 109.16 ng/ml

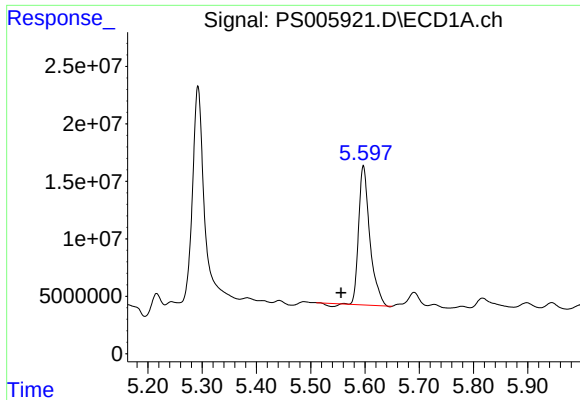

#4 2,4-DCAA


R.T.: 5.597 min
Delta R.T.: 0.041 min
Response: 171035068
Conc: 117.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

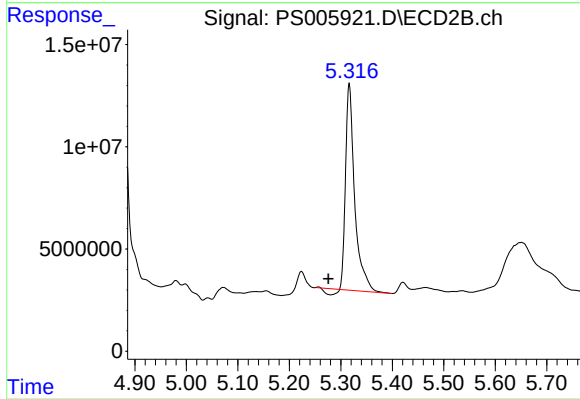


#4 2,4-DCAA

R.T.: 5.317 min
Delta R.T.: 0.041 min
Response: 122169080
Conc: 122.82 ng/ml

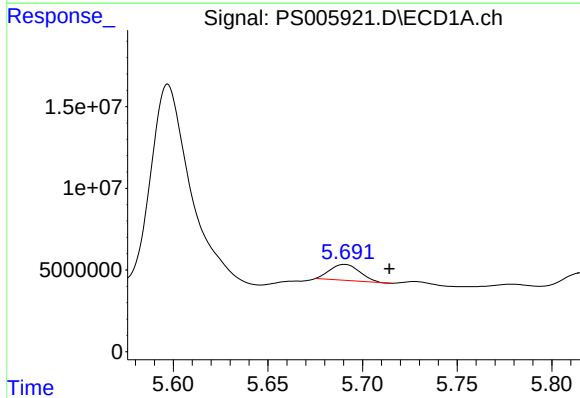


#5 DICAMBA

R.T.: 5.690 min
Delta R.T.: -0.024 min
Response: 10635874
Conc: 1.78 ng/ml

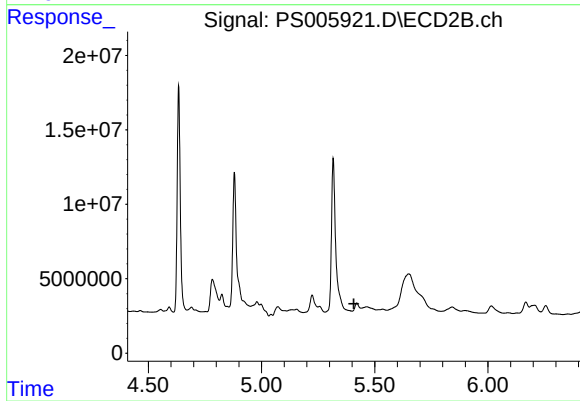

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

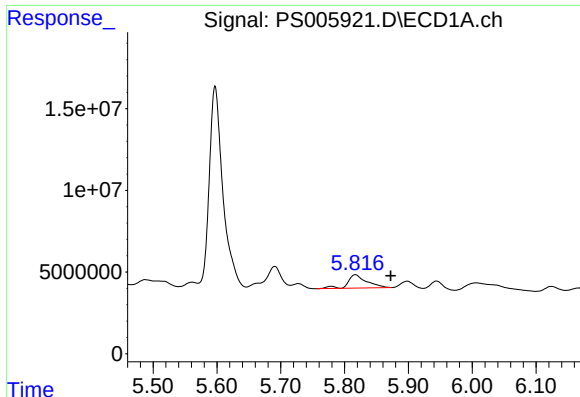

#6 MCPP


R.T.: 5.817 min
Delta R.T.: -0.056 min
Response: 16821409
Conc: 3.63 ug/ml

Instrument :
ECD_S
ClientSampleId :

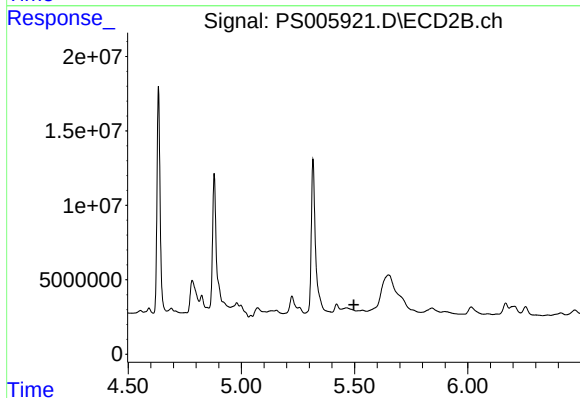


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

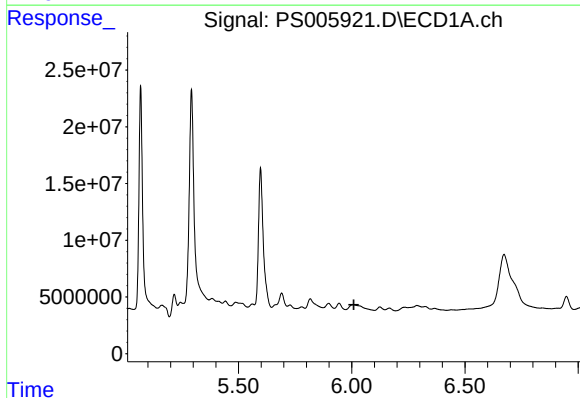


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

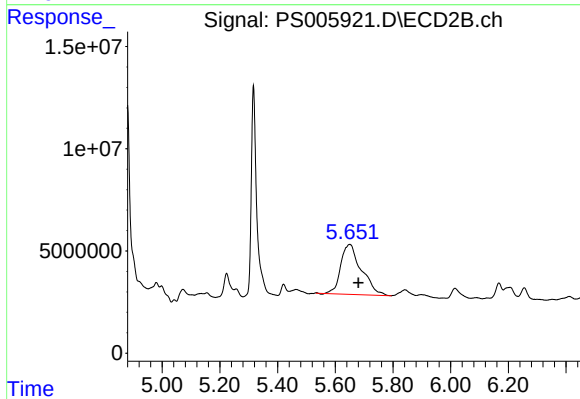

#7 MCPA


R.T.: 5.650 min
Delta R.T.: -0.031 min
Response: 121117086
Conc: 28.78 ug/ml

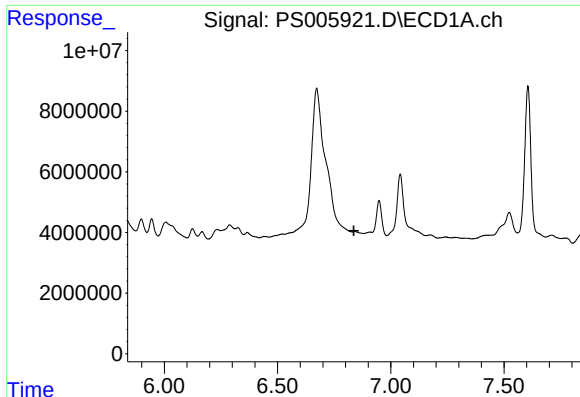

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

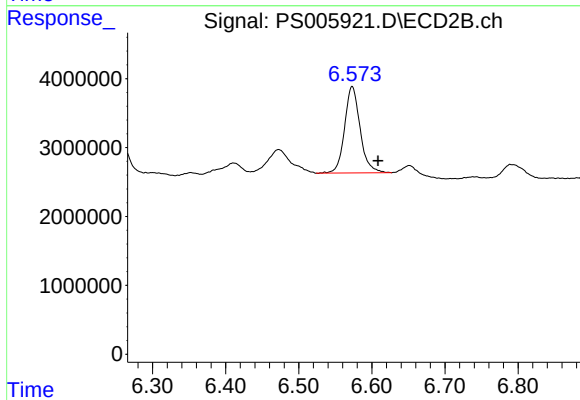


#10 Pentachlorophenol

R.T.: 6.573 min
Delta R.T.: -0.035 min
Response: 18542534
Conc: 1.43 ng/ml

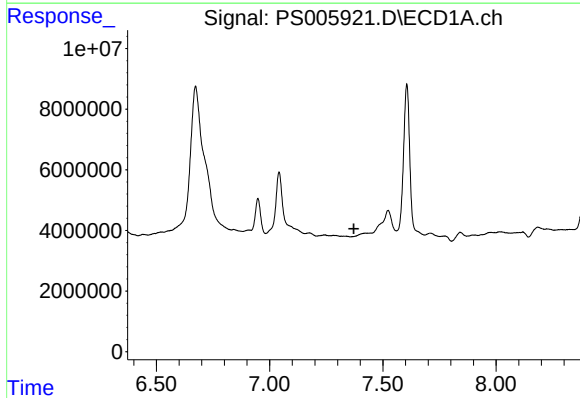


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

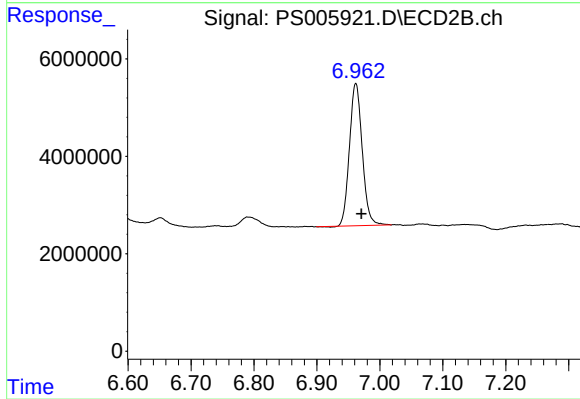

#11 2,4,5-TP (SILVEX)


R.T.: 6.962 min
Delta R.T.: -0.009 min
Response: 41172104
Conc: 7.94 ng/ml

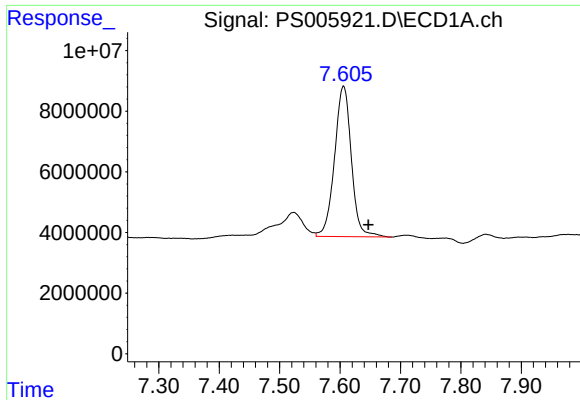

#12 2,4,5-T

R.T.: 7.606 min
Delta R.T.: -0.041 min
Response: 95898640
Conc: 11.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

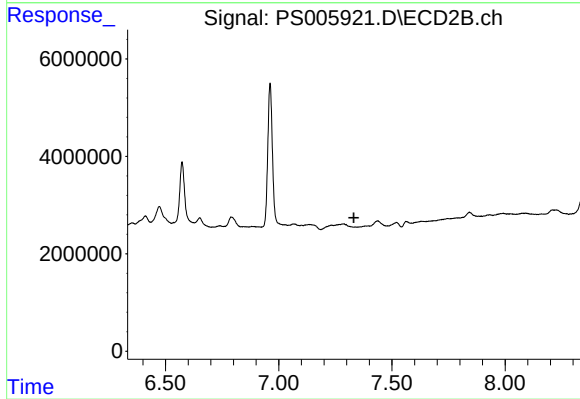

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.