

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 23:15
 Operator : SM\AJ
 Sample : K4131-36
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:45:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.292	270.2E6	176.7E6	186.267	177.623
Target Compounds							
1) T	Dalapon	2.071	0.000	32320871	0	17.440	N.D. #
2) T	3,5-DICHL...	0.000	4.610	0	189.5E6	N.D.	146.084
3) T	4-Nitroph...	5.361	0.000	5195505	0	8.637	N.D. #
5) T	DICAMBA	5.667	0.000	8467603	0	1.418	N.D. #
7) T	MCPA	0.000	5.620	0	126.6E6	N.D.	30.080
8) T	DICHLORPROP	6.305	0.000	4827255	0	3.357	N.D. #
10) T	Pentachlo...	0.000	6.549	0	23960263	N.D.	1.846
11) T	2,4,5-TP ...	0.000	6.939	0	65853509	N.D.	12.695
12) T	2,4,5-T	7.582	0.000	142.3E6	0	17.048	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 23:15
Operator : SM\AJ
Sample : K4131-36
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:45:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

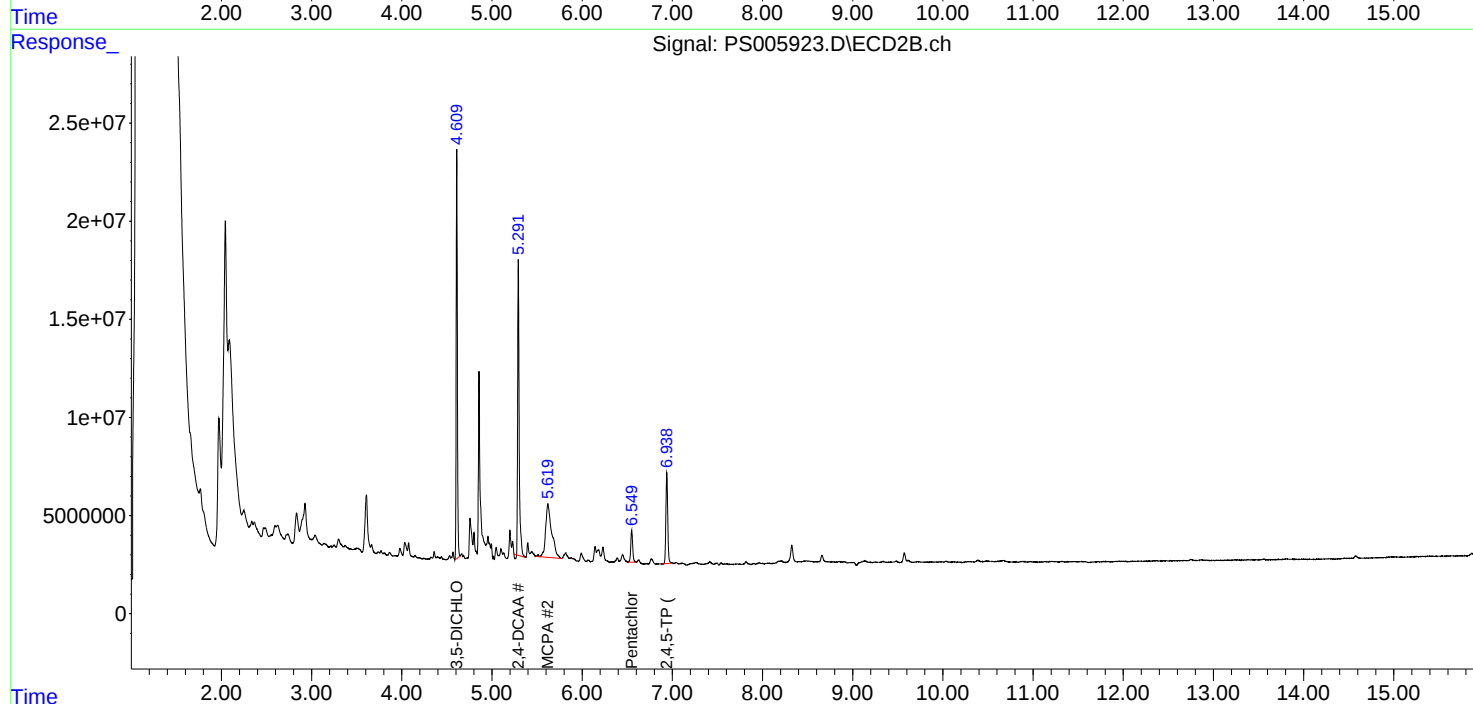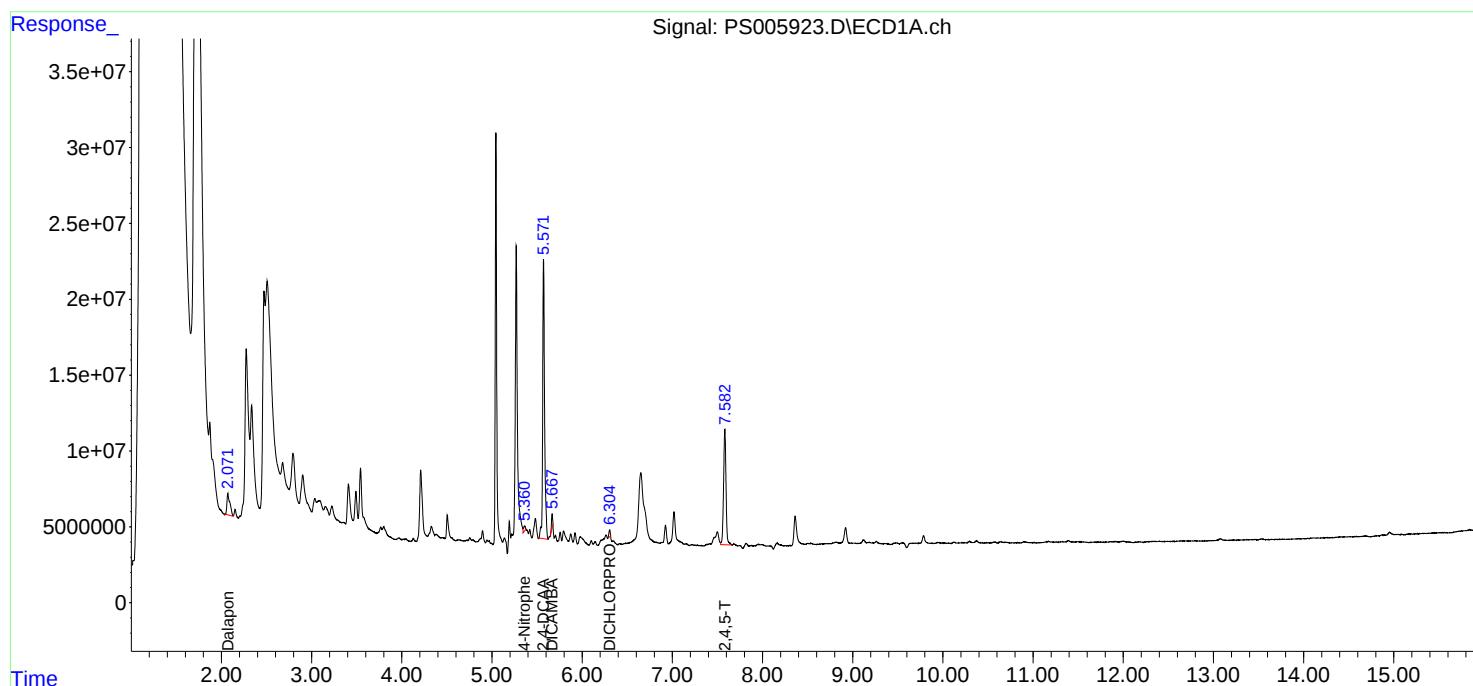


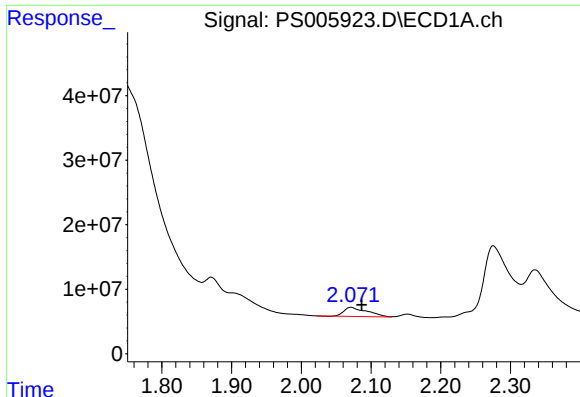

#1 Dalapon


R.T.: 2.071 min
Delta R.T.: -0.016 min
Response: 32320871
Conc: 17.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

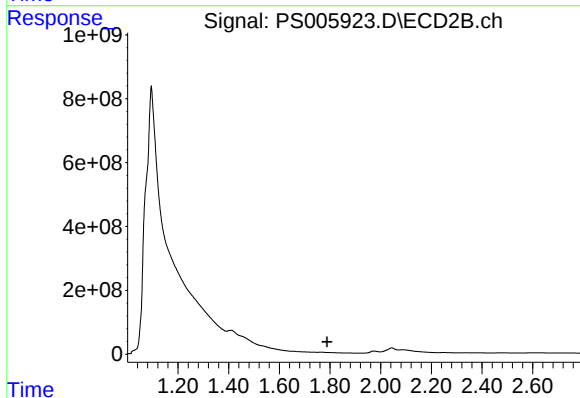


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

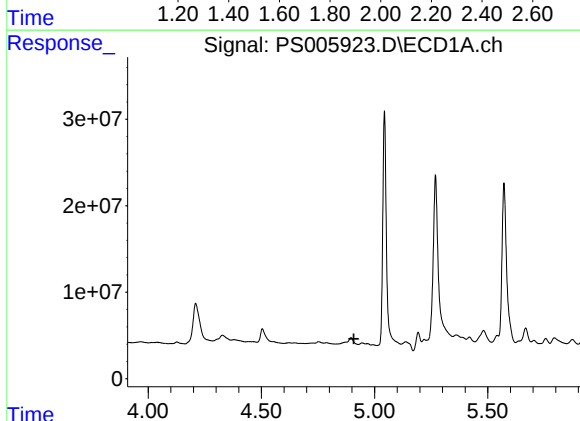


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

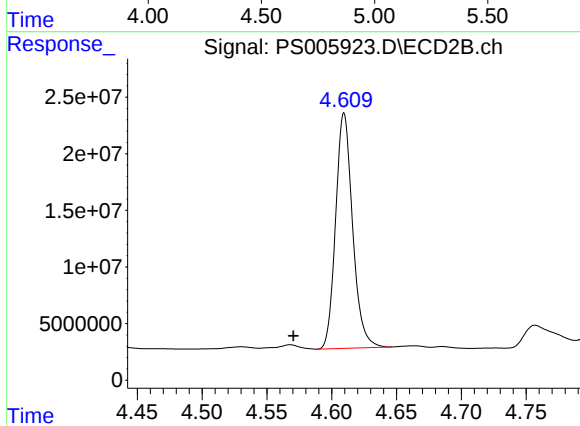

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.610 min
Delta R.T.: 0.039 min
Response: 189516676
Conc: 146.08 ng/ml

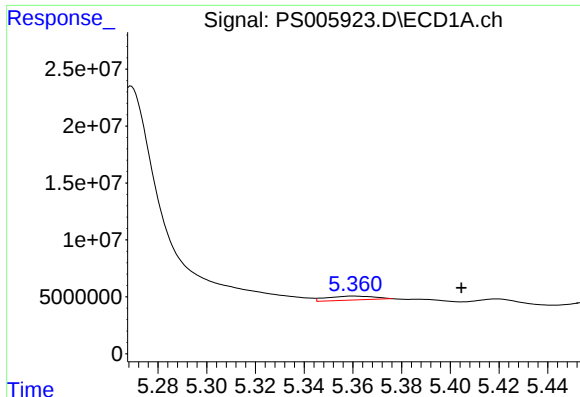

#3 4-Nitrophenol


R.T.: 5.361 min
Delta R.T.: -0.044 min
Response: 5195505
Conc: 8.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

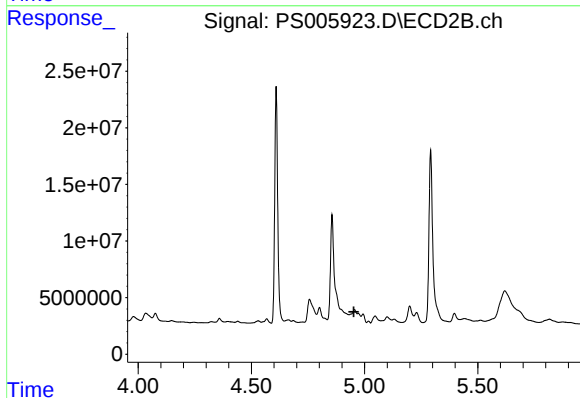


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

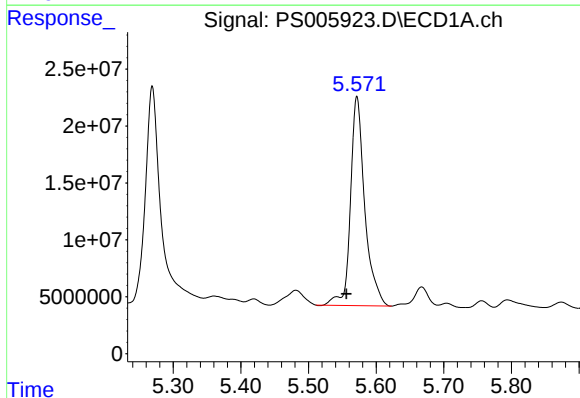


#4 2,4-DCAA

R.T.: 5.572 min
Delta R.T.: 0.016 min
Response: 270239571
Conc: 186.27 ng/ml

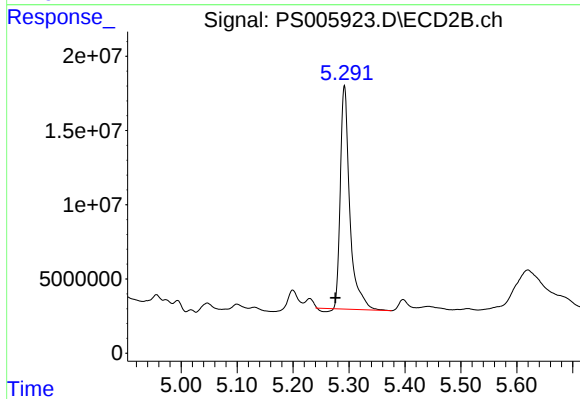

#4 2,4-DCAA


R.T.: 5.292 min
Delta R.T.: 0.016 min
Response: 176678201
Conc: 177.62 ng/ml

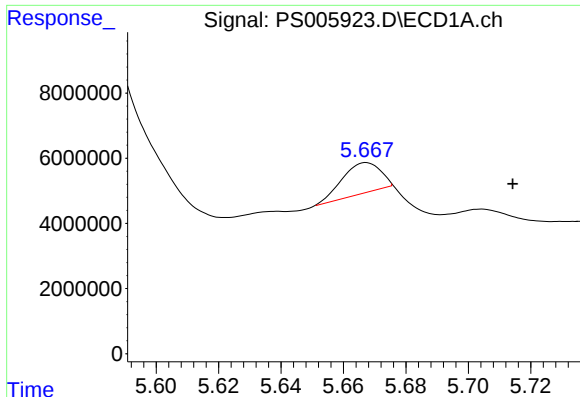

#5 DICAMBA


R.T.: 5.667 min
Delta R.T.: -0.047 min
Response: 8467603
Conc: 1.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

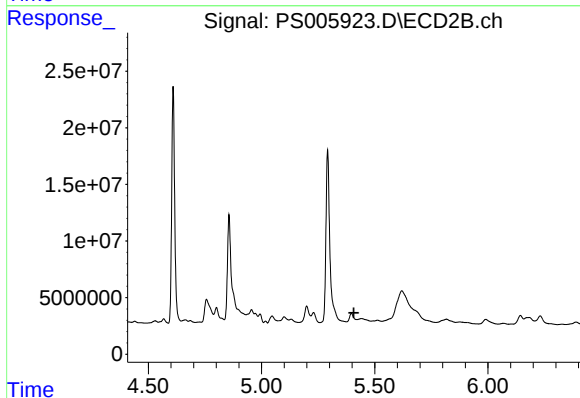


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

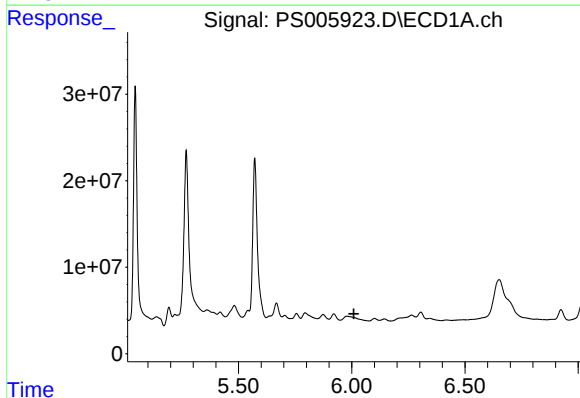


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

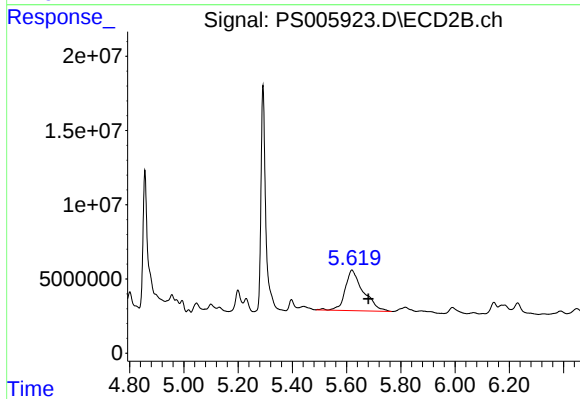

#7 MCPA


R.T.: 5.620 min
Delta R.T.: -0.061 min
Response: 126609153
Conc: 30.08 ug/ml

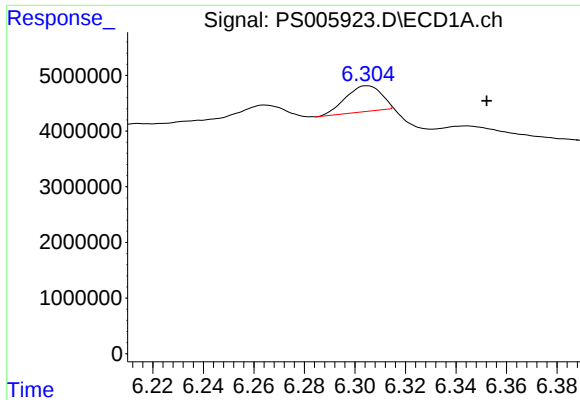

#8 DICHLORPROP


R.T.: 6.305 min
Delta R.T.: -0.047 min
Response: 4827255
Conc: 3.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

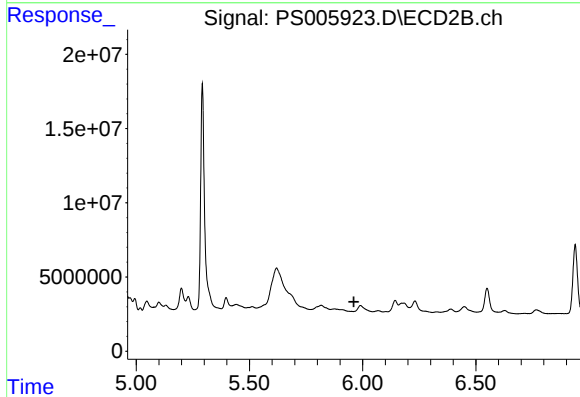


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.961 min
Response: 0
Conc: N.D.

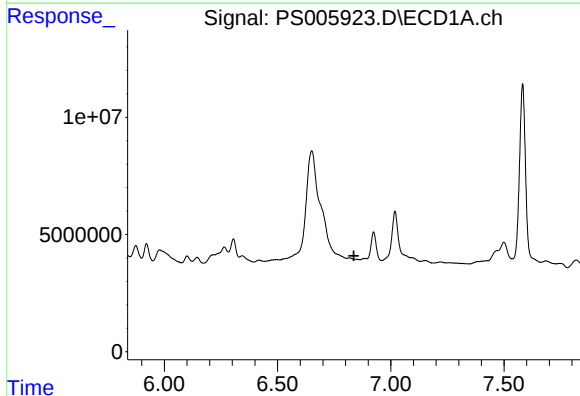


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

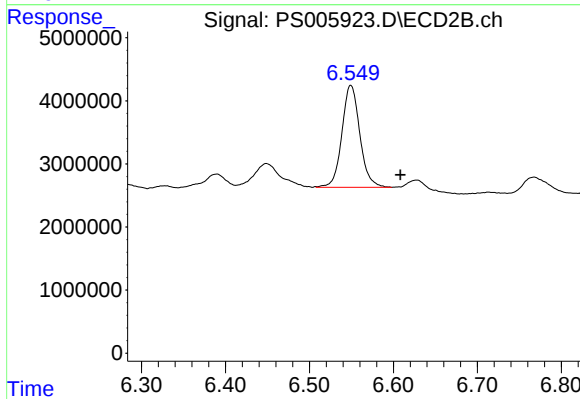

#10 Pentachlorophenol


R.T.: 6.549 min
Delta R.T.: -0.059 min
Response: 23960263
Conc: 1.85 ng/ml

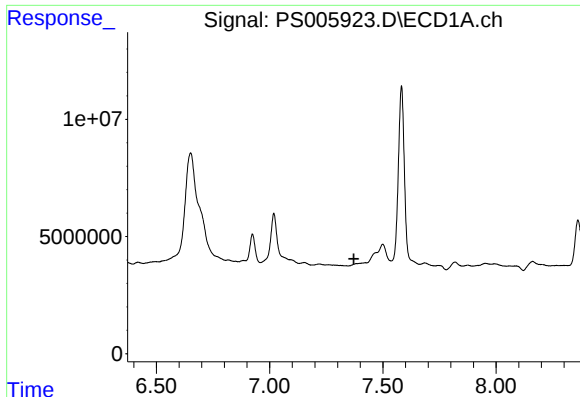

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

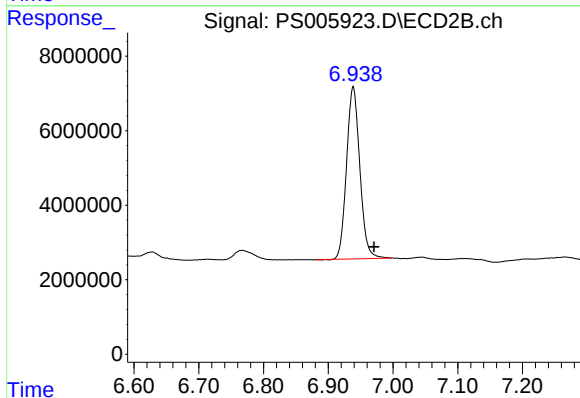


#11 2,4,5-TP (SILVEX)

R.T.: 6.939 min
Delta R.T.: -0.032 min
Response: 65853509
Conc: 12.70 ng/ml

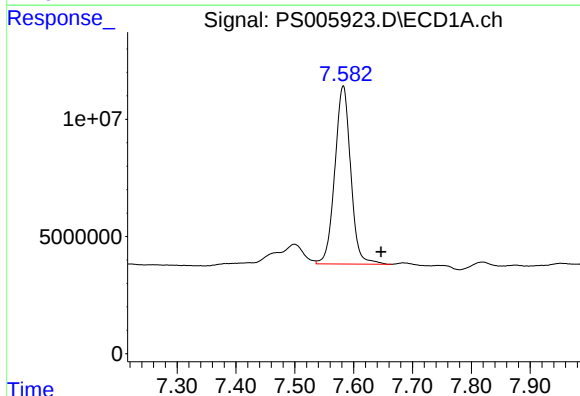

#12 2,4,5-T

R.T.: 7.582 min
Delta R.T.: -0.065 min
Response: 142294113
Conc: 17.05 ng/ml

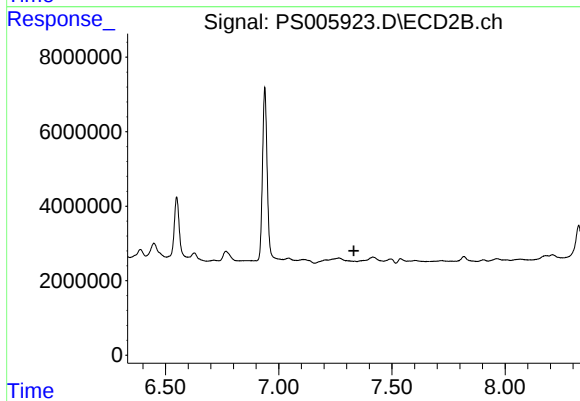

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.