

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 23:37
 Operator : SM\AJ
 Sample : K4135-21
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 1S-A1-A4-COMP-(0-1)

Manual Integrations
 APPROVED

Ankita
 8/7/2019 5:47:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:45:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	5.556	5.277	265.4E6	188.3E6	182.921m	189.262
------	----------	-------	-------	---------	---------	----------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 23:37
Operator : SM\AJ
Sample : K4135-21
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
1S-A1-A4-COMP-(0-1)


Manual Integrations
APPROVED

Ankita
8/7/2019 5:47:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:45:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

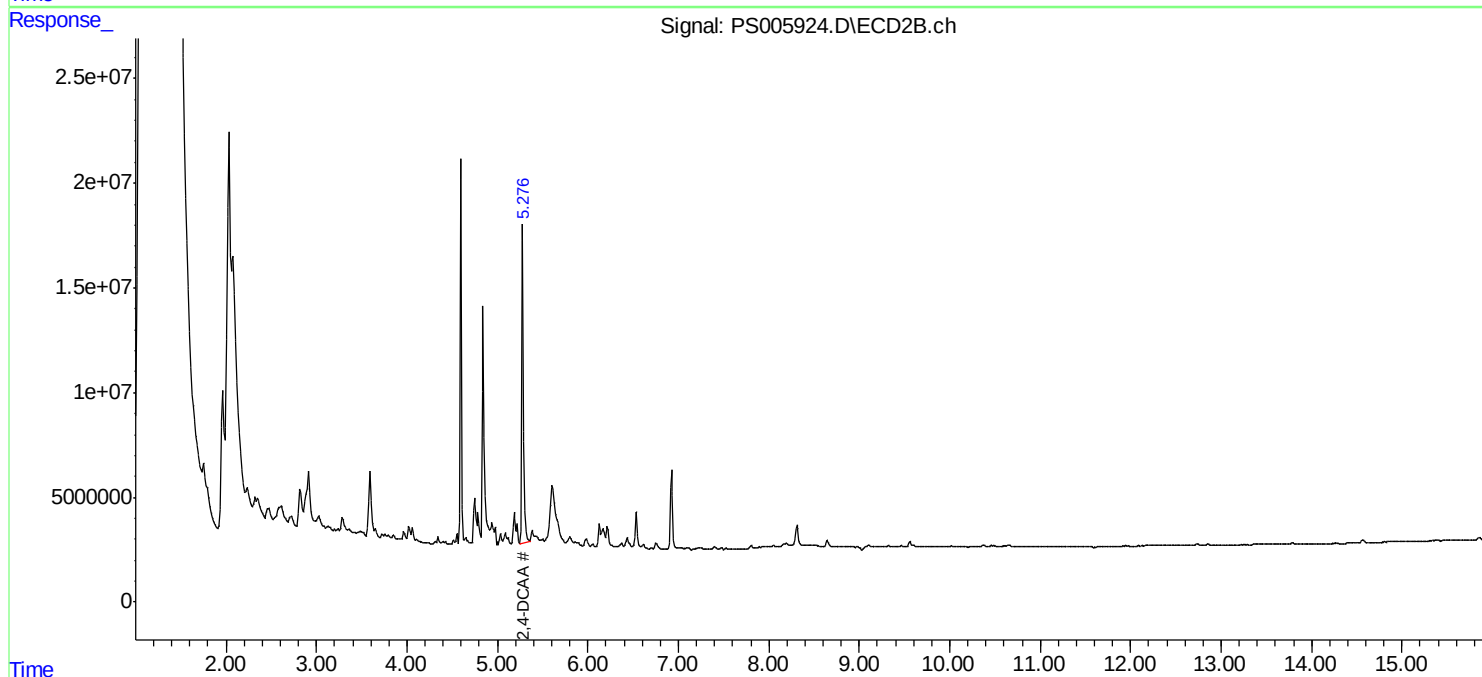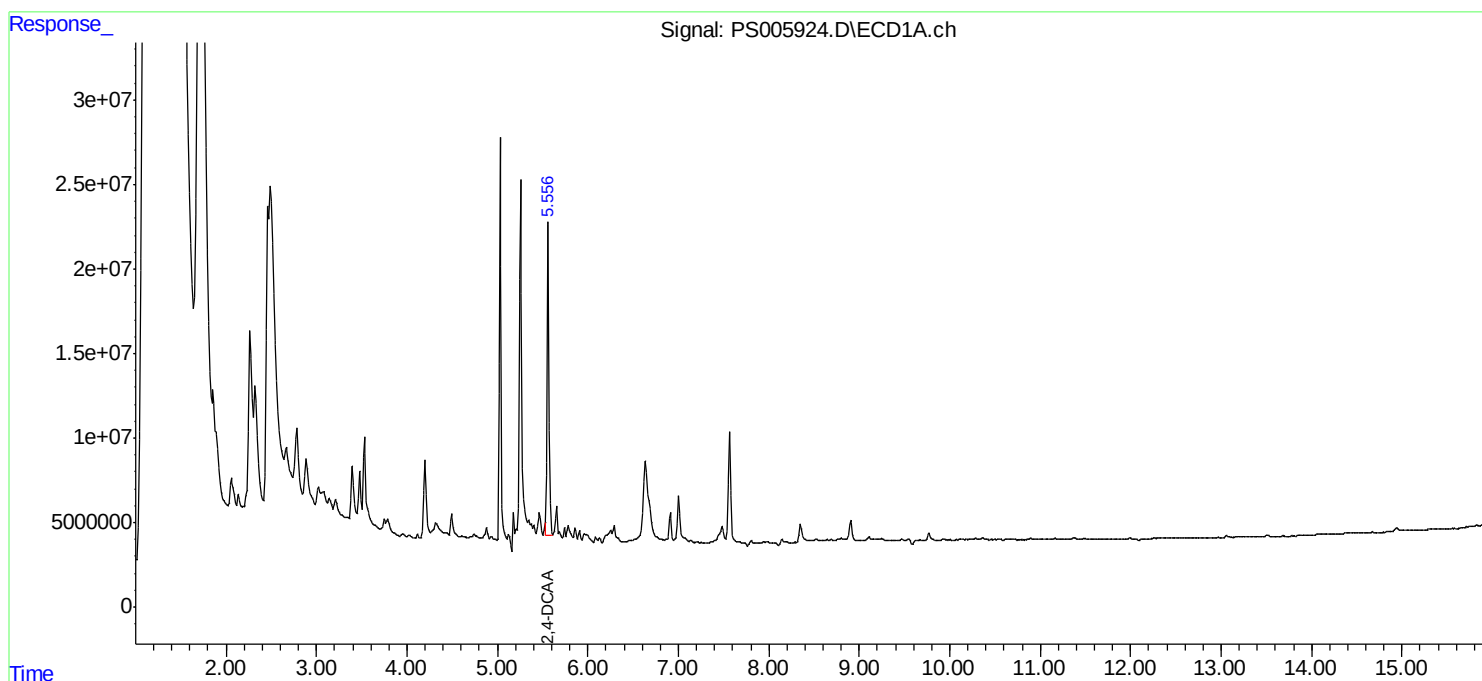

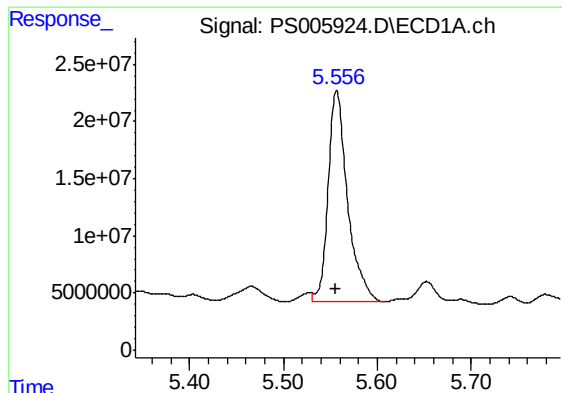


#4 2,4-DCAA

R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 265384395
Conc: 182.92 ng/ml m

Instrument :
ECD_S
ClientSampleId :
1S-A1-A4-COMP-(0-1)

Manual Integrations
APPROVED

Ankita
8/7/2019 5:47:45 PM

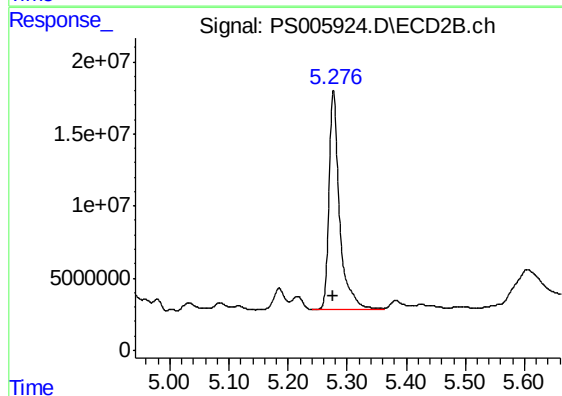

#4 2,4-DCAA

R.T.: 5.277 min
Delta R.T.: 0.001 min
Response: 188254924
Conc: 189.26 ng/ml