

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
 Data File : PS005937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2019 12:19
 Operator : SM\AJ
 Sample : PB121976TB
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 05:24:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.586	5.304	727.8E6	503.6E6	501.637	506.291
Target Compounds							
2) T	3,5-DICHL...	0.000	4.623	0	124.2E6	N.D.	95.753
5) T	DICAMBA	0.000	5.410	0	6151057	N.D.	1.648
6) T	MCP	5.810	5.473	44817781	89034443	9.673	31.260 #
9) T	2,4-D	6.637	0.000	629.5E6	0	420.010	N.D. #
10) T	Pentachlo...	6.872	6.638	19364465	17063234	<MDL	1.314 #
12) T	2,4,5-T	7.594	0.000	116.7E6	0	13.981	N.D. #
14) T	DINOSEB	9.303	0.000	20638861	0	3.178	N.D. #
15) T	Picloram	9.166	9.116	315.2E6	238.3E6	26.925	31.717
16) T	DCPA	9.576	0.000	33659602	0	3.310	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
Data File : PS005937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2019 12:19
Operator : SM\AJ
Sample : PB121976TB
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 05:24:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

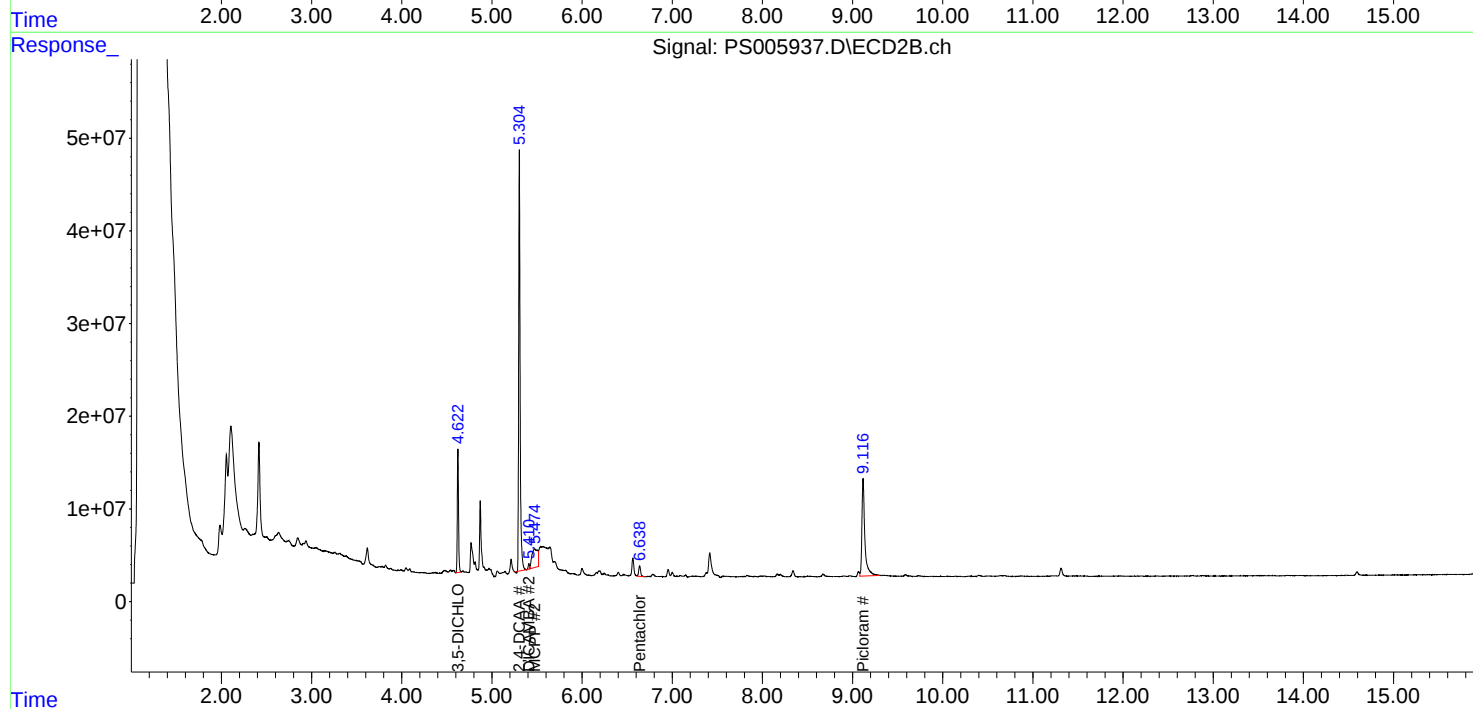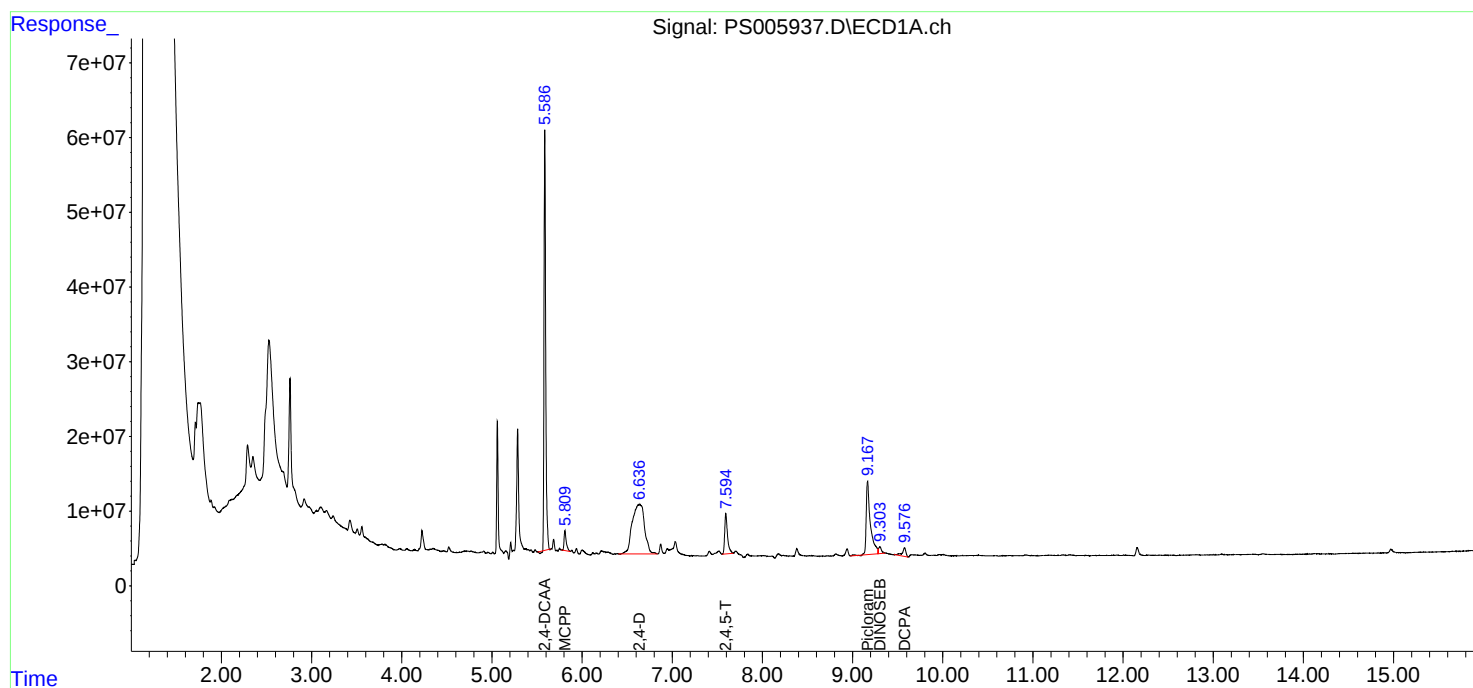


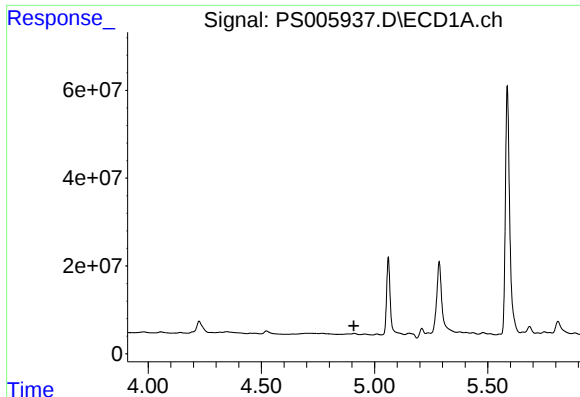

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

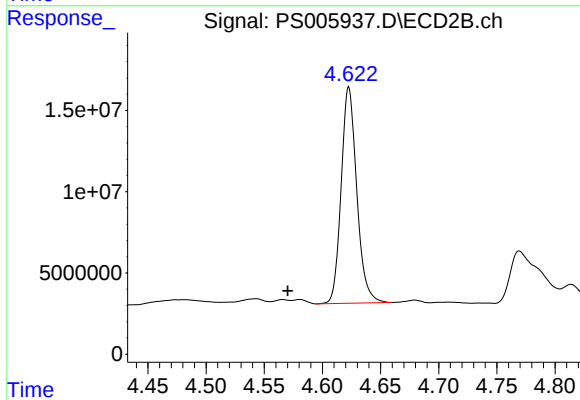


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.623 min
Delta R.T.: 0.053 min
Response: 124222202
Conc: 95.75 ng/ml

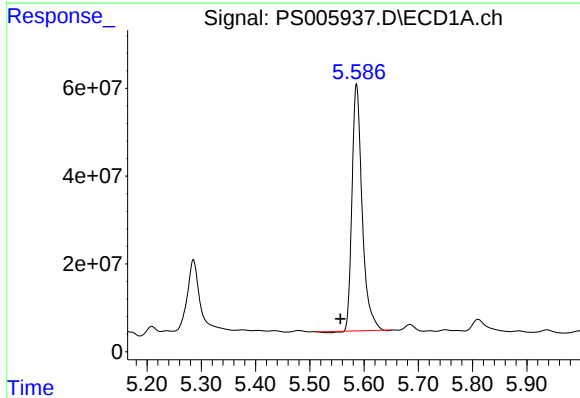


#4 2,4-DCAA

R.T.: 5.586 min
Delta R.T.: 0.030 min
Response: 727783457
Conc: 501.64 ng/ml

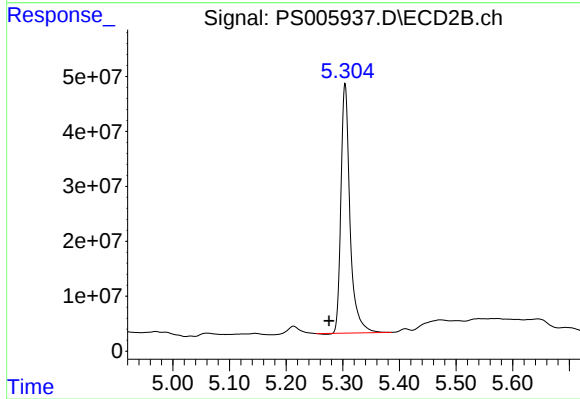

#4 2,4-DCAA


R.T.: 5.304 min
Delta R.T.: 0.028 min
Response: 503596394
Conc: 506.29 ng/ml

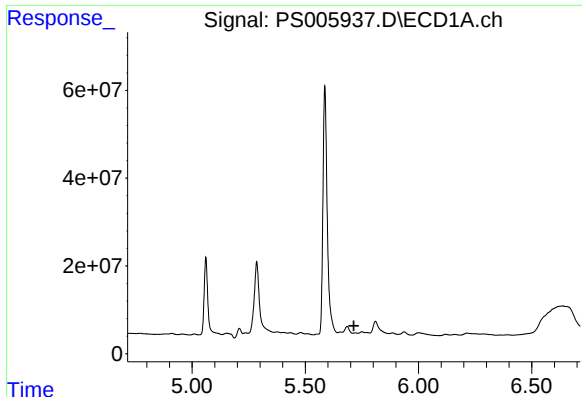

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.714 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

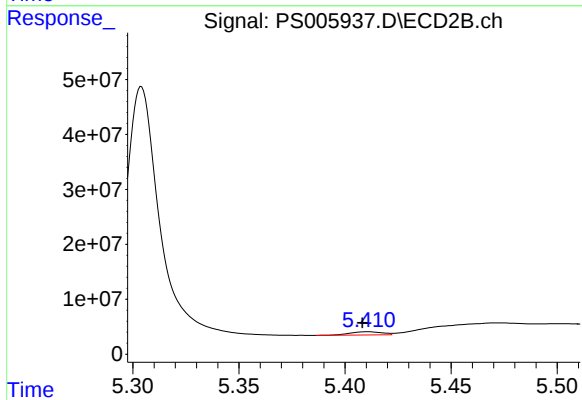


#5 DICAMBA

R.T.: 5.410 min
Delta R.T.: 0.002 min
Response: 6151057
Conc: 1.65 ng/ml

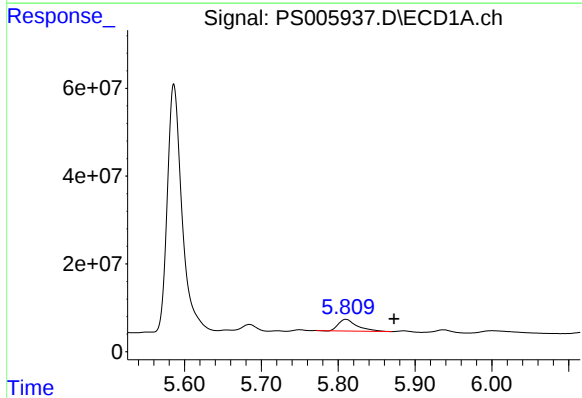


#6 MCP

R.T.: 5.810 min
Delta R.T.: -0.063 min
Response: 44817781
Conc: 9.67 ug/ml

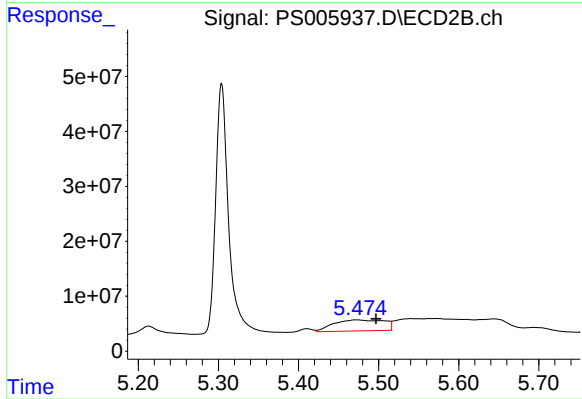

#6 MCP


R.T.: 5.473 min
Delta R.T.: -0.024 min
Response: 89034443
Conc: 31.26 ug/ml

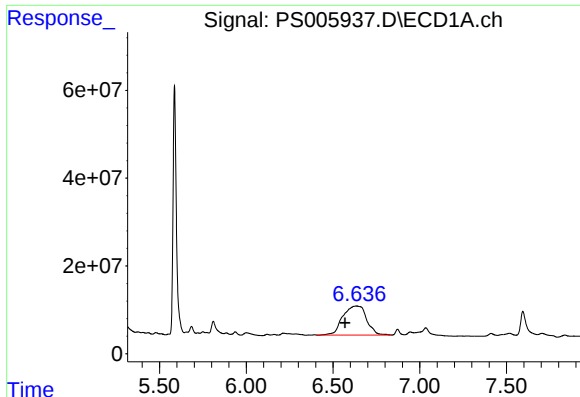

#9 2,4-D


R.T.: 6.637 min
Delta R.T.: 0.068 min
Response: 629456344
Conc: 420.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

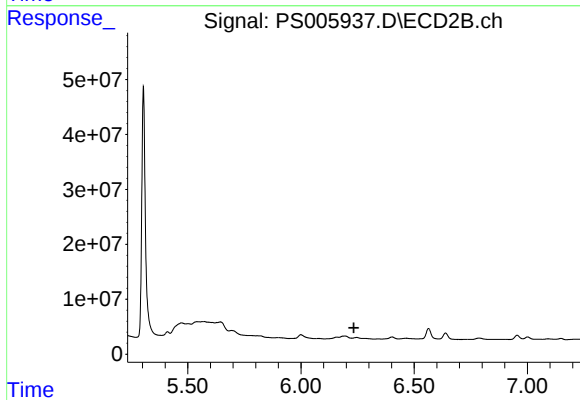


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

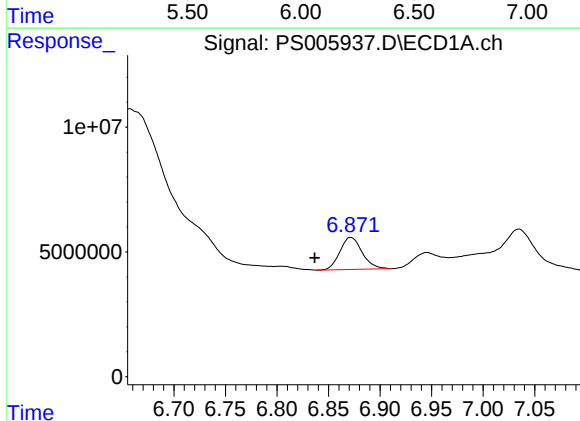


#10 Pentachlorophenol

R.T.: 6.872 min
Delta R.T.: 0.035 min
Response: 19364465
Conc: N.D.

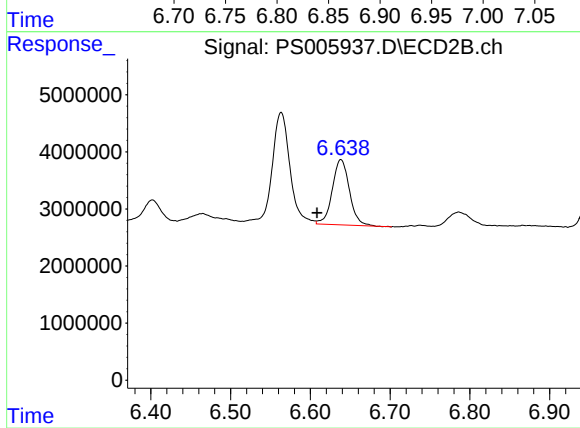

#10 Pentachlorophenol


R.T.: 6.638 min
Delta R.T.: 0.030 min
Response: 17063234
Conc: 1.31 ng/ml

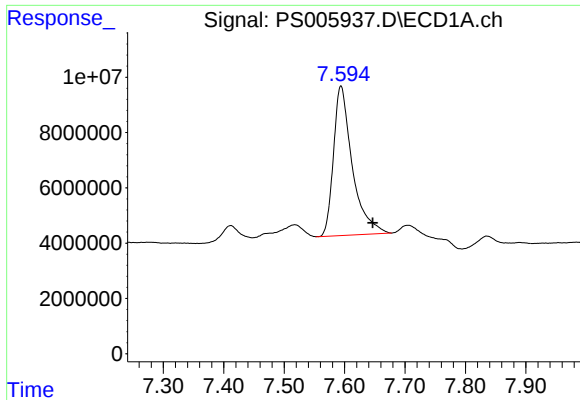

#12 2,4,5-T


R.T.: 7.594 min
Delta R.T.: -0.053 min
Response: 116692474
Conc: 13.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

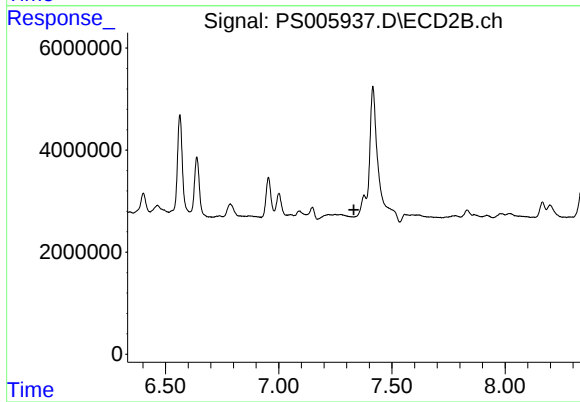


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

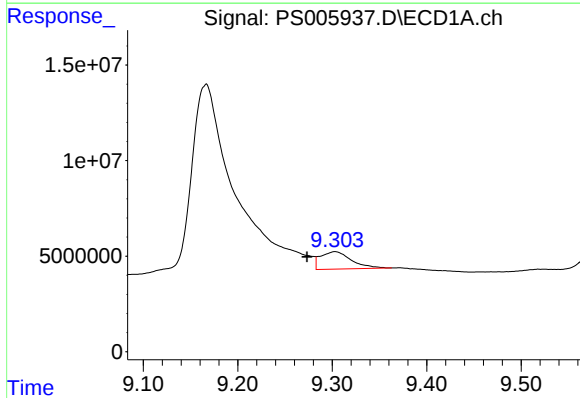


#14 DINOSEB

R.T.: 9.303 min
Delta R.T.: 0.030 min
Response: 20638861
Conc: 3.18 ng/ml

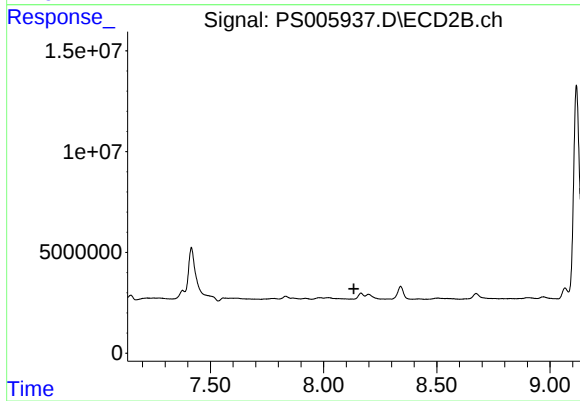

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.134 min
Response: 0
Conc: N.D.

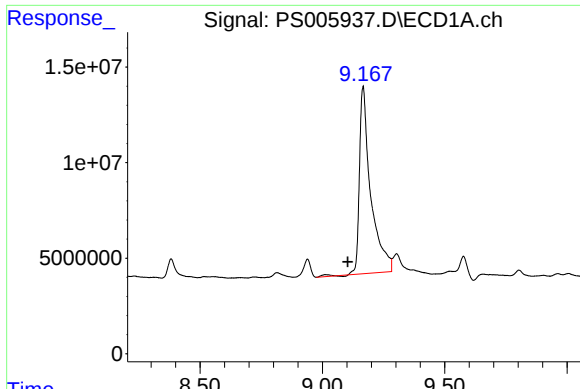

#15 Picloram


R.T.: 9.166 min
Delta R.T.: 0.062 min
Response: 315160386
Conc: 26.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

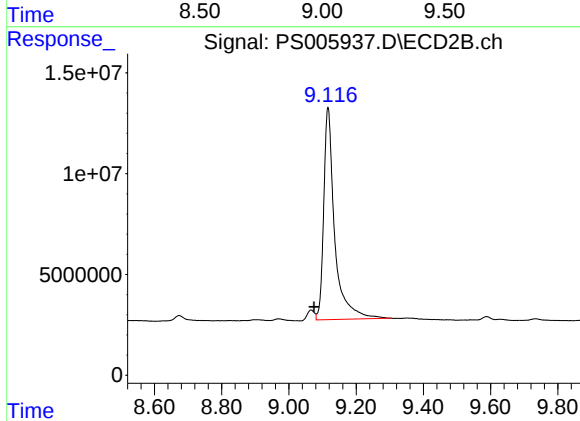


#15 Picloram

R.T.: 9.116 min
Delta R.T.: 0.041 min
Response: 238263311
Conc: 31.72 ng/ml

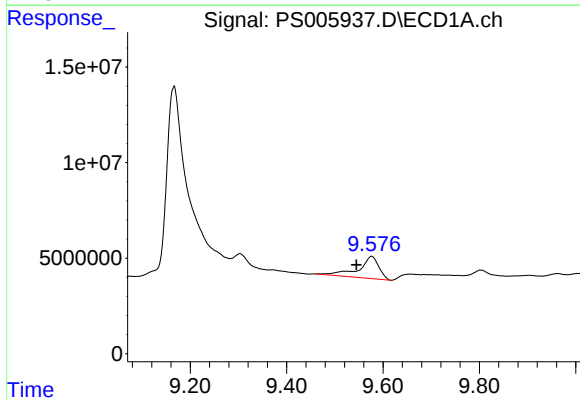

#16 DCPA

R.T.: 9.576 min
Delta R.T.: 0.031 min
Response: 33659602
Conc: 3.31 ng/ml

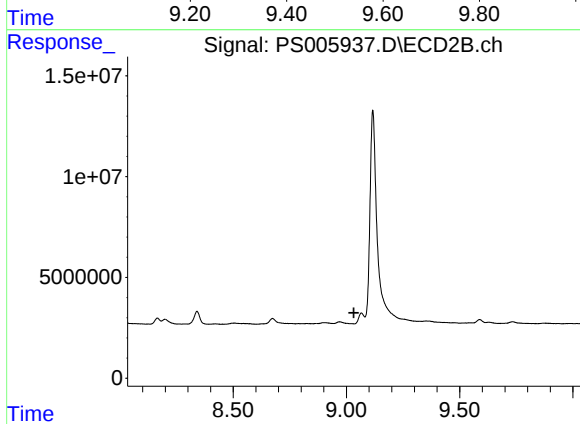

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.033 min
Response: 0
Conc: N.D.