

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
 Data File : PS005938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2019 12:41
 Operator : SM\AJ
 Sample : K4129-15
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 05:24:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.554	5.274	747.5E6	506.4E6	515.221	509.086
Target Compounds							
2) T	3,5-DICHL...	0.000	4.593	0	120.8E6	N.D.	93.150
3) T	4-Nitroph...	5.343	0.000	6079536	0	10.107	N.D. #
5) T	DICAMBA	5.778	0.000	20560824	0	3.443	N.D. #
9) T	2,4-D	6.634	0.000	169.5E6	0	113.077	N.D. #
11) T	2,4,5-TP ...	0.000	6.923	0	18637249	N.D.	3.593



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
Data File : PS005938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2019 12:41
Operator : SM\AJ
Sample : K4129-15
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 05:24:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

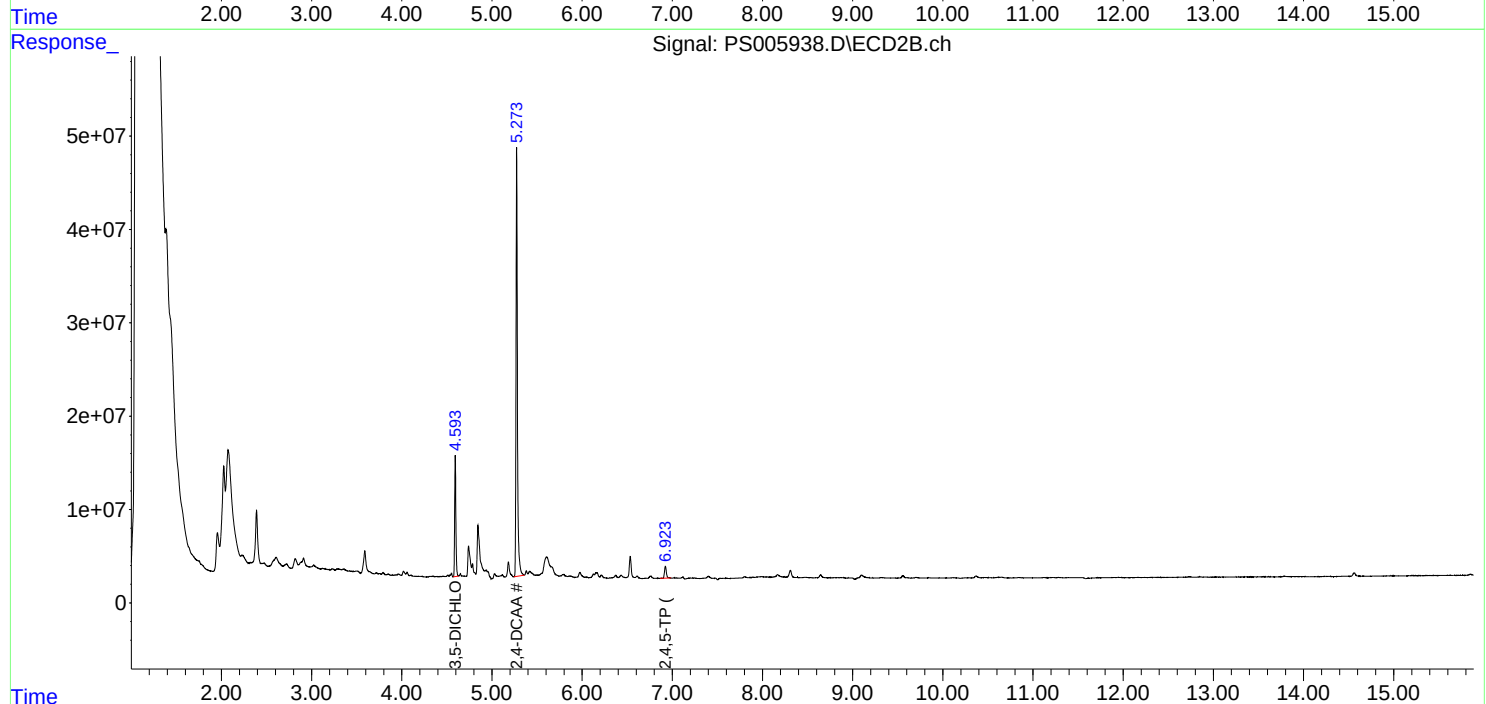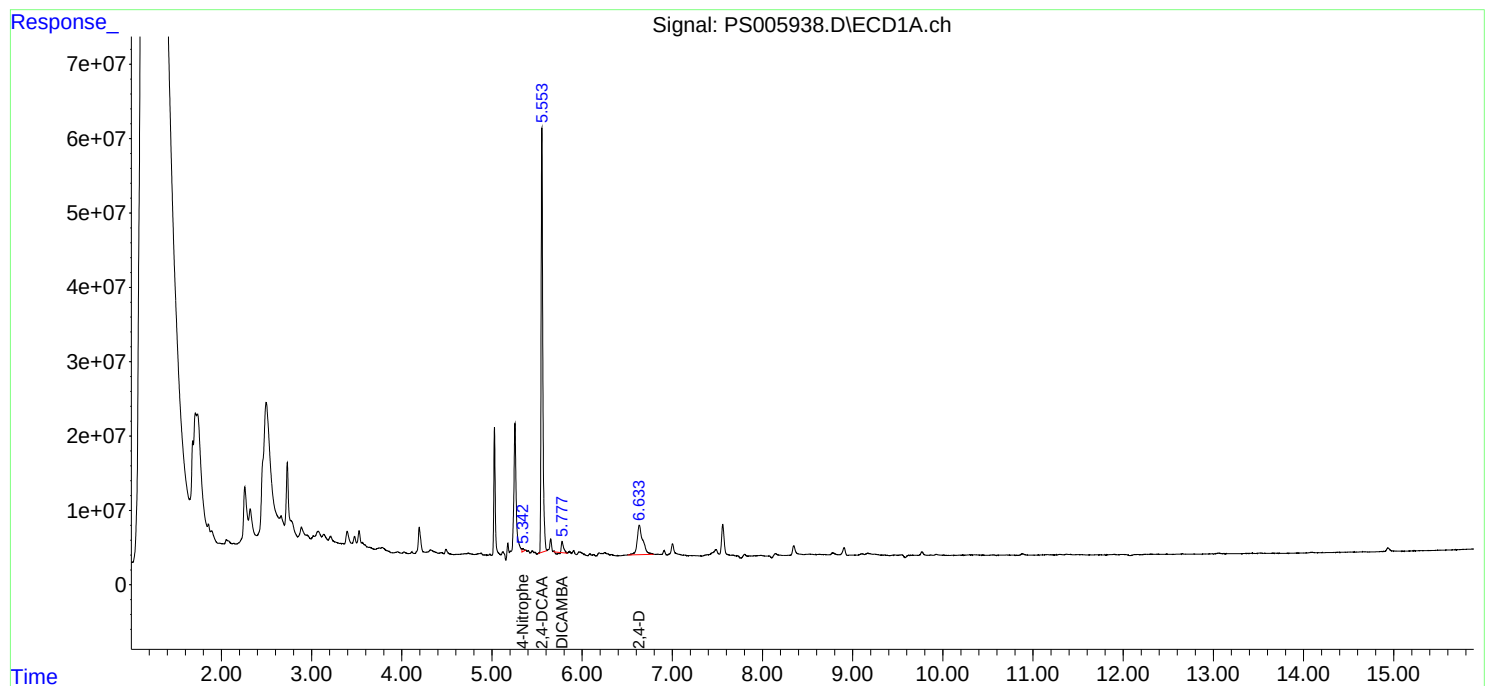


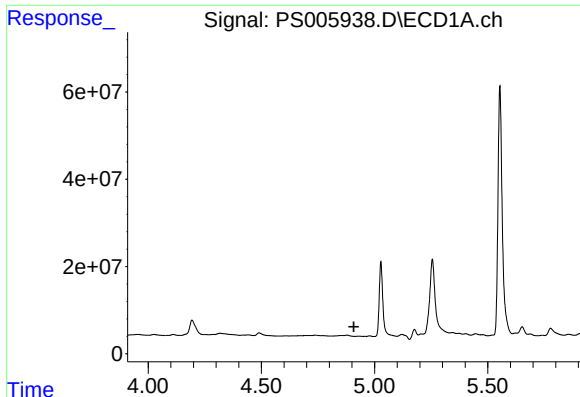

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

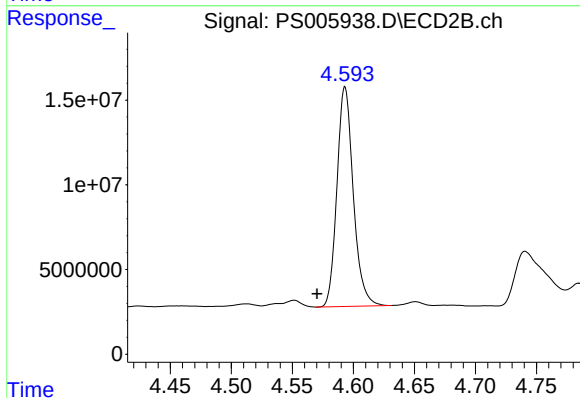


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.593 min
Delta R.T.: 0.023 min
Response: 120844245
Conc: 93.15 ng/ml

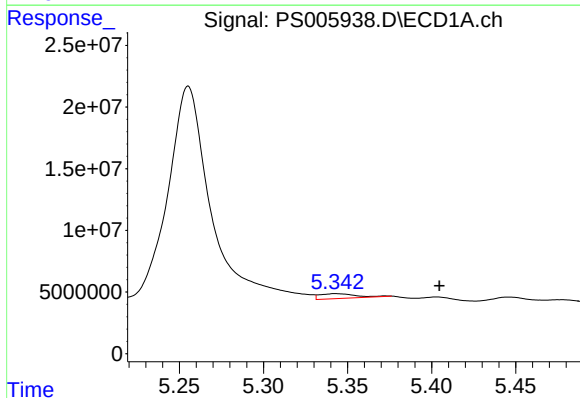


#3 4-Nitrophenol

R.T.: 5.343 min
Delta R.T.: -0.061 min
Response: 6079536
Conc: 10.11 ng/ml

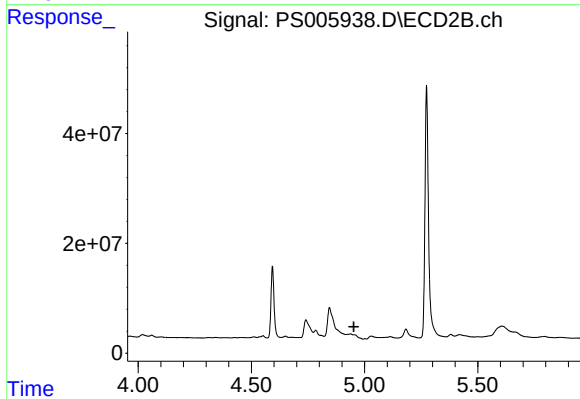

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

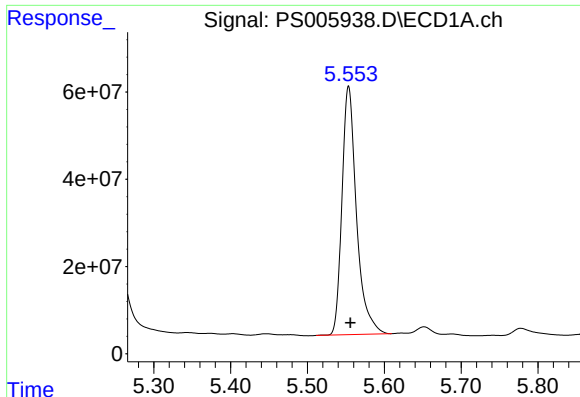

#4 2,4-DCAA


R.T.: 5.554 min
Delta R.T.: -0.003 min
Response: 747491908
Conc: 515.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

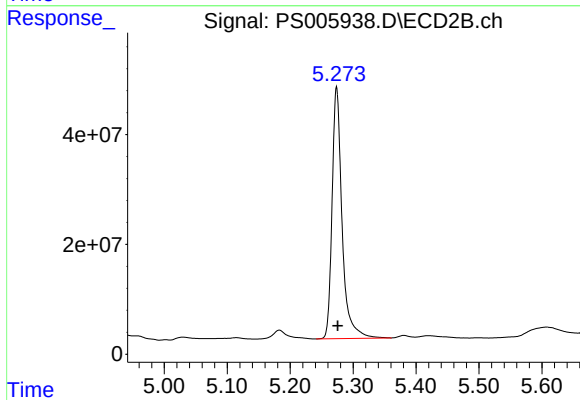


#4 2,4-DCAA

R.T.: 5.274 min
Delta R.T.: -0.002 min
Response: 506377045
Conc: 509.09 ng/ml

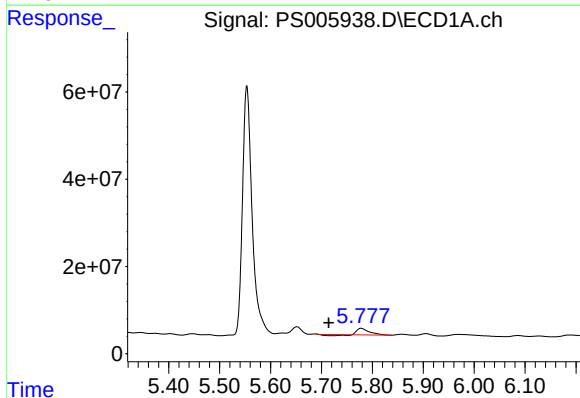


#5 DICAMBA

R.T.: 5.778 min
Delta R.T.: 0.064 min
Response: 20560824
Conc: 3.44 ng/ml

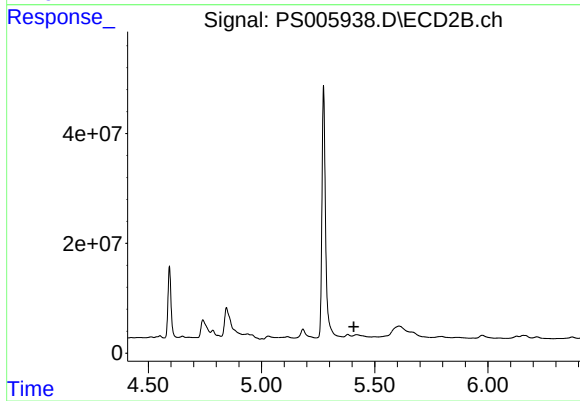

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

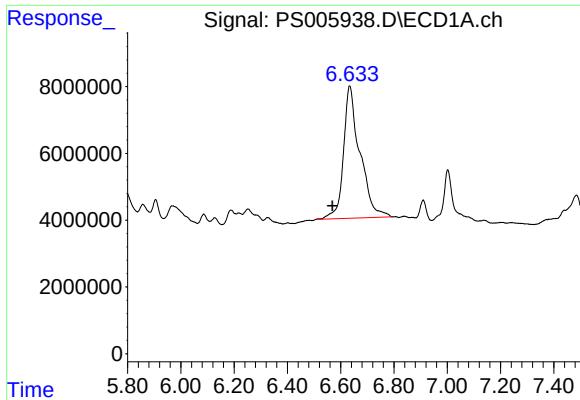

#9 2,4-D


R.T.: 6.634 min
Delta R.T.: 0.065 min
Response: 169465052
Conc: 113.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

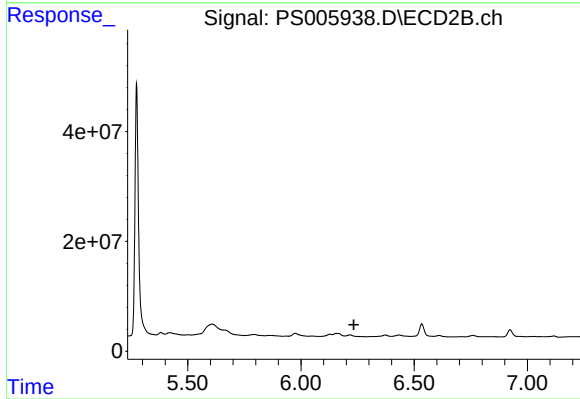


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

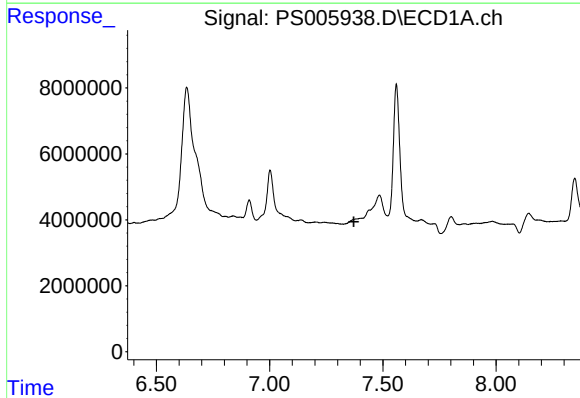

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.372 min
Response: 0
Conc: N.D.

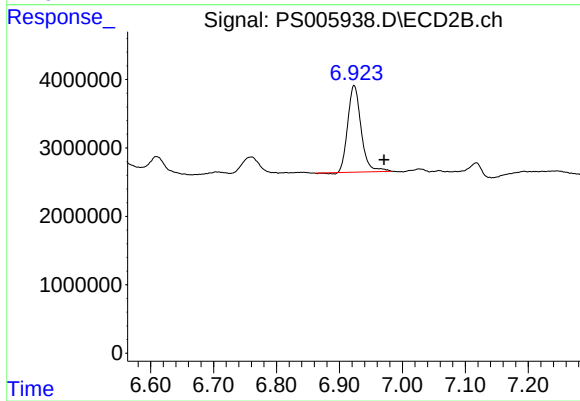

#11 2,4,5-TP (SILVEX)

R.T.: 6.923 min
Delta R.T.: -0.047 min
Response: 18637249
Conc: 3.59 ng/ml