

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
 Data File : PS005949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2019 17:09
 Operator : SM\AJ
 Sample : K4130-40
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 05:27:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.591	5.312	588.2E6	393.9E6	405.410	396.046
Target Compounds							
2) T	3,5-DICHL...	0.000	4.631	0	131.6E6	N.D.	101.458
3) T	4-Nitroph...	0.000	4.893	0	37634604	N.D.	75.971
5) T	DICAMBA	5.689	0.000	10736082	0	1.798	N.D. #
7) T	MCPA	0.000	5.645	0	116.5E6	N.D.	27.674
10) T	Pentachlo...	0.000	6.571	0	27971567	N.D.	2.154
11) T	2,4,5-TP ...	0.000	6.960	0	58272685	N.D.	11.234
12) T	2,4,5-T	7.604	0.000	134.3E6	0	16.088	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
Data File : PS005949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2019 17:09
Operator : SM\AJ
Sample : K4130-40
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 05:27:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

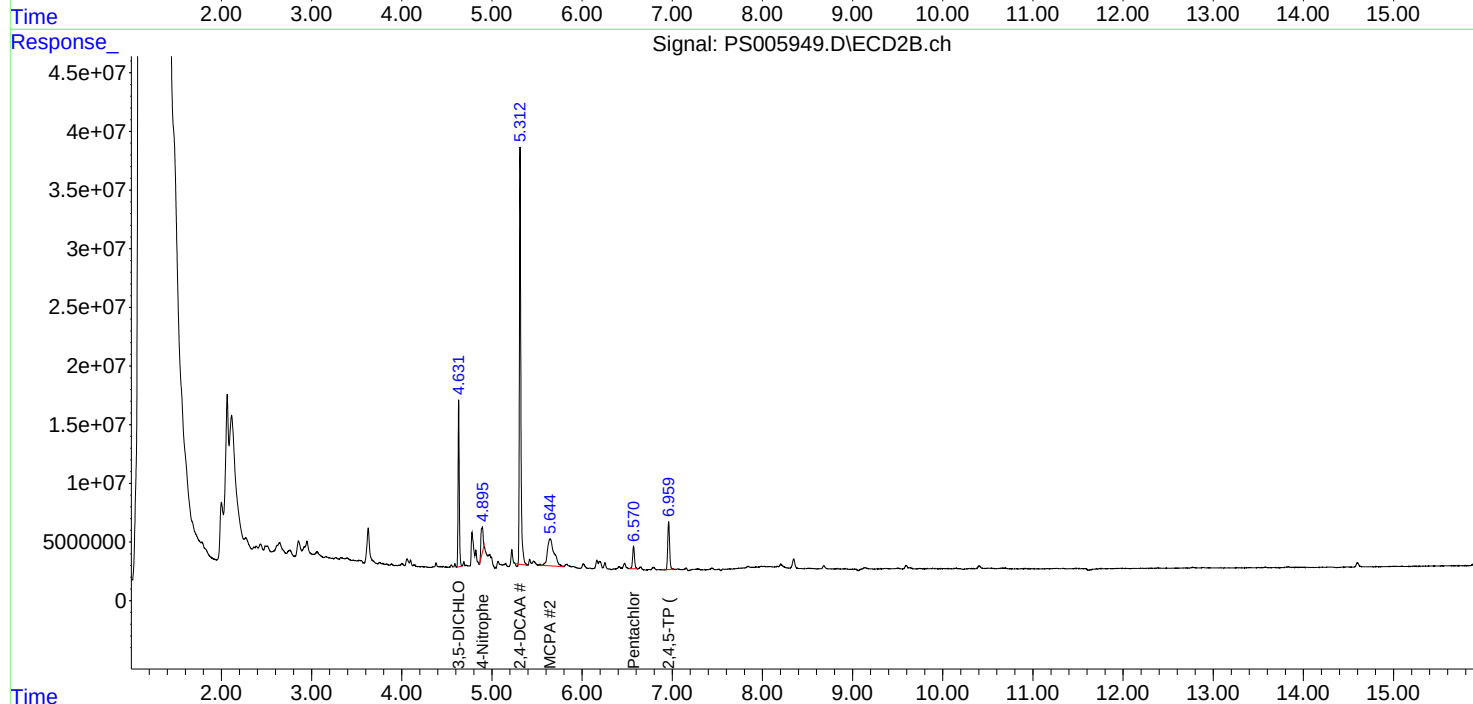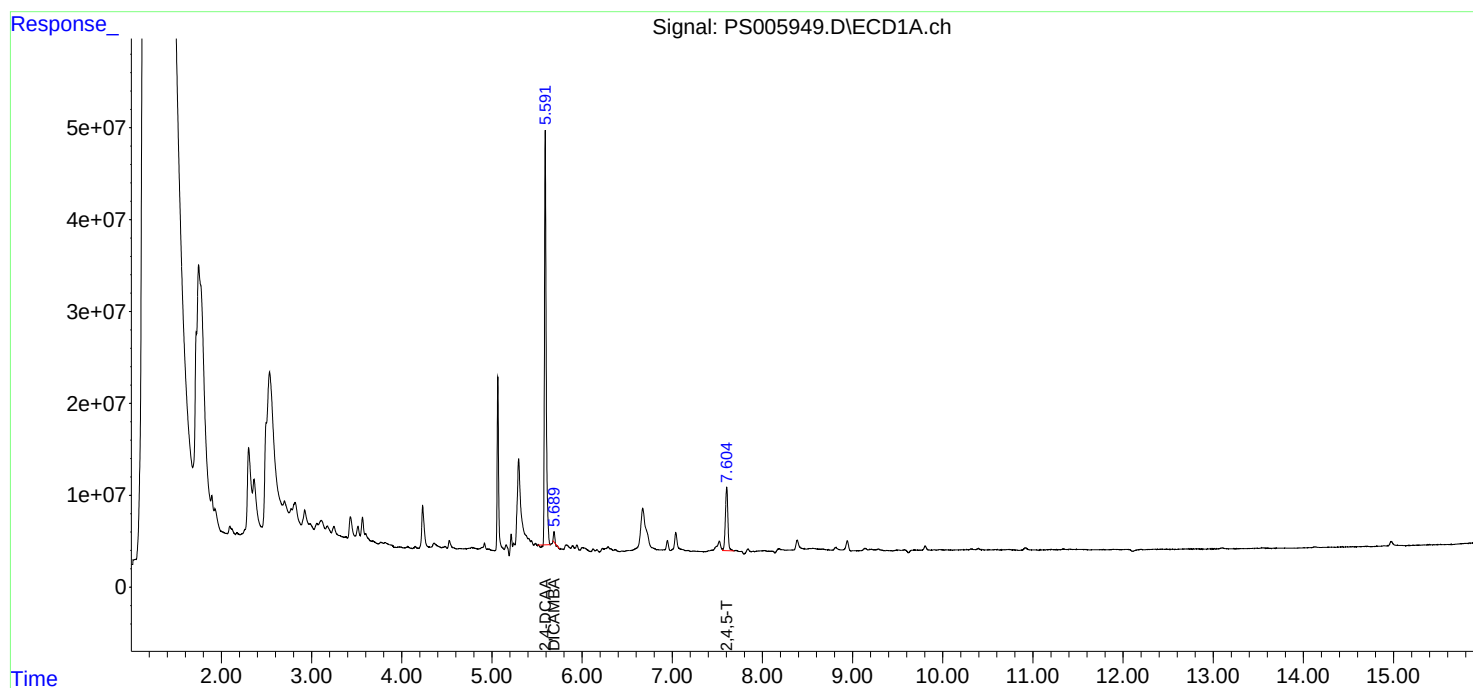


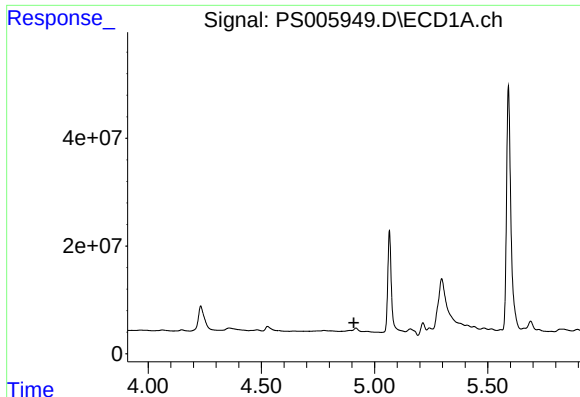

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

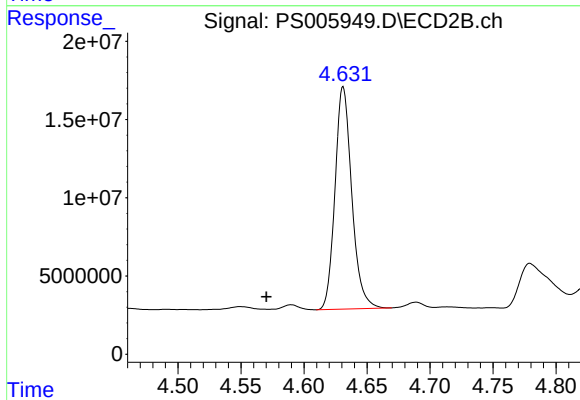


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.631 min
Delta R.T.: 0.061 min
Response: 131623092
Conc: 101.46 ng/ml

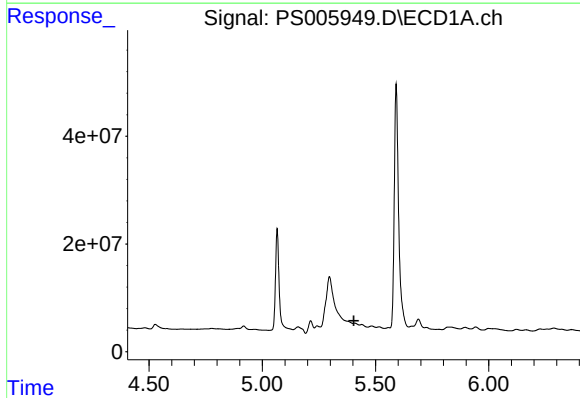


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

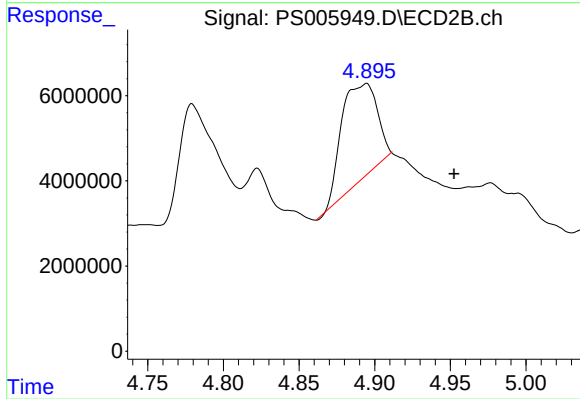

#3 4-Nitrophenol


R.T.: 4.893 min
Delta R.T.: -0.059 min
Response: 37634604
Conc: 75.97 ng/ml

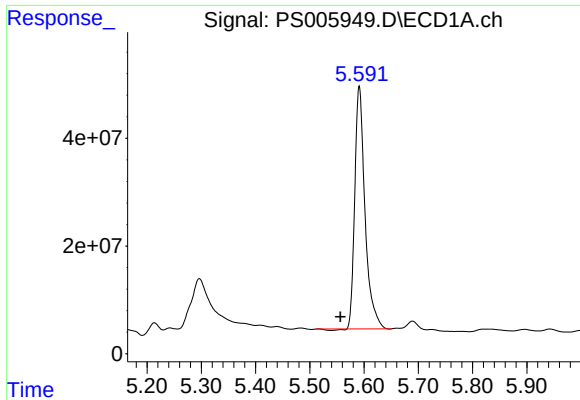

#4 2,4-DCAA


R.T.: 5.591 min
Delta R.T.: 0.035 min
Response: 588176414
Conc: 405.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

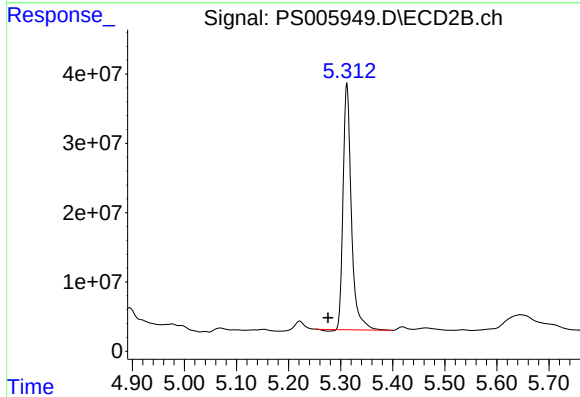


#4 2,4-DCAA

R.T.: 5.312 min
Delta R.T.: 0.036 min
Response: 393938707
Conc: 396.05 ng/ml

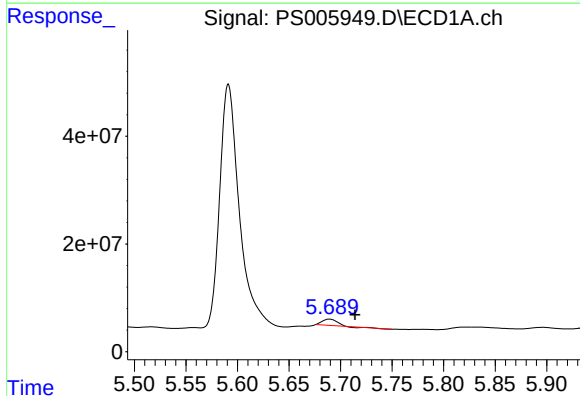


#5 DICAMBA

R.T.: 5.689 min
Delta R.T.: -0.025 min
Response: 10736082
Conc: 1.80 ng/ml

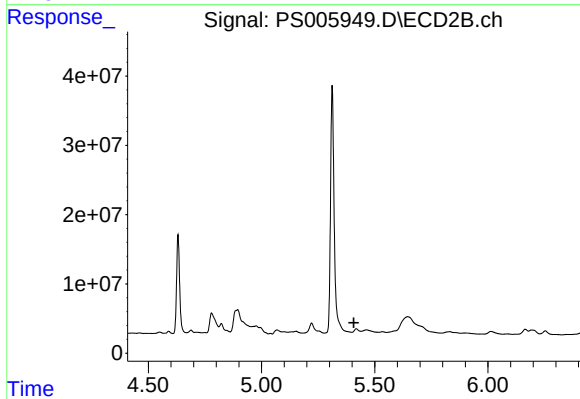

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

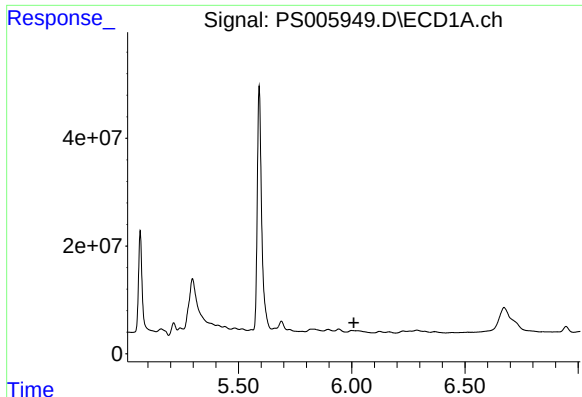

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

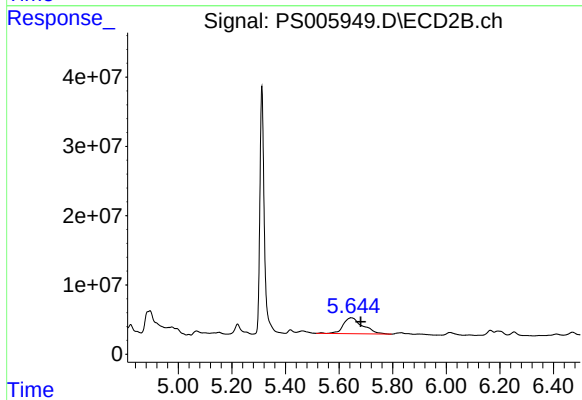


#7 MCPA

R.T.: 5.645 min
Delta R.T.: -0.035 min
Response: 116479337
Conc: 27.67 ug/ml

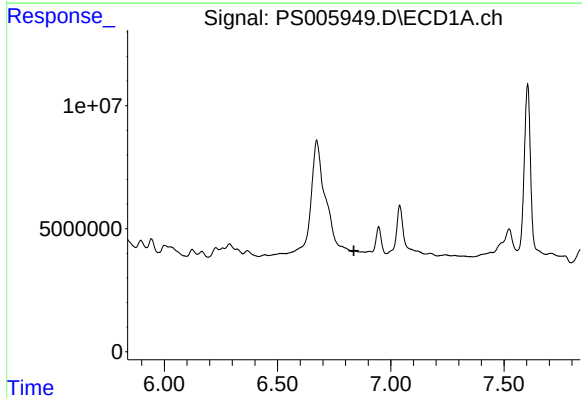


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

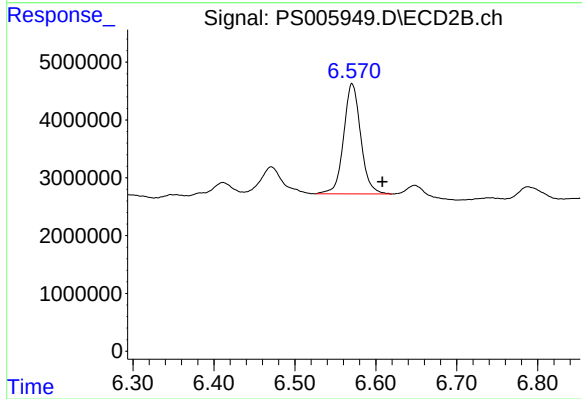

#10 Pentachlorophenol


R.T.: 6.571 min
Delta R.T.: -0.037 min
Response: 27971567
Conc: 2.15 ng/ml

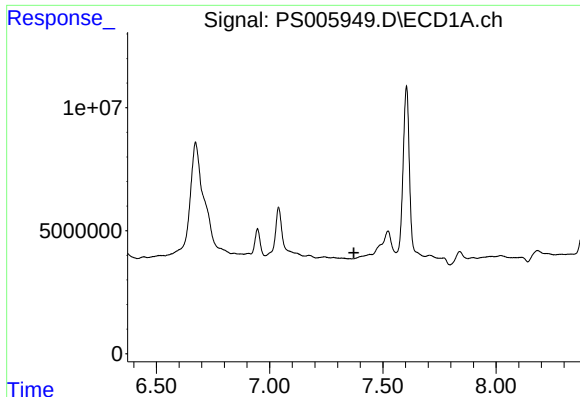

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

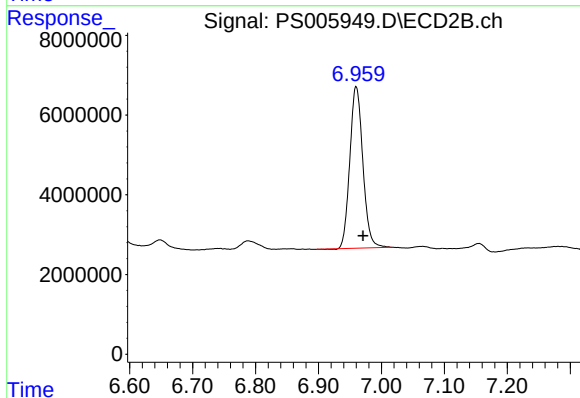


#11 2,4,5-TP (SILVEX)

R.T.: 6.960 min
Delta R.T.: -0.011 min
Response: 58272685
Conc: 11.23 ng/ml

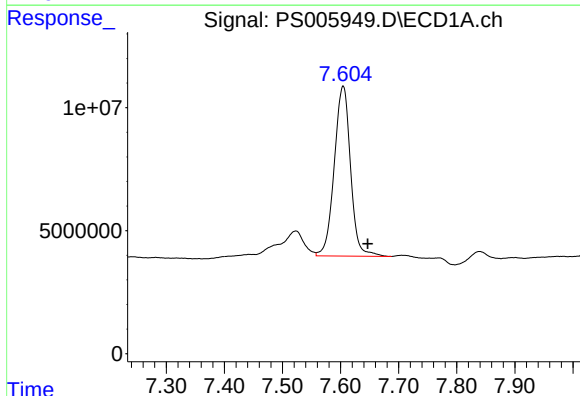

#12 2,4,5-T

R.T.: 7.604 min
Delta R.T.: -0.043 min
Response: 134278282
Conc: 16.09 ng/ml

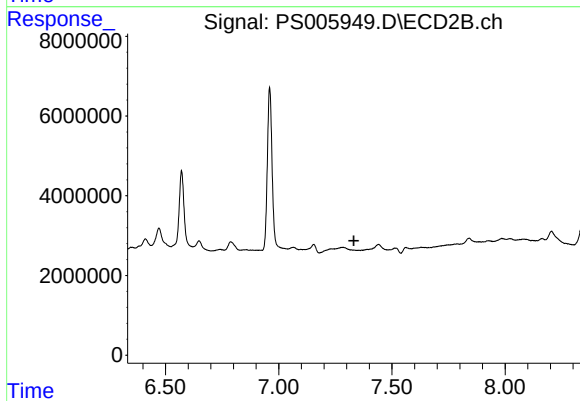

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.