

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
 Data File : PS005959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2019 20:51
 Operator : SM\AJ
 Sample : K4135-36
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 05:30:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.552	5.273	597.1E6	410.5E6	411.545	412.708
Target Compounds							
2) T	3,5-DICHL...	0.000	4.592	0	163.7E6	N.D.	126.205
3) T	4-Nitroph...	5.343	0.000	10791954	0	17.941	N.D. #
9) T	2,4-D	6.633	0.000	251.3E6	0	167.657	N.D. #
10) T	Pentachlo...	6.906	0.000	17010258	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.922	0	49415721	N.D.	9.526
12) T	2,4,5-T	0.000	7.388	0	36387253	N.D.	7.654
15) T	Picloram	9.138	9.087	238.9E6	139.8E6	20.412	18.613
16) T	DCPA	0.000	9.087	0	139.8E6	N.D.	21.204



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
Data File : PS005959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2019 20:51
Operator : SM\AJ
Sample : K4135-36
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 05:30:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

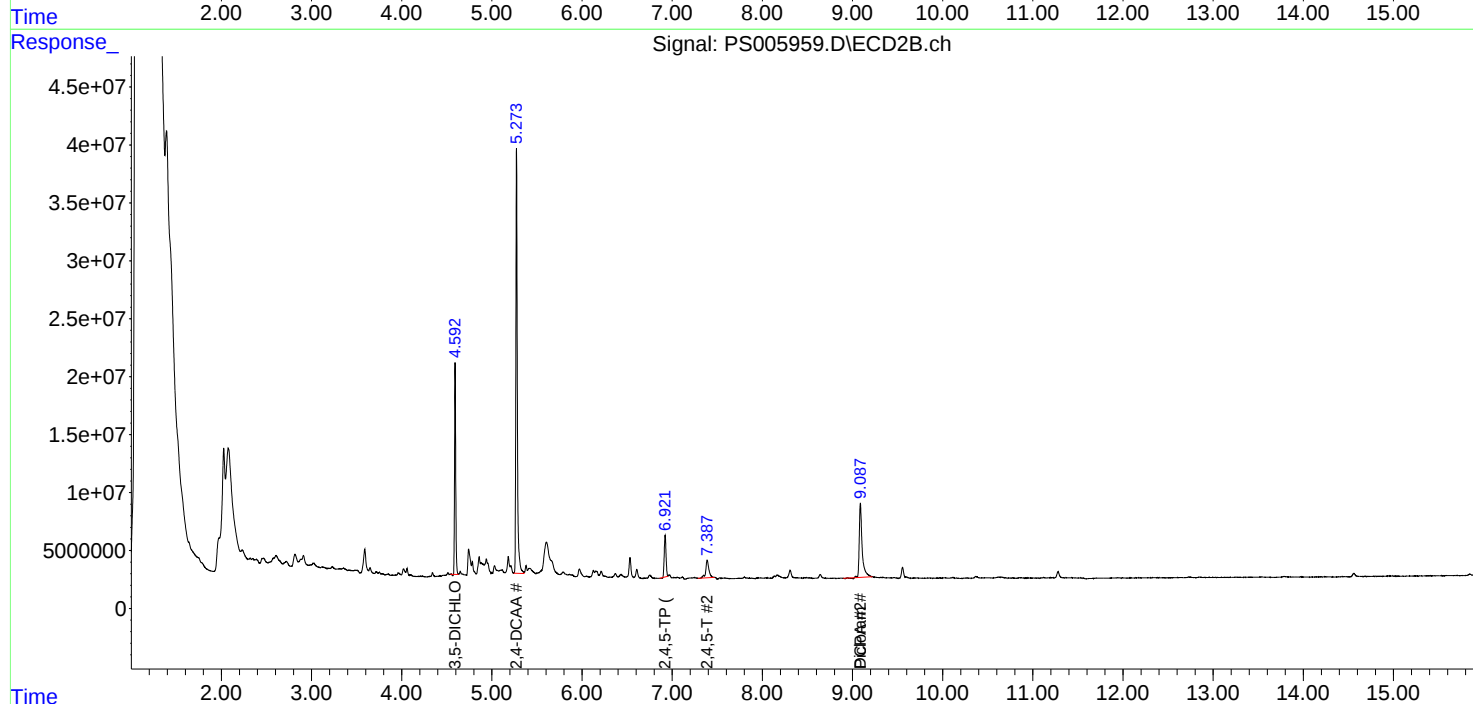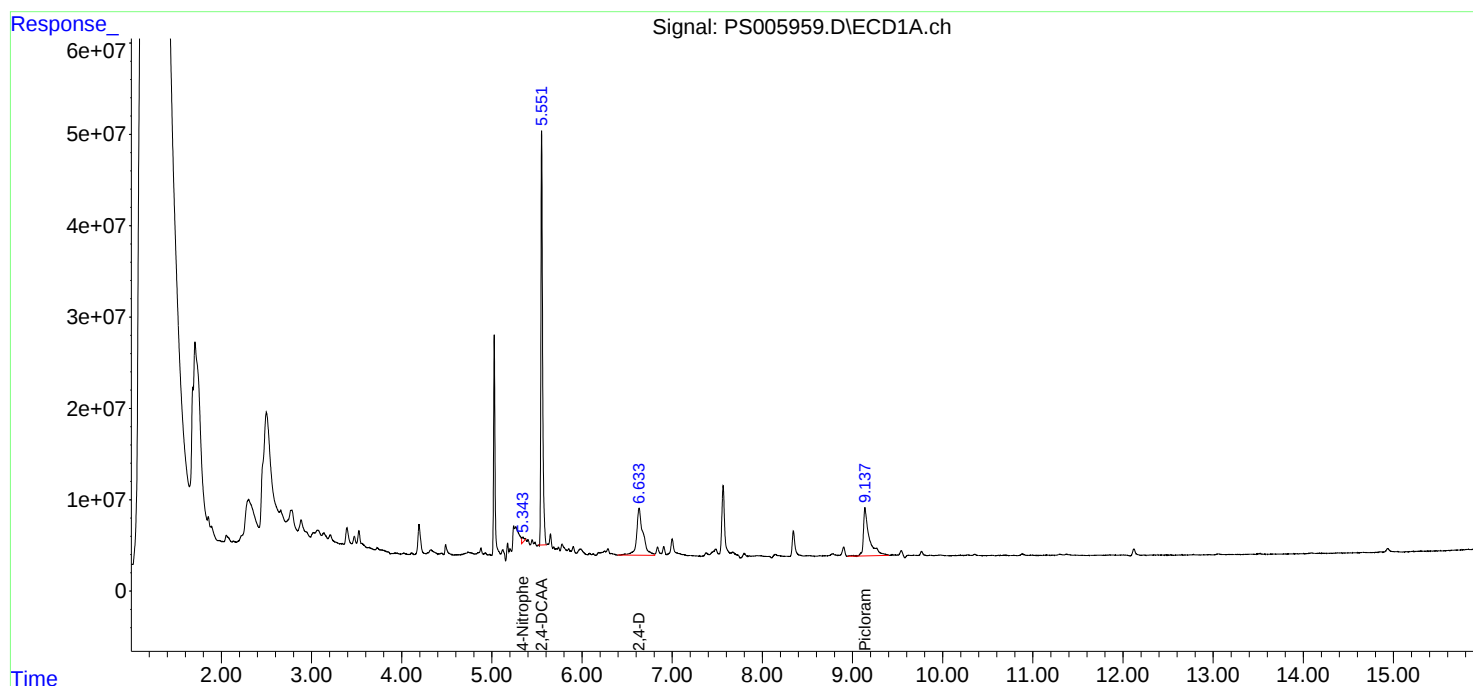


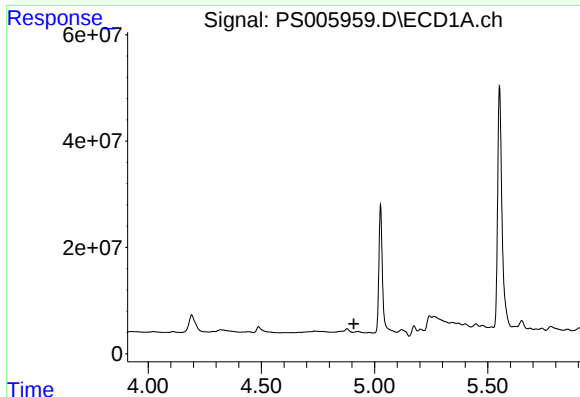

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

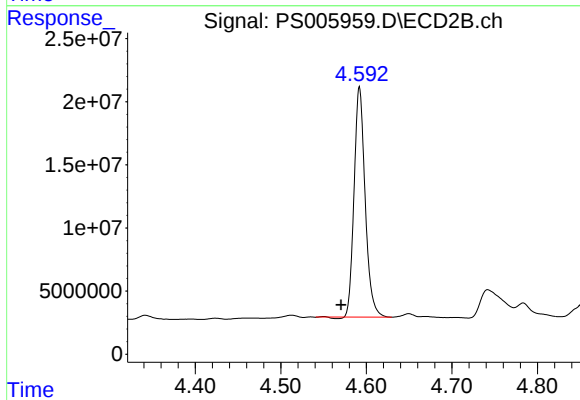


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.592 min
Delta R.T.: 0.022 min
Response: 163727940
Conc: 126.21 ng/ml

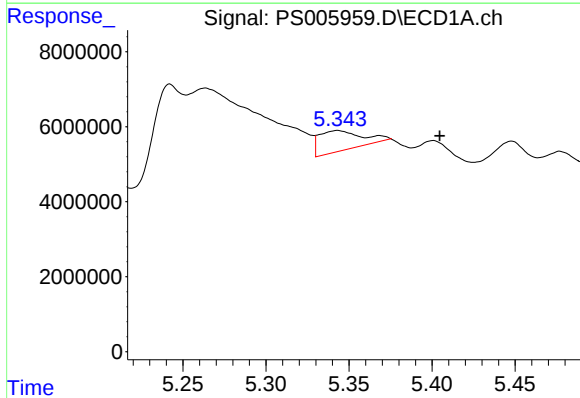


#3 4-Nitrophenol

R.T.: 5.343 min
Delta R.T.: -0.062 min
Response: 10791954
Conc: 17.94 ng/ml

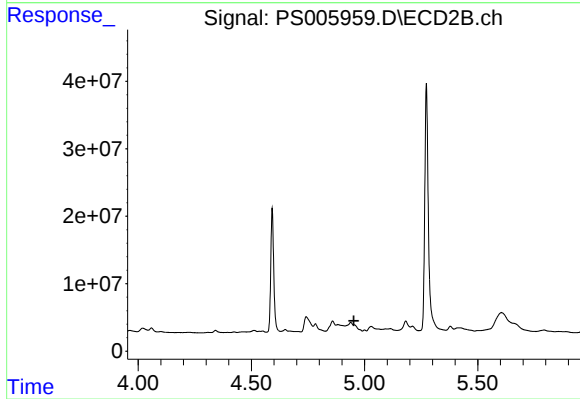

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

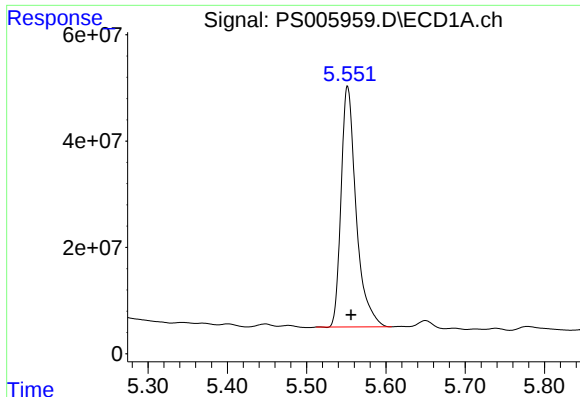

#4 2,4-DCAA


R.T.: 5.552 min
Delta R.T.: -0.004 min
Response: 597077378
Conc: 411.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

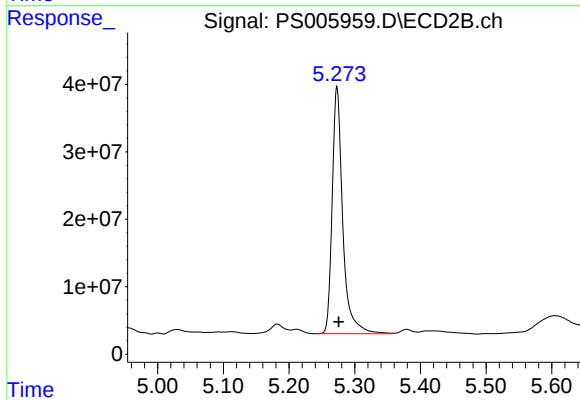


#4 2,4-DCAA

R.T.: 5.273 min
Delta R.T.: -0.003 min
Response: 410511536
Conc: 412.71 ng/ml

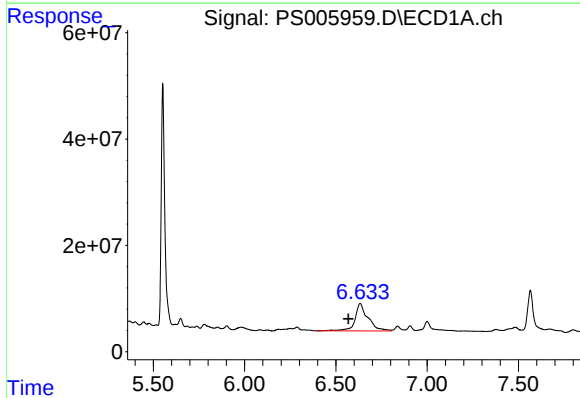


#9 2,4-D

R.T.: 6.633 min
Delta R.T.: 0.064 min
Response: 251262428
Conc: 167.66 ng/ml

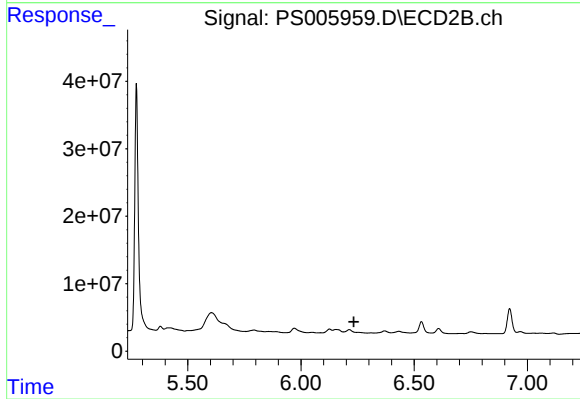

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.

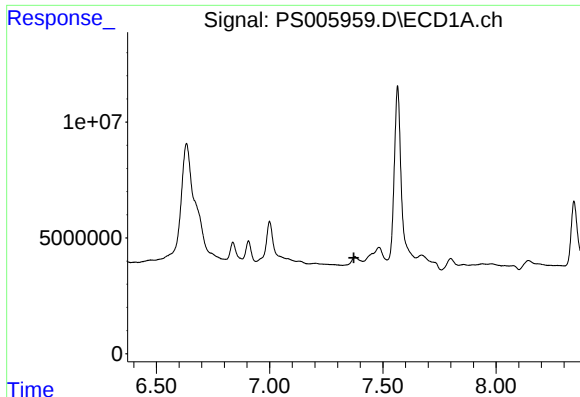

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

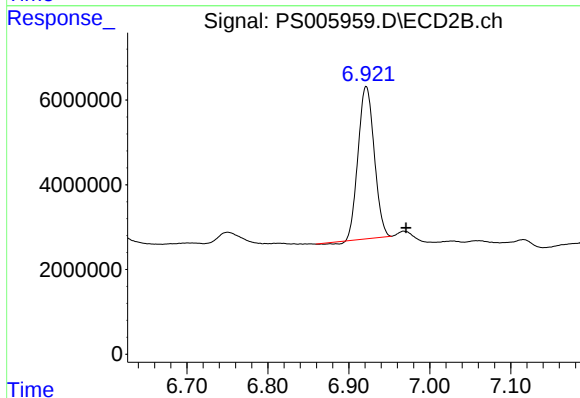


#11 2,4,5-TP (SILVEX)

R.T.: 6.922 min
Delta R.T.: -0.049 min
Response: 49415721
Conc: 9.53 ng/ml

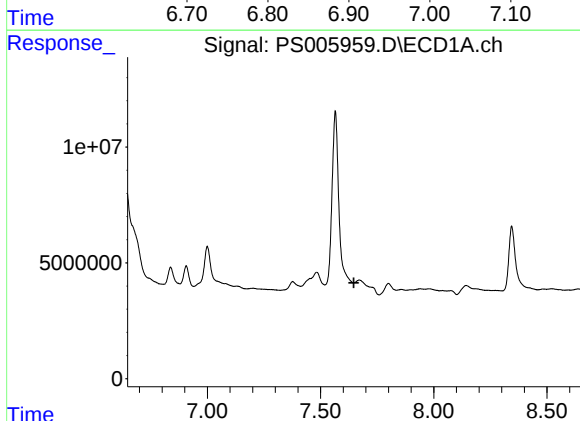


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.647 min
Response: 0
Conc: N.D.

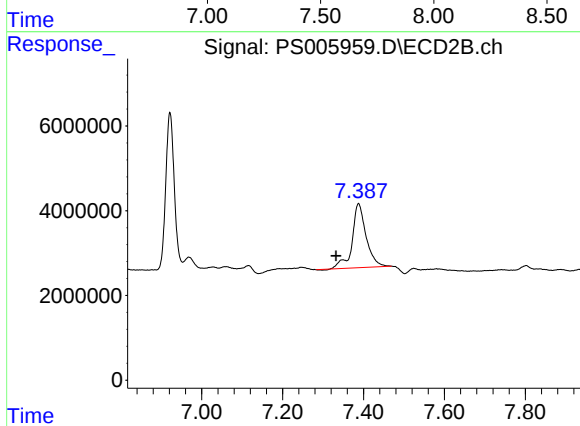

#12 2,4,5-T


R.T.: 7.388 min
Delta R.T.: 0.056 min
Response: 36387253
Conc: 7.65 ng/ml

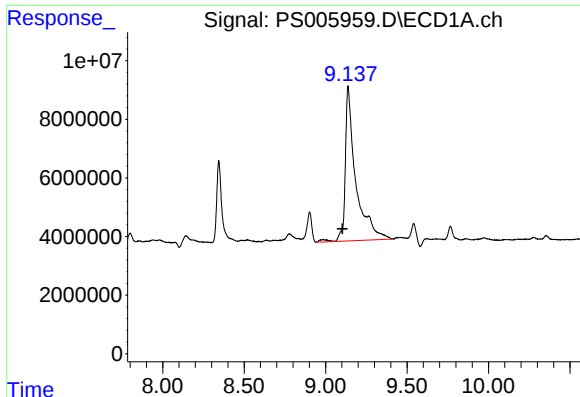

#15 Picloram


R.T.: 9.138 min
Delta R.T.: 0.034 min
Response: 238917635
Conc: 20.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

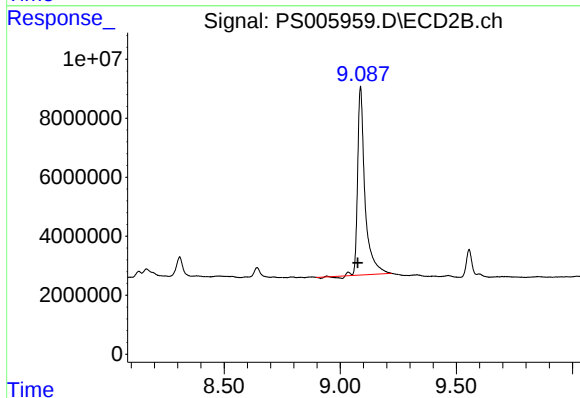


#15 Picloram

R.T.: 9.087 min
Delta R.T.: 0.012 min
Response: 139822330
Conc: 18.61 ng/ml

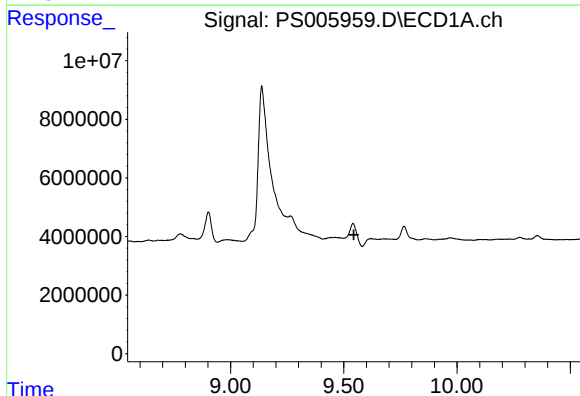

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.545 min
Response: 0
Conc: N.D.

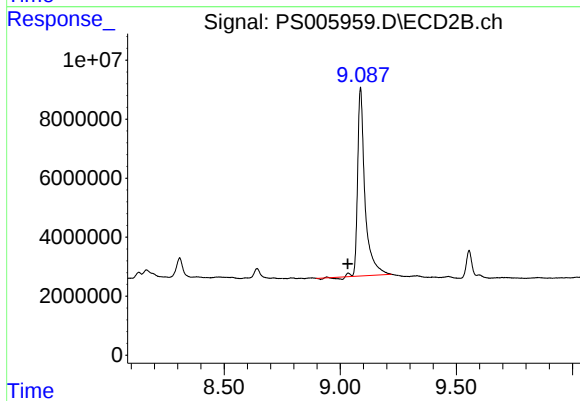

#16 DCPA

R.T.: 9.087 min
Delta R.T.: 0.054 min
Response: 139822330
Conc: 21.20 ng/ml