

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
 Data File : PS005949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2019 17:09
 Operator : SM\AJ
 Sample : K4130-40
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 1S-H-(0-30)-COMP

Manual Integrations
 APPROVED

Ankita
 8/8/2019 2:45:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 05:27:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	5.591	5.312	598.4E6	403.5E6	412.448m 405.645m
------	----------	-------	-------	---------	---------	-------------------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080719\
Data File : PS005949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2019 17:09
Operator : SM\AJ
Sample : K4130-40
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
1S-H-(0-30)-COMP


Manual Integrations
APPROVED

Ankita
8/8/2019 2:45:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 05:27:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

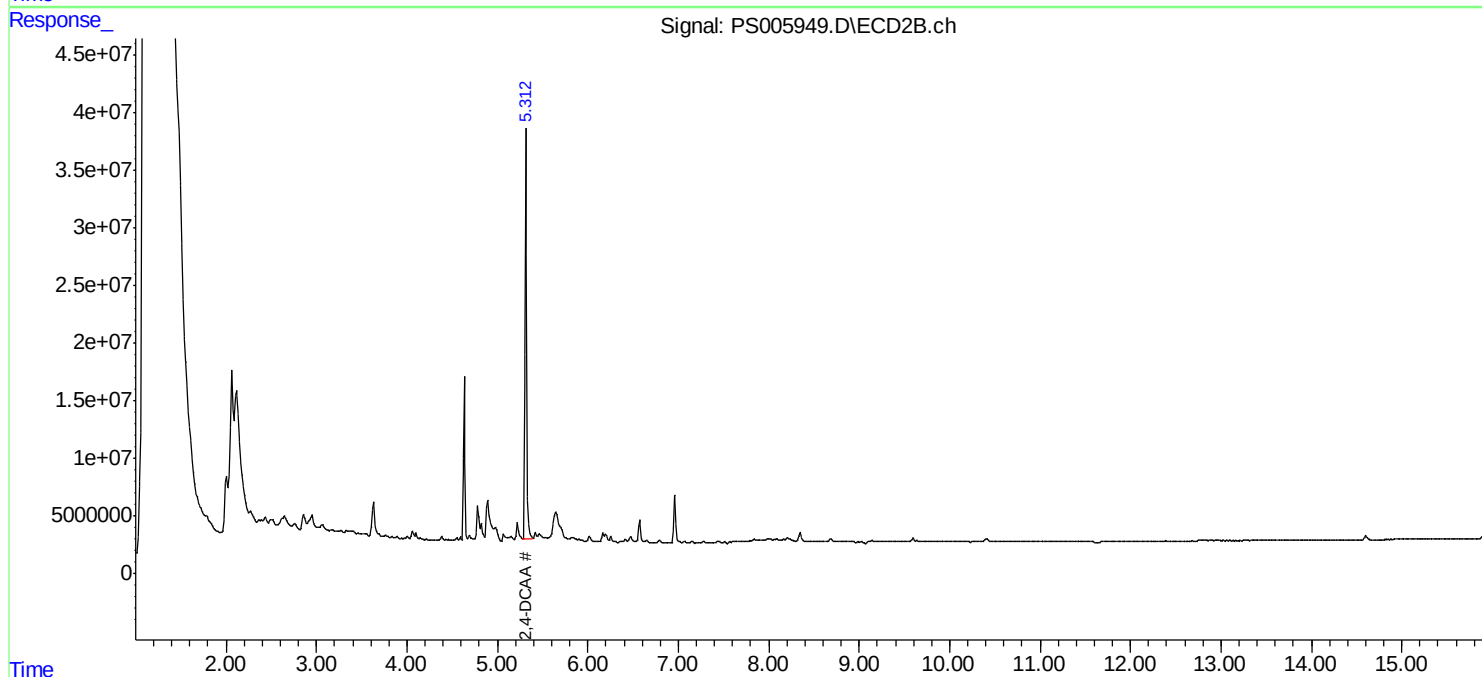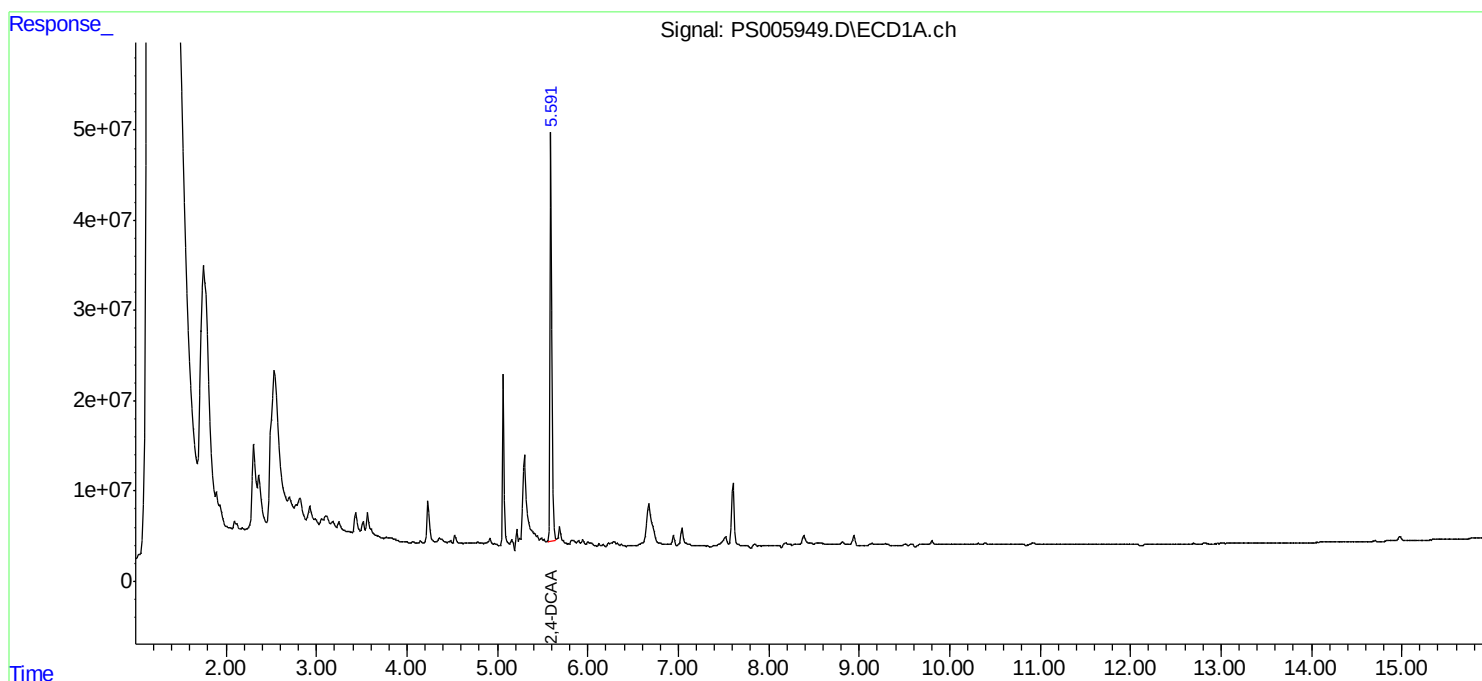

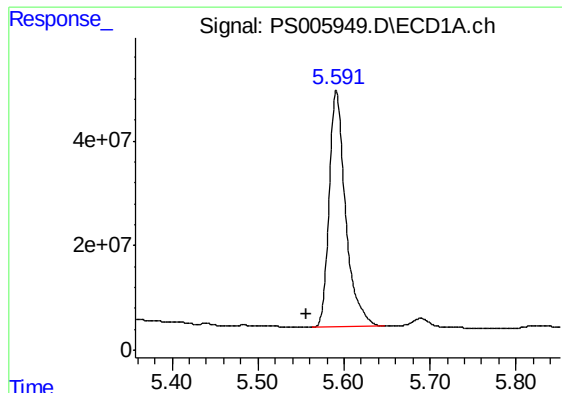


#4 2,4-DCAA

R.T.: 5.591 min
Delta R.T.: 0.035 min
Response: 598387045
Conc: 412.45 ng/ml m

Instrument :
ECD_S
ClientSampleId :
1S-H-(0-30)-COMP

Manual Integrations
APPROVED

Ankita
8/8/2019 2:45:21 PM

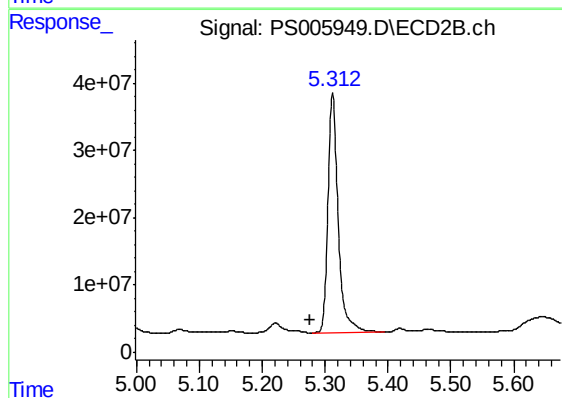

#4 2,4-DCAA

R.T.: 5.312 min
Delta R.T.: 0.036 min
Response: 403486201
Conc: 405.64 ng/ml m