

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080720\
 Data File : PS011657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2020 08:50
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 05:56:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.483	0.000	17804570	0	13.305	N.D.	#
5) T	DICAMBA	0.000	7.153	0	10964219	N.D.	4.788	
6) T	MCP	0.000	7.153	0	10964219	N.D.	5.746	
8) T	DICHLORPROP	0.000	7.758	0	3440650	N.D.	5.716	
11) T	2,4,5-TP ...	0.000	8.850	0	2402931	N.D.	<MDL	
15) T	Picloram	10.986	11.031	18404922	6241565	2.917	1.427	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080720\
Data File : PS011657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2020 08:50
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 05:56:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

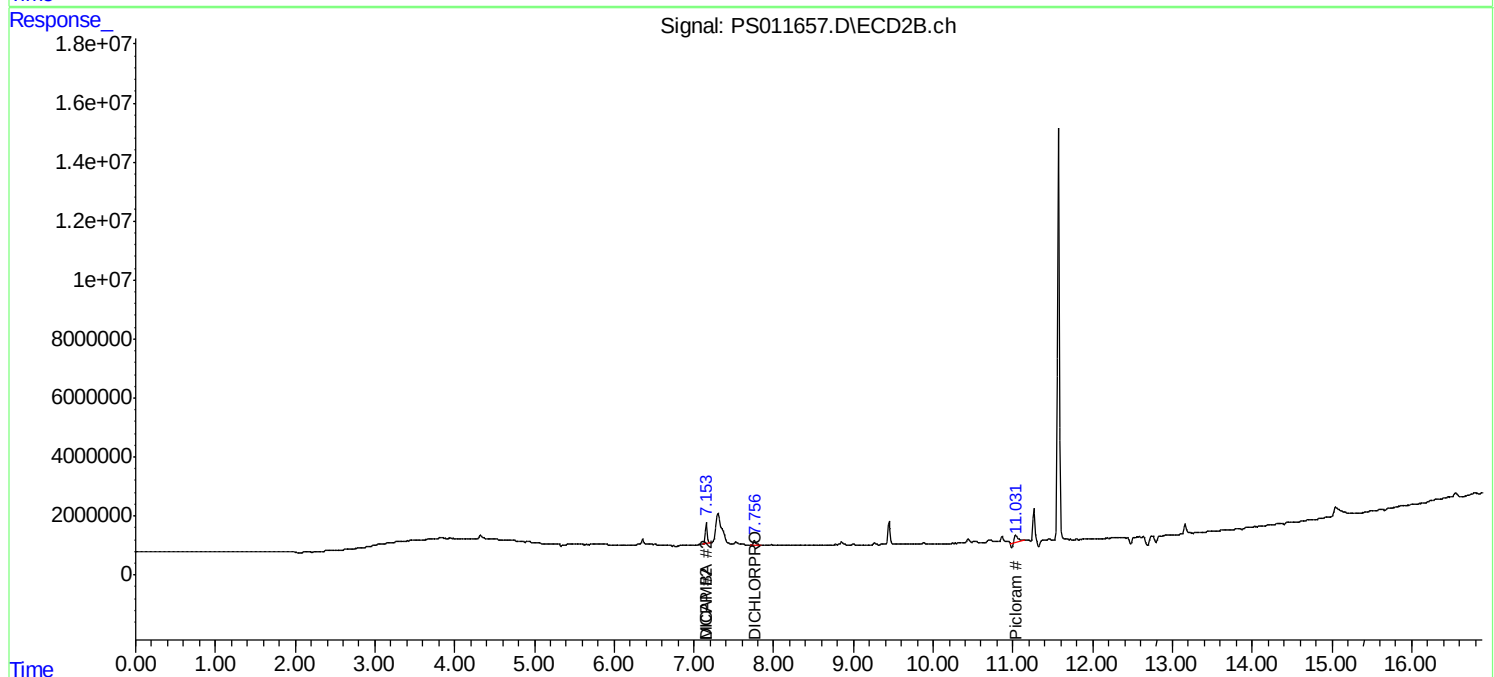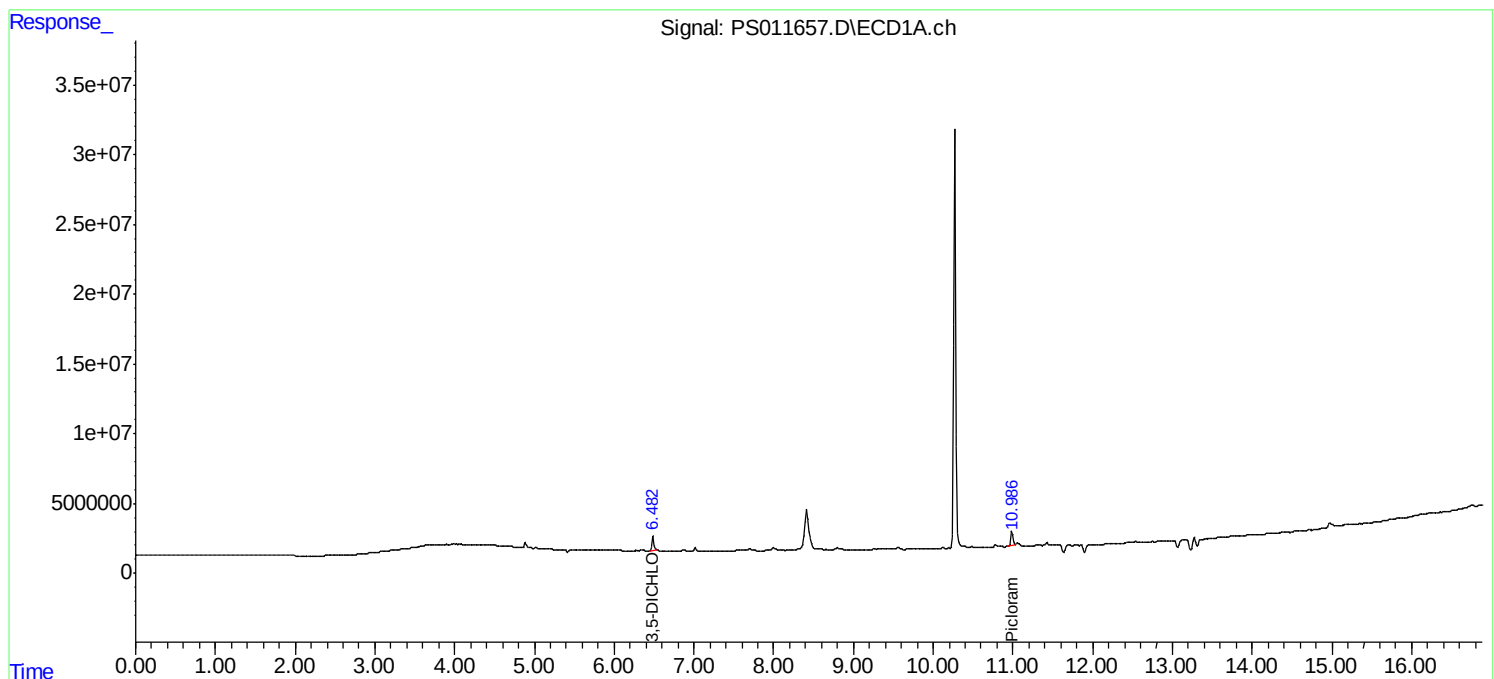


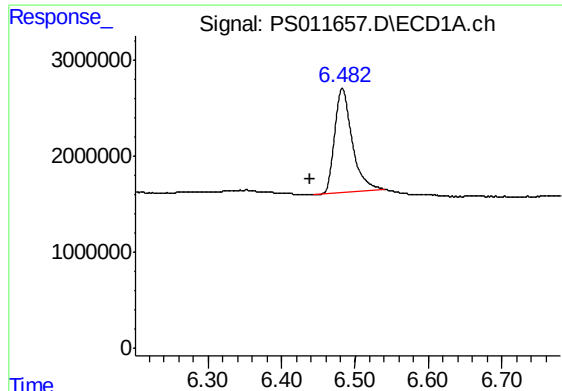

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.483 min
Delta R.T.: 0.043 min
Response: 17804570
Conc: 13.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

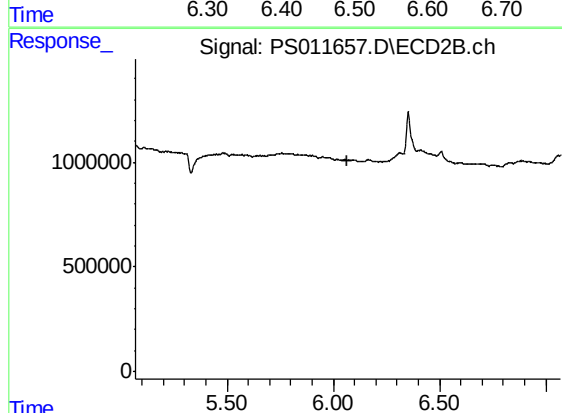


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

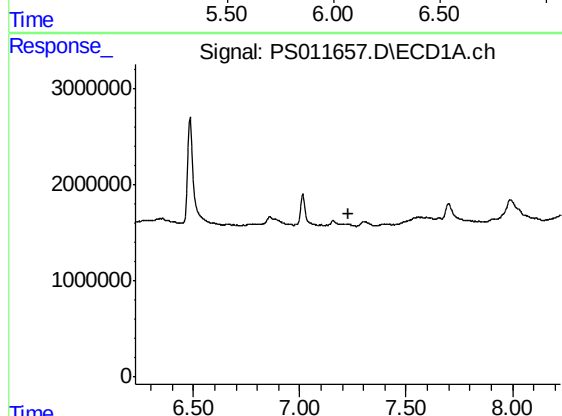


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.226 min
Response: 0
Conc: N.D.

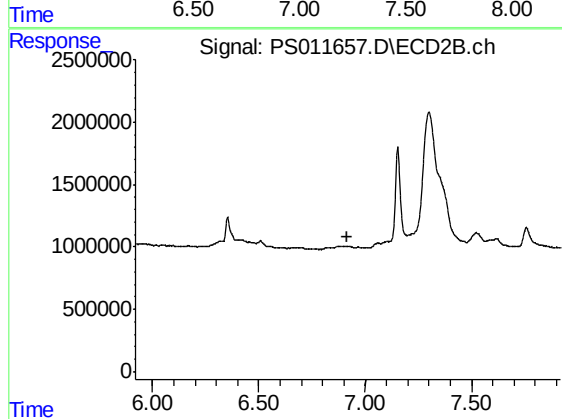

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.918 min
Response: 0
Conc: N.D.

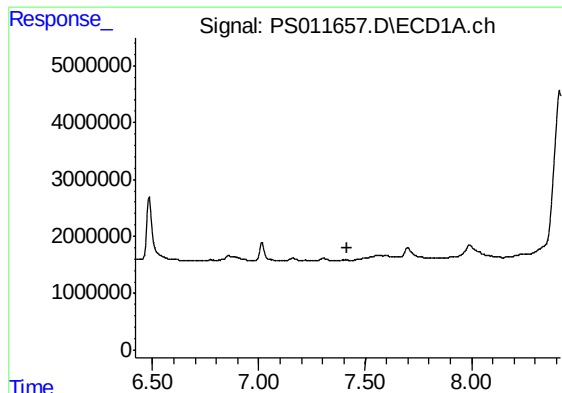

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

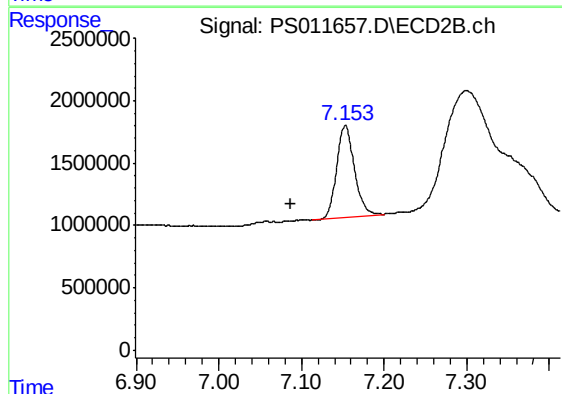


#5 DICAMBA

R.T.: 7.153 min
Delta R.T.: 0.065 min
Response: 10964219
Conc: 4.79 ng/ml

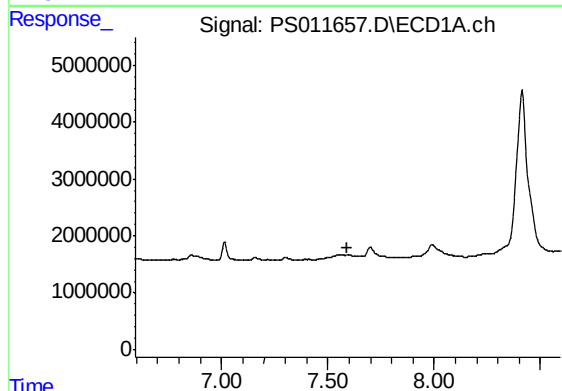


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.594 min
Response: 0
Conc: N.D.

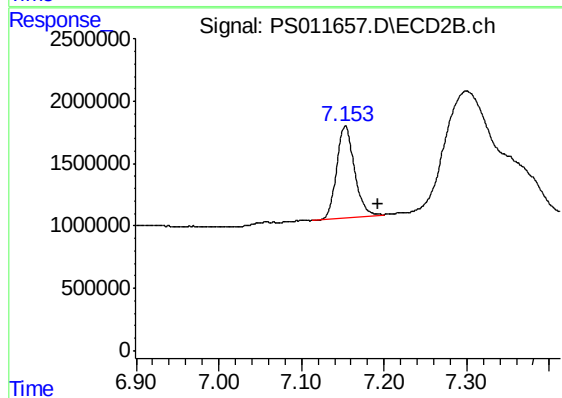

#6 MCPP


R.T.: 7.153 min
Delta R.T.: -0.039 min
Response: 10964219
Conc: 5.75 ug/ml

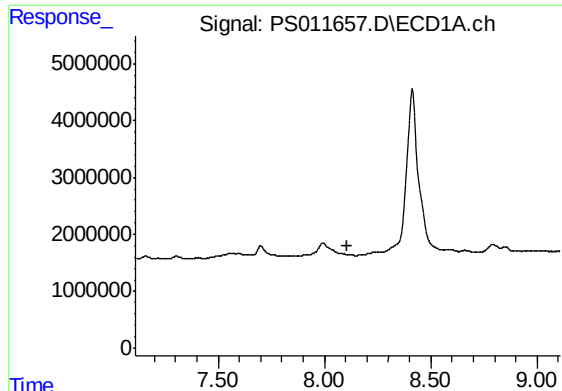

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.110 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

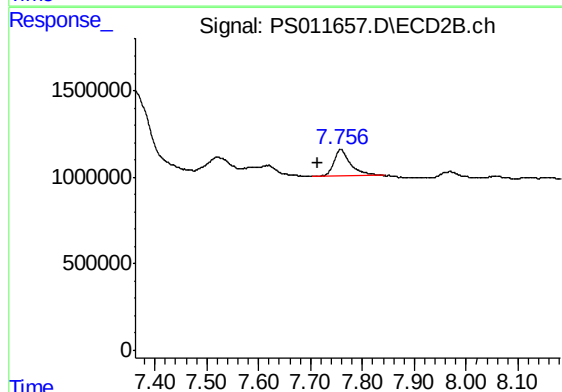


#8 DICHLORPROP

R.T.: 7.758 min
Delta R.T.: 0.044 min
Response: 3440650
Conc: 5.72 ng/ml

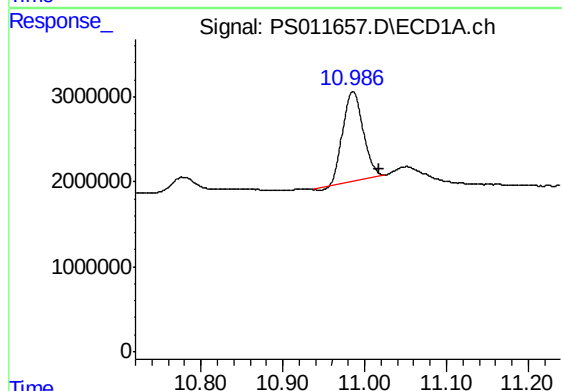

#15 Picloram

R.T.: 10.986 min
Delta R.T.: -0.032 min
Response: 18404922
Conc: 2.92 ng/ml

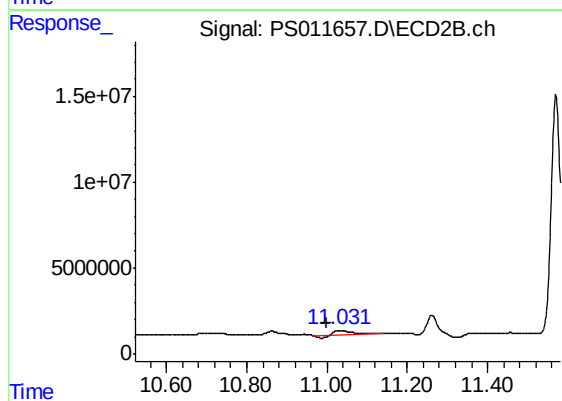

#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.031 min
Response: 6241565
Conc: 1.43 ng/ml