

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080725\
 Data File : PS031377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2025 11:14
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 03:20:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:11:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.288	0.000	339285	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.452	0.000	312717	0	<MDL	N.D. #
3) T	4-Nitroph...	7.081	0.000	867274	0	<MDL	N.D. #
5) T	DICAMBA	7.477	0.000	245504	0	<MDL	N.D. #
6) T	MCP	7.678	0.000	2641721	0	<MDL	N.D. #
7) T	MCPA	7.815	8.257f	552359	92107033	<MDL	32.831 #
8) T	DICHLORPROP	8.191	0.000	560574	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.302	9.892	358694	16611026	<MDL	1.266 #
12) T	2,4,5-T	9.566f	0.000	1240793	0	<MDL	N.D. #
13) T	2,4-DB	10.178	0.000	538231	0	<MDL	N.D. #
14) T	DINOSEB	11.362	0.000	472376	0	<MDL	N.D. #
15) T	Picloram	11.210	12.445f	676158	1644891	<MDL	<MDL #
16) T	DCPA	11.676	0.000	926448	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080725\
Data File : PS031377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2025 11:14
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 03:20:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:11:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

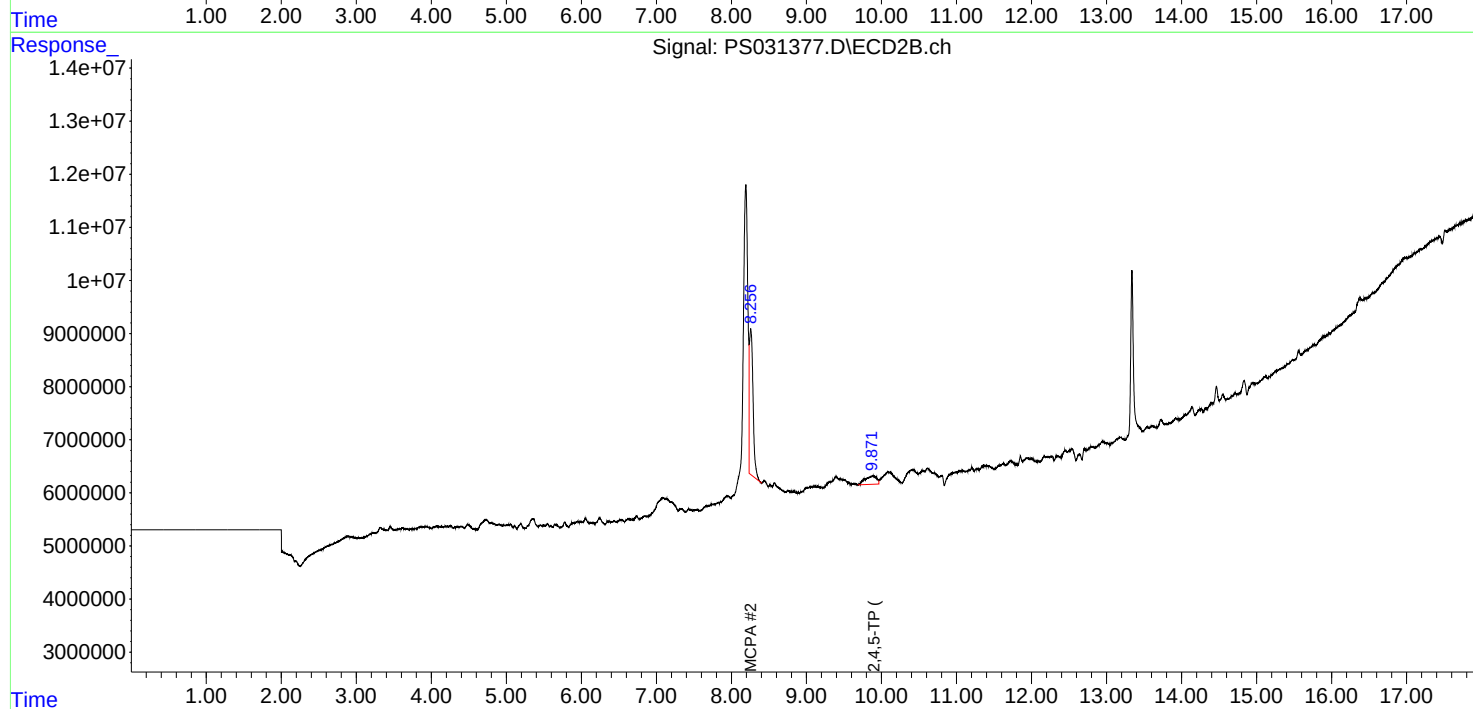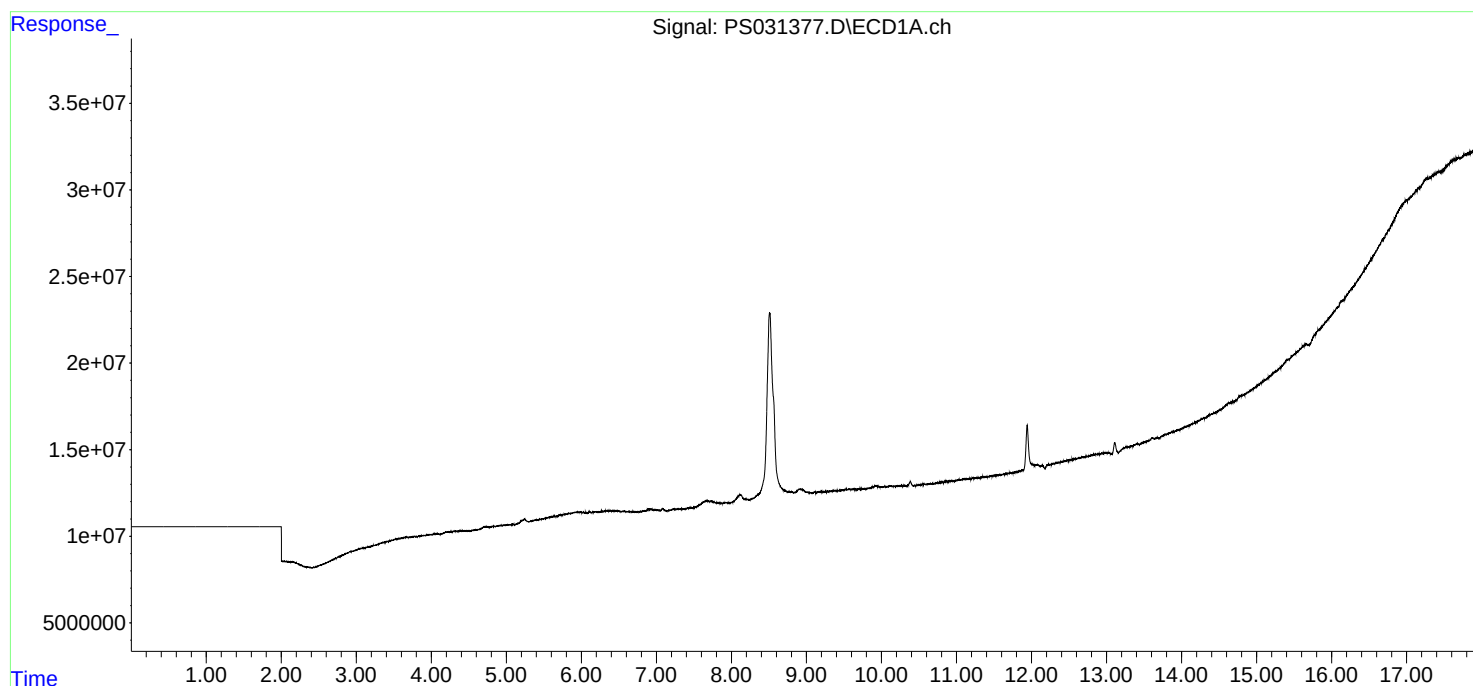


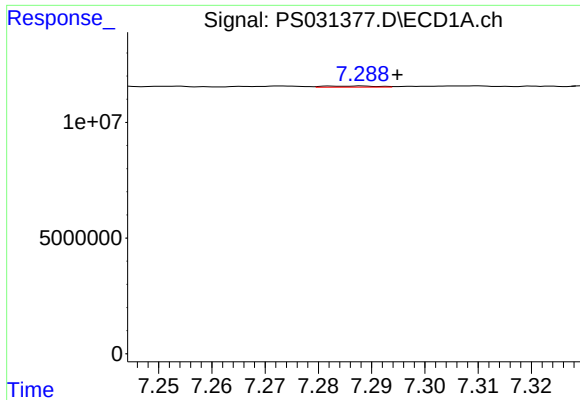

#4 2,4-DCAA


R.T.: 7.288 min
Delta R.T.: -0.007 min
Response: 339285
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

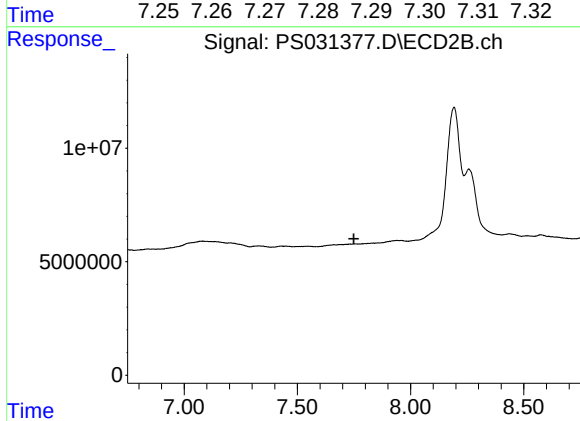


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.749 min
Response: 0
Conc: N.D.

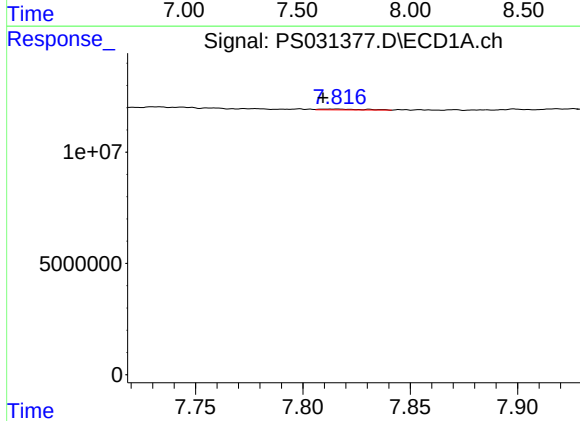


#7 MCPA

R.T.: 7.815 min
Delta R.T.: 0.006 min
Response: 552359
Conc: N.D.

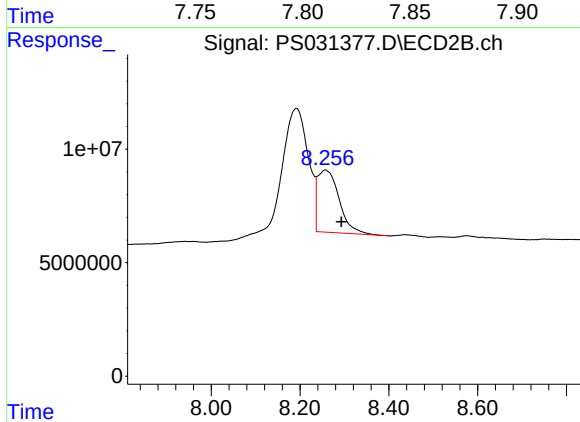

#7 MCPA


R.T.: 8.257 min
Delta R.T.: -0.036 min
Response: 92107033
Conc: 32.83 ug/ml

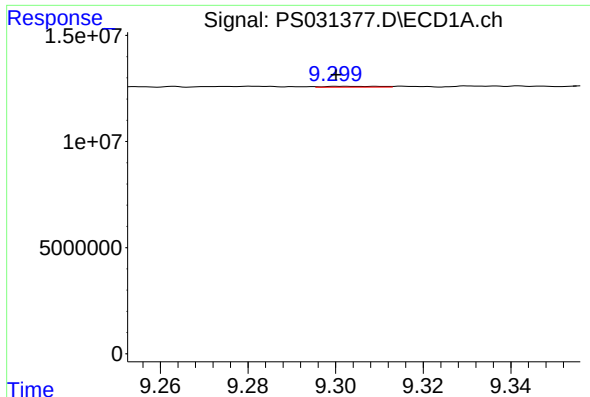

#11 2,4,5-TP (SILVEX)

R.T.: 9.302 min
Delta R.T.: 0.002 min
Response: 358694
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

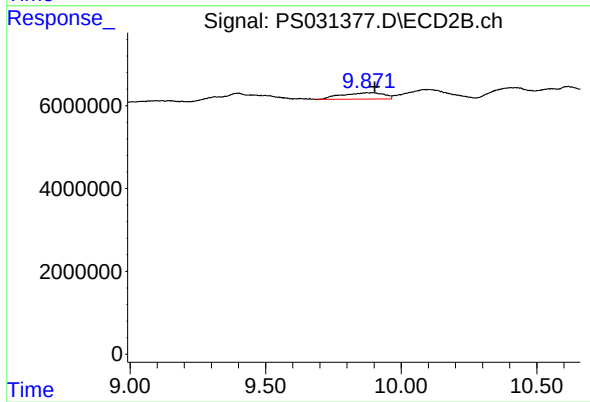

#11 2,4,5-TP (SILVEX)

R.T.: 9.892 min
Delta R.T.: -0.010 min
Response: 16611026
Conc: 1.27 ng/ml