

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080725\
 Data File : PS031385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2025 14:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 04:24:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.298	7.767	2364194	1087663	<MDL	1.287 #
Target Compounds							
2) T	3,5-DICHL...	6.483	0.000	3592158	0	<MDL	N.D. #
5) T	DICAMBA	0.000	7.993f	0	1586323	N.D.	<MDL
7) T	MCPA	0.000	8.260f	0	71869975	N.D.	25.617
8) T	DICHLORPROP	8.196	0.000	1646397	0	<MDL	N.D. #
10) T	Pentachlo...	8.719	9.514	1817666	14393512	<MDL	<MDL #
11) T	2,4,5-TP ...	9.301	9.905	2203517	8228852	<MDL	<MDL #
12) T	2,4,5-T	9.603	0.000	4958529	0	<MDL	N.D. #
13) T	2,4-DB	10.164	10.910	1488293	7571987	<MDL	7.848 #
14) T	DINOSEB	11.368	0.000	2219791	0	<MDL	N.D. #
15) T	Picloram	11.214	12.428f	19752133	17762158	1.513	1.013 #
16) T	DCPA	11.673	12.327	11816080	979173	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080725\
Data File : PS031385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2025 14:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 04:24:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

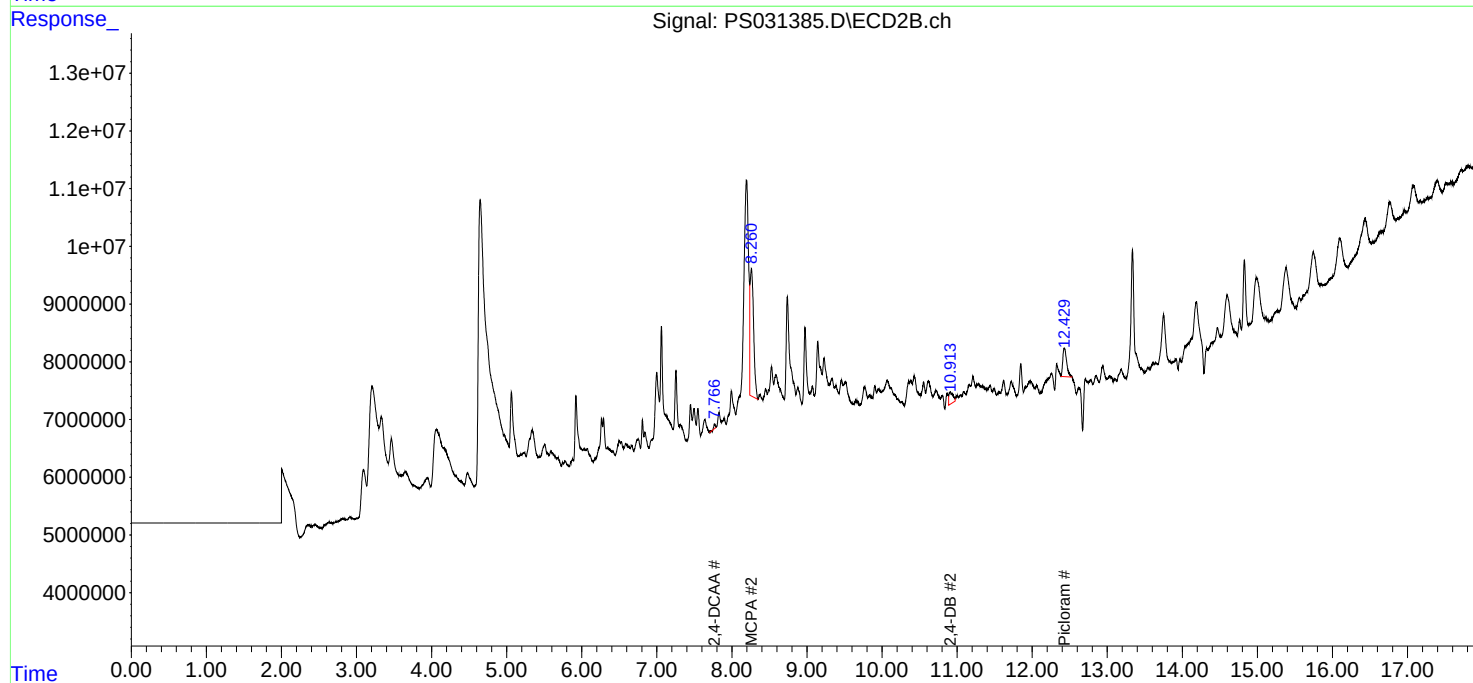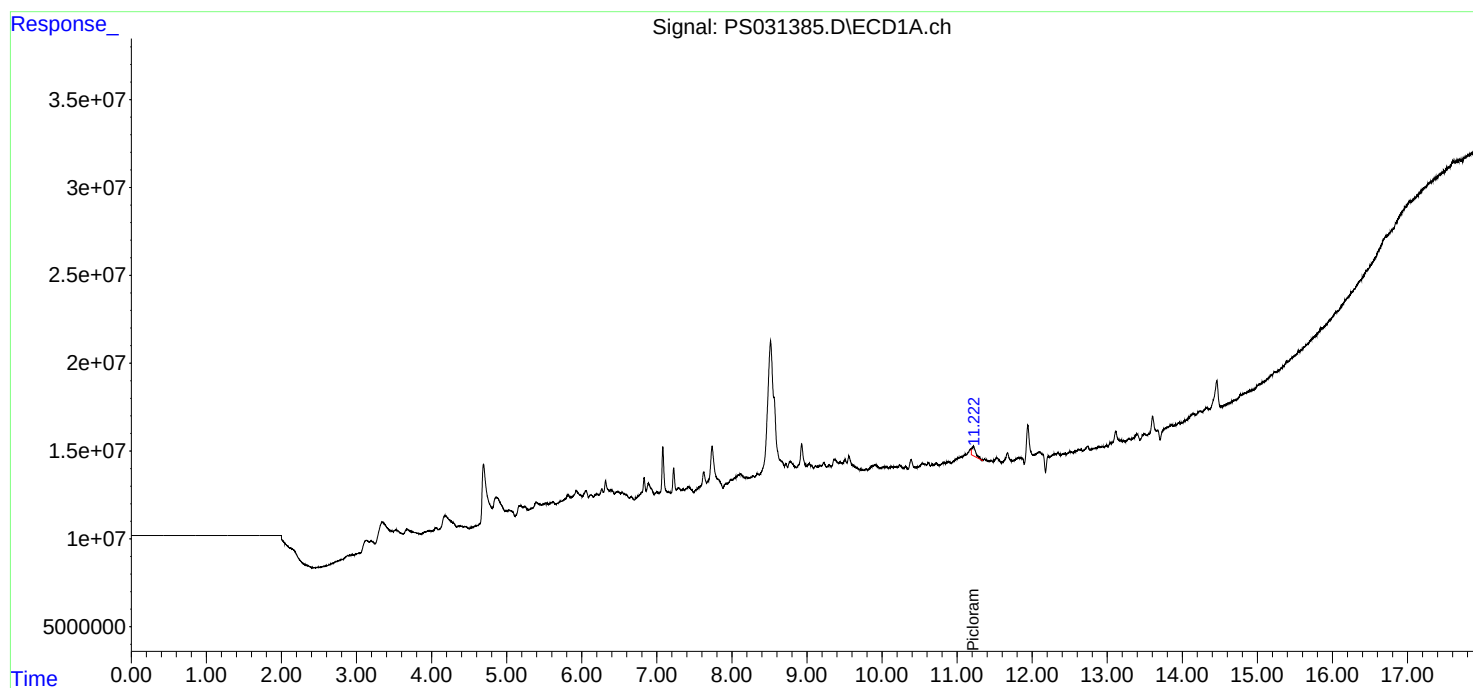


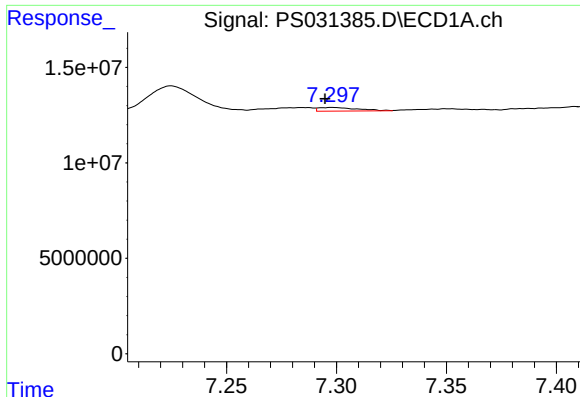

#4 2,4-DCAA


R.T.: 7.298 min
Delta R.T.: 0.003 min
Response: 2364194
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

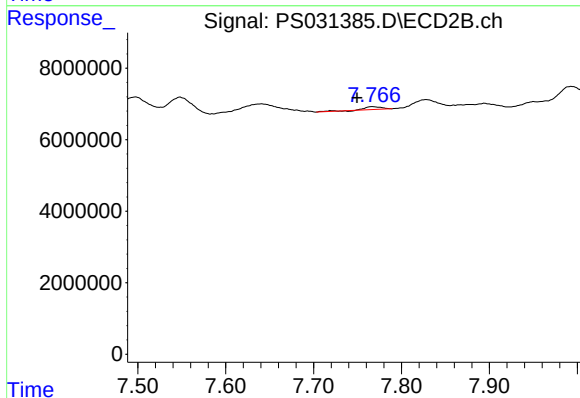


#4 2,4-DCAA

R.T.: 7.767 min
Delta R.T.: 0.018 min
Response: 1087663
Conc: 1.29 ng/ml

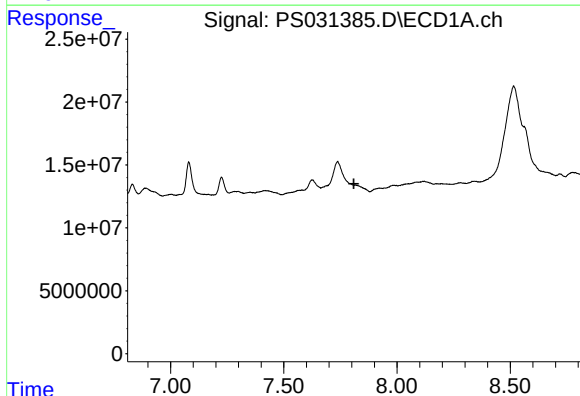


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.809 min
Response: 0
Conc: N.D.

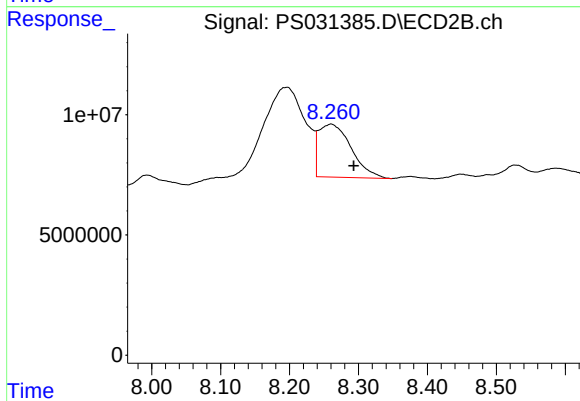

#7 MCPA


R.T.: 8.260 min
Delta R.T.: -0.033 min
Response: 71869975
Conc: 25.62 ug/ml

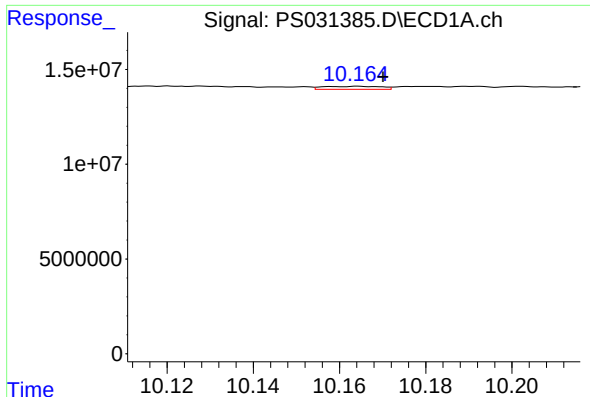

#13 2,4-DB


R.T.: 10.164 min
Delta R.T.: -0.006 min
Response: 1488293
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

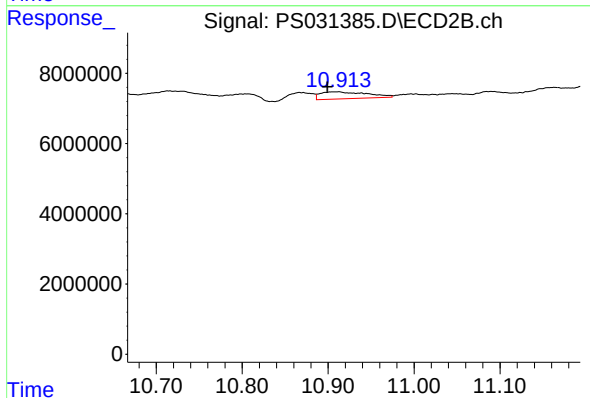


#13 2,4-DB

R.T.: 10.910 min
Delta R.T.: 0.011 min
Response: 7571987
Conc: 7.85 ng/ml

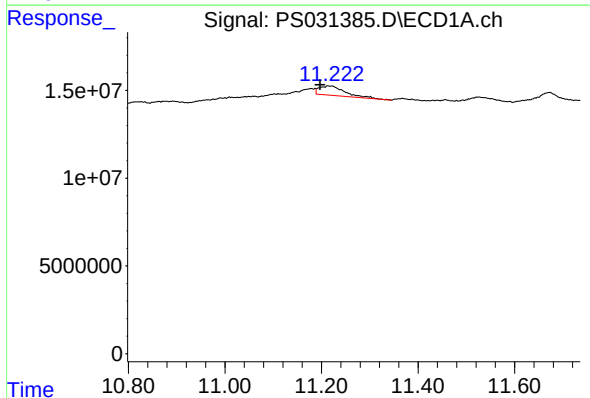

#15 Picloram

R.T.: 11.214 min
Delta R.T.: 0.016 min
Response: 19752133
Conc: 1.51 ng/ml

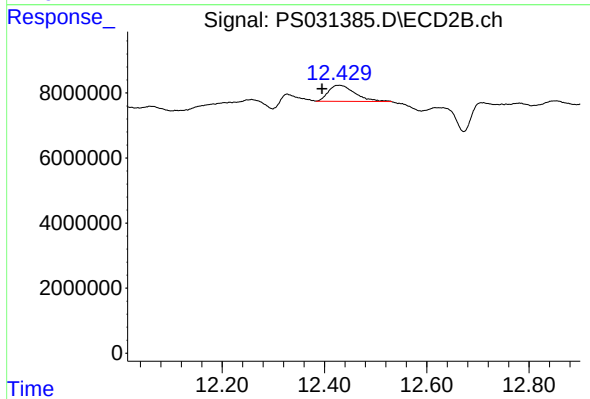

#15 Picloram

R.T.: 12.428 min
Delta R.T.: 0.032 min
Response: 17762158
Conc: 1.01 ng/ml