

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080822\
 Data File : PS020226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 12:46
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 19:25:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	6.760	1377.6E6	433.7E6	467.181	532.229
Target Compounds							
1) T	Dalapon	3.004	0.000	478004	0	<MDL	N.D. #
3) T	4-Nitroph...	6.990f	0.000	903308	0	<MDL	N.D. #
6) T	MCP	7.558	0.000	508139	0	<MDL	N.D. #
7) T	MCPA	7.688	0.000	1252718	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.612f	0	1190343	N.D.	1.273
9) T	2,4-D	8.363f	0.000	28631327	0	9.507	N.D. #
10) T	Pentachlo...	8.601	0.000	871152	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.157	0.000	1527010	0	<MDL	N.D. #
12) T	2,4,5-T	9.393f	0.000	38705400	0	2.132	N.D. #
13) T	2,4-DB	9.949f	0.000	6841633	0	1.875	N.D. #
15) T	Picloram	10.958	10.841	3754015	34876668	<MDL	4.623 #
16) T	DCPA	11.404	0.000	3189263	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080822\
Data File : PS020226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 12:46
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 19:25:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

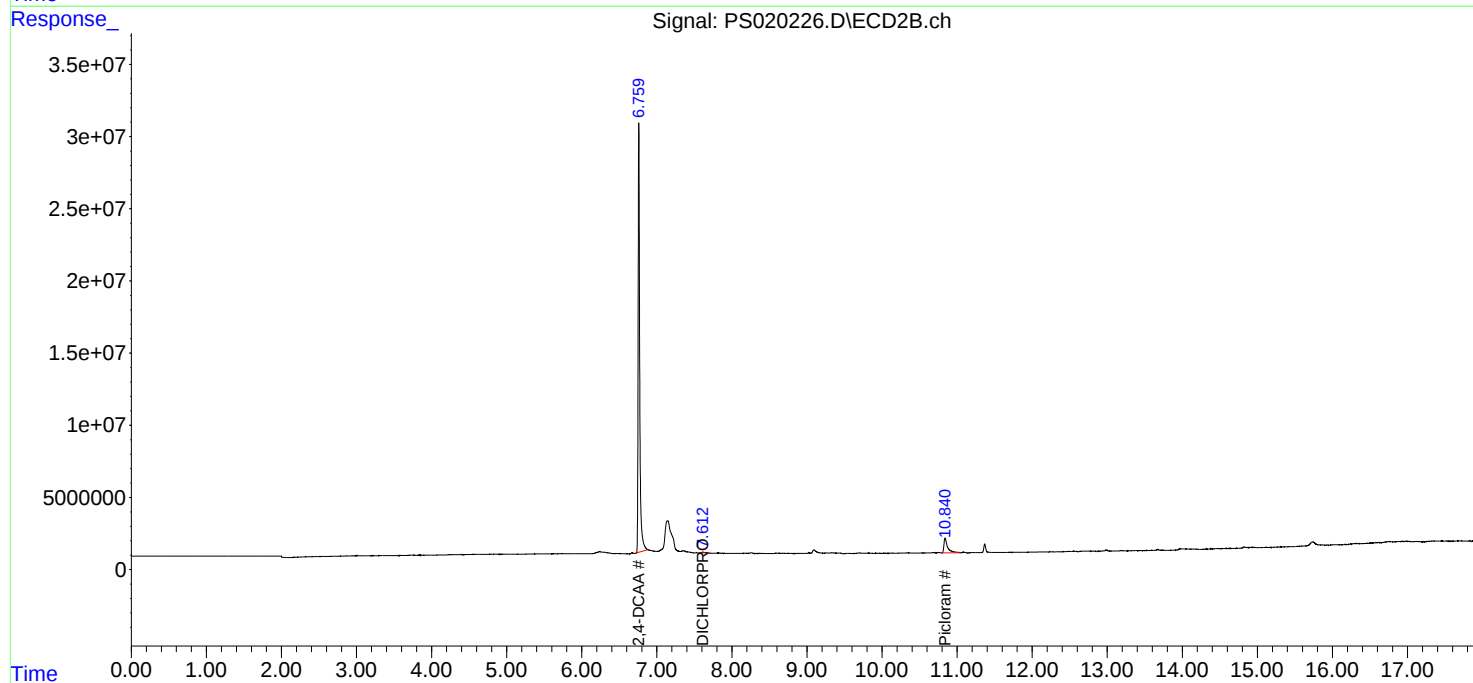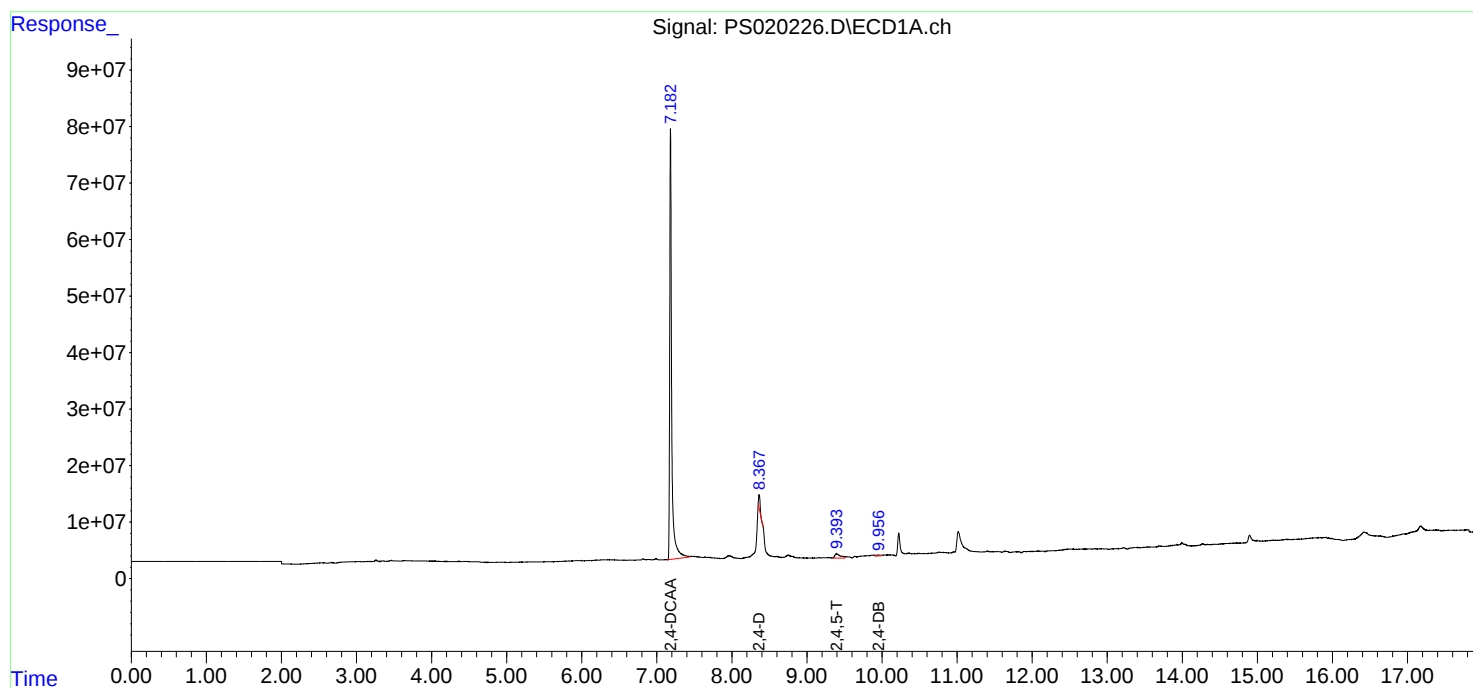


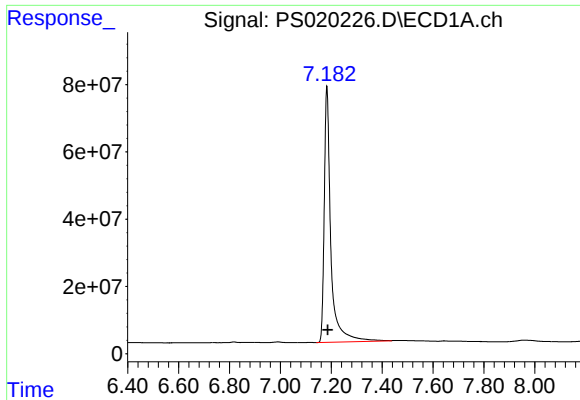

#4 2,4-DCAA


R.T.: 7.182 min
Delta R.T.: -0.003 min
Response: 1377587013
Conc: 467.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

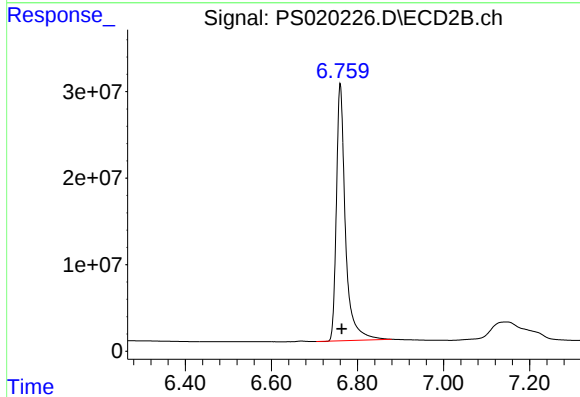


#4 2,4-DCAA

R.T.: 6.760 min
Delta R.T.: -0.004 min
Response: 433743009
Conc: 532.23 ng/ml

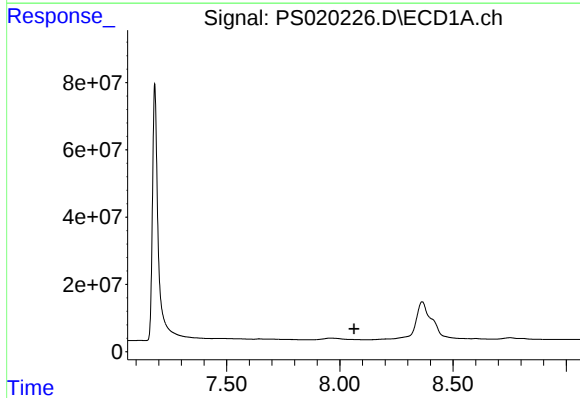


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.062 min
Response: 0
Conc: N.D.

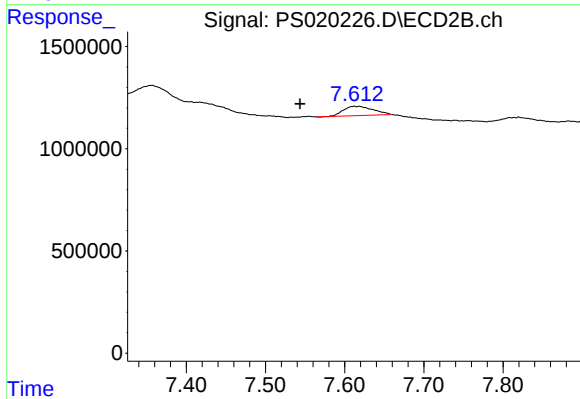

#8 DICHLORPROP


R.T.: 7.612 min
Delta R.T.: 0.068 min
Response: 1190343
Conc: 1.27 ng/ml

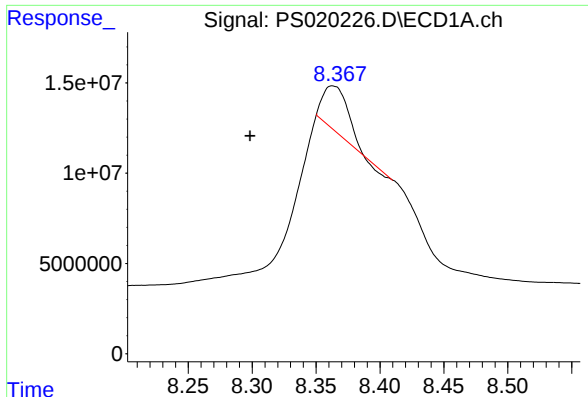

#9 2,4-D


R.T.: 8.363 min
Delta R.T.: 0.065 min
Response: 28631327
Conc: 9.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

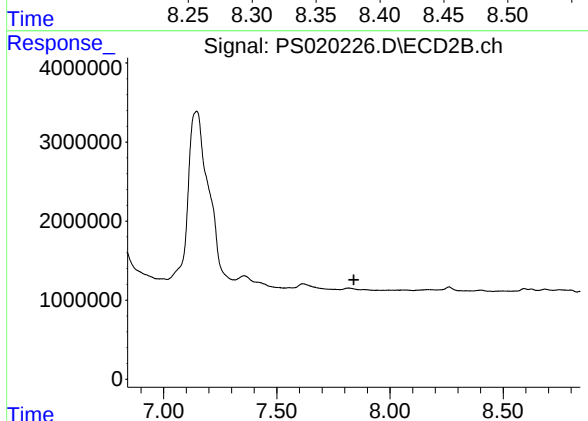


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.840 min
Response: 0
Conc: N.D.

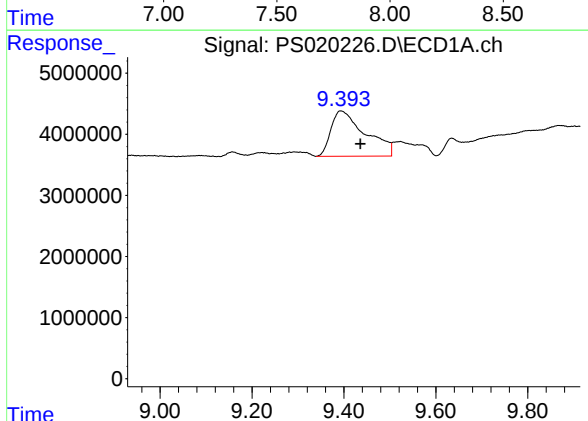


#12 2,4,5-T

R.T.: 9.393 min
Delta R.T.: -0.043 min
Response: 38705400
Conc: 2.13 ng/ml

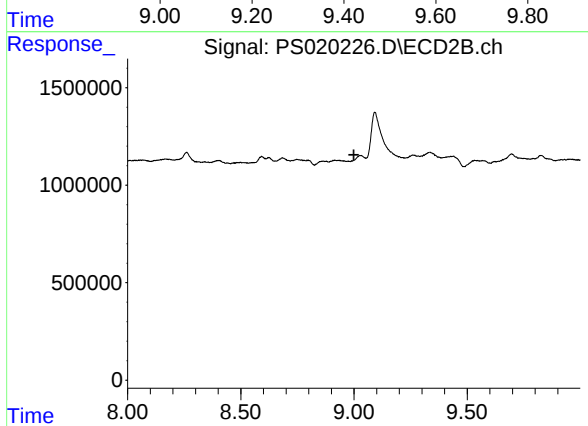

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.999 min
Response: 0
Conc: N.D.

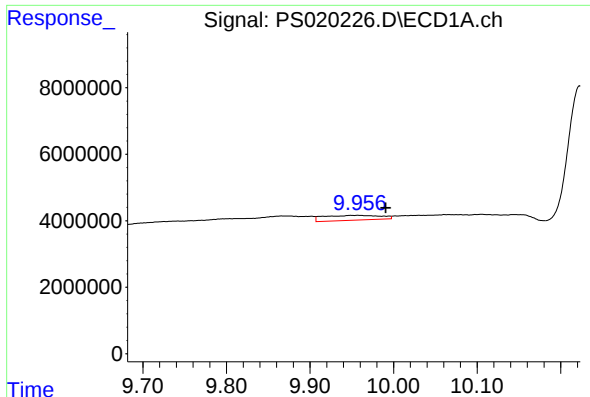

#13 2,4-DB


R.T.: 9.949 min
Delta R.T.: -0.041 min
Response: 6841633
Conc: 1.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

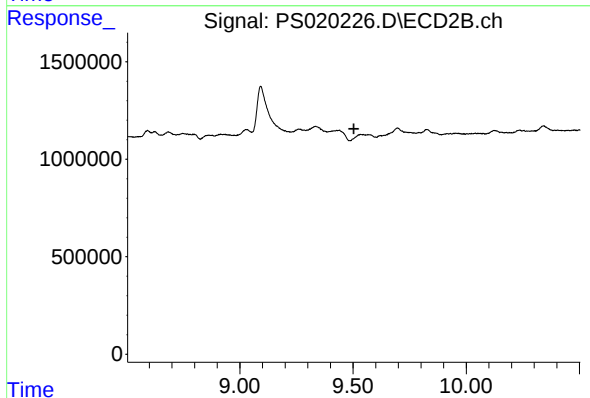


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.503 min
Response: 0
Conc: N.D.

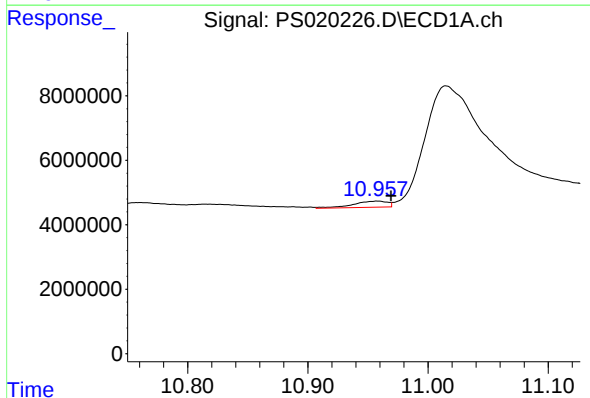

#15 Picloram

R.T.: 10.958 min
Delta R.T.: -0.012 min
Response: 3754015
Conc: N.D.

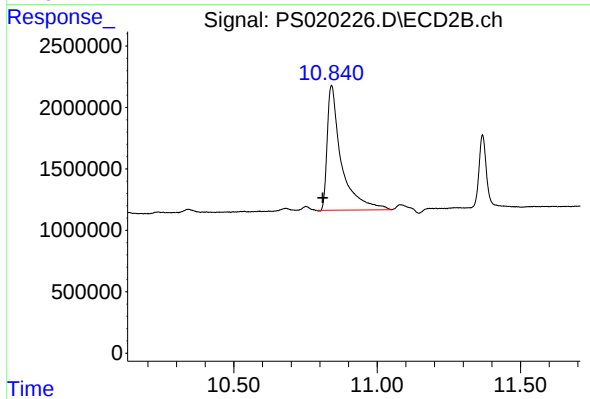

#15 Picloram

R.T.: 10.841 min
Delta R.T.: 0.031 min
Response: 34876668
Conc: 4.62 ng/ml