

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080824\
 Data File : PS027331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2024 09:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 05:09:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	7.743	1237.3E6	923.6E6	491.934	496.620
Target Compounds							
2) T	3,5-DICHL...	6.341	6.652f	111.2E6	158428	27.936	<MDL #
3) T	4-Nitroph...	6.973	0.000	15112928	0	9.997	N.D. #
5) T	DICAMBA	0.000	7.939	0	4344521	N.D.	<MDL
6) T	MCP	7.500f	8.047	3583958	38093030	<MDL	6.690 #
8) T	DICHLORPROP	8.088	8.651	1018044	133052	<MDL	<MDL #
9) T	2,4-D	8.299	0.000	268.3E6	0	94.116	N.D. #
10) T	Pentachlo...	0.000	9.507	0	868703	N.D.	<MDL
11) T	2,4,5-TP ...	9.129	9.904	3526571	2325768	<MDL	<MDL #
12) T	2,4,5-T	9.445	10.309	1925077	851737	<MDL	<MDL #
14) T	DINOSEB	11.175f	11.267	2264298	357714	<MDL	<MDL #
15) T	Picloram	10.988f	12.344	102.9E6	59772353	5.336	3.313 #
16) T	DCPA	11.483	0.000	1388865	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080824\
Data File : PS027331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2024 09:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 05:09:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

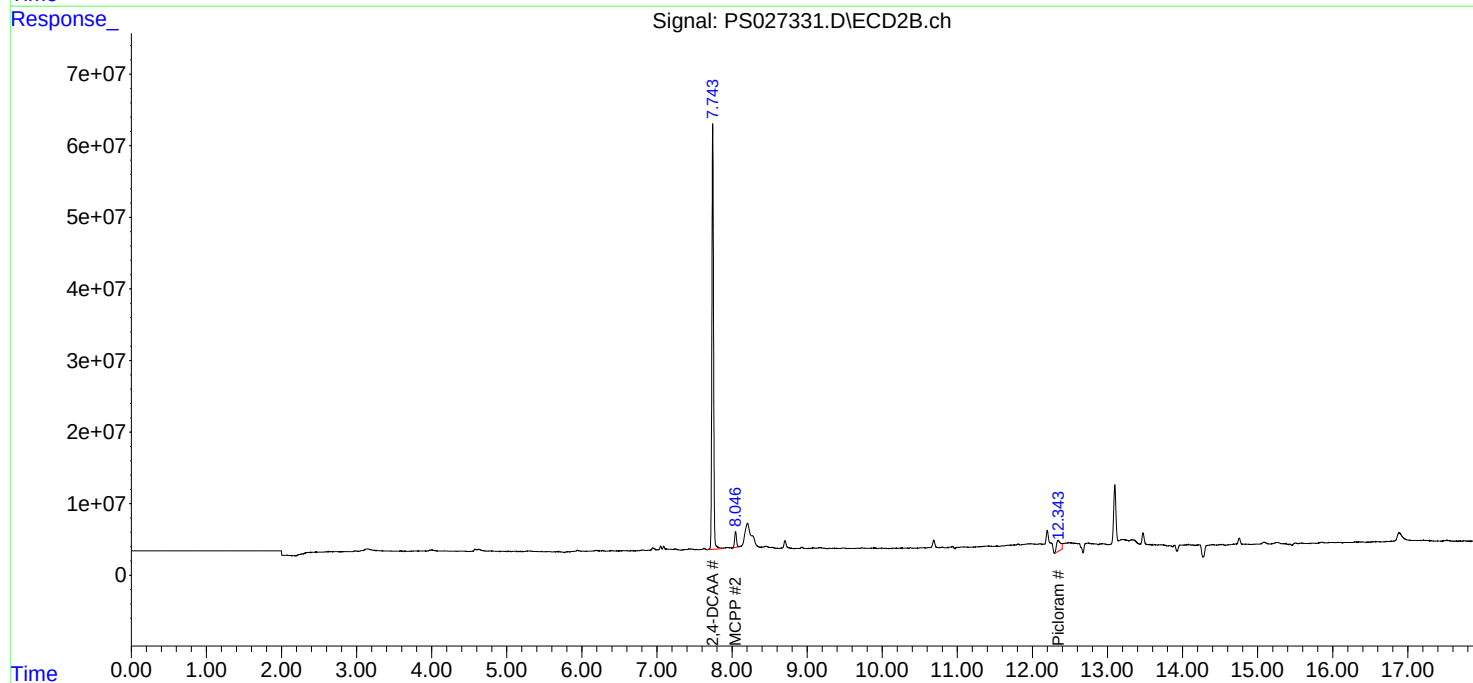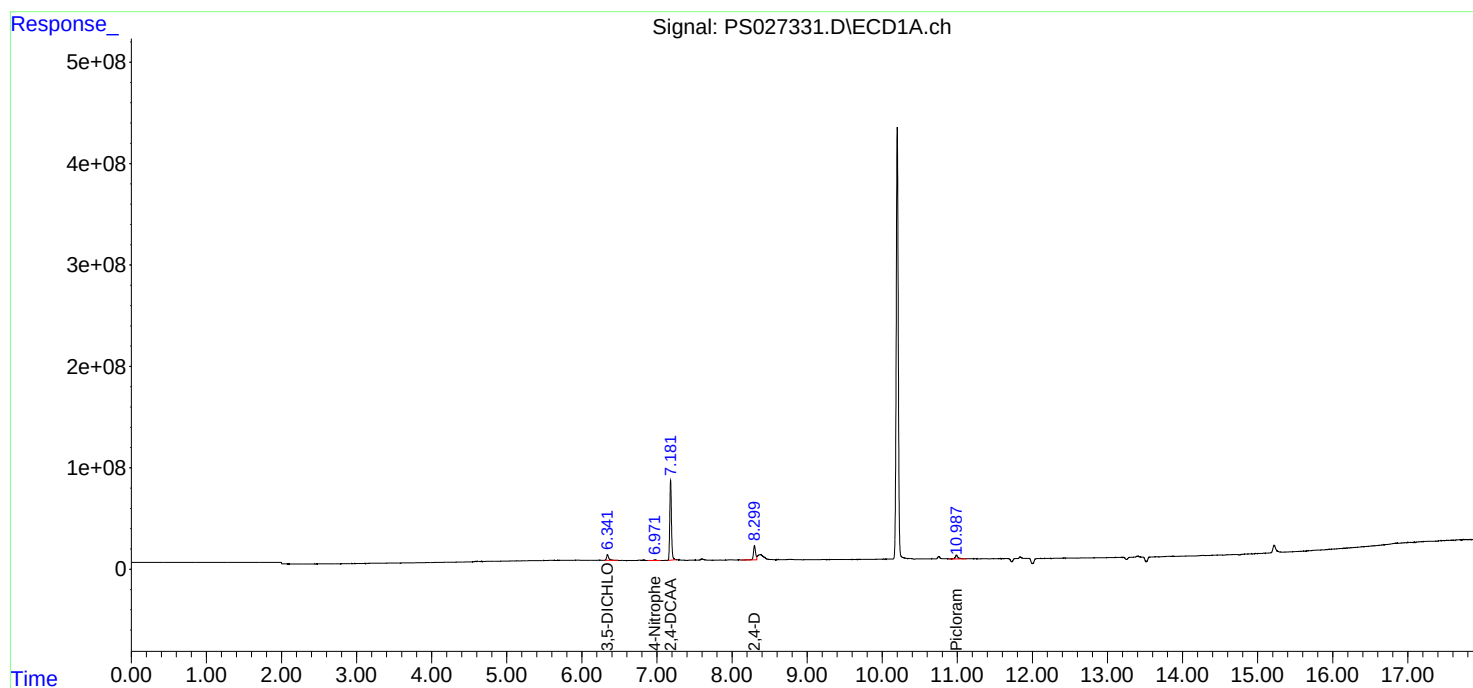


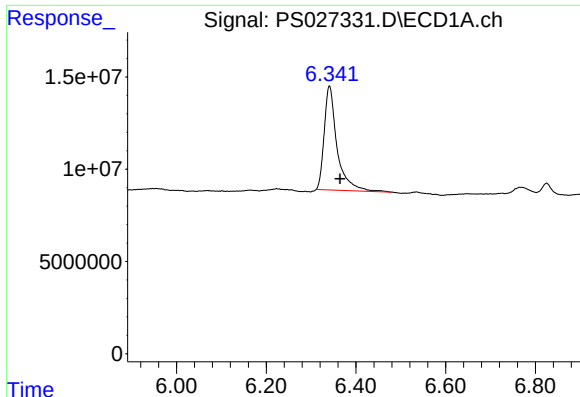

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.341 min
Delta R.T.: -0.023 min
Response: 111231961
Conc: 27.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

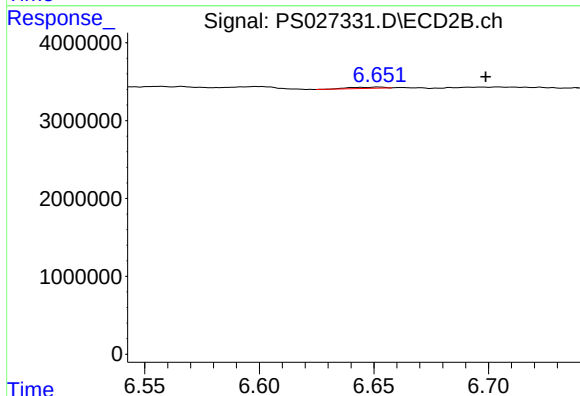


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.652 min
Delta R.T.: -0.047 min
Response: 158428
Conc: N.D.

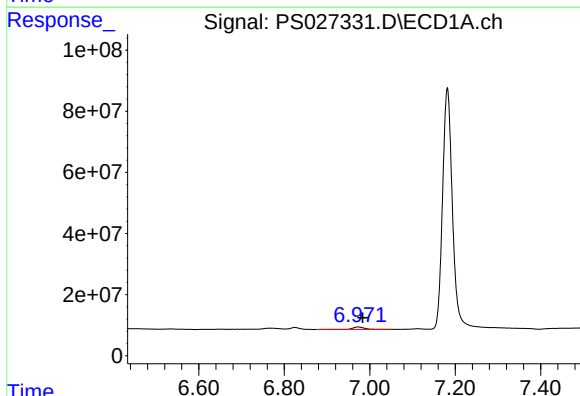


#3 4-Nitrophenol

R.T.: 6.973 min
Delta R.T.: -0.011 min
Response: 15112928
Conc: 10.00 ng/ml

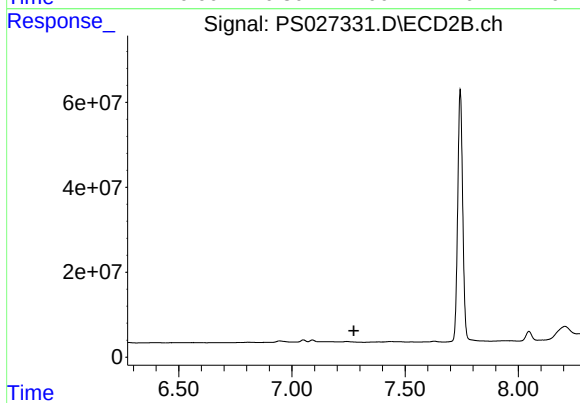

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.

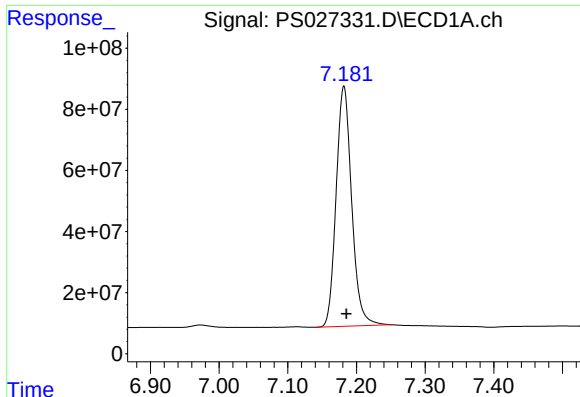

#4 2,4-DCAA


R.T.: 7.182 min
Delta R.T.: -0.004 min
Response: 1237271244
Conc: 491.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

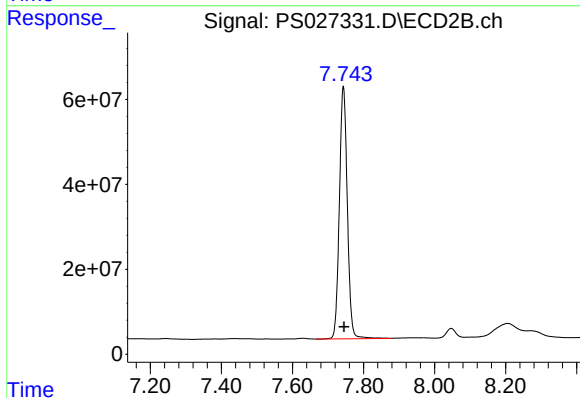


#4 2,4-DCAA

R.T.: 7.743 min
Delta R.T.: -0.002 min
Response: 923599420
Conc: 496.62 ng/ml

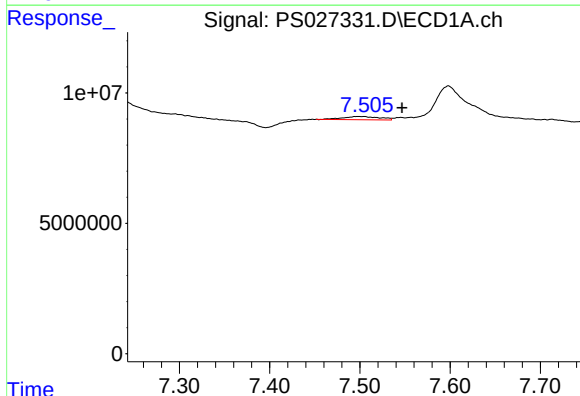


#6 MCP

R.T.: 7.500 min
Delta R.T.: -0.047 min
Response: 3583958
Conc: N.D.

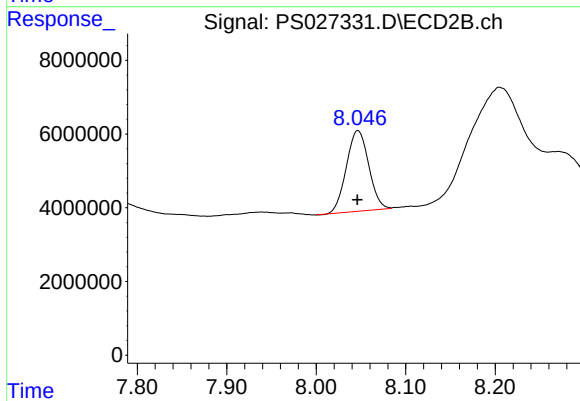

#6 MCP


R.T.: 8.047 min
Delta R.T.: 0.000 min
Response: 38093030
Conc: 6.69 ug/ml

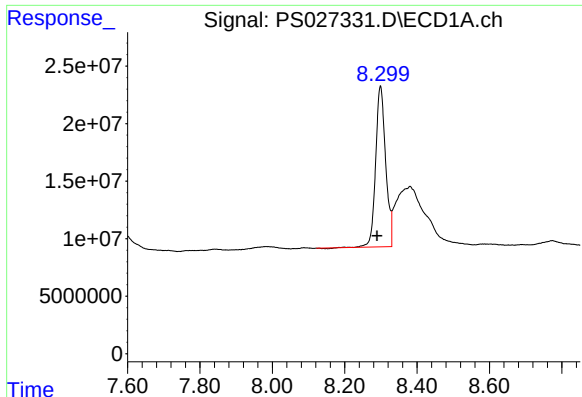

#9 2,4-D


R.T.: 8.299 min
Delta R.T.: 0.010 min
Response: 268335963
Conc: 94.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

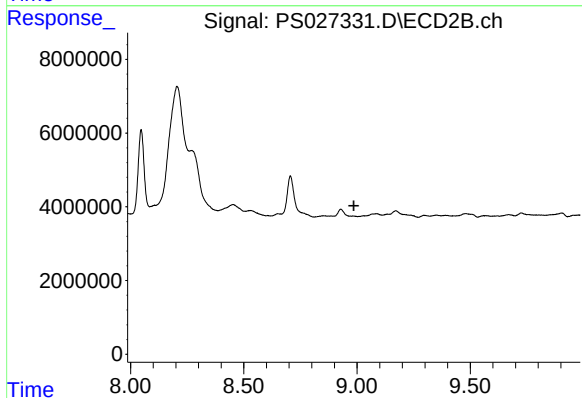


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.986 min
Response: 0
Conc: N.D.

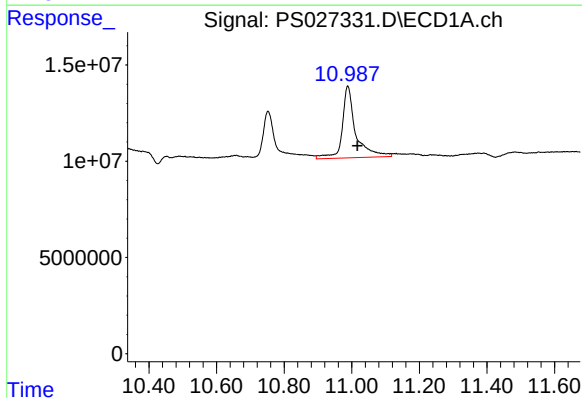

#15 Picloram

R.T.: 10.988 min
Delta R.T.: -0.028 min
Response: 102880441
Conc: 5.34 ng/ml

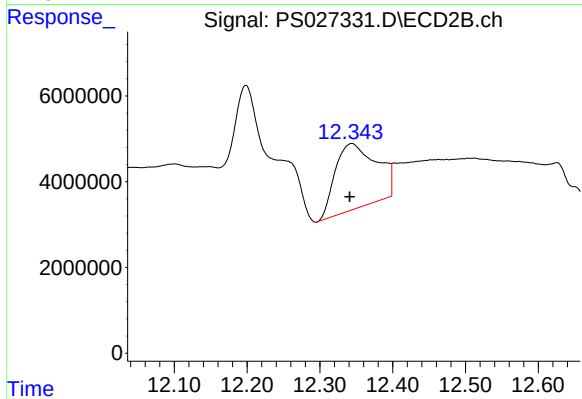

#15 Picloram

R.T.: 12.344 min
Delta R.T.: 0.003 min
Response: 59772353
Conc: 3.31 ng/ml