

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080825\
 Data File : PS031394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 09:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 03:25:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.293	7.747	1290.0E6	413.6E6	406.444	489.292
Target Compounds							
1) T	Dalapon	0.000	2.648f	0	48107097	N.D.	18.078
2) T	3,5-DICHL...	6.465	0.000	1299359	0	<MDL	N.D. #
3) T	4-Nitroph...	7.088	0.000	2066419	0	2.003	N.D. #
5) T	DICAMBA	7.475	0.000	997949	0	<MDL	N.D. #
7) T	MCPA	7.827	8.251f	655200	50755564	<MDL	18.091 #
8) T	DICHLORPROP	8.195	0.000	510536	0	<MDL	N.D. #
10) T	Pentachlo...	8.719	9.516	4414438	4205005	<MDL	<MDL #
11) T	2,4,5-TP ...	9.301	9.905	8404609	16009239	<MDL	1.221 #
12) T	2,4,5-T	9.605	0.000	897786	0	<MDL	N.D. #
14) T	DINOSEB	11.374	11.276	2774803	2424708	<MDL	<MDL #
15) T	Picloram	11.174	12.441f	5742539	-380574	<MDL	N.D. #
16) T	DCPA	11.670	0.000	3486539	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080825\
Data File : PS031394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 09:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 03:25:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

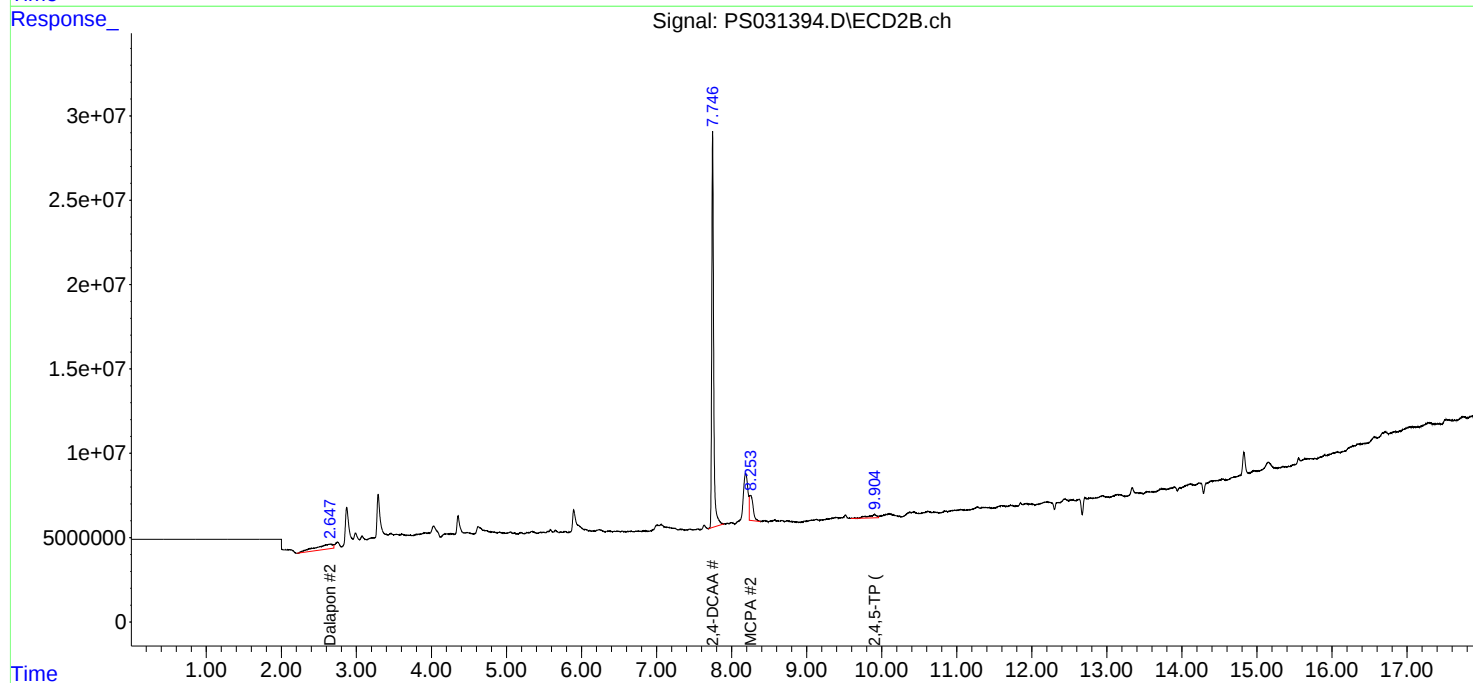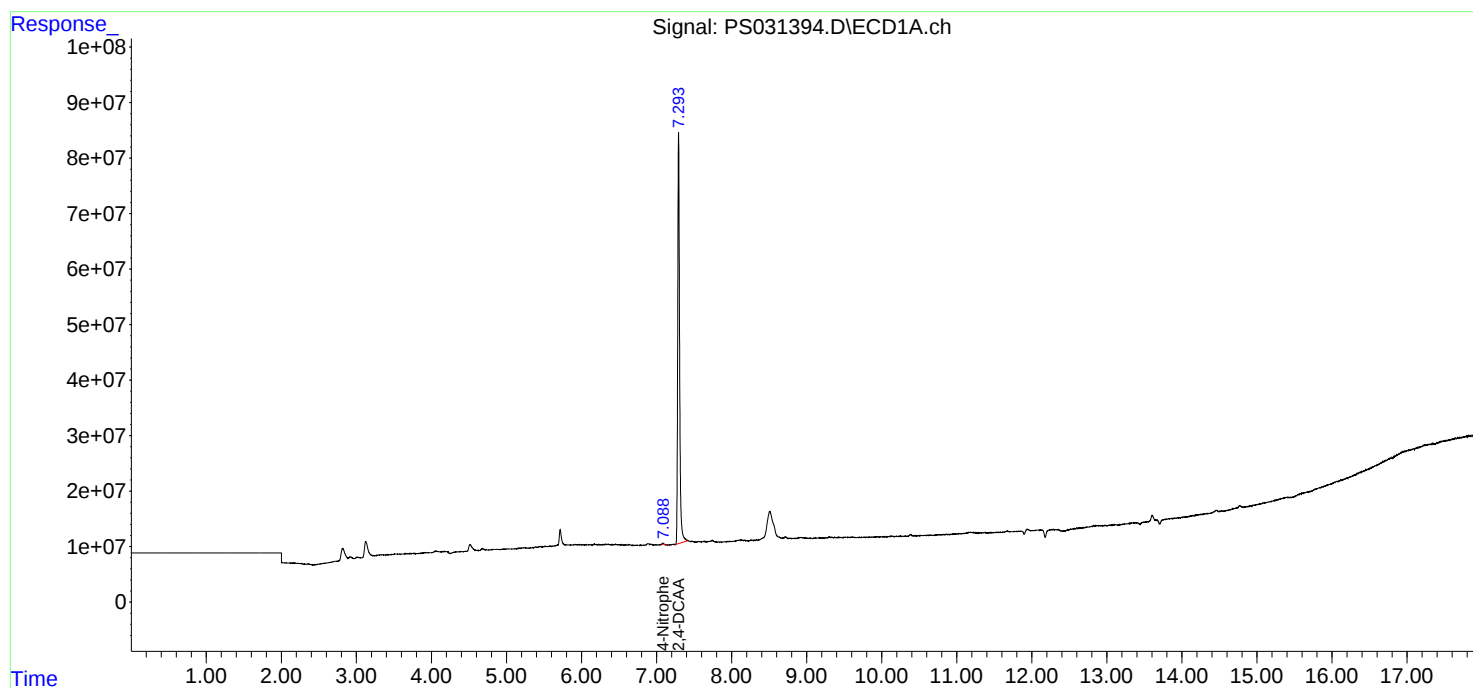


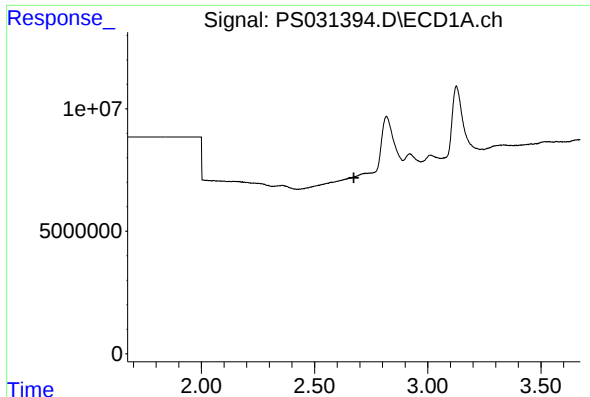

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

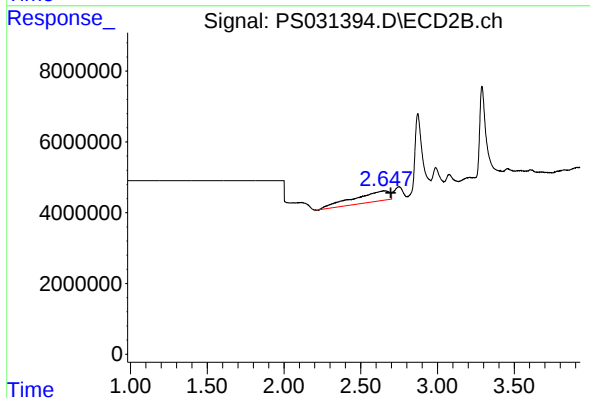


#1 Dalapon

R.T.: 2.648 min
Delta R.T.: -0.047 min
Response: 48107097
Conc: 18.08 ng/ml

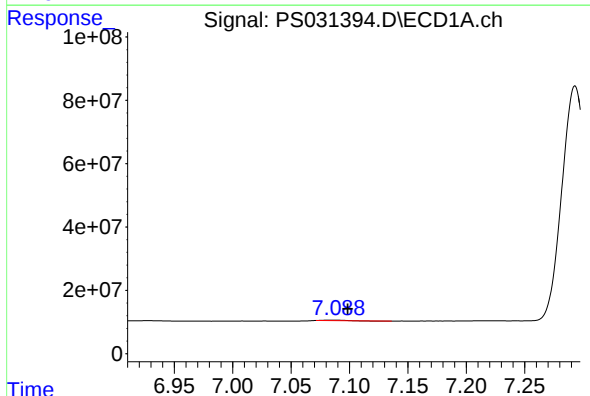


#3 4-Nitrophenol

R.T.: 7.088 min
Delta R.T.: -0.011 min
Response: 2066419
Conc: 2.00 ng/ml

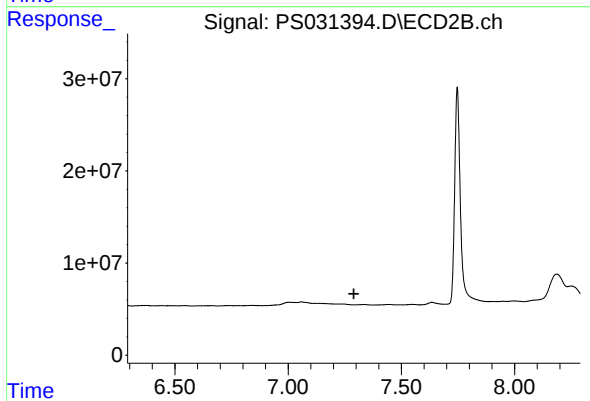

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.291 min
Response: 0
Conc: N.D.

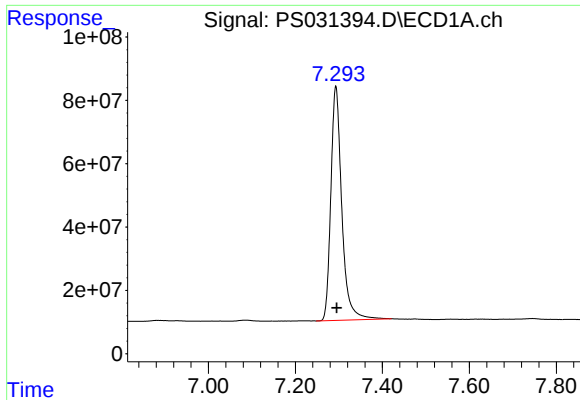

#4 2,4-DCAA


R.T.: 7.293 min
Delta R.T.: -0.002 min
Response: 1290049954
Conc: 406.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

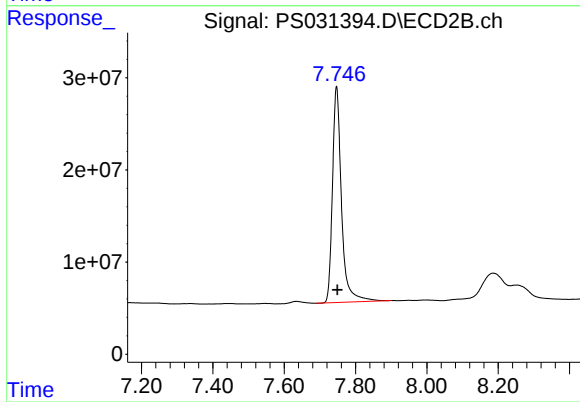


#4 2,4-DCAA

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 413618197
Conc: 489.29 ng/ml

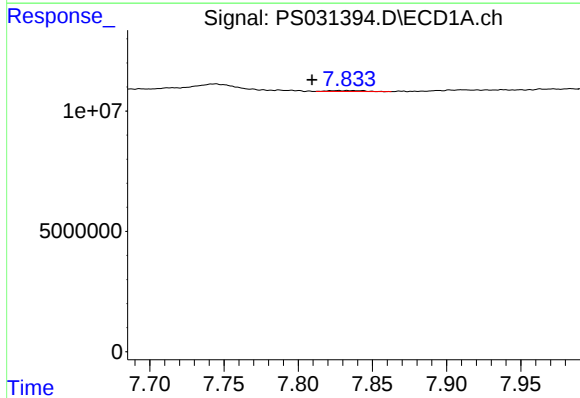


#7 MCPA

R.T.: 7.827 min
Delta R.T.: 0.018 min
Response: 655200
Conc: N.D.

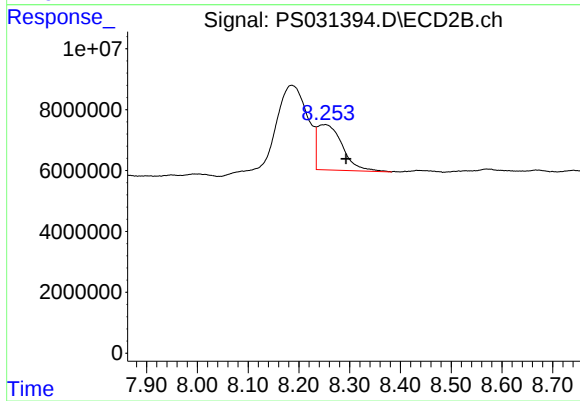

#7 MCPA


R.T.: 8.251 min
Delta R.T.: -0.042 min
Response: 50755564
Conc: 18.09 ug/ml

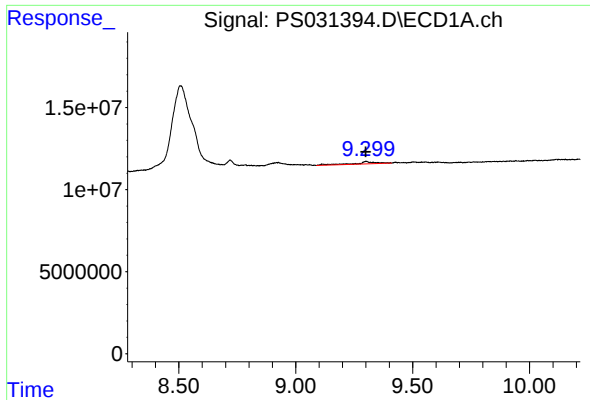

#11 2,4,5-TP (SILVEX)

R.T.: 9.301 min
Delta R.T.: 0.000 min
Response: 8404609
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

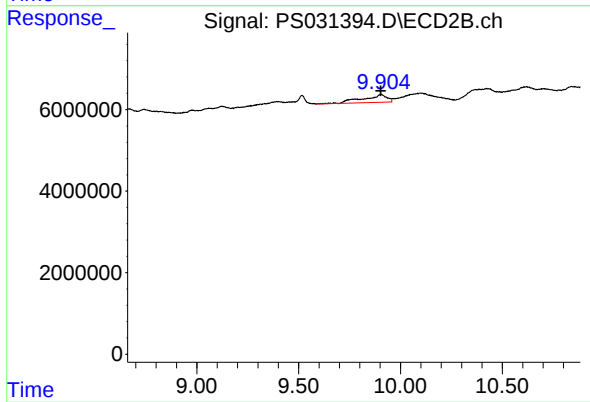

#11 2,4,5-TP (SILVEX)

R.T.: 9.905 min
Delta R.T.: 0.002 min
Response: 16009239
Conc: 1.22 ng/ml