

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080825\
 Data File : PS031400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 12:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 03:28:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.293	7.746	1335.6E6	401.0E6	420.806	474.360
Target Compounds							
1) T	Dalapon	0.000	2.658f	0	11064602	N.D.	4.158
2) T	3,5-DICHL...	6.455	0.000	822375	0	<MDL	N.D. #
3) T	4-Nitroph...	7.081	7.250f	3459801	-477722	3.354	N.D. #
5) T	DICAMBA	7.468	7.974f	829588	8105737	<MDL	1.426 #
6) T	MCPD	7.617f	0.000	1113774	0	<MDL	N.D. #
7) T	MCPA	7.828	8.259f	7092920	98675682	<MDL	35.172 #
8) T	DICHLORPROP	8.215f	0.000	686126	0	<MDL	N.D. #
10) T	Pentachlo...	8.721	0.000	3406313	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.302	0.000	8663164	0	<MDL	N.D. #
12) T	2,4,5-T	9.594	0.000	3859395	0	<MDL	N.D. #
13) T	2,4-DB	10.184	0.000	269.1E6	0	140.019	N.D. #
14) T	DINOSEB	11.375	11.320f	409002	3504156	<MDL	<MDL #
16) T	DCPA	11.663	12.311	8869864	4659823	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080825\
Data File : PS031400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 12:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 03:28:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

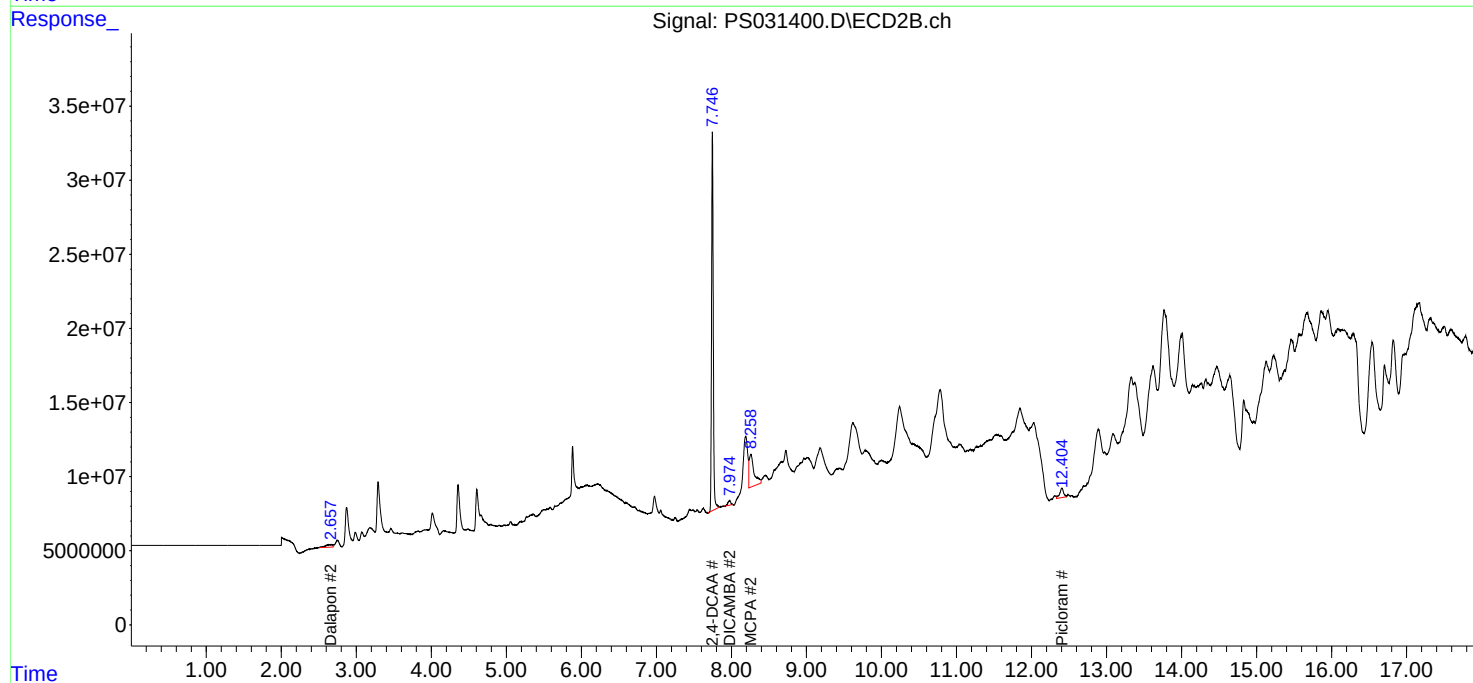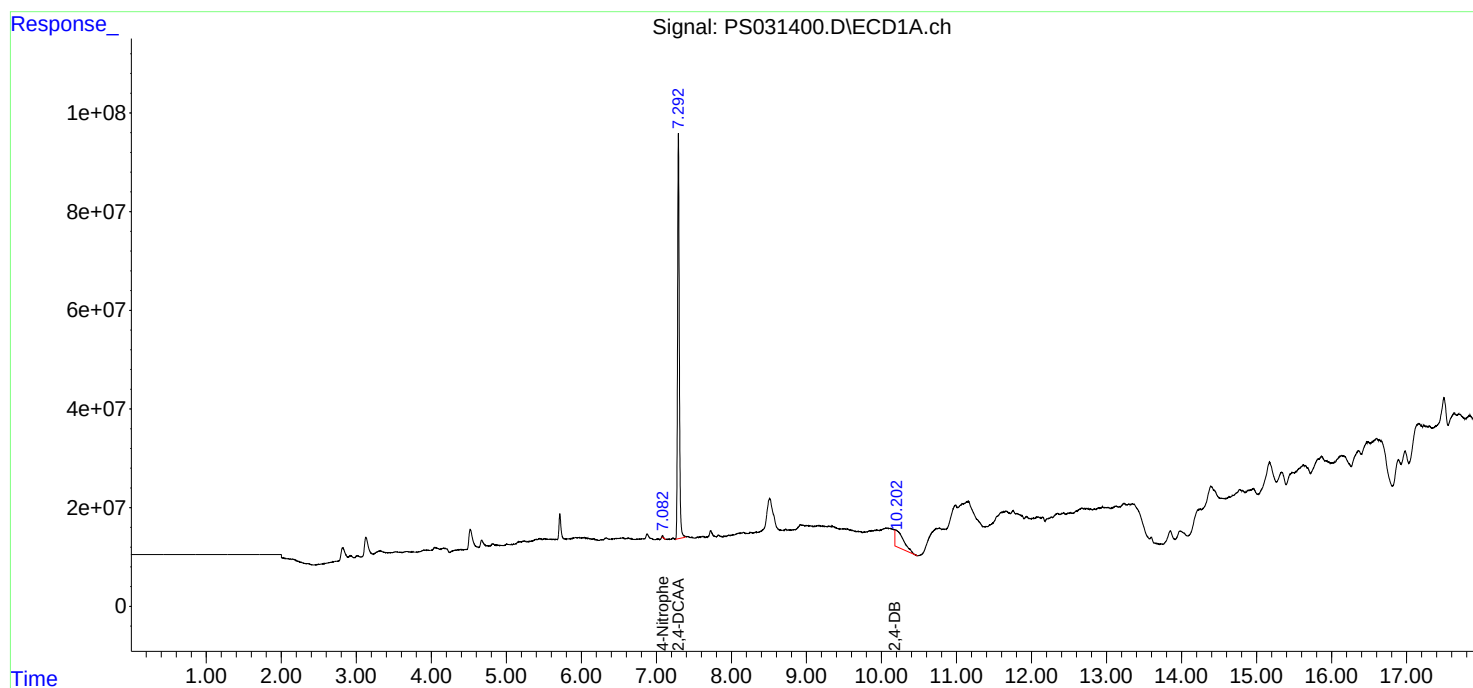


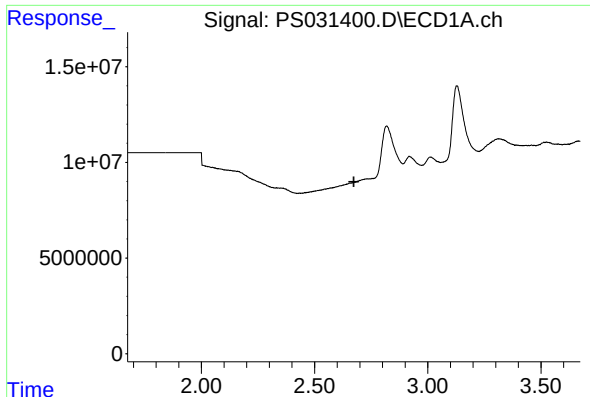

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

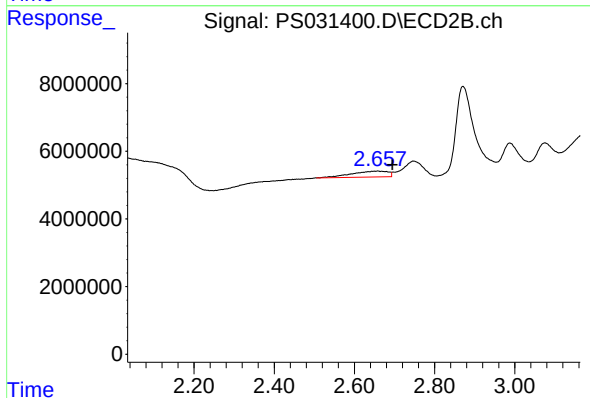


#1 Dalapon

R.T.: 2.658 min
Delta R.T.: -0.037 min
Response: 11064602
Conc: 4.16 ng/ml

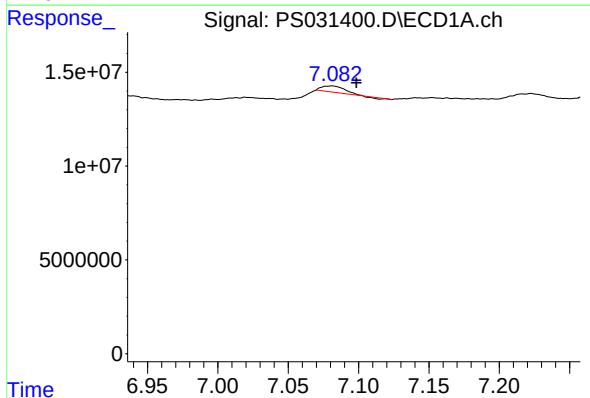


#3 4-Nitrophenol

R.T.: 7.081 min
Delta R.T.: -0.017 min
Response: 3459801
Conc: 3.35 ng/ml

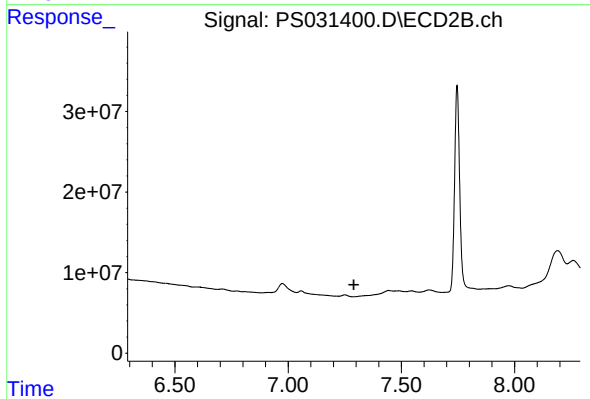

#3 4-Nitrophenol


R.T.: 7.250 min
Delta R.T.: -0.041 min
Response: -477722
Conc: N.D.

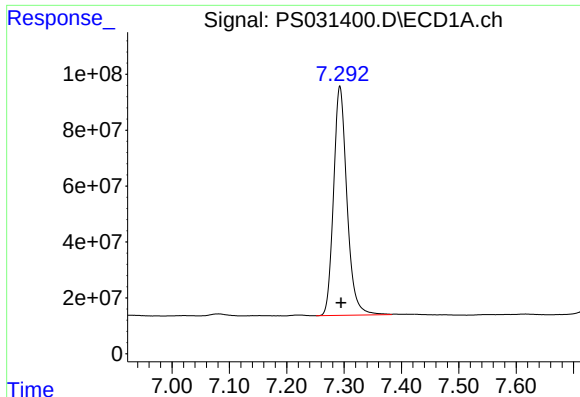

#4 2,4-DCAA


R.T.: 7.293 min
Delta R.T.: -0.002 min
Response: 1335634465
Conc: 420.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

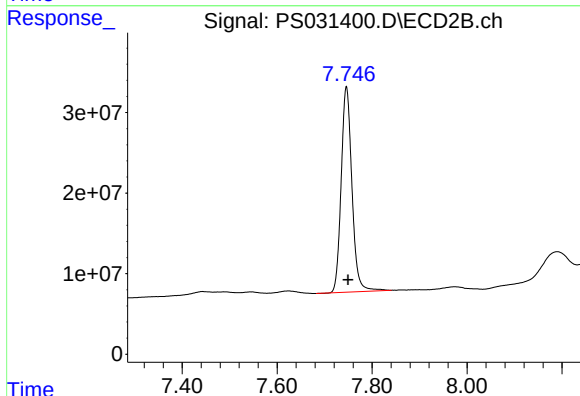


#4 2,4-DCAA

R.T.: 7.746 min
Delta R.T.: -0.003 min
Response: 400995000
Conc: 474.36 ng/ml

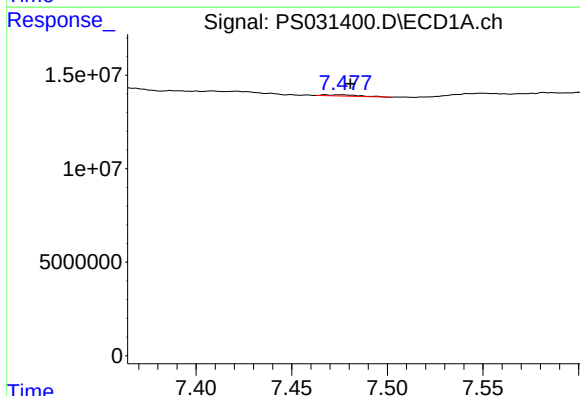


#5 DICAMBA

R.T.: 7.468 min
Delta R.T.: -0.013 min
Response: 829588
Conc: N.D.

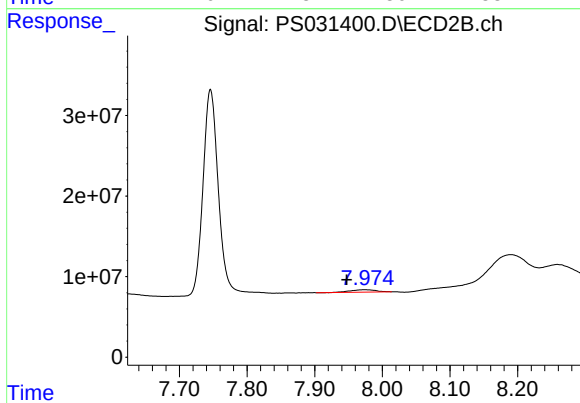

#5 DICAMBA


R.T.: 7.974 min
Delta R.T.: 0.027 min
Response: 8105737
Conc: 1.43 ng/ml

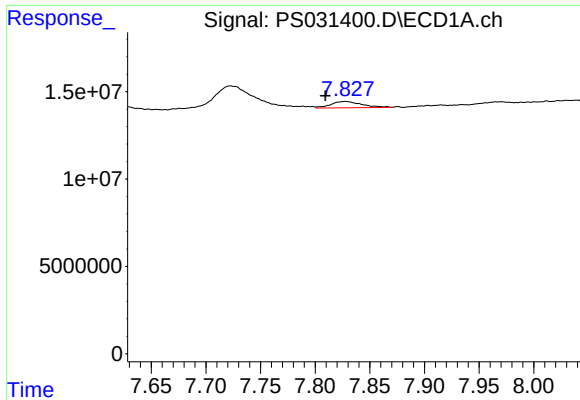

#7 MCPA


R.T.: 7.828 min
Delta R.T.: 0.018 min
Response: 7092920
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

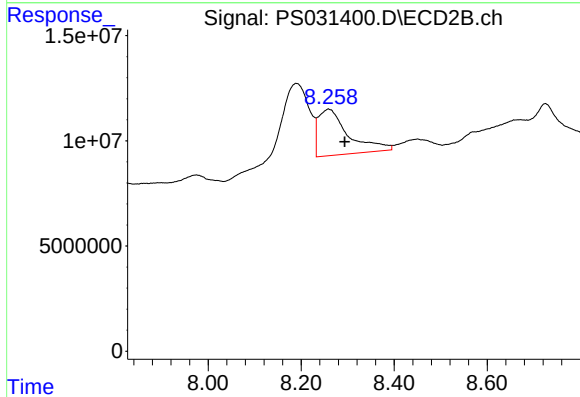


#7 MCPA

R.T.: 8.259 min
Delta R.T.: -0.034 min
Response: 98675682
Conc: 35.17 ug/ml

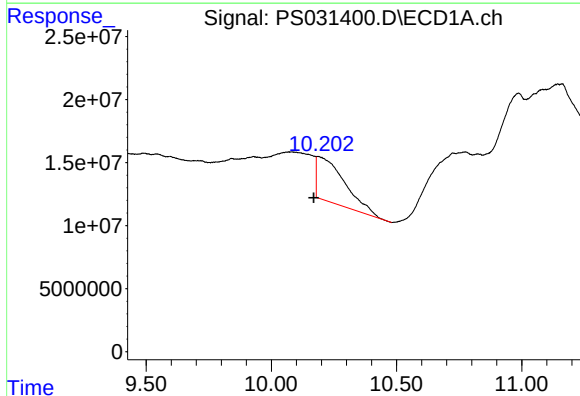


#13 2,4-DB

R.T.: 10.184 min
Delta R.T.: 0.014 min
Response: 269077824
Conc: 140.02 ng/ml

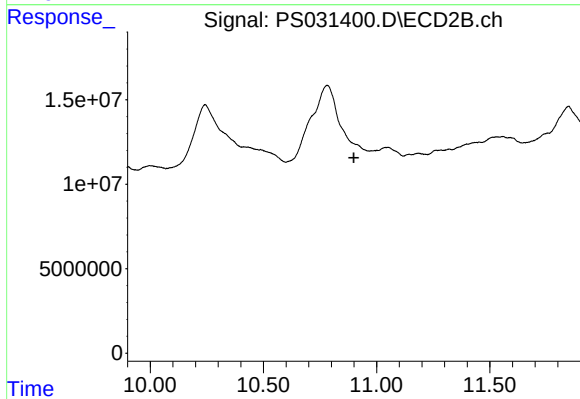

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.899 min
Response: 0
Conc: N.D.

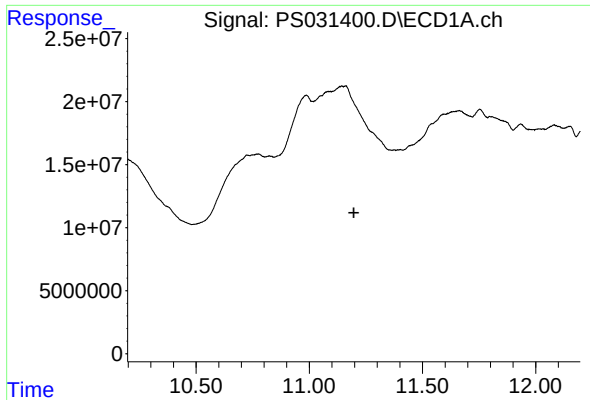

#15 Picloram

R.T.: 11.160 min
Delta R.T.: -0.037 min
Response: -30176716
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

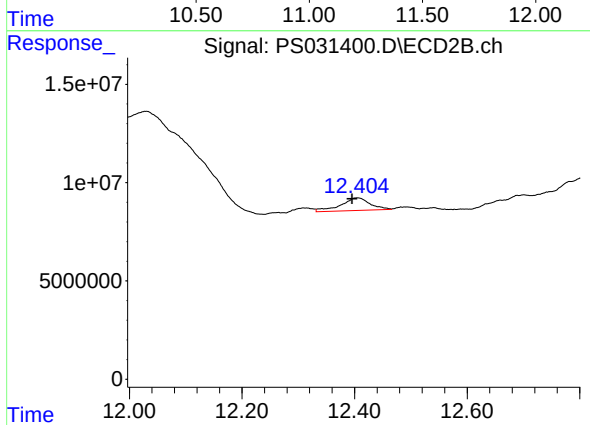

#15 Picloram

R.T.: 12.404 min
Delta R.T.: 0.009 min
Response: 23251058
Conc: 1.33 ng/ml