

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080919\
 Data File : PS005965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 10:25
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 03:04:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.539	5.254	604.4E6	280.5E6	416.583	281.960 #
Target Compounds							
5) T	DICAMBA	0.000	5.429	0	106.7E6	N.D.	28.592
6) T	MCPD	0.000	5.523	0	31441749	N.D.	11.039
9) T	2,4-D	6.582	0.000	484.4E6	0	323.241	N.D. #
14) T	DINOSEB	9.264	0.000	49805935	0	7.670	N.D. #
15) T	Picloram	0.000	9.125	0	31877542	N.D.	4.243



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080919\
Data File : PS005965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 10:25
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 03:04:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

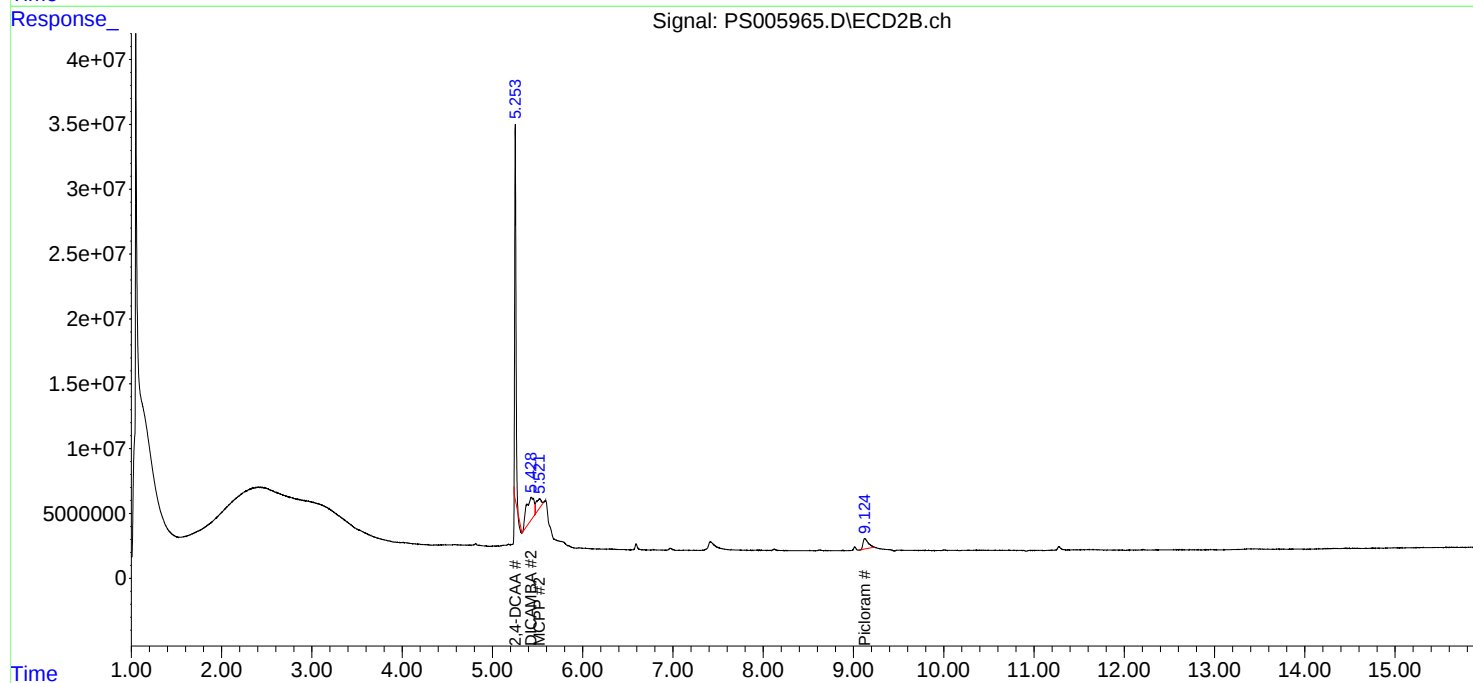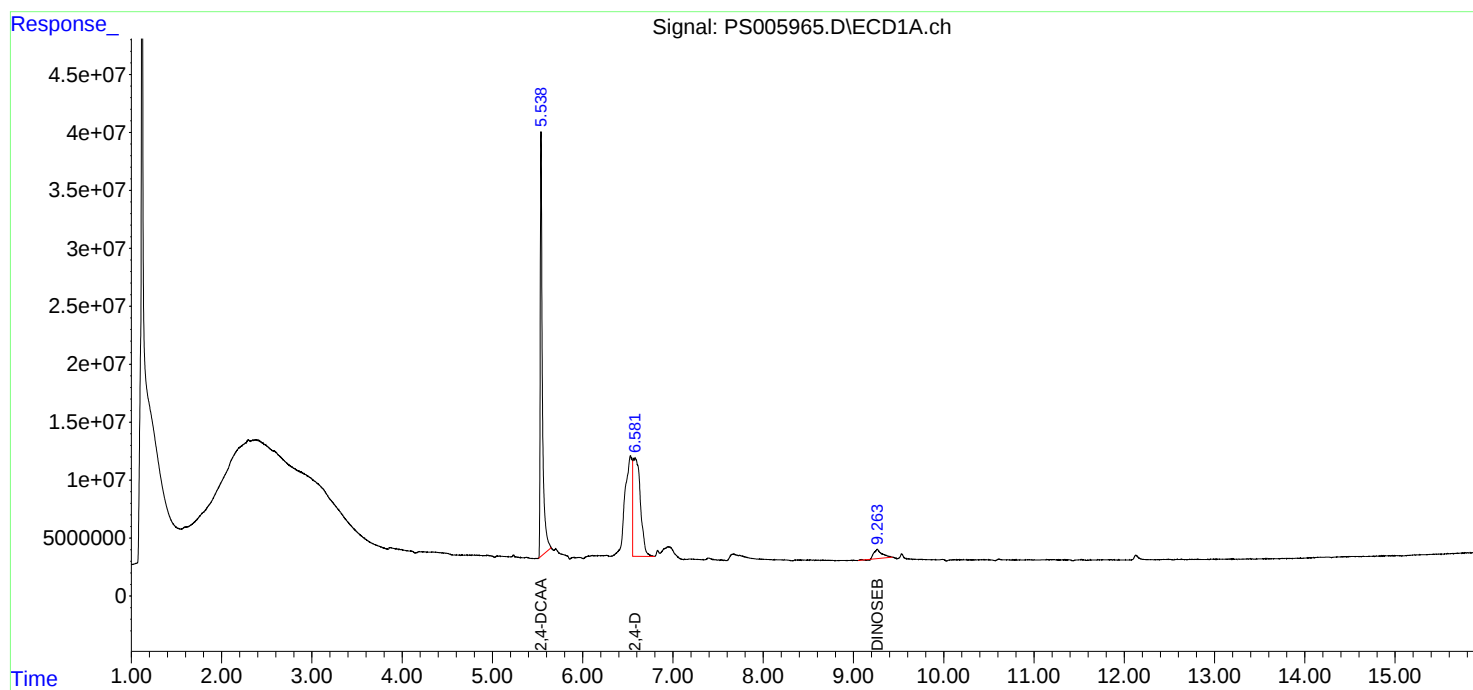


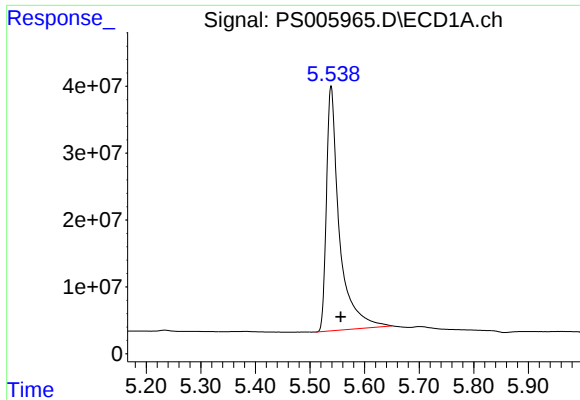

#4 2,4-DCAA


R.T.: 5.539 min
Delta R.T.: -0.017 min
Response: 604385779
Conc: 416.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

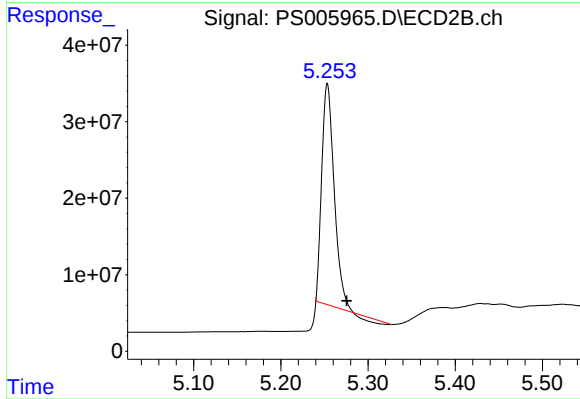


#4 2,4-DCAA

R.T.: 5.254 min
Delta R.T.: -0.022 min
Response: 280459435
Conc: 281.96 ng/ml

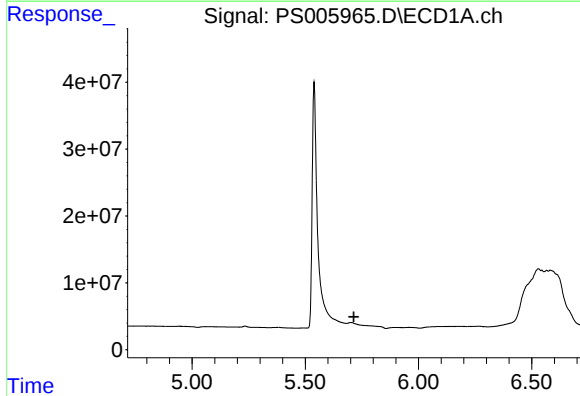


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.714 min
Response: 0
Conc: N.D.

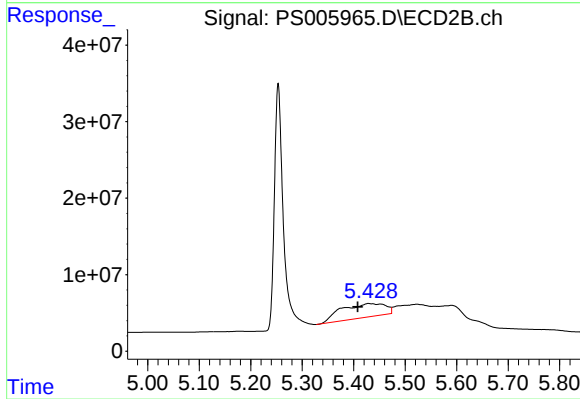

#5 DICAMBA


R.T.: 5.429 min
Delta R.T.: 0.021 min
Response: 106733973
Conc: 28.59 ng/ml

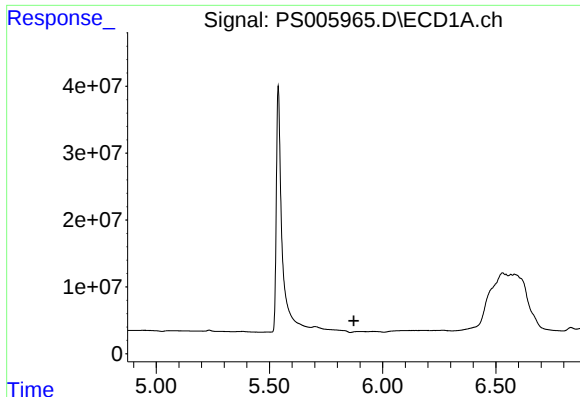

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.873 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

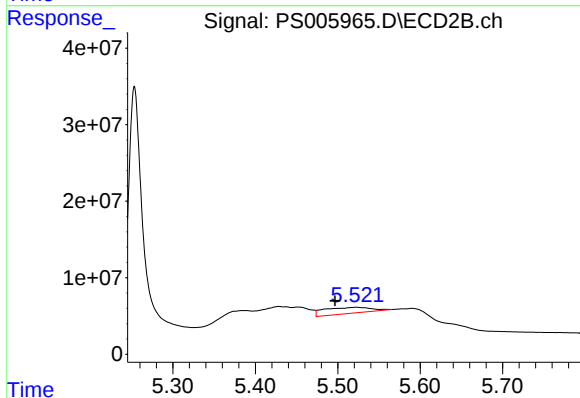


#6 MCP

R.T.: 5.523 min
Delta R.T.: 0.026 min
Response: 31441749
Conc: 11.04 ug/ml

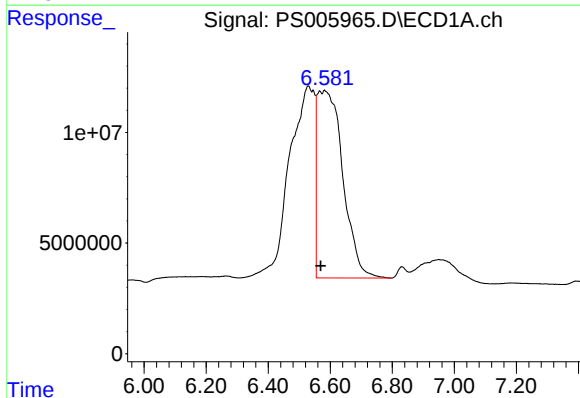


#9 2,4-D

R.T.: 6.582 min
Delta R.T.: 0.013 min
Response: 484430797
Conc: 323.24 ng/ml

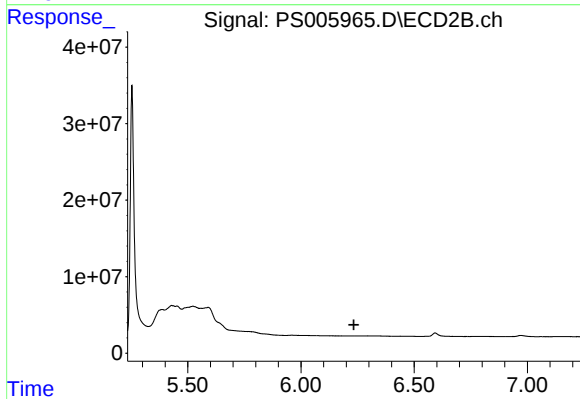

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.

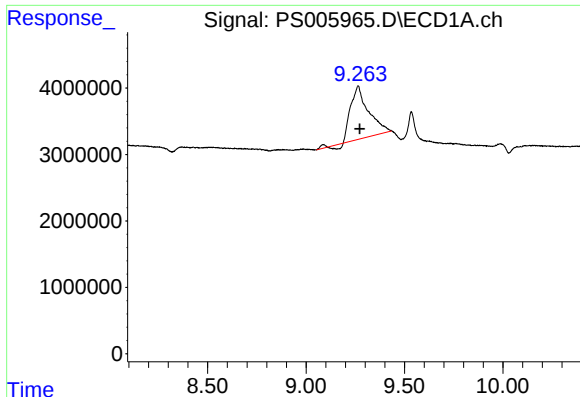

#14 DINOSEB


R.T.: 9.264 min
Delta R.T.: -0.009 min
Response: 49805935
Conc: 7.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

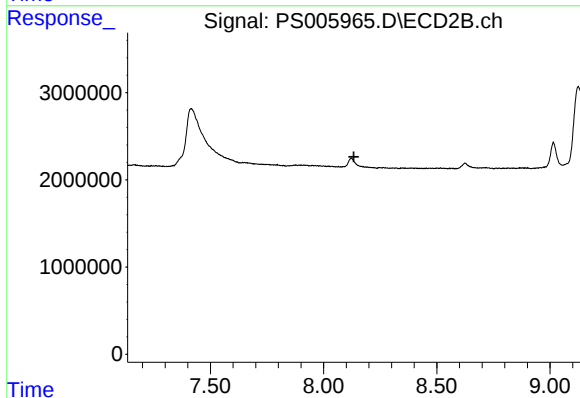


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.134 min
Response: 0
Conc: N.D.

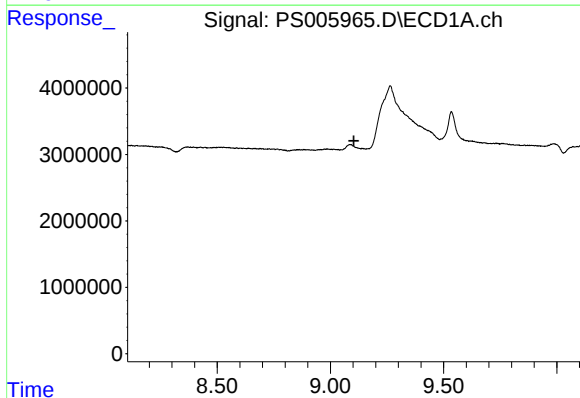

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.104 min
Response: 0
Conc: N.D.

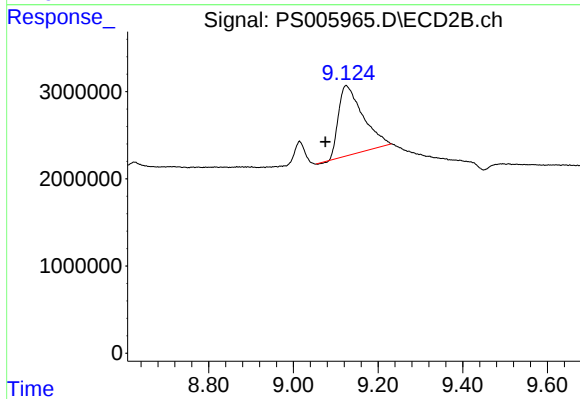

#15 Picloram

R.T.: 9.125 min
Delta R.T.: 0.050 min
Response: 31877542
Conc: 4.24 ng/ml