

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080919\
 Data File : PS005969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 11:53
 Operator : SM\AJ
 Sample : PB122081TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 03:06:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.293	704.6E6	467.6E6	485.642	470.057
Target Compounds							
2) T	3,5-DICHL...	0.000	4.612	0	200.3E6	N.D.	154.389
3) T	4-Nitroph...	5.362	0.000	8137784	0	13.529	N.D. #
5) T	DICAMBA	5.669	5.399	7794106	22644560	1.305	6.066 #
6) T	MCP	5.875	0.000	14888278	0	3.213	N.D. #
7) T	MCPA	5.977	5.682	44402429	36804204	6.804	8.744 #
8) T	DICHLORPROP	0.000	5.987	0	28718219	N.D.	31.096
10) T	Pentachlo...	0.000	6.552	0	19083268	N.D.	1.470
12) T	2,4,5-T	7.577	0.000	57632942	0	6.905	N.D. #
15) T	Picloram	9.169	9.113	28722618	21258322	2.454	2.830



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080919\
Data File : PS005969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 11:53
Operator : SM\AJ
Sample : PB122081TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 03:06:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

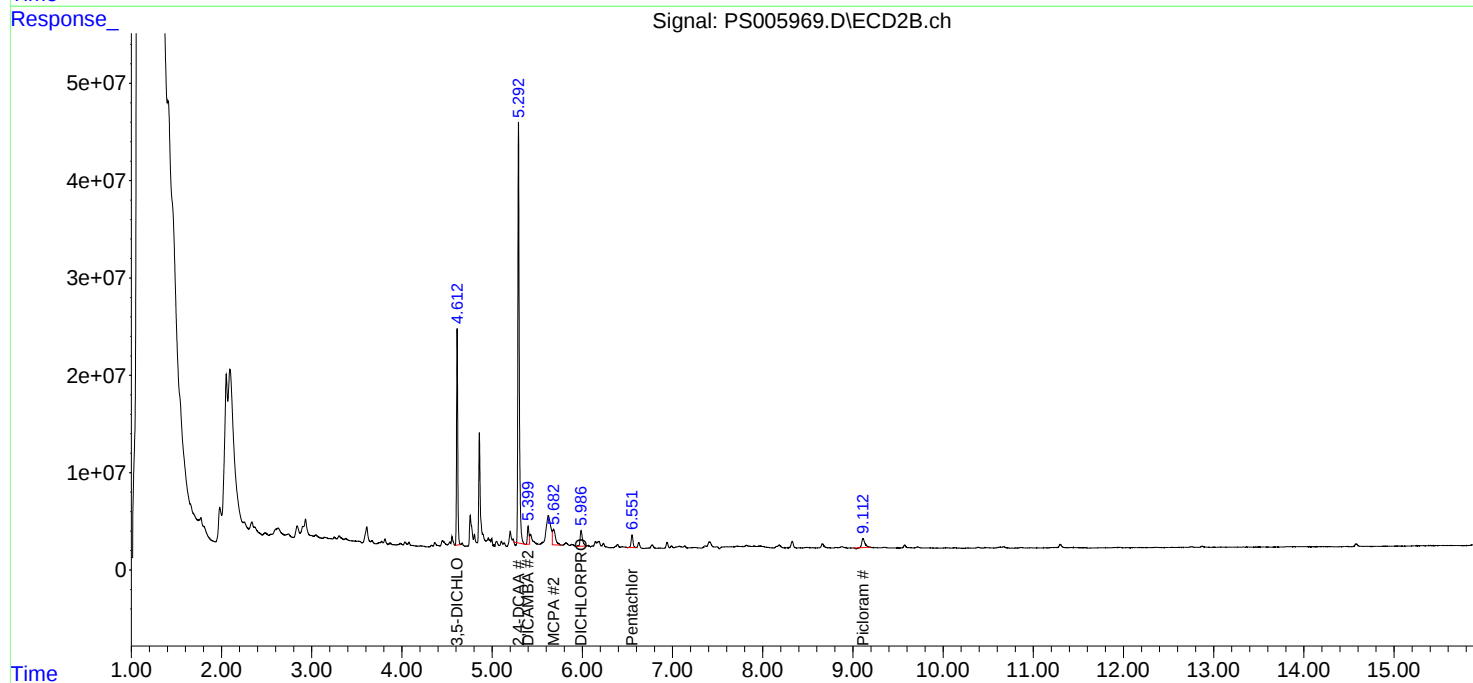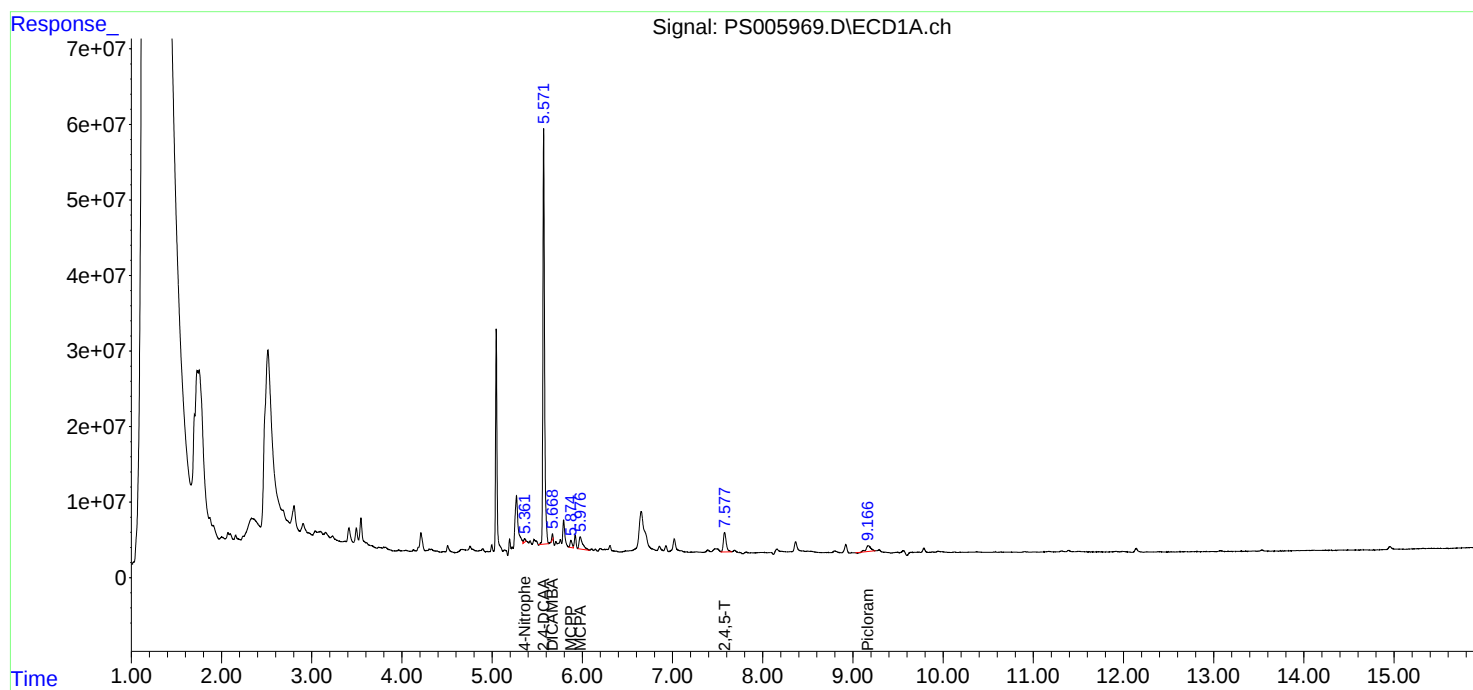


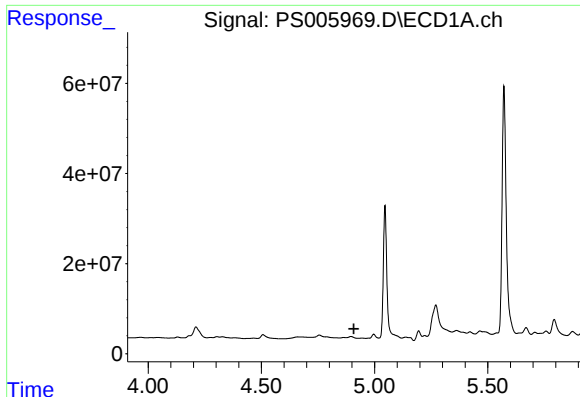

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

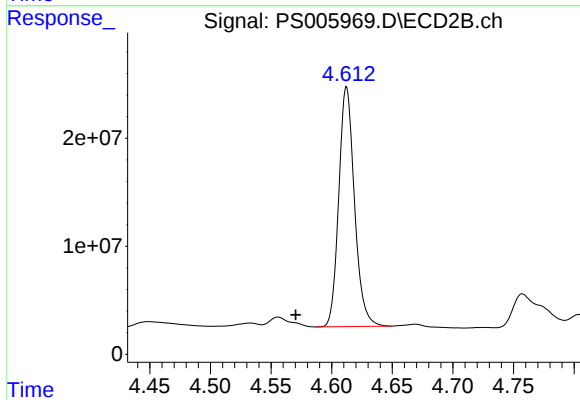


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.612 min
Delta R.T.: 0.042 min
Response: 200291140
Conc: 154.39 ng/ml

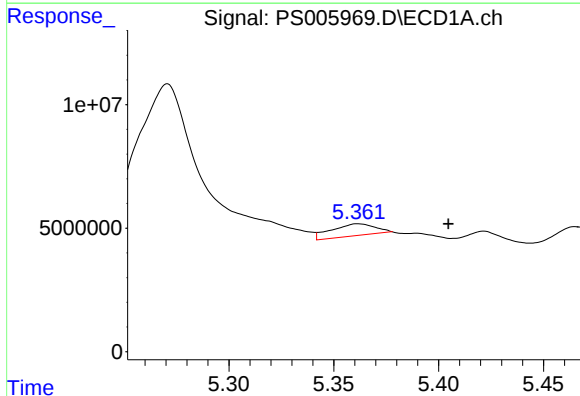


#3 4-Nitrophenol

R.T.: 5.362 min
Delta R.T.: -0.043 min
Response: 8137784
Conc: 13.53 ng/ml

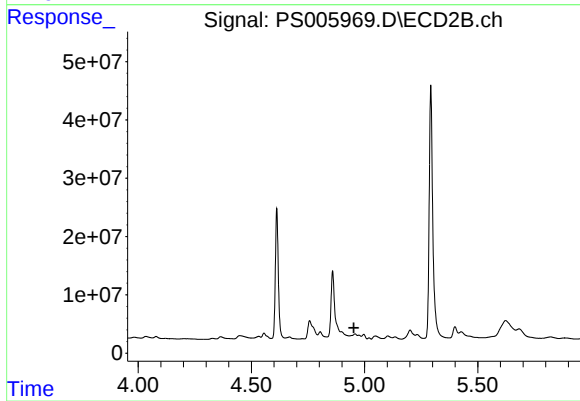

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

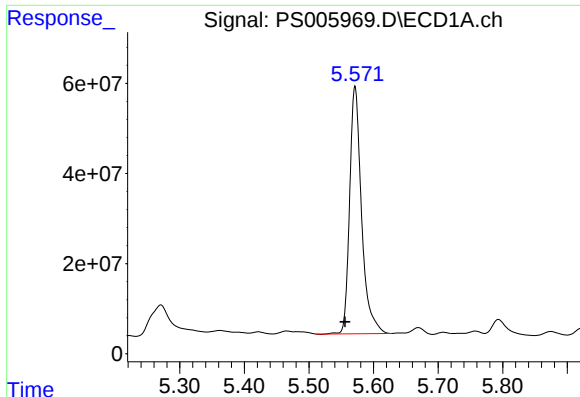

#4 2,4-DCAA


R.T.: 5.572 min
Delta R.T.: 0.015 min
Response: 704577501
Conc: 485.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

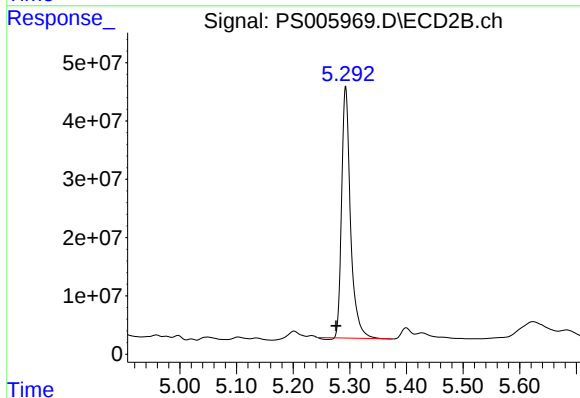


#4 2,4-DCAA

R.T.: 5.293 min
Delta R.T.: 0.017 min
Response: 467555732
Conc: 470.06 ng/ml

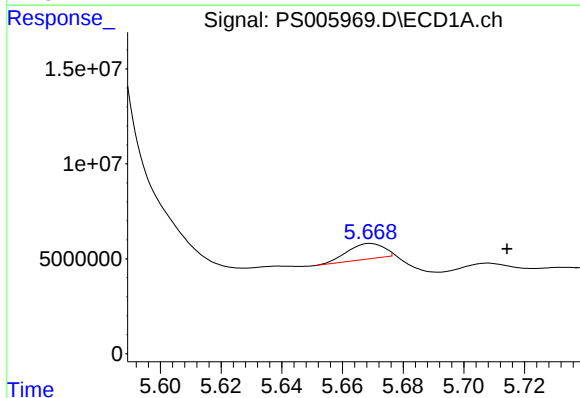


#5 DICAMBA

R.T.: 5.669 min
Delta R.T.: -0.045 min
Response: 7794106
Conc: 1.31 ng/ml

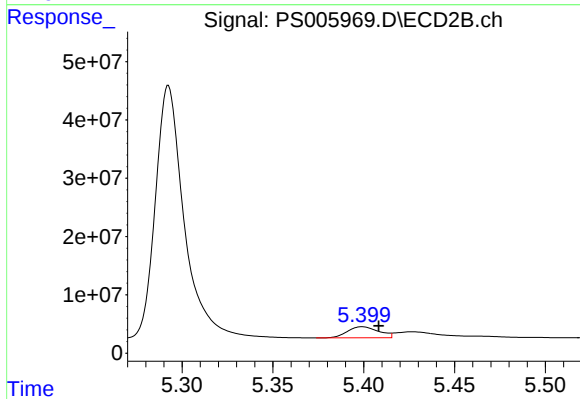

#5 DICAMBA


R.T.: 5.399 min
Delta R.T.: -0.009 min
Response: 22644560
Conc: 6.07 ng/ml

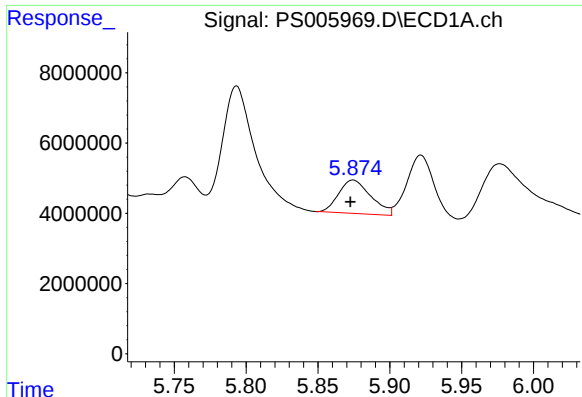

#6 MCPP


R.T.: 5.875 min
Delta R.T.: 0.002 min
Response: 14888278
Conc: 3.21 ug/ml

Instrument :
ECD_S
ClientSampleId :

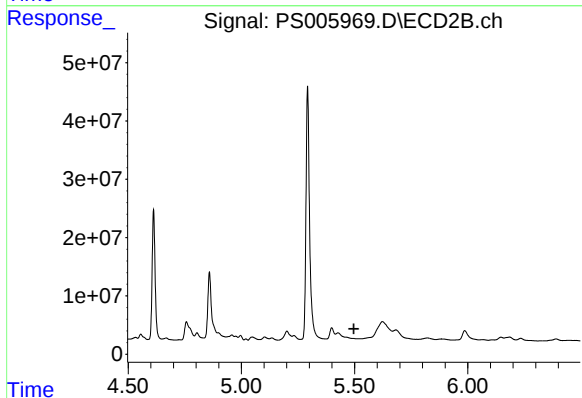


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

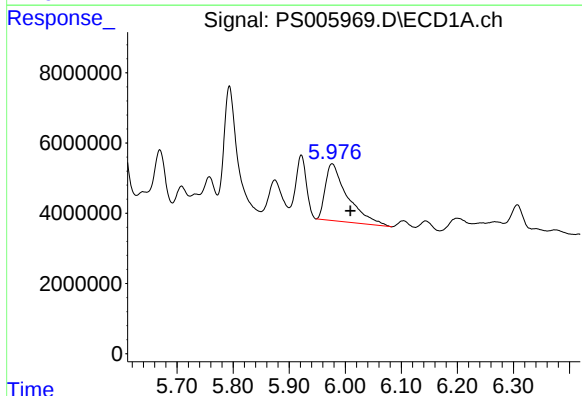


#7 MCPA

R.T.: 5.977 min
Delta R.T.: -0.032 min
Response: 44402429
Conc: 6.80 ug/ml

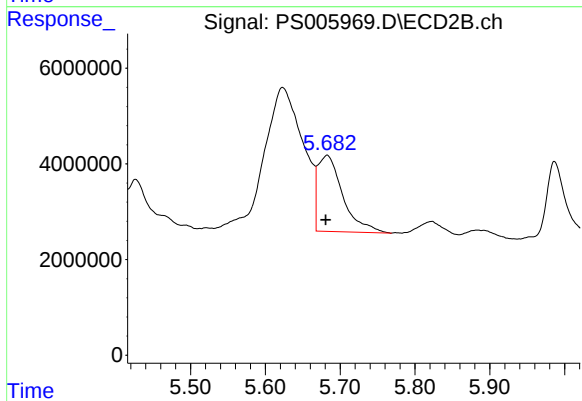

#7 MCPA


R.T.: 5.682 min
Delta R.T.: 0.002 min
Response: 36804204
Conc: 8.74 ug/ml

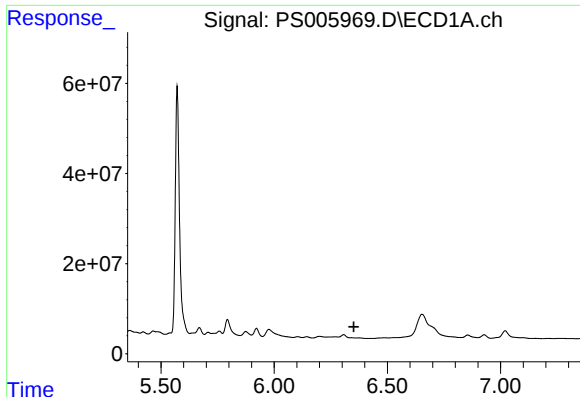

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

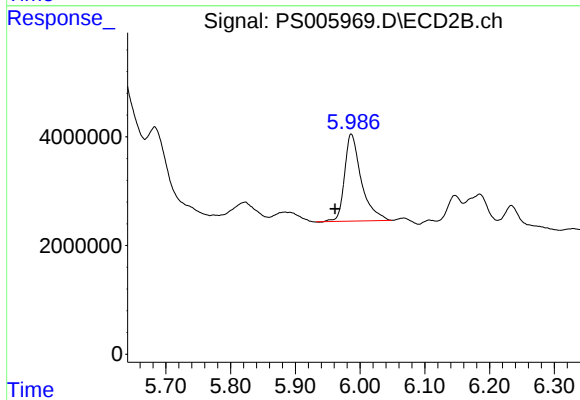


#8 DICHLORPROP

R.T.: 5.987 min
Delta R.T.: 0.025 min
Response: 28718219
Conc: 31.10 ng/ml

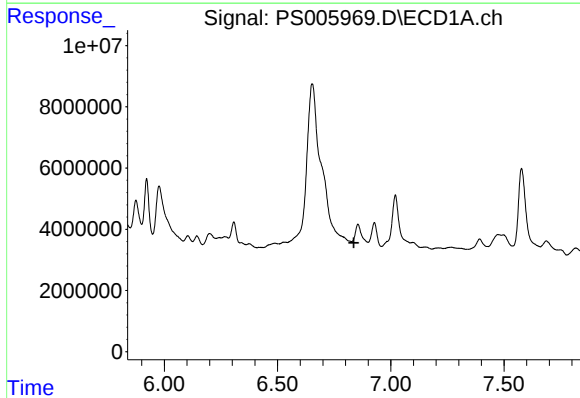


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

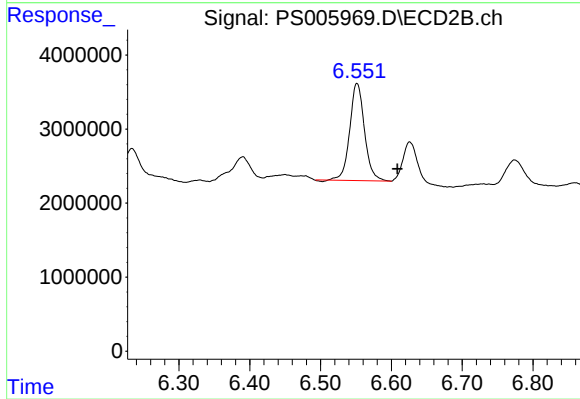

#10 Pentachlorophenol


R.T.: 6.552 min
Delta R.T.: -0.057 min
Response: 19083268
Conc: 1.47 ng/ml

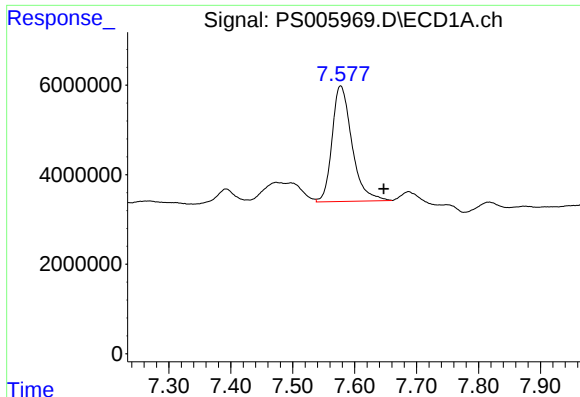

#12 2,4,5-T


R.T.: 7.577 min
Delta R.T.: -0.069 min
Response: 57632942
Conc: 6.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

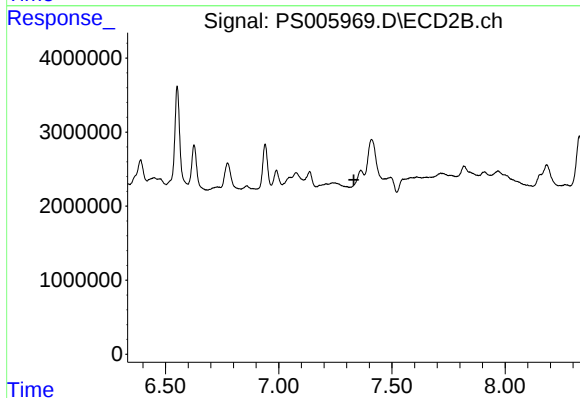


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

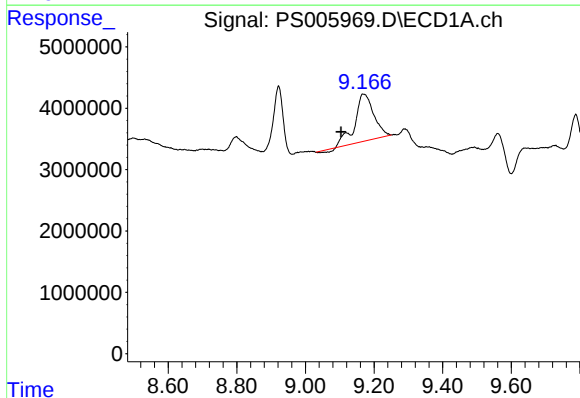

#15 Picloram

R.T.: 9.169 min
Delta R.T.: 0.065 min
Response: 28722618
Conc: 2.45 ng/ml

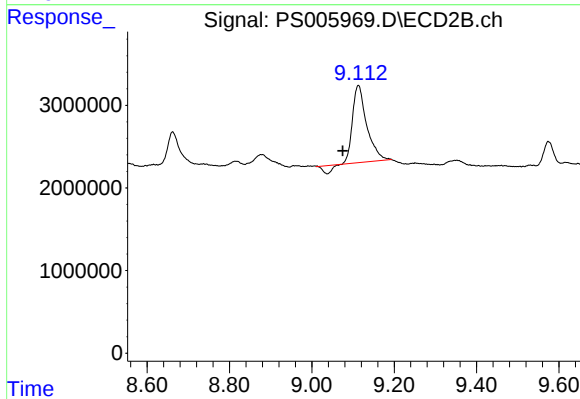

#15 Picloram

R.T.: 9.113 min
Delta R.T.: 0.038 min
Response: 21258322
Conc: 2.83 ng/ml