

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080919\
 Data File : PS005982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 17:03
 Operator : SM\AJ
 Sample : K4152-31
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 03:12:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.573	5.293	629.4E6	428.7E6	433.791	430.965
Target Compounds							
1) T	Dalapon	2.072	0.000	21370659	0	11.531	N.D. #
2) T	3,5-DICHL...	0.000	4.613	0	208.1E6	N.D.	160.430
3) T	4-Nitroph...	5.363	0.000	4091115	0	6.801	N.D. #
5) T	DICAMBA	5.669	5.399	5845123	11079921	<MDL	2.968 #
6) T	MCP	5.924	0.000	13884577	0	2.997	N.D. #
7) T	MCPA	0.000	5.624	0	136.4E6	N.D.	32.403
10) T	Pentachlo...	0.000	6.552	0	24387981	N.D.	1.878
11) T	2,4,5-TP ...	0.000	6.942	0	16232057	N.D.	3.129
12) T	2,4,5-T	7.578	0.000	84636662	0	10.140	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080919\
Data File : PS005982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 17:03
Operator : SM\AJ
Sample : K4152-31
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 03:12:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

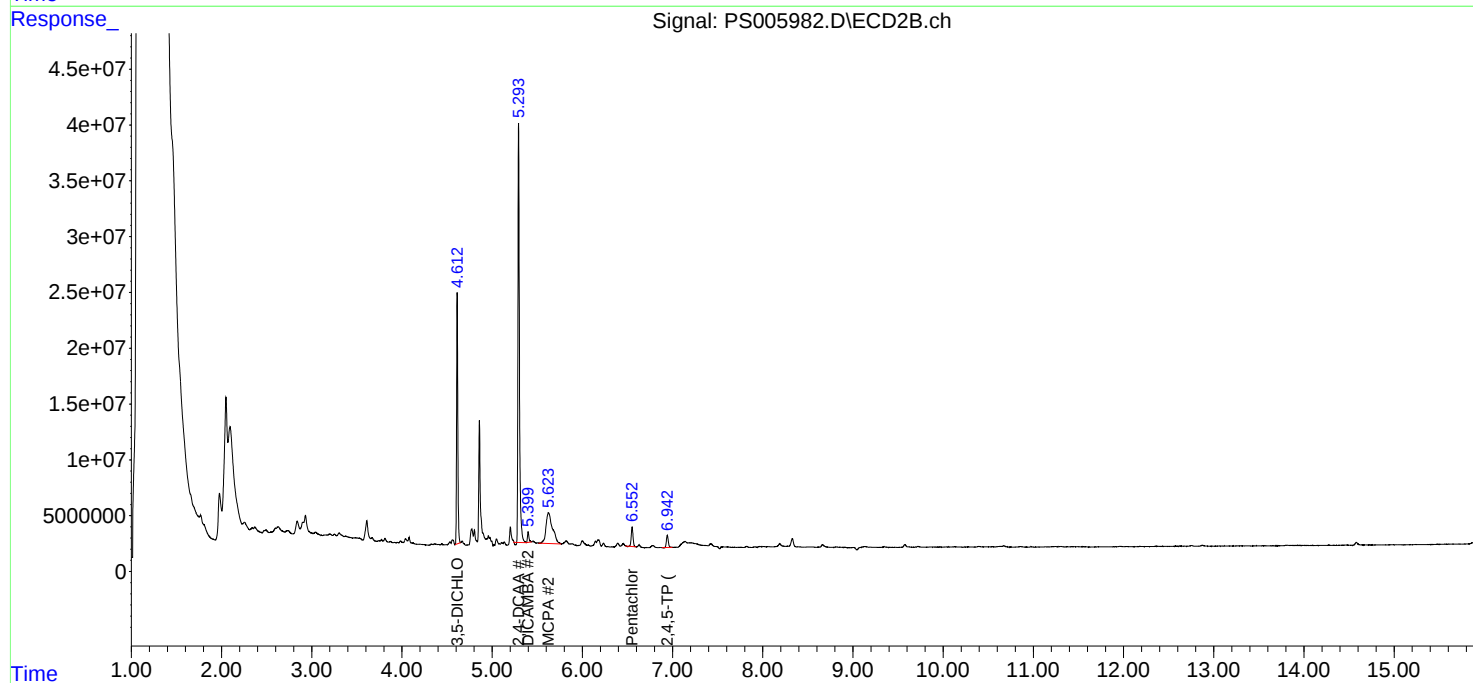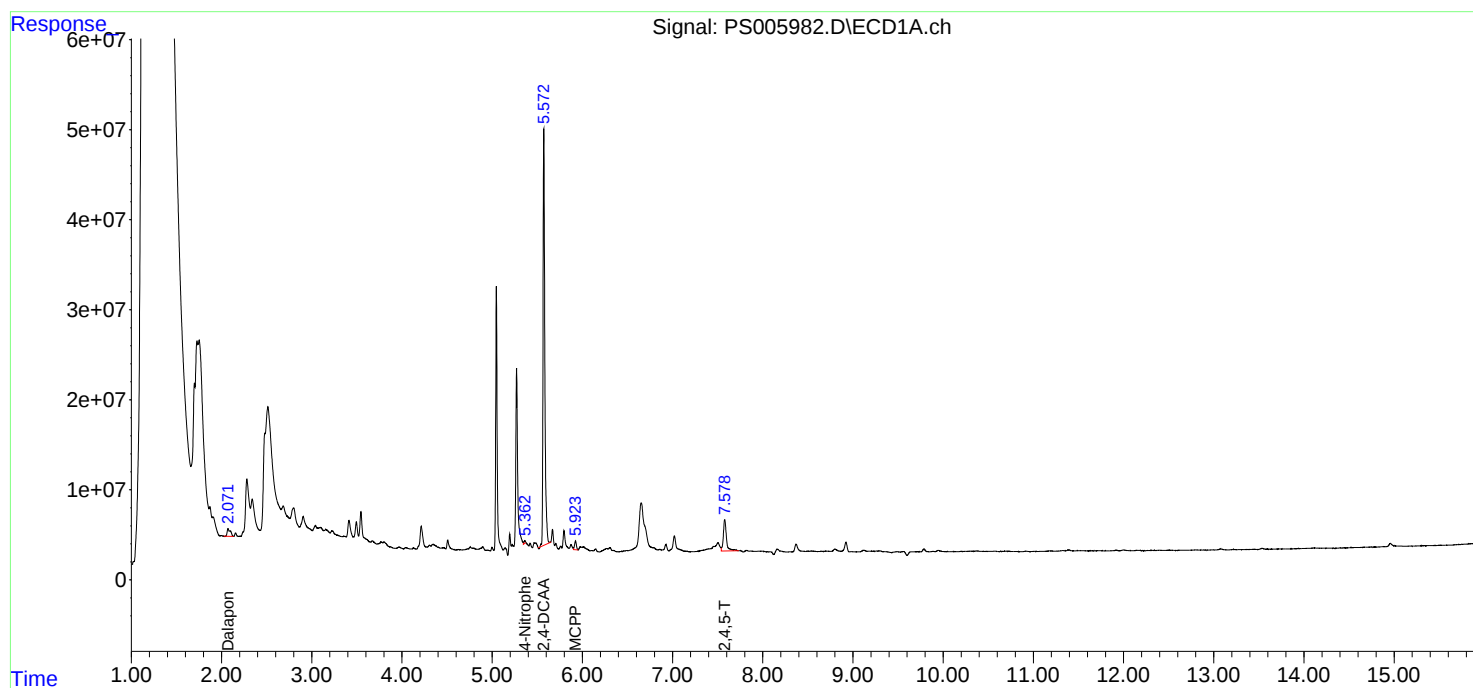


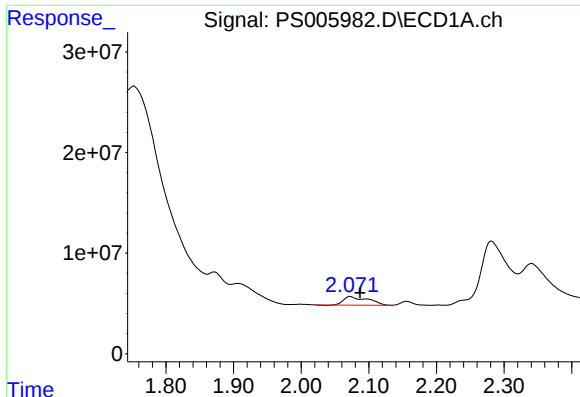

#1 Dalapon


R.T.: 2.072 min
Delta R.T.: -0.015 min
Response: 21370659
Conc: 11.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

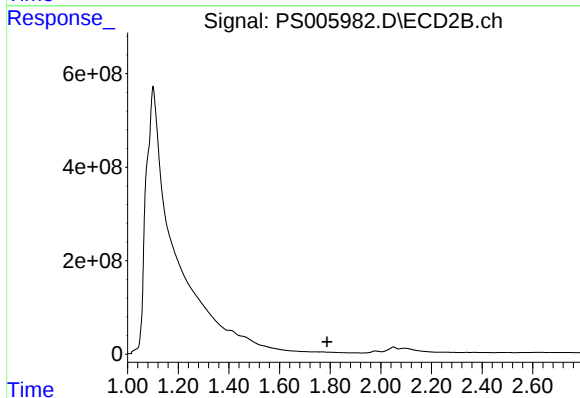


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

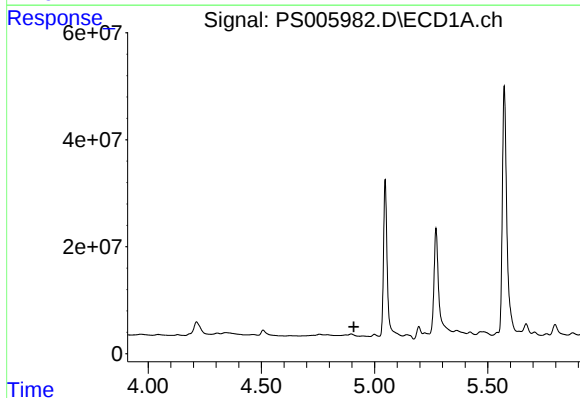


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

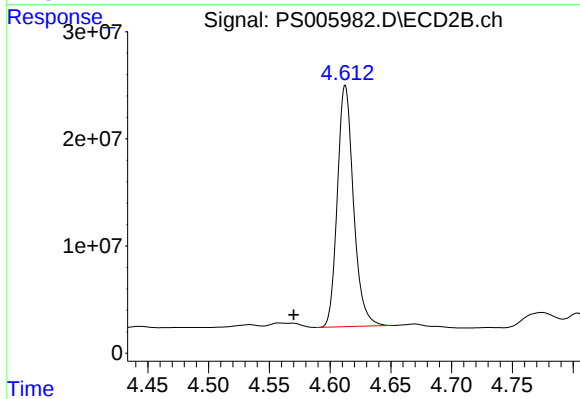

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.613 min
Delta R.T.: 0.042 min
Response: 208127984
Conc: 160.43 ng/ml

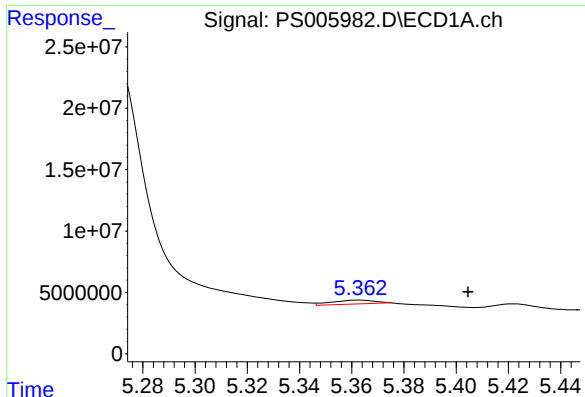

#3 4-Nitrophenol


R.T.: 5.363 min
Delta R.T.: -0.042 min
Response: 4091115
Conc: 6.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

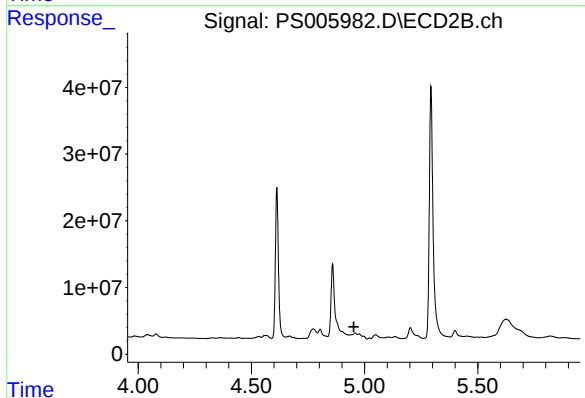


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

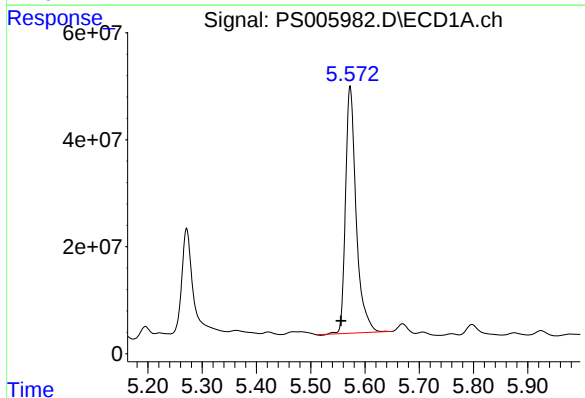


#4 2,4-DCAA

R.T.: 5.573 min
Delta R.T.: 0.017 min
Response: 629351054
Conc: 433.79 ng/ml

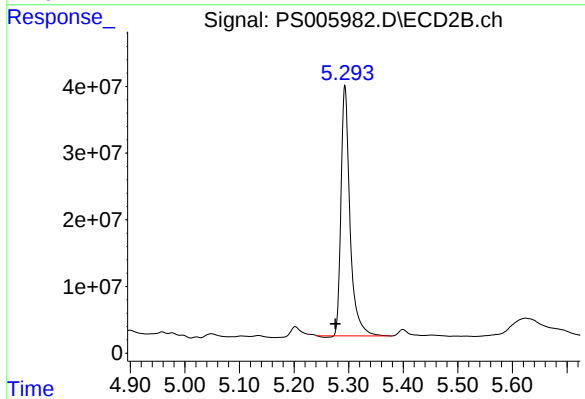

#4 2,4-DCAA


R.T.: 5.293 min
Delta R.T.: 0.018 min
Response: 428671464
Conc: 430.96 ng/ml

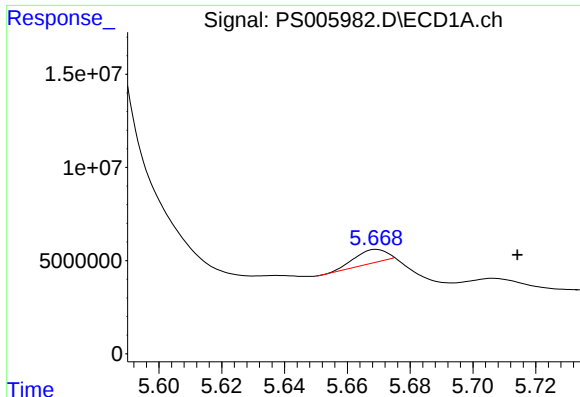

#5 DICAMBA


R.T.: 5.669 min
Delta R.T.: -0.045 min
Response: 5845123
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

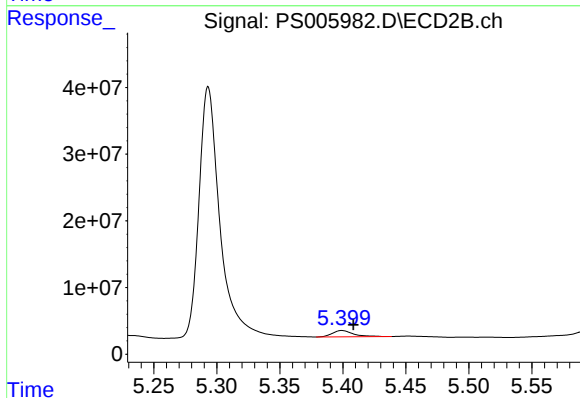


#5 DICAMBA

R.T.: 5.399 min
Delta R.T.: -0.009 min
Response: 11079921
Conc: 2.97 ng/ml

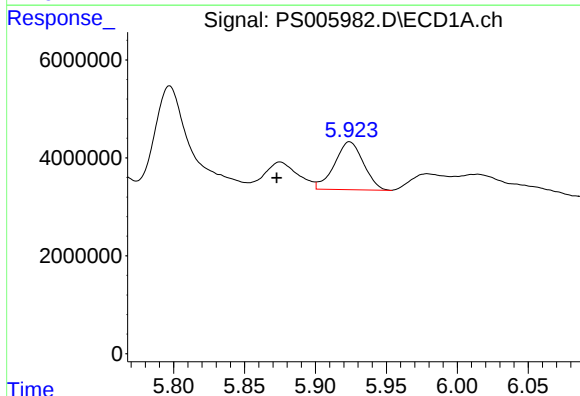


#6 MCP

R.T.: 5.924 min
Delta R.T.: 0.052 min
Response: 13884577
Conc: 3.00 ug/ml

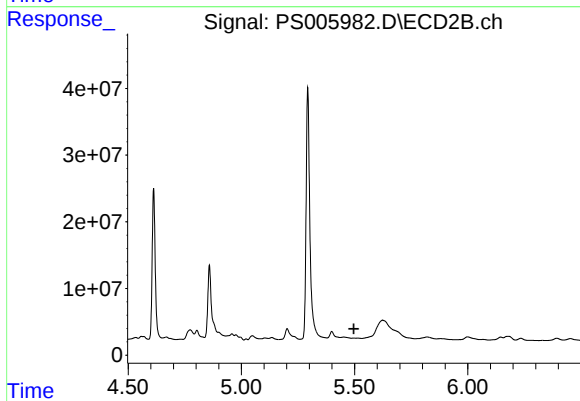

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

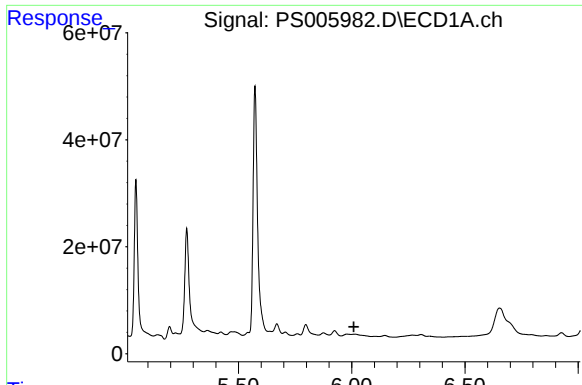

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

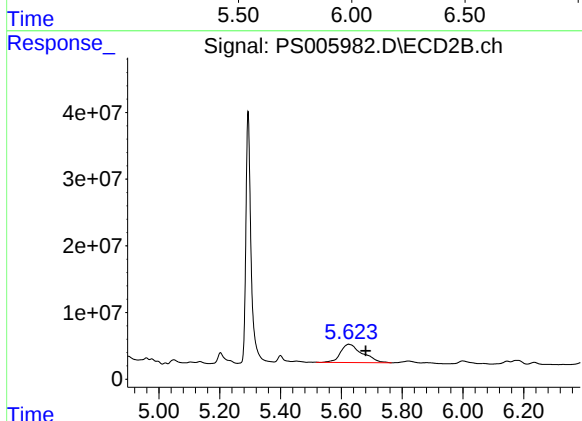


#7 MCPA

R.T.: 5.624 min
Delta R.T.: -0.057 min
Response: 136386589
Conc: 32.40 ug/ml

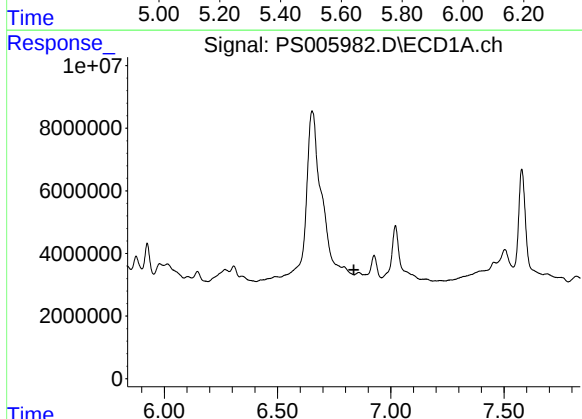


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

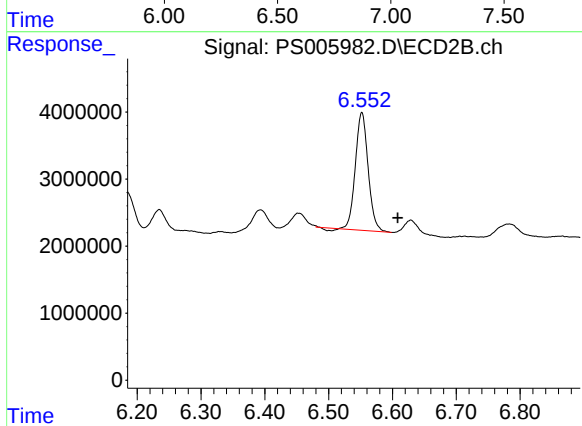

#10 Pentachlorophenol


R.T.: 6.552 min
Delta R.T.: -0.056 min
Response: 24387981
Conc: 1.88 ng/ml

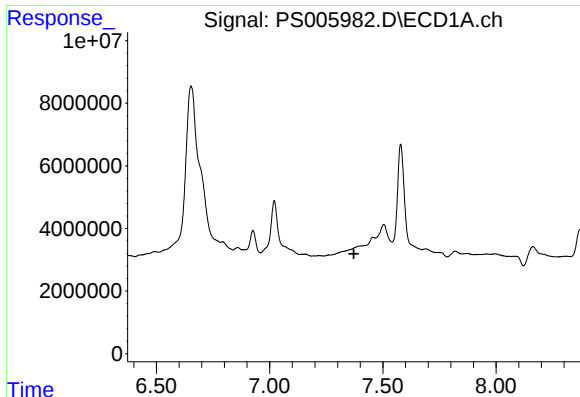

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

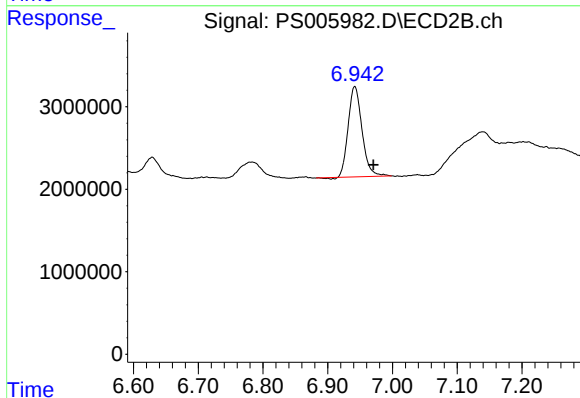


#11 2,4,5-TP (SILVEX)

R.T.: 6.942 min
Delta R.T.: -0.029 min
Response: 16232057
Conc: 3.13 ng/ml

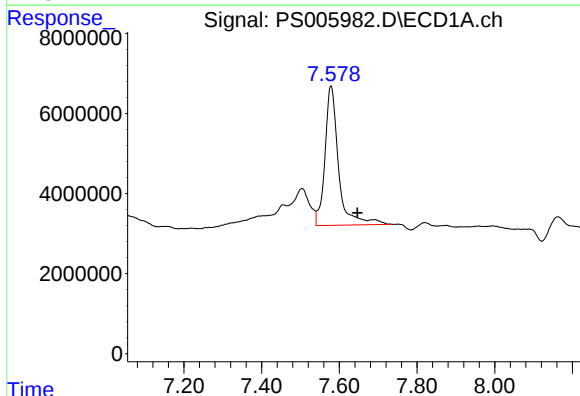

#12 2,4,5-T

R.T.: 7.578 min
Delta R.T.: -0.068 min
Response: 84636662
Conc: 10.14 ng/ml

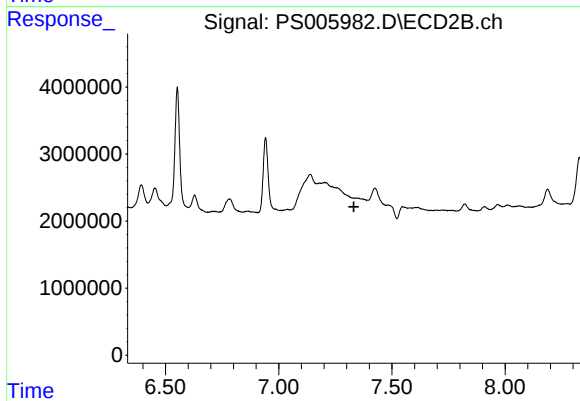

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.