

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080919\
 Data File : PS005983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 17:25
 Operator : SM\AJ
 Sample : K4152-36
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 03:13:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.570	5.291	555.7E6	378.5E6	382.996	380.521
Target Compounds							
2) T	3,5-DICHL...	0.000	4.610	0	198.9E6	N.D.	153.280
3) T	4-Nitroph...	5.360	0.000	5701097	0	9.478	N.D. #
5) T	DICAMBA	5.667	0.000	8421406	0	1.410	N.D. #
7) T	MCPA	0.000	5.622	0	134.7E6	N.D.	32.001
10) T	Pentachlo...	0.000	6.549	0	20203881	N.D.	1.556
11) T	2,4,5-TP ...	0.000	6.938	0	27622555	N.D.	5.325
12) T	2,4,5-T	7.580	0.000	78245630	0	9.374	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080919\
Data File : PS005983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 17:25
Operator : SM\AJ
Sample : K4152-36
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 03:13:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

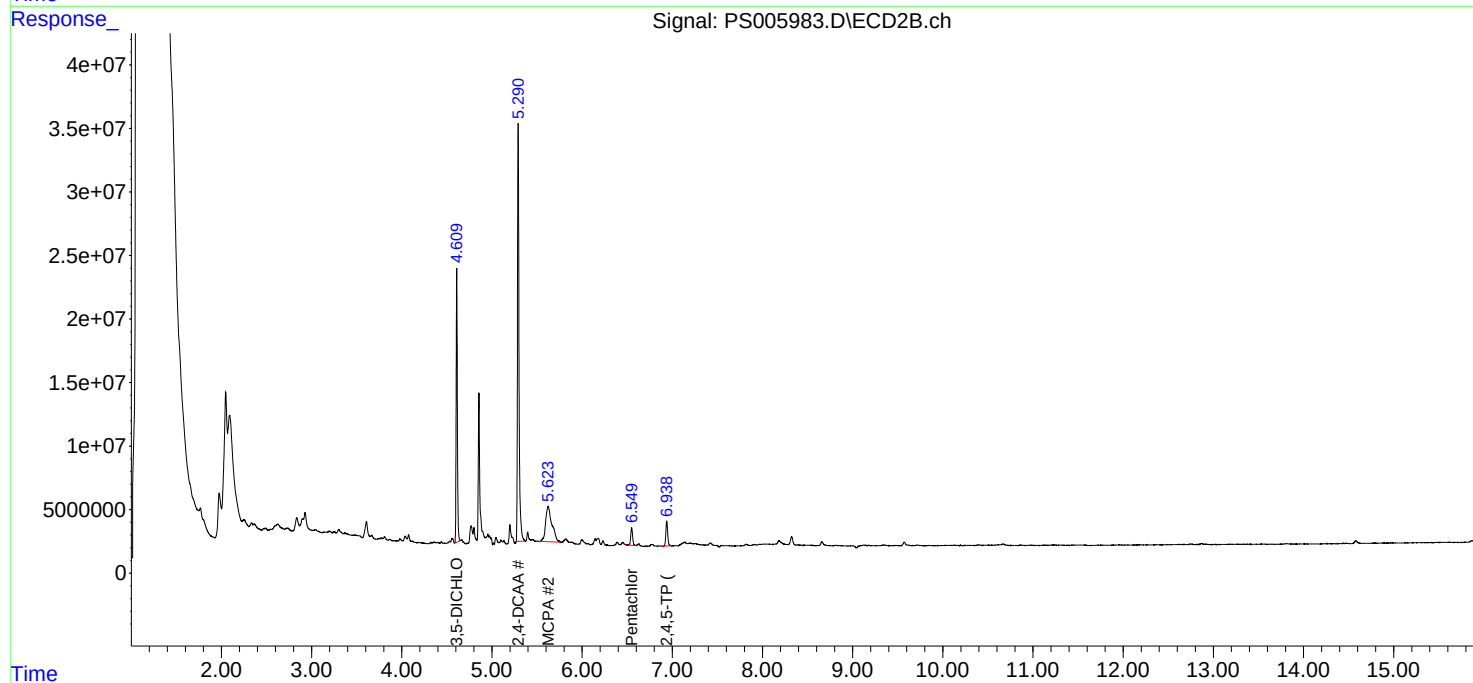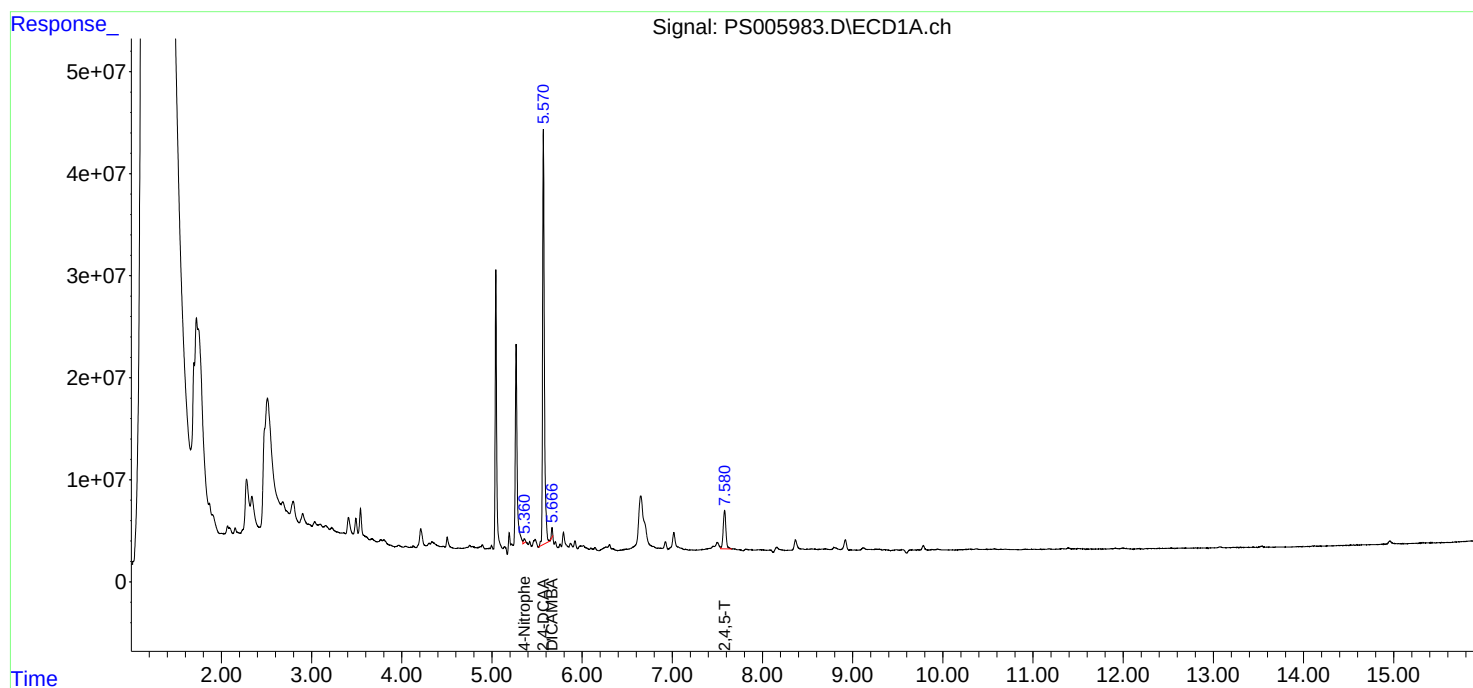


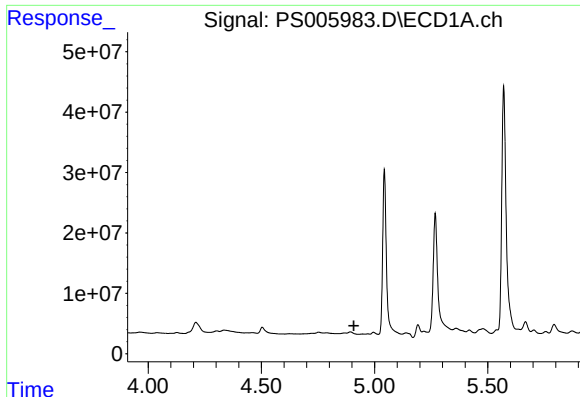

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

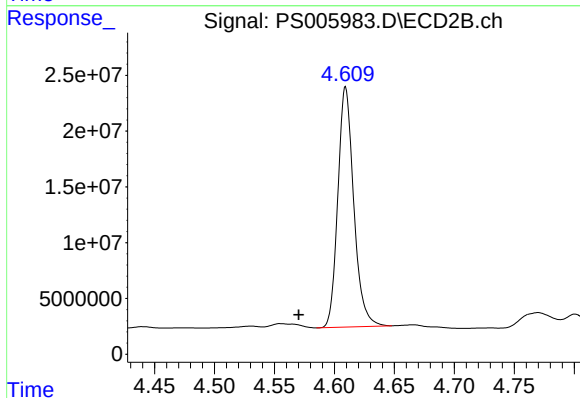


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.610 min
Delta R.T.: 0.039 min
Response: 198852273
Conc: 153.28 ng/ml

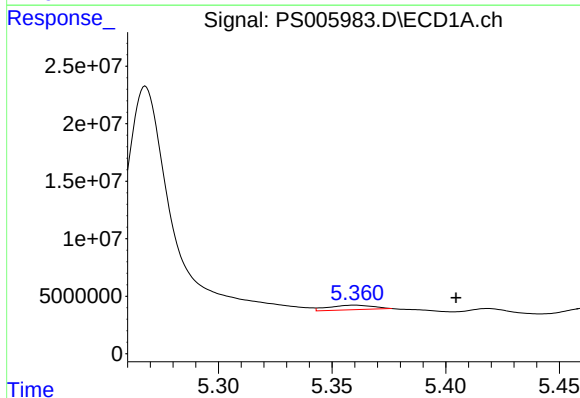


#3 4-Nitrophenol

R.T.: 5.360 min
Delta R.T.: -0.045 min
Response: 5701097
Conc: 9.48 ng/ml

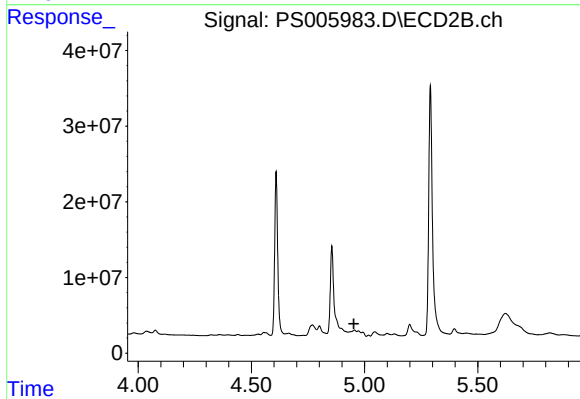

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

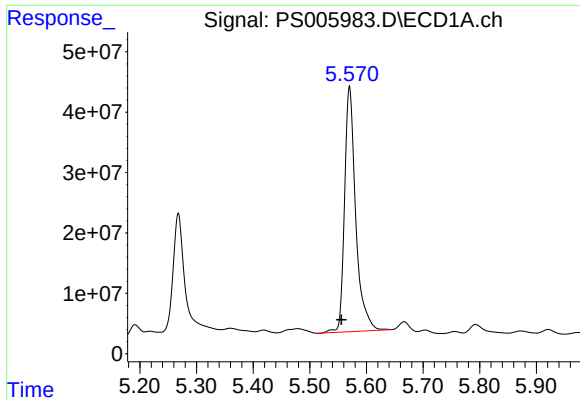

#4 2,4-DCAA


R.T.: 5.570 min
Delta R.T.: 0.014 min
Response: 555657476
Conc: 383.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

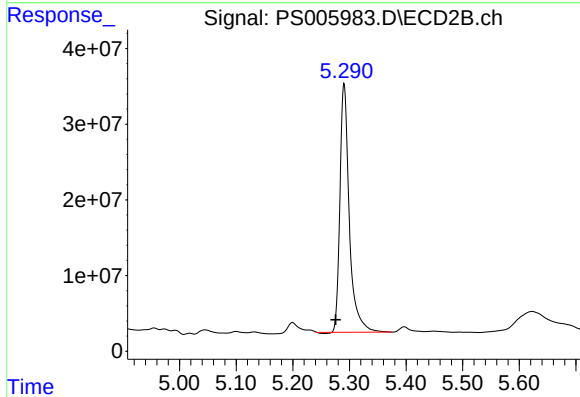


#4 2,4-DCAA

R.T.: 5.291 min
Delta R.T.: 0.015 min
Response: 378496178
Conc: 380.52 ng/ml

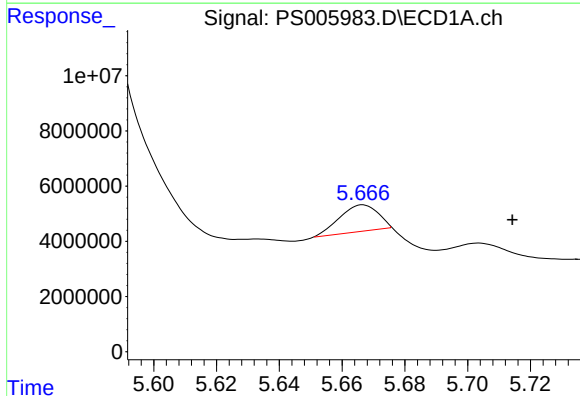


#5 DICAMBA

R.T.: 5.667 min
Delta R.T.: -0.048 min
Response: 8421406
Conc: 1.41 ng/ml

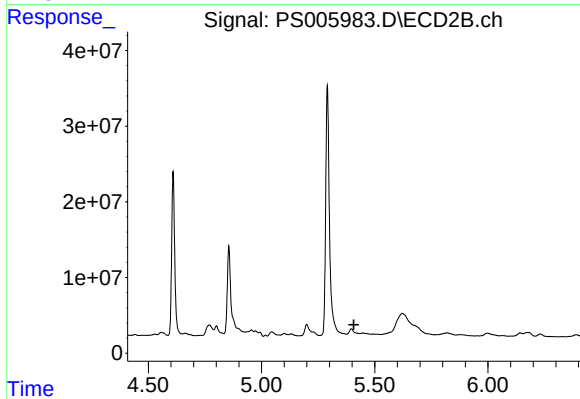

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

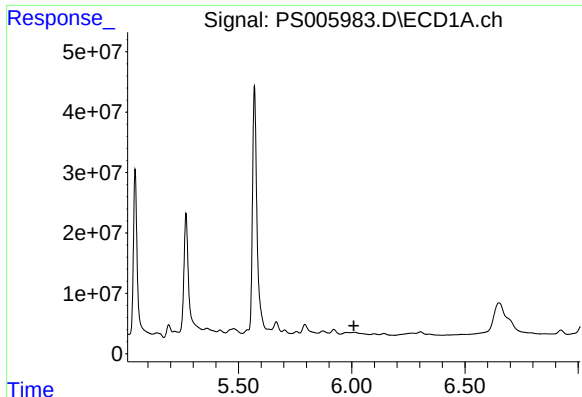

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

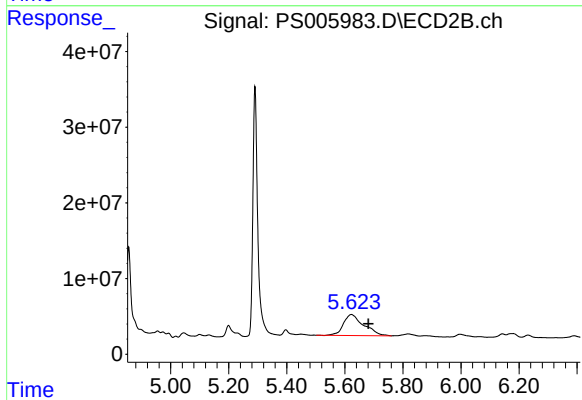


#7 MCPA

R.T.: 5.622 min
Delta R.T.: -0.058 min
Response: 134693303
Conc: 32.00 ug/ml

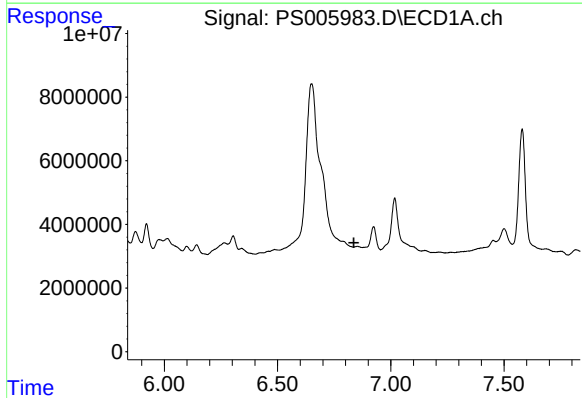


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

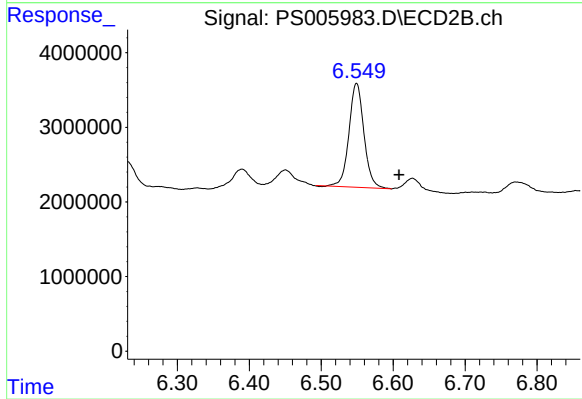

#10 Pentachlorophenol


R.T.: 6.549 min
Delta R.T.: -0.059 min
Response: 20203881
Conc: 1.56 ng/ml

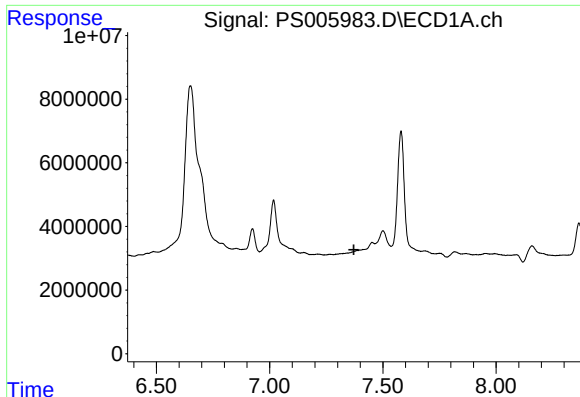

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

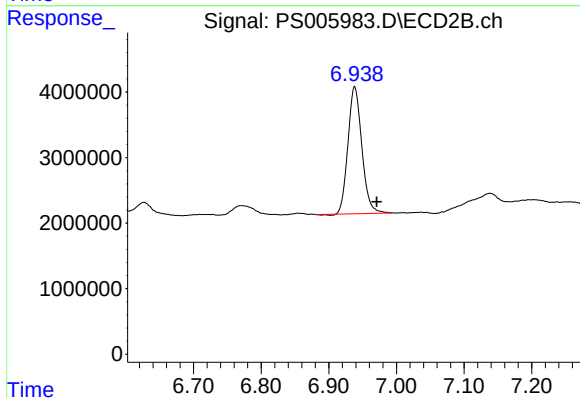


#11 2,4,5-TP (SILVEX)

R.T.: 6.938 min
Delta R.T.: -0.032 min
Response: 2762255
Conc: 5.33 ng/ml

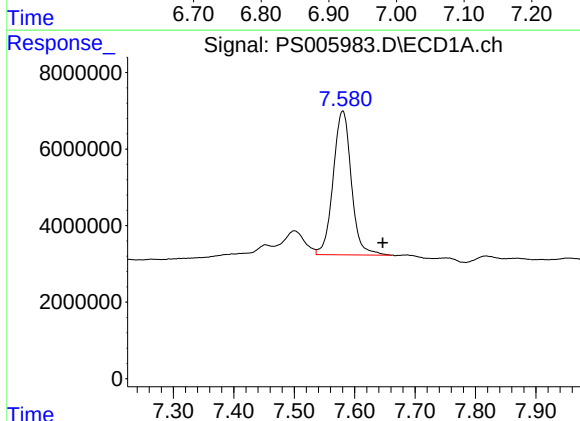

#12 2,4,5-T

R.T.: 7.580 min
Delta R.T.: -0.067 min
Response: 78245630
Conc: 9.37 ng/ml

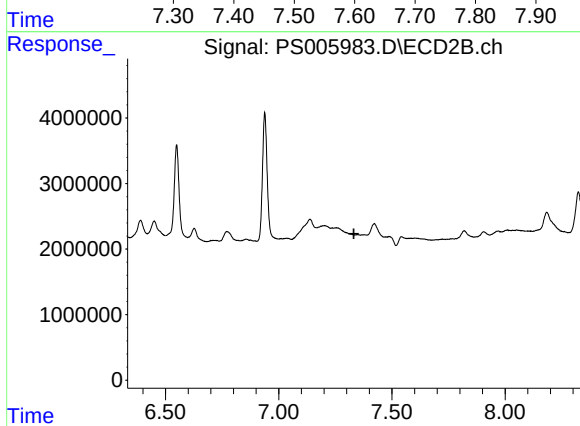

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.