

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080922\
 Data File : PS020228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 09:08
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 13:07:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.119f	0.000	930868	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.988	0.000	201025	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.448f	0.000	31606704	0	8.125	N.D. #
5) T	DICAMBA	7.352	6.985f	39219	6213489	<MDL	1.743 #
6) T	MCP	7.522	6.985	383401	6213489	<MDL	2.278 #
7) T	MCPA	7.678	0.000	329191	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.150	0.000	105095	0	<MDL	N.D. #
12) T	2,4,5-T	9.411	0.000	12422324	0	<MDL	N.D. #
13) T	2,4-DB	10.006	0.000	2566098	0	<MDL	N.D. #
15) T	Picloram	10.945	10.845	94148703	14420914	2.978	1.911 #
16) T	DCPA	11.406	0.000	2578035	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080922\
Data File : PS020228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 09:08
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 13:07:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

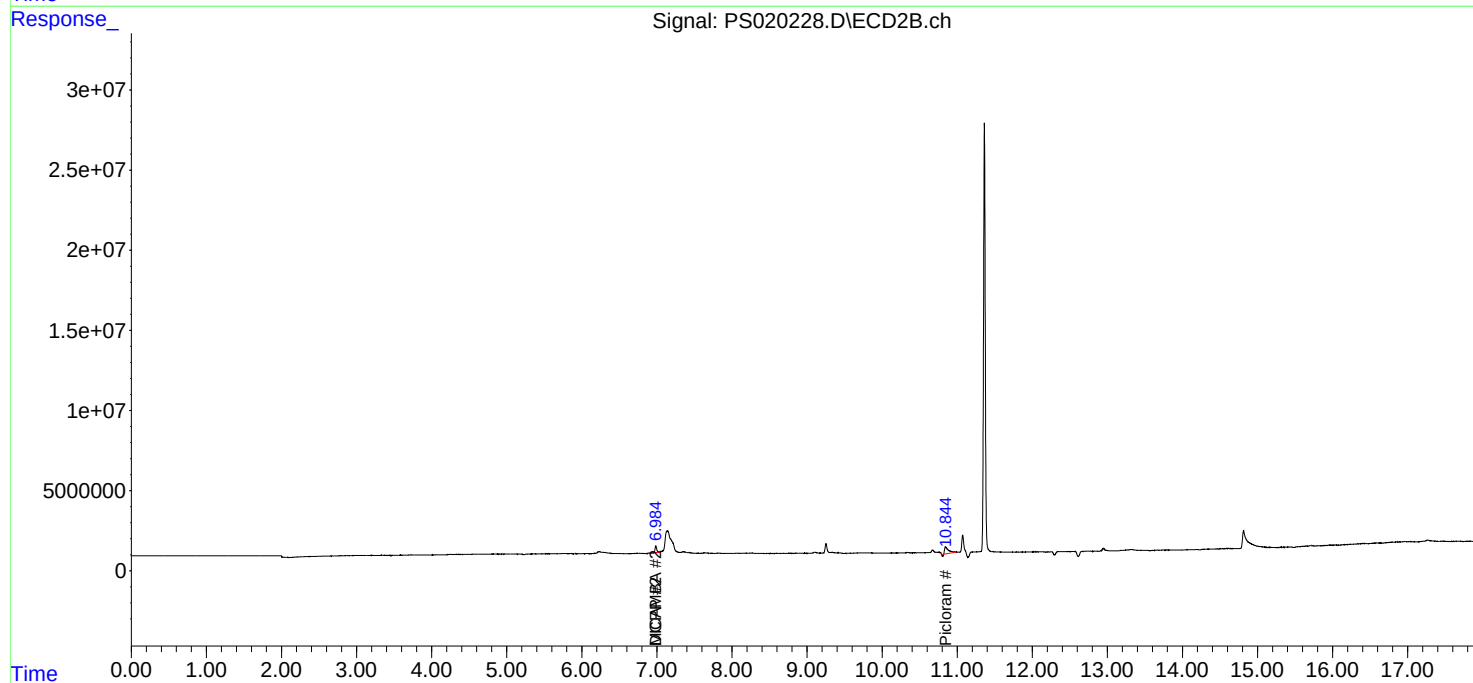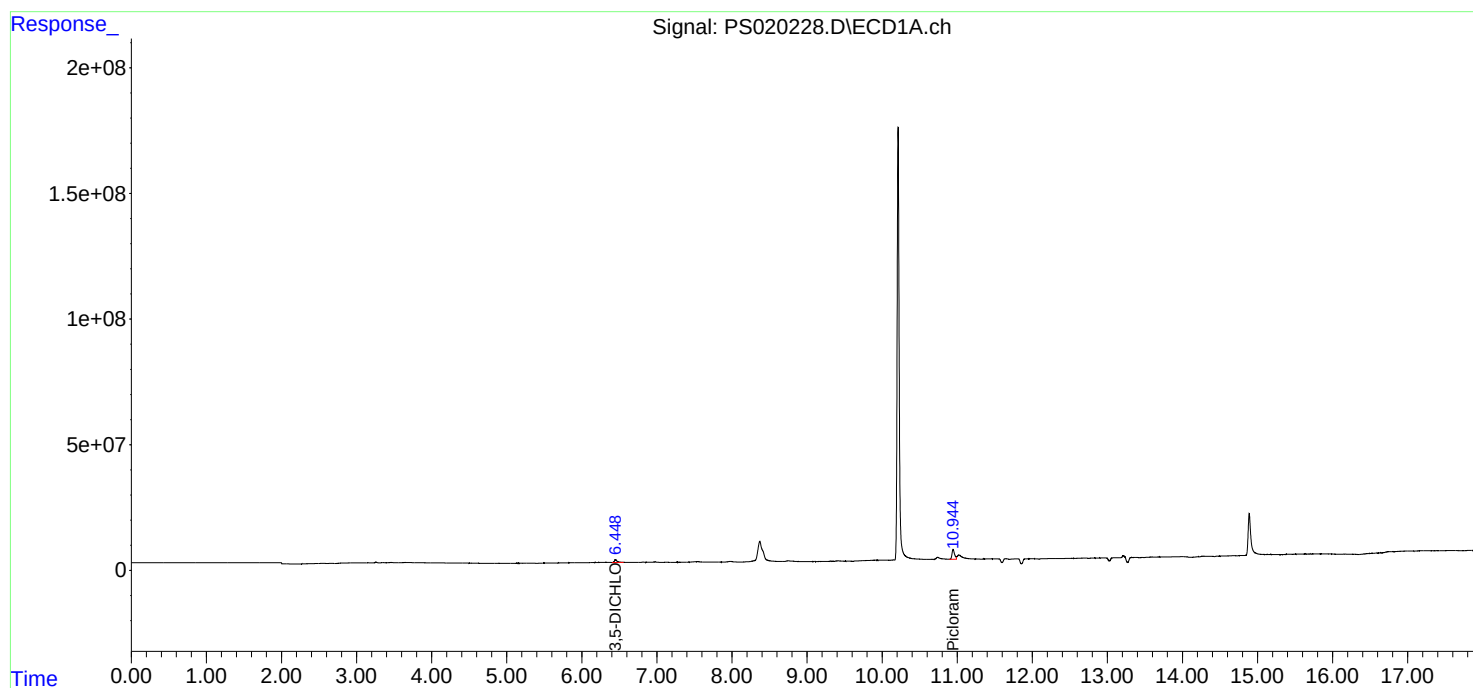


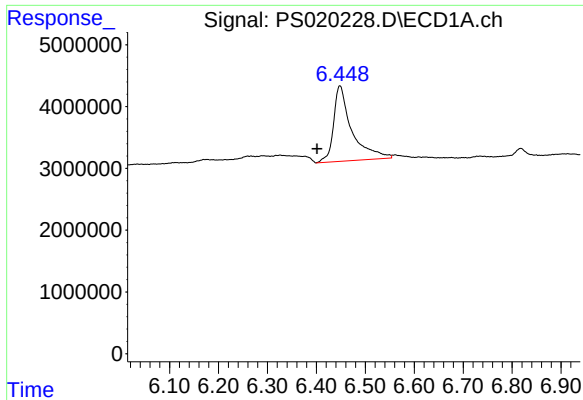

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.448 min
Delta R.T.: 0.047 min
Response: 31606704
Conc: 8.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

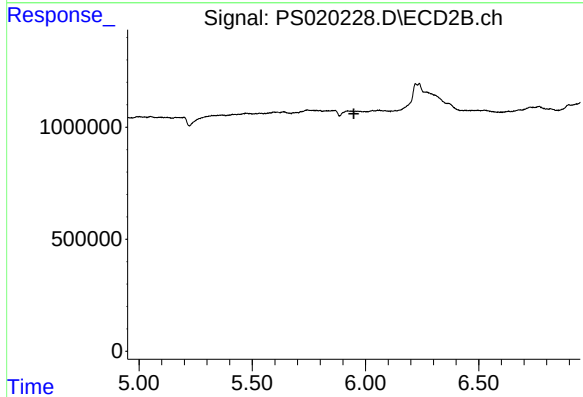


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

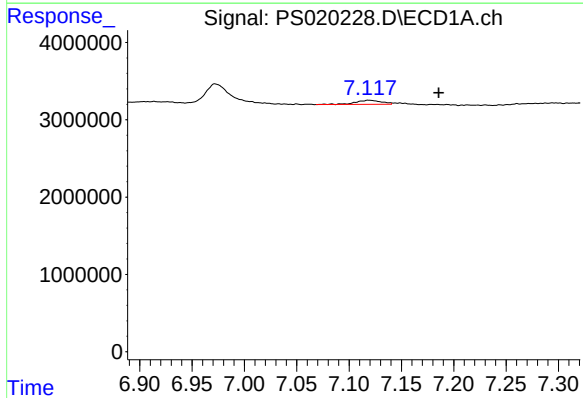


#4 2,4-DCAA

R.T.: 7.119 min
Delta R.T.: -0.067 min
Response: 930868
Conc: N.D.

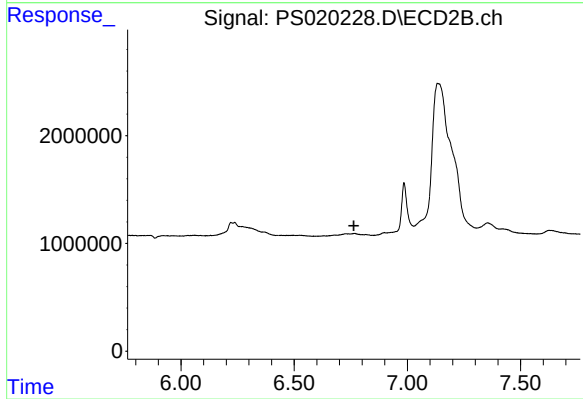

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

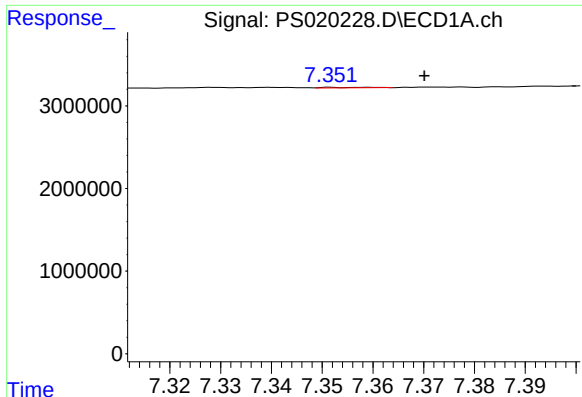

#5 DICAMBA


R.T.: 7.352 min
Delta R.T.: -0.018 min
Response: 39219
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

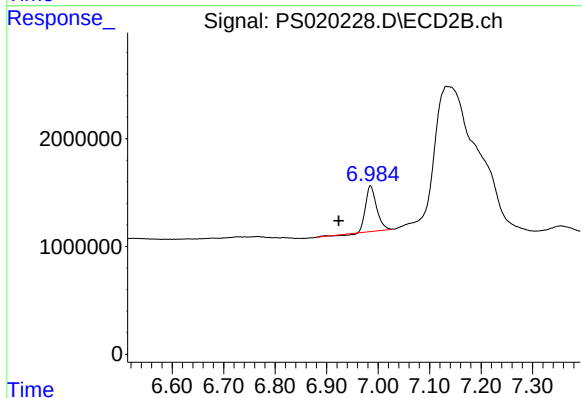


#5 DICAMBA

R.T.: 6.985 min
Delta R.T.: 0.062 min
Response: 6213489
Conc: 1.74 ng/ml

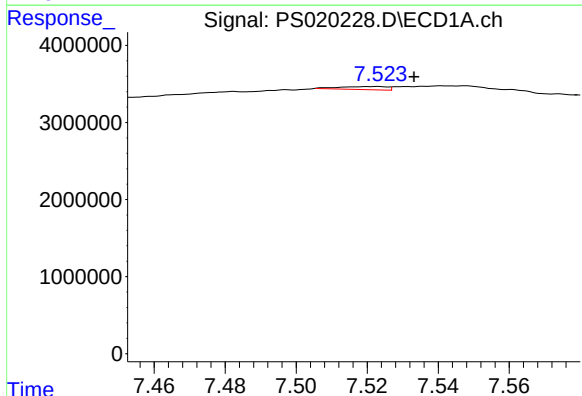


#6 MCP

R.T.: 7.522 min
Delta R.T.: -0.011 min
Response: 383401
Conc: N.D.

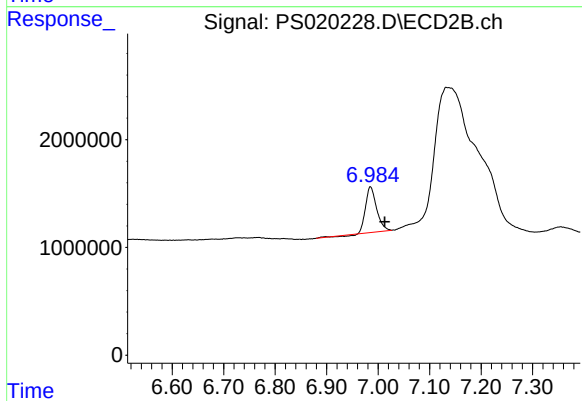

#6 MCP


R.T.: 6.985 min
Delta R.T.: -0.028 min
Response: 6213489
Conc: 2.28 ug/ml

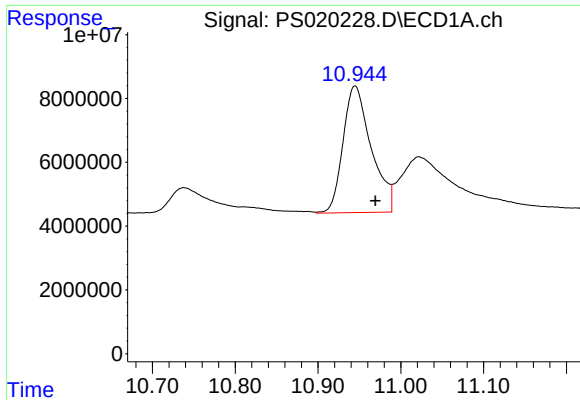

#15 Picloram

R.T.: 10.945 min
Delta R.T.: -0.024 min
Response: 94148703
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

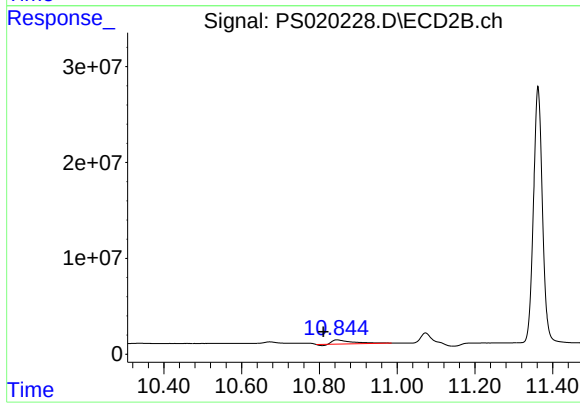

#15 Picloram

R.T.: 10.845 min
Delta R.T.: 0.035 min
Response: 14420914
Conc: 1.91 ng/ml