

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080922\
 Data File : PS020229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 09:32
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 13:08:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.183	6.760	1394.1E6	437.2E6	472.790	536.439
Target Compounds							
1) T	Dalapon	3.046f	0.000	1062520	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.451f	0.000	1486386	0	<MDL	N.D. #
3) T	4-Nitroph...	6.992f	0.000	841189	0	<MDL	N.D. #
6) T	MCP	7.479f	0.000	1382490	0	<MDL	N.D. #
7) T	MCPA	7.649	0.000	451924	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.165	0.000	488502	0	<MDL	N.D. #
12) T	2,4,5-T	9.415	0.000	10075022	0	<MDL	N.D. #
13) T	2,4-DB	10.013	0.000	510555	0	<MDL	N.D. #
14) T	DINOSEB	11.202f	0.000	1577401	0	<MDL	N.D. #
15) T	Picloram	10.964	10.856f	8737610	7749658	<MDL	1.027 #
16) T	DCPA	11.410	0.000	1541373	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080922\
Data File : PS020229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 09:32
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 13:08:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

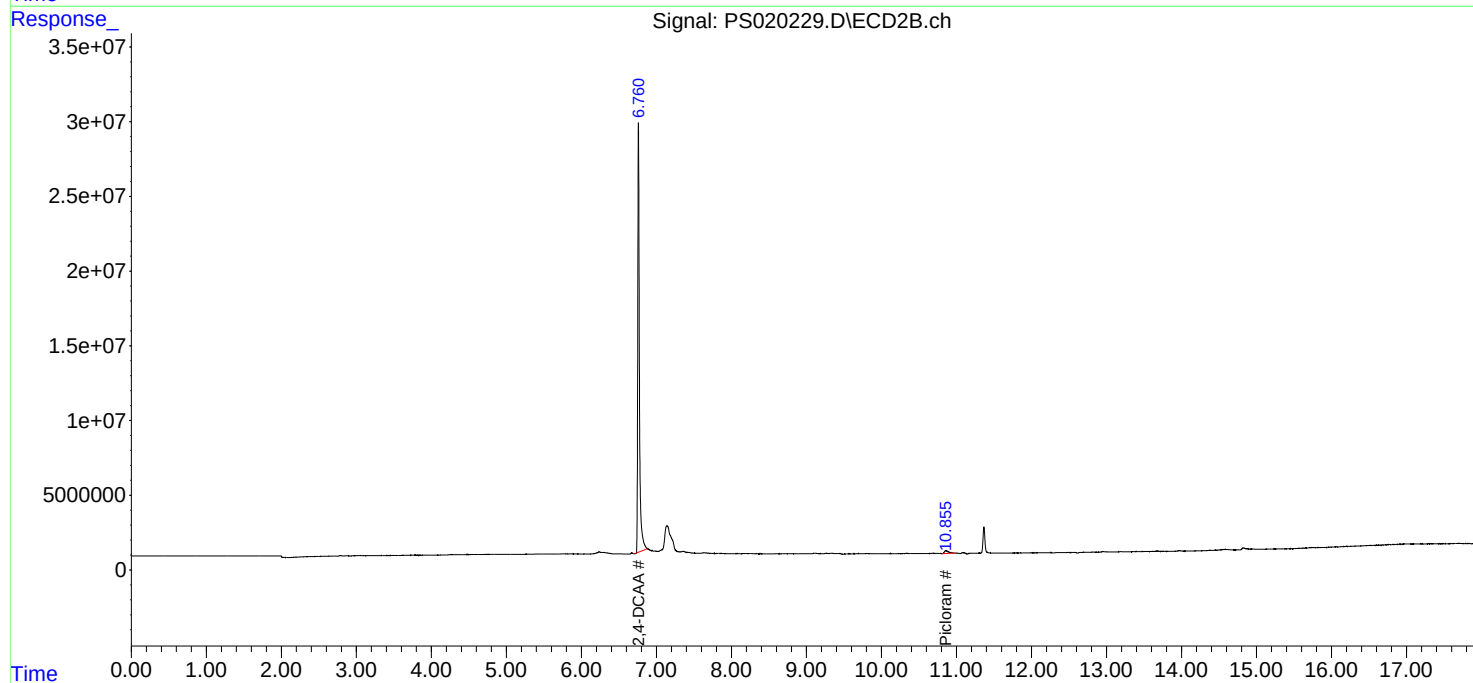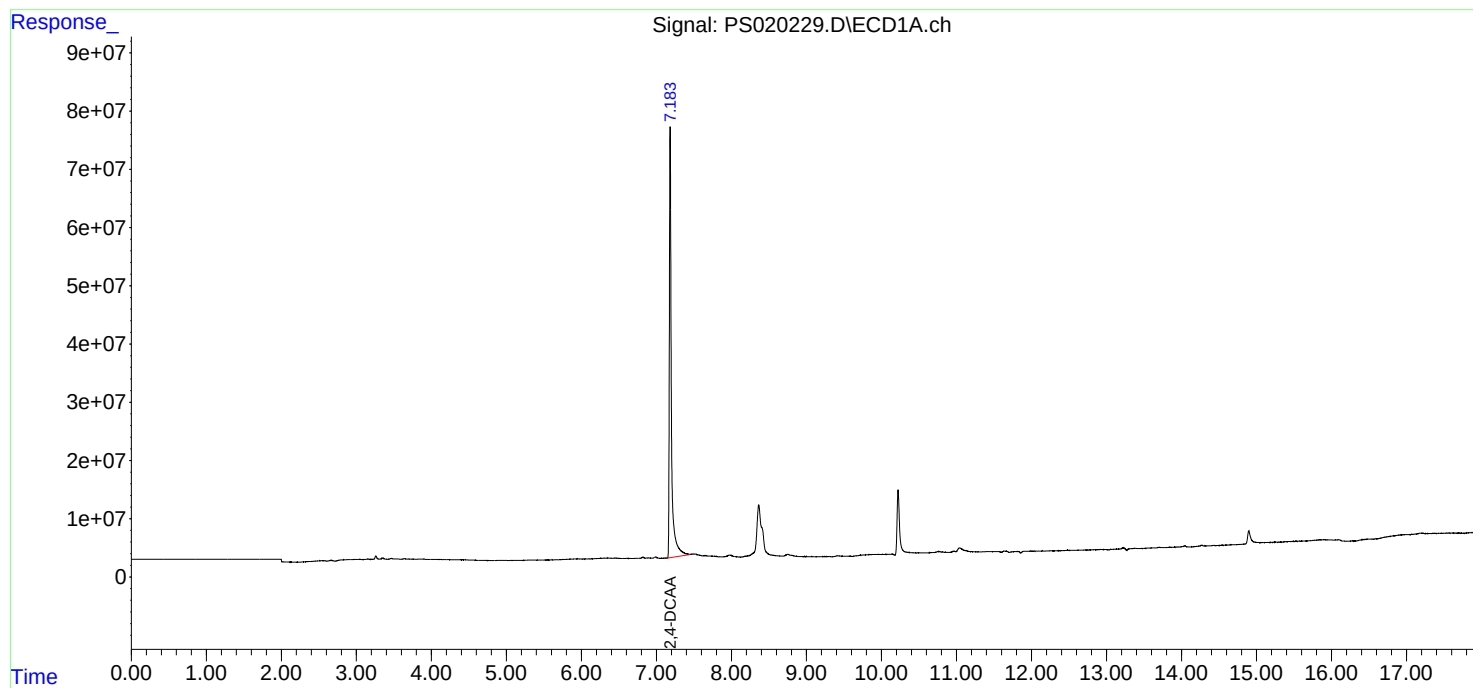


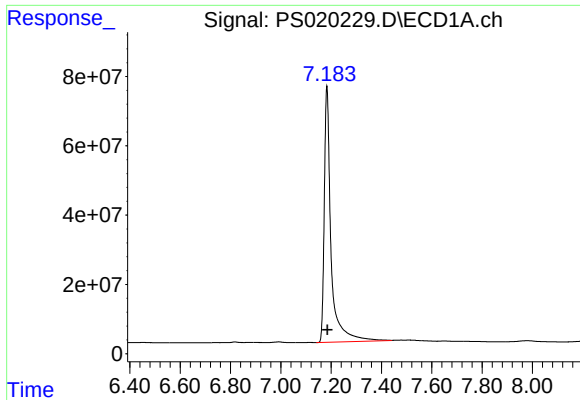

#4 2,4-DCAA


R.T.: 7.183 min
Delta R.T.: -0.002 min
Response: 1394126187
Conc: 472.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

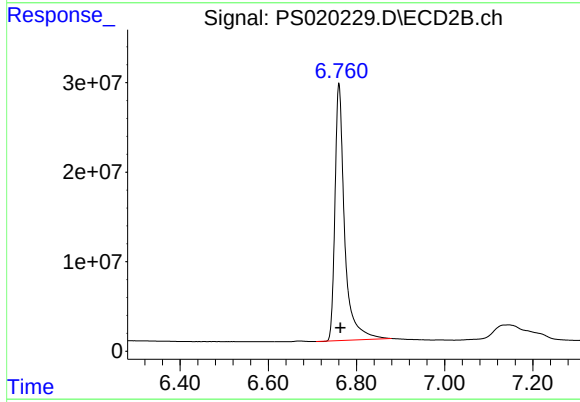


#4 2,4-DCAA

R.T.: 6.760 min
Delta R.T.: -0.003 min
Response: 437174225
Conc: 536.44 ng/ml

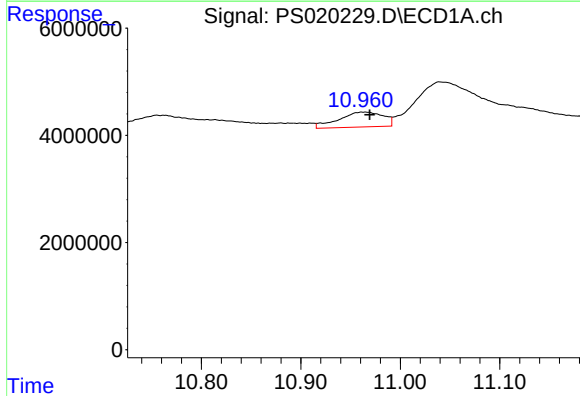

#15 Picloram

R.T.: 10.964 min
Delta R.T.: -0.005 min
Response: 8737610
Conc: N.D.

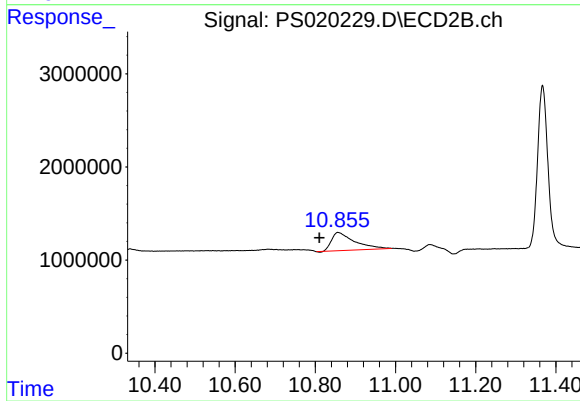

#15 Picloram

R.T.: 10.856 min
Delta R.T.: 0.046 min
Response: 7749658
Conc: 1.03 ng/ml