

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080922\
 Data File : PS020235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 12:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 15:52:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.757	1371.2E6	439.9E6	465.023	539.801
Target Compounds							
1) T	Dalapon	3.044f	0.000	992680	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.435	0.000	325236	0	<MDL	N.D. #
7) T	MCPA	7.633f	0.000	7471006	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.576	0	2567228	N.D.	2.745
9) T	2,4-D	8.365f	0.000	55950207	0	18.578	N.D. #
11) T	2,4,5-TP ...	9.192f	0.000	7936375	0	<MDL	N.D. #
12) T	2,4,5-T	9.438	9.058f	6030652	1446816	<MDL	<MDL #
13) T	2,4-DB	9.960	0.000	2723091	0	<MDL	N.D. #
15) T	Picloram	10.978	10.825	13895873	5389849	<MDL	<MDL #
16) T	DCPA	11.398	0.000	6294467	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080922\
Data File : PS020235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 12:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 15:52:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

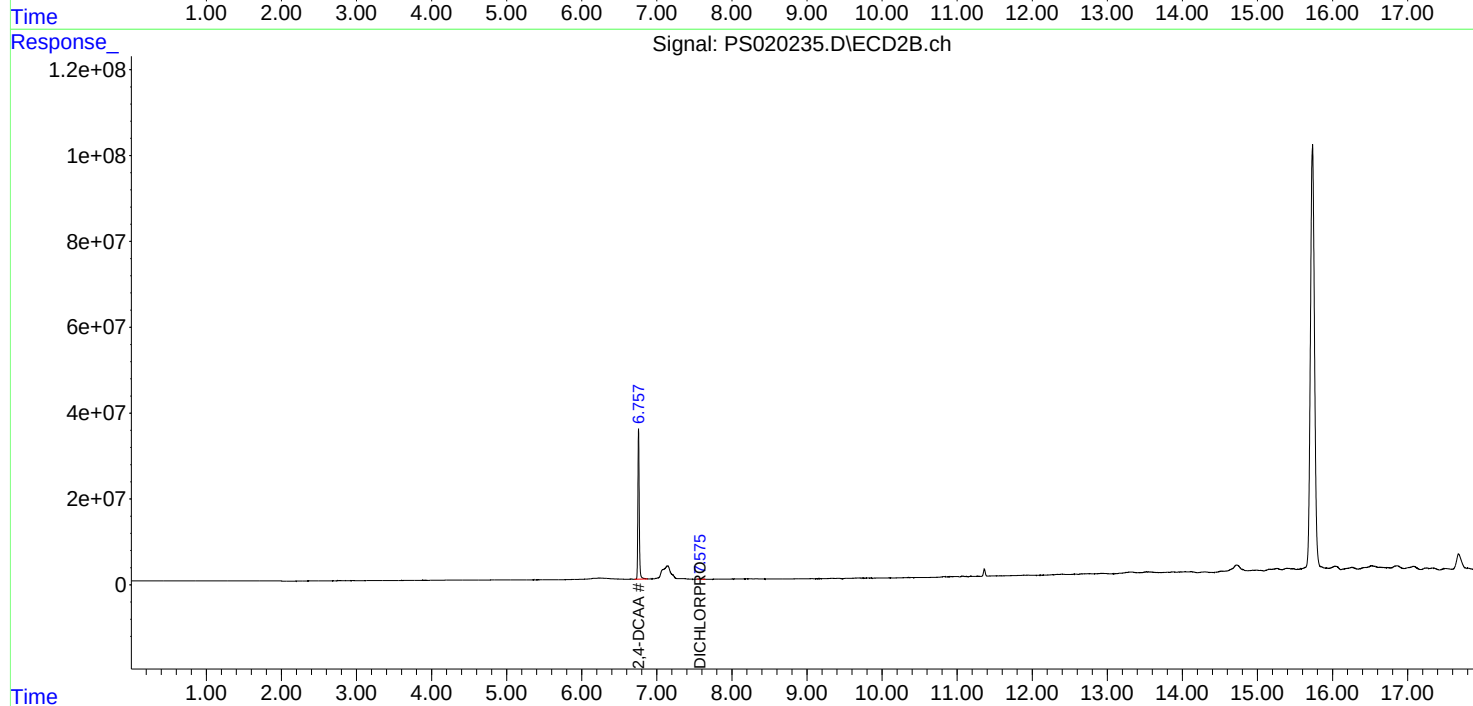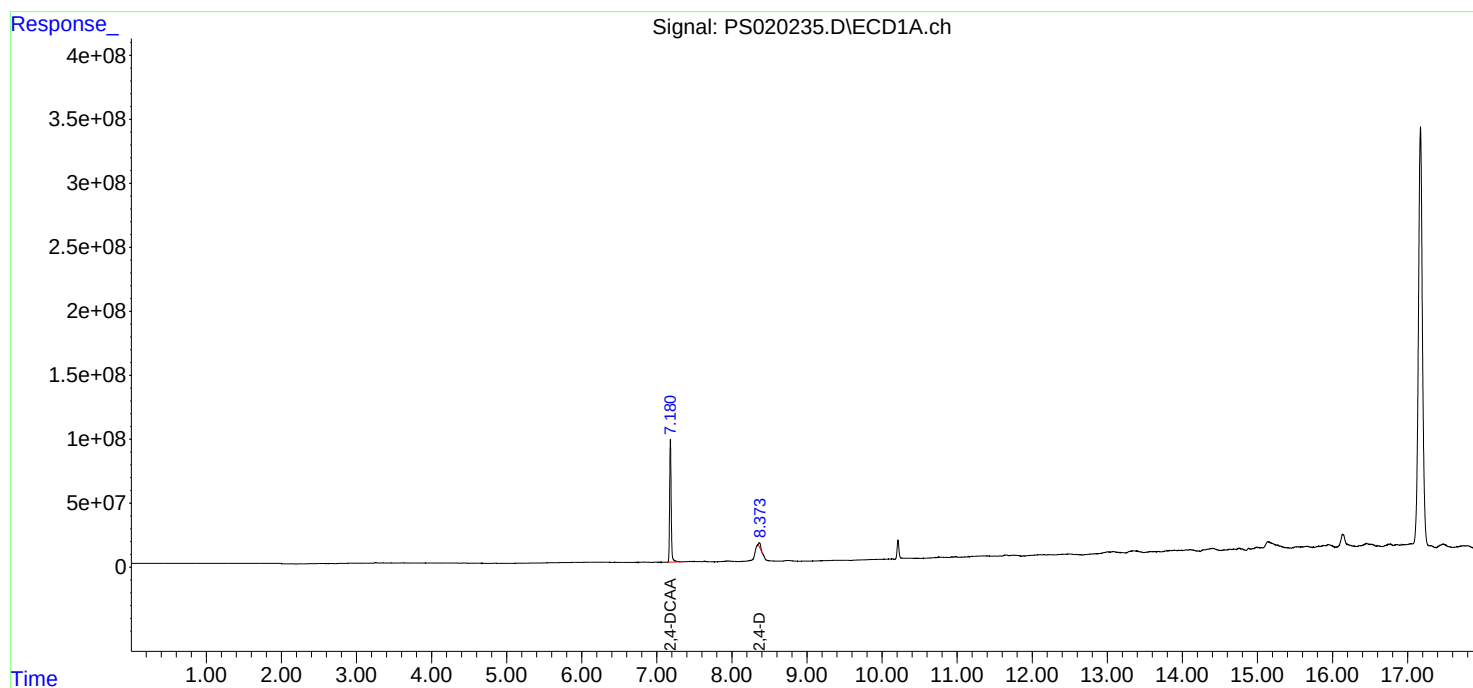


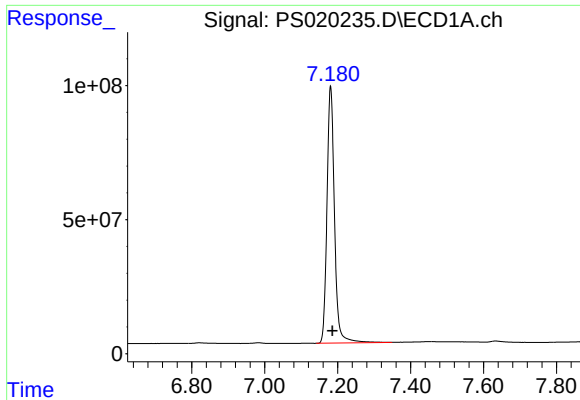

#4 2,4-DCAA


R.T.: 7.181 min
Delta R.T.: -0.005 min
Response: 1371223427
Conc: 465.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

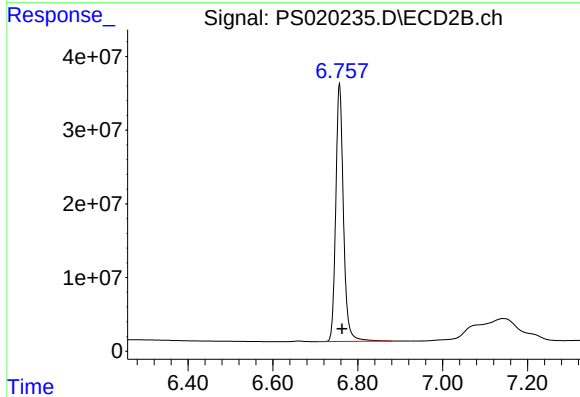


#4 2,4-DCAA

R.T.: 6.757 min
Delta R.T.: -0.007 min
Response: 439914071
Conc: 539.80 ng/ml

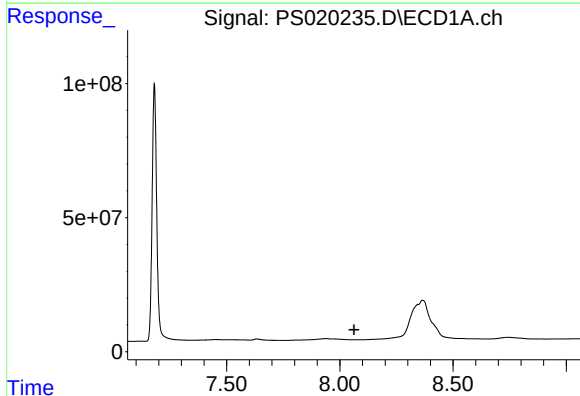


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.062 min
Response: 0
Conc: N.D.

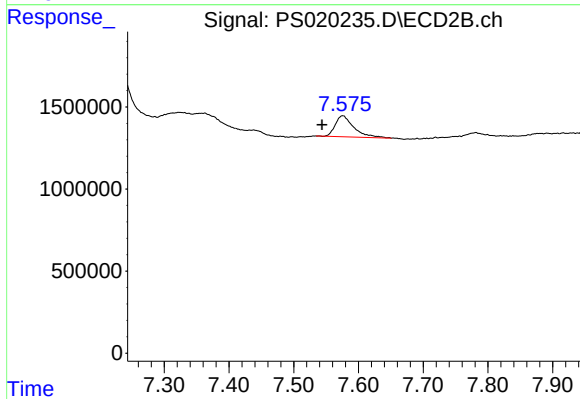

#8 DICHLORPROP


R.T.: 7.576 min
Delta R.T.: 0.032 min
Response: 2567228
Conc: 2.75 ng/ml

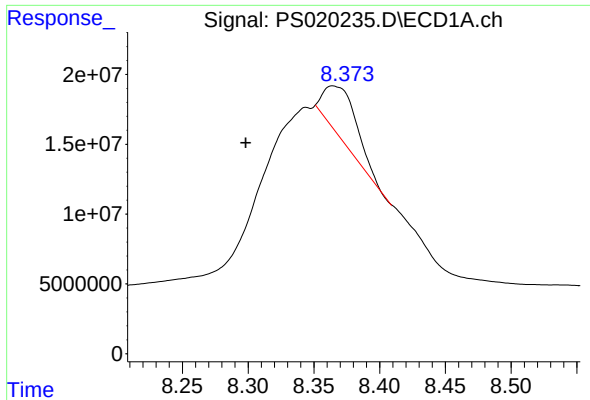

#9 2,4-D

R.T.: 8.365 min
Delta R.T.: 0.067 min
Response: 55950207
Conc: 18.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

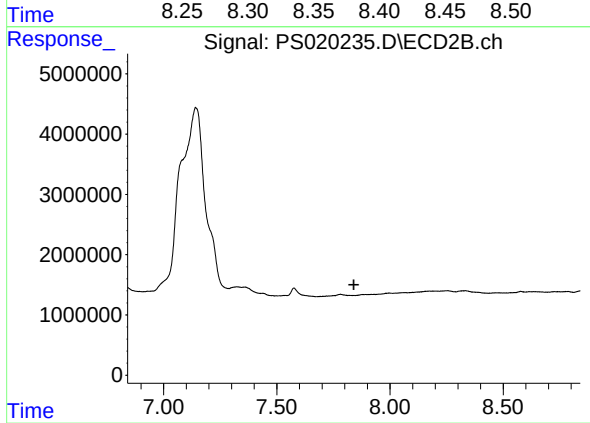

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.840 min
Response: 0
Conc: N.D.