

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080922\
 Data File : PS020247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 20:30
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:37:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.179	6.757	1448.4E6	459.3E6	491.204	563.576
Target Compounds							
1) T	Dalapon	3.044	0.000	709491	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.436	0.000	364769	0	<MDL	N.D. #
7) T	MCPA	7.634f	0.000	6325710	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.584	0	1753162	N.D.	1.875
10) T	Pentachlo...	8.598	0.000	711820	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.117	0.000	11716212	0	<MDL	N.D. #
12) T	2,4,5-T	9.444	9.068f	11865890	2241790	<MDL	<MDL #
13) T	2,4-DB	9.956	9.520	7934108	895853	2.174	1.317 #
14) T	DINOSEB	11.106	0.000	9004305	0	<MDL	N.D. #
15) T	Picloram	10.996	10.834	19761846	4670209	<MDL	<MDL #
16) T	DCPA	11.408	10.752	5044518	2217324	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080922\
Data File : PS020247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 20:30
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:37:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

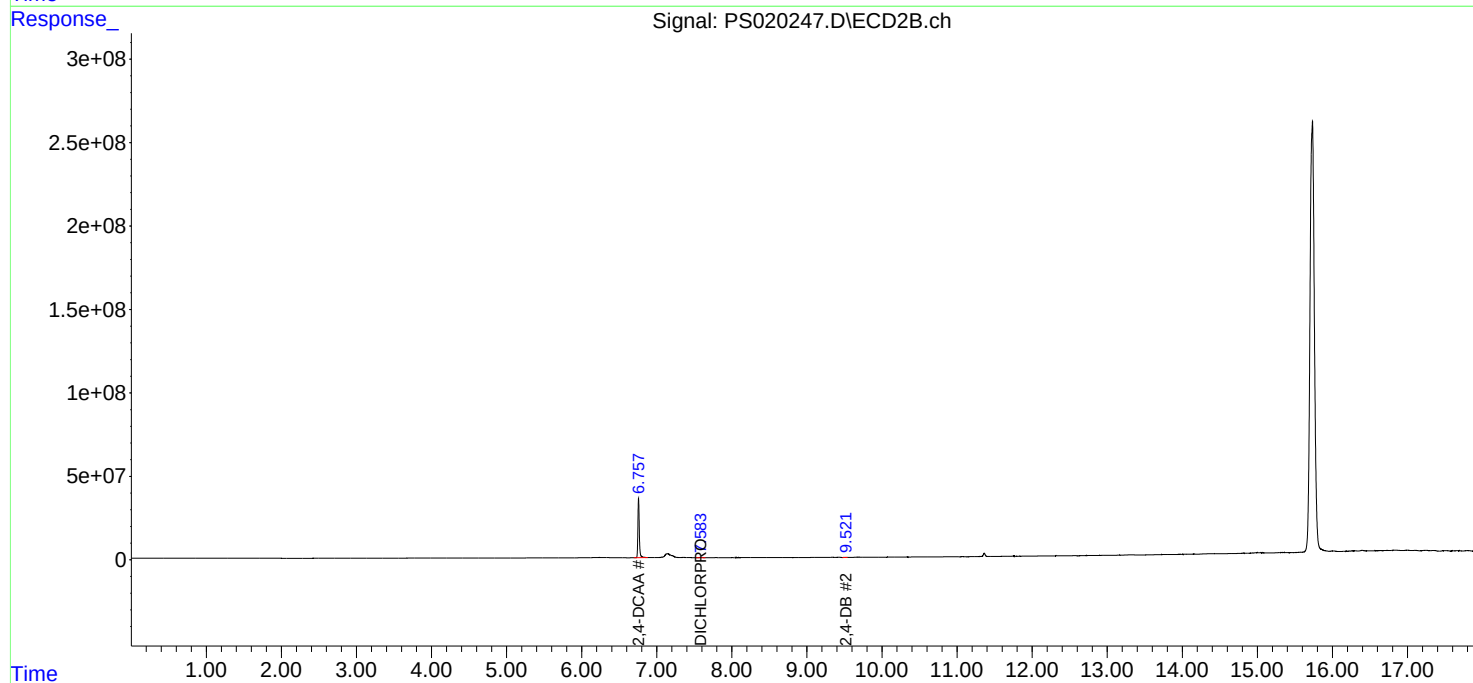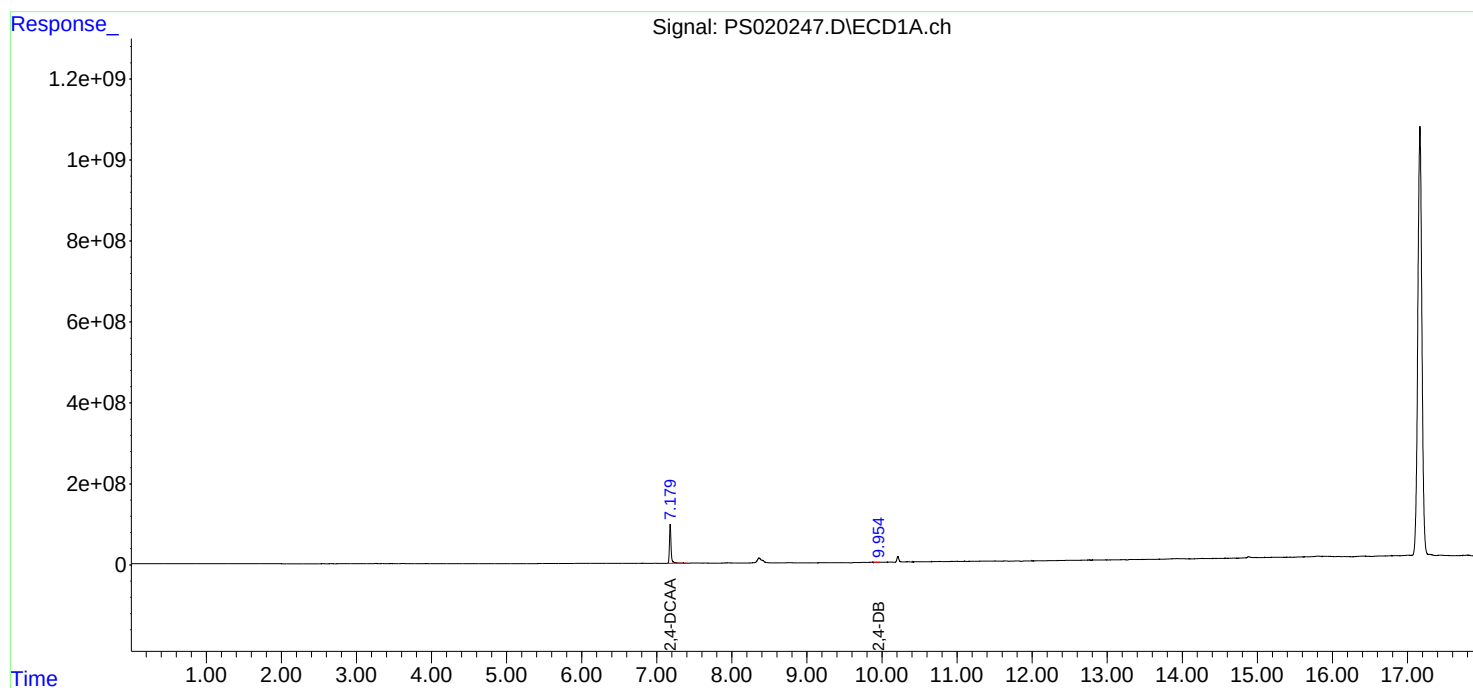


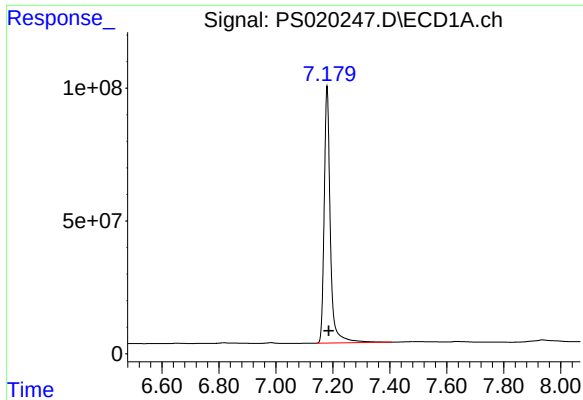

#4 2,4-DCAA


R.T.: 7.179 min
Delta R.T.: -0.006 min
Response: 1448424870
Conc: 491.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

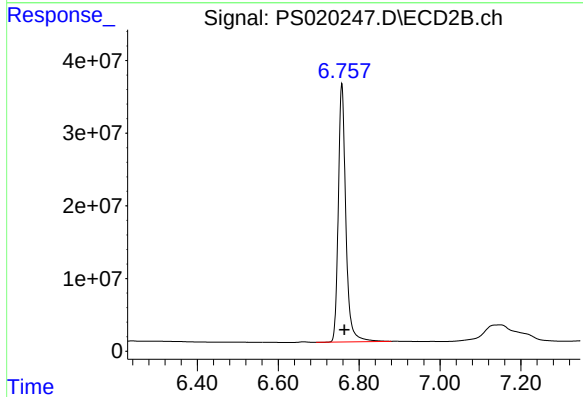


#4 2,4-DCAA

R.T.: 6.757 min
Delta R.T.: -0.006 min
Response: 459289612
Conc: 563.58 ng/ml

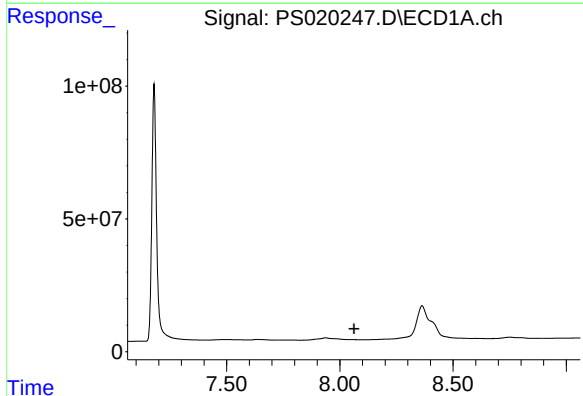


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.062 min
Response: 0
Conc: N.D.

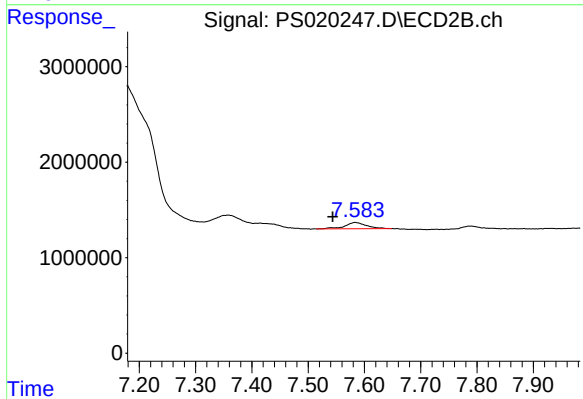

#8 DICHLORPROP


R.T.: 7.584 min
Delta R.T.: 0.040 min
Response: 1753162
Conc: 1.87 ng/ml

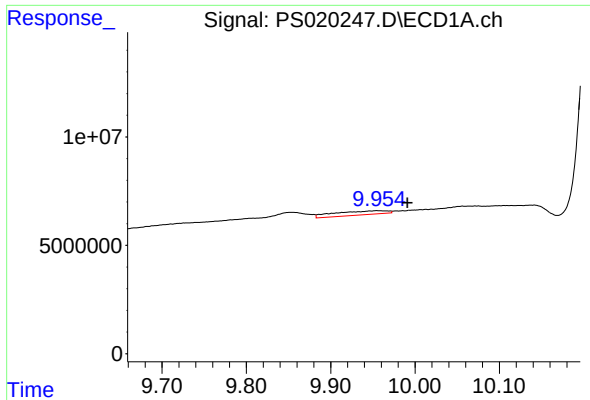

#13 2,4-DB

R.T.: 9.956 min
Delta R.T.: -0.035 min
Response: 7934108
Conc: 2.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

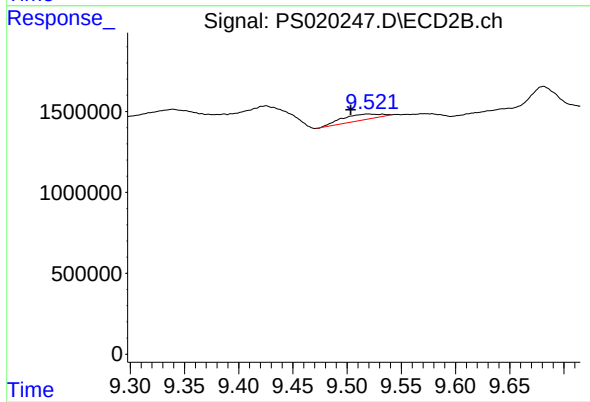

#13 2,4-DB

R.T.: 9.520 min
Delta R.T.: 0.016 min
Response: 895853
Conc: 1.32 ng/ml