

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081018\
 Data File : PS001434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2018 20:46
 Operator : UA
 Sample : J4393-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 06:36:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.613	11.033	42899929	46406215	231.204	255.155
Target Compounds							
1) T	Dalapon	2.962	2.400	5068007	4711964	21.373	20.678
2) T	3,5-DICHL...	0.000	9.121	0	1199527	N.D.	4.709 #
3) T	4-Nitroph...	0.000	10.252	0	21295046	N.D.	208.900 #
5) T	DICAMBA	0.000	11.277	0	6571441	N.D.	9.588 #
6) T	MCPD	12.305	11.519	9990063	2668524	19.876	6.150 #
7) T	MCPA	12.581	0.000	17633360	0	22.359	N.D. #
9) T	2,4-D	0.000	12.877	0	3865824	N.D.	16.291 #
14) T	DINOSEB	0.000	15.728	0	17490615	N.D.	24.607 #
15) T	Picloram	0.000	16.916	0	18187743	N.D.	13.194 #
16) T	DCPA	0.000	16.972	0	12857709	N.D.	8.902 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081018\
Data File : PS001434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2018 20:46
Operator : UA
Sample : J4393-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 06:36:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

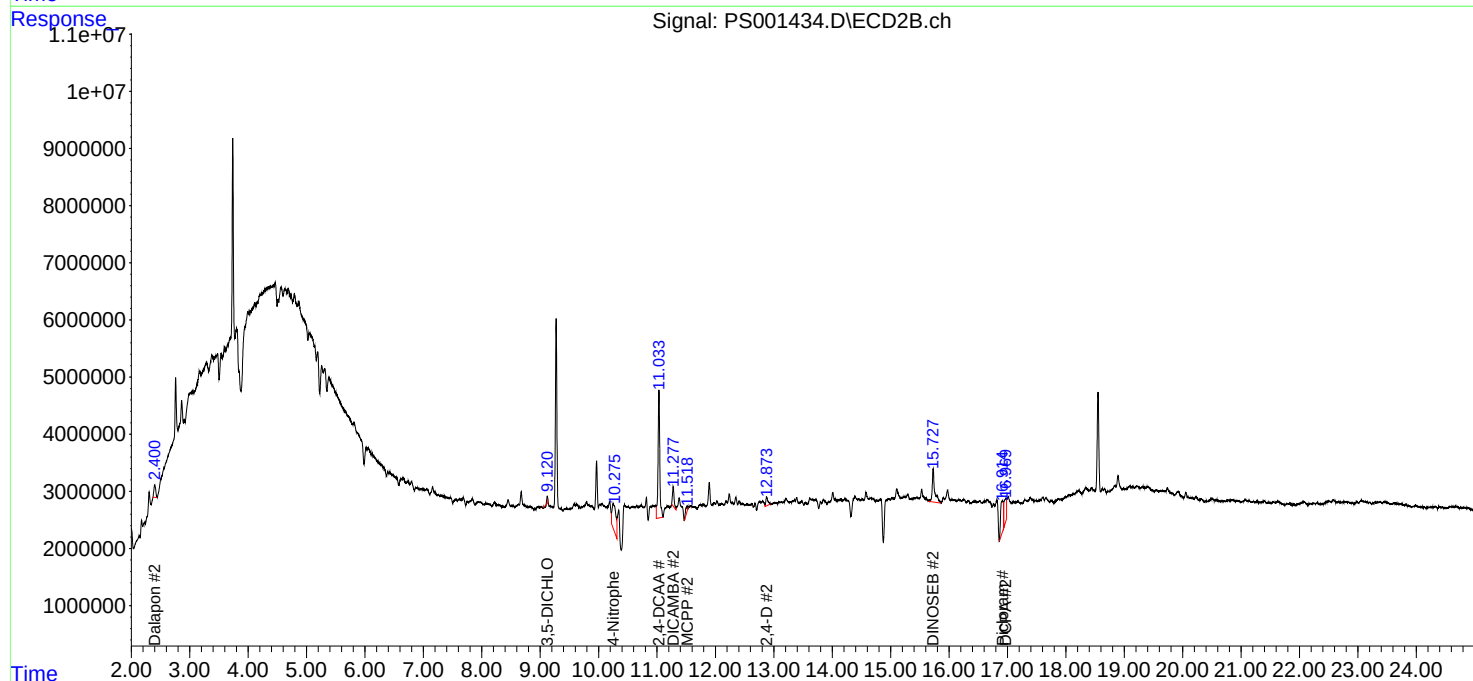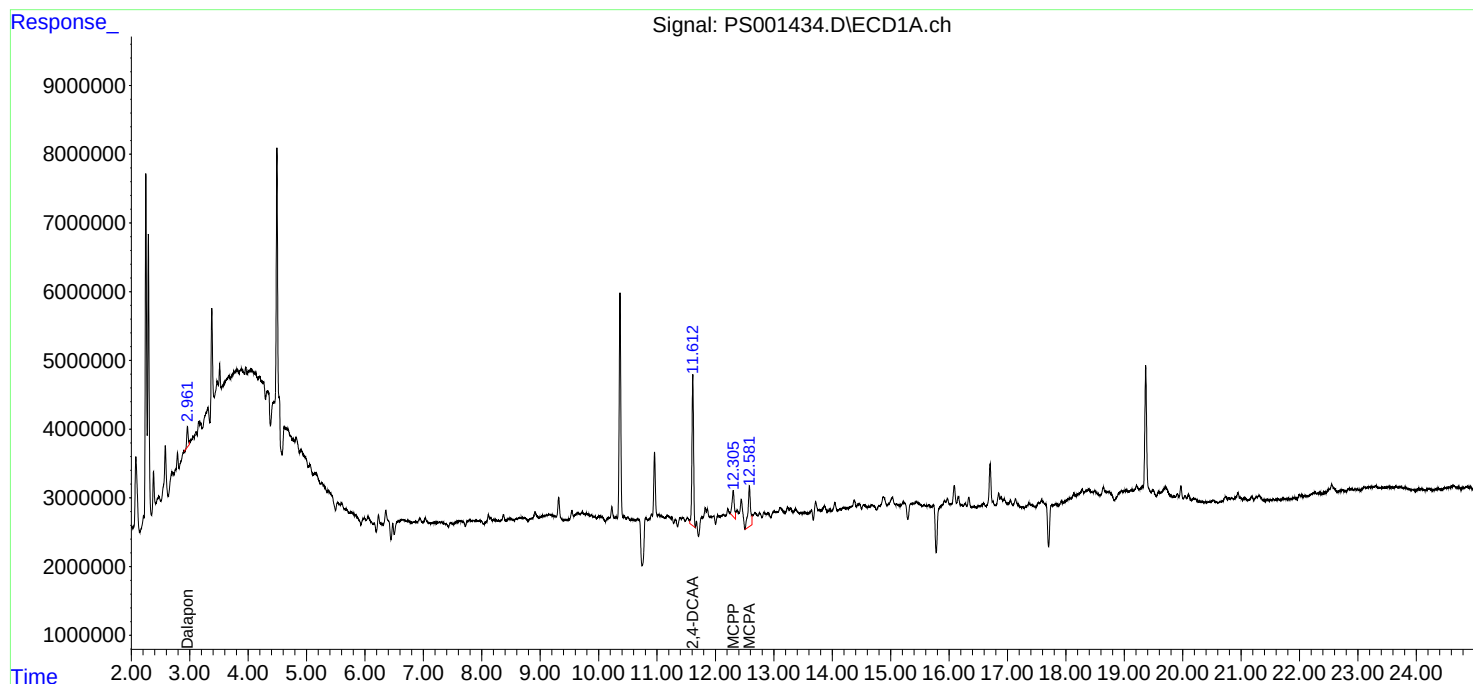


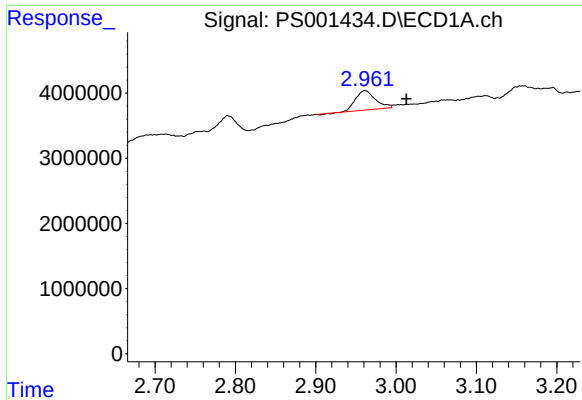

#1 Dalapon


R.T.: 2.962 min
Delta R.T.: -0.051 min
Response: 5068007
Conc: 21.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

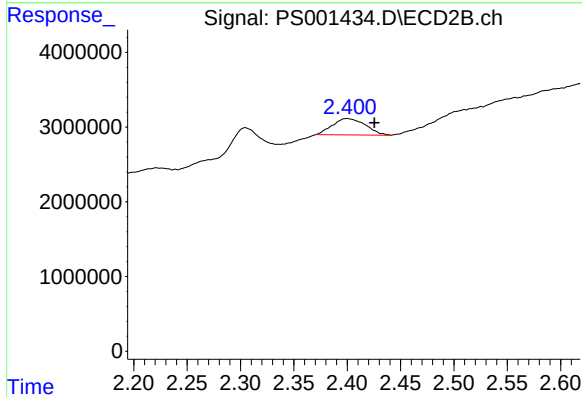


#1 Dalapon

R.T.: 2.400 min
Delta R.T.: -0.026 min
Response: 4711964
Conc: 20.68 ng/ml

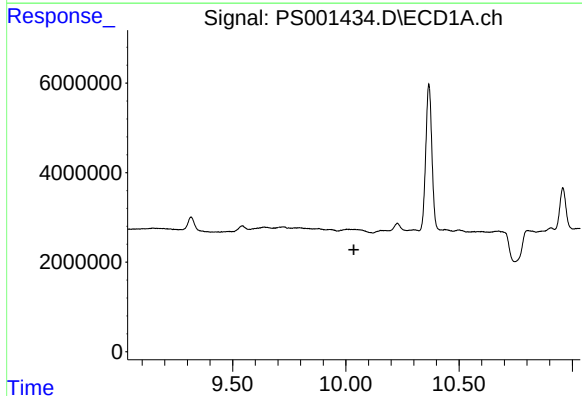


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

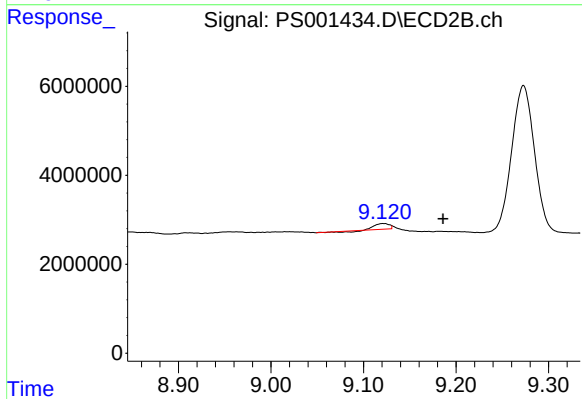

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.121 min
Delta R.T.: -0.065 min
Response: 1199527
Conc: 4.71 ng/ml

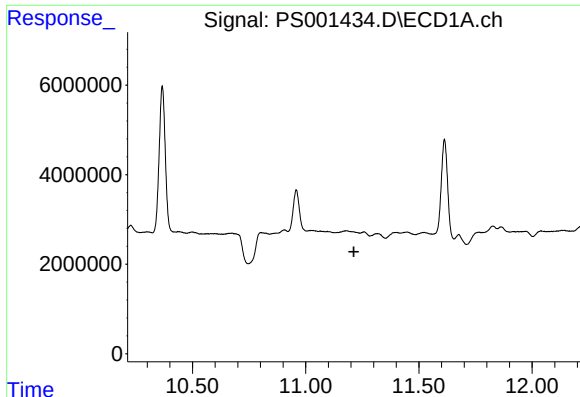

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

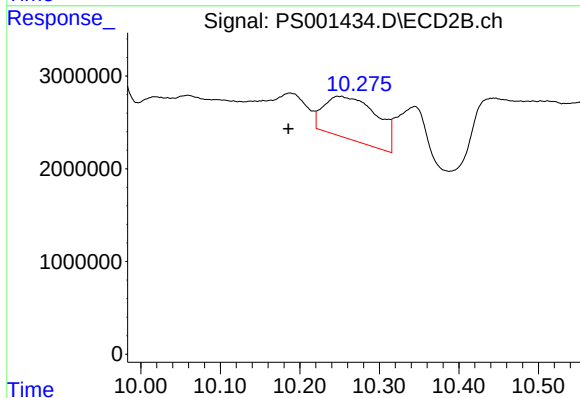


#3 4-Nitrophenol

R.T.: 10.252 min
Delta R.T.: 0.067 min
Response: 21295046
Conc: 208.90 ng/ml

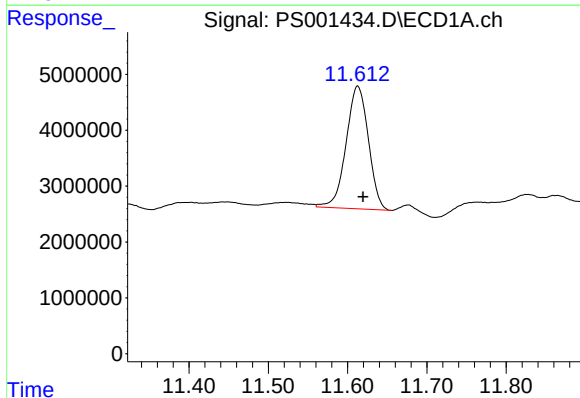


#4 2,4-DCAA

R.T.: 11.613 min
Delta R.T.: -0.007 min
Response: 42899929
Conc: 231.20 ng/ml

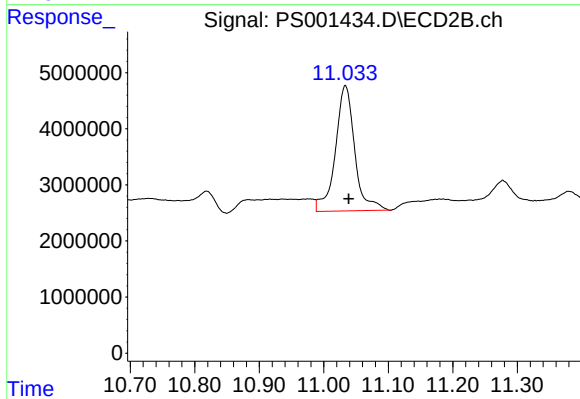

#4 2,4-DCAA


R.T.: 11.033 min
Delta R.T.: -0.005 min
Response: 46406215
Conc: 255.15 ng/ml

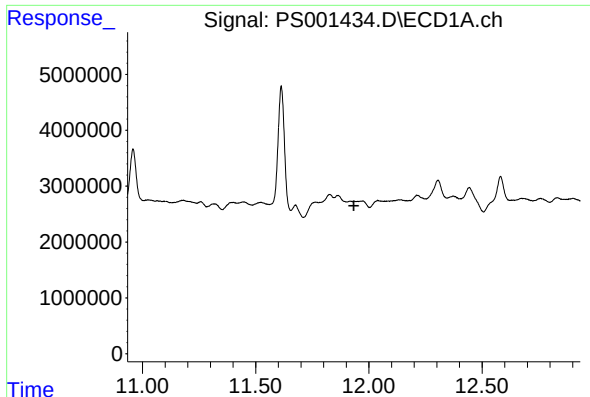

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

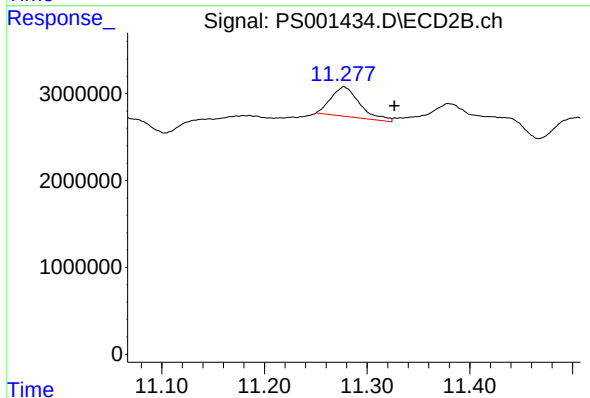


#5 DICAMBA

R.T.: 11.277 min
Delta R.T.: -0.049 min
Response: 6571441
Conc: 9.59 ng/ml

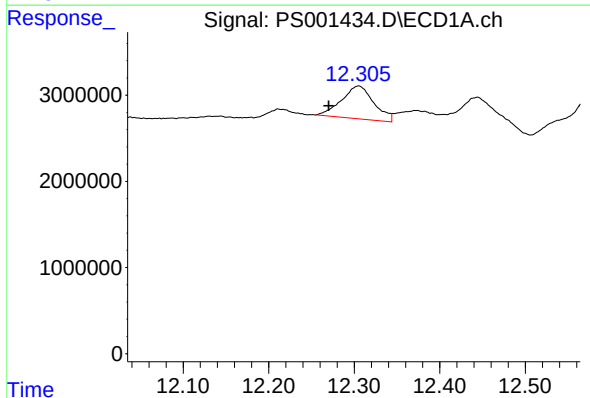


#6 MCP

R.T.: 12.305 min
Delta R.T.: 0.035 min
Response: 9990063
Conc: 19.88 ug/ml

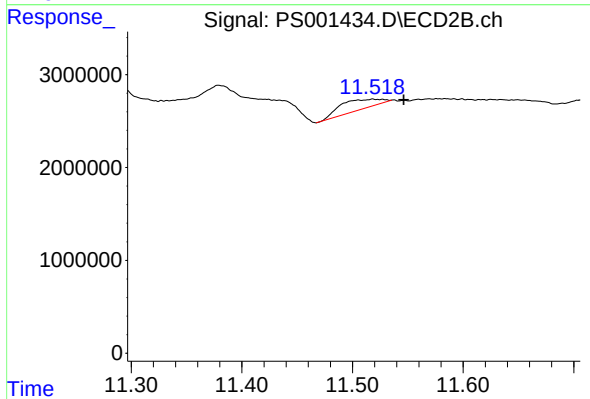

#6 MCP


R.T.: 11.519 min
Delta R.T.: -0.028 min
Response: 2668524
Conc: 6.15 ug/ml

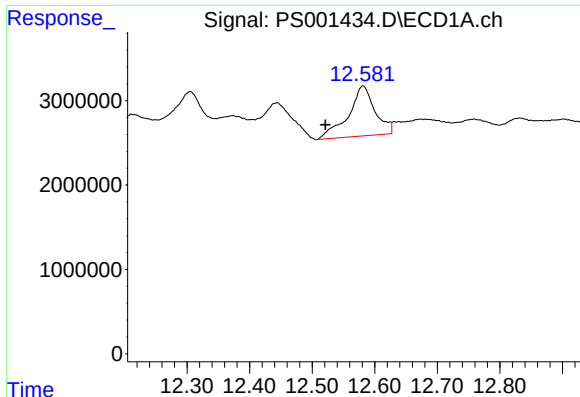

#7 MCPA


R.T.: 12.581 min
Delta R.T.: 0.060 min
Response: 17633360
Conc: 22.36 ug/ml

Instrument :
ECD_S
ClientSampleId :

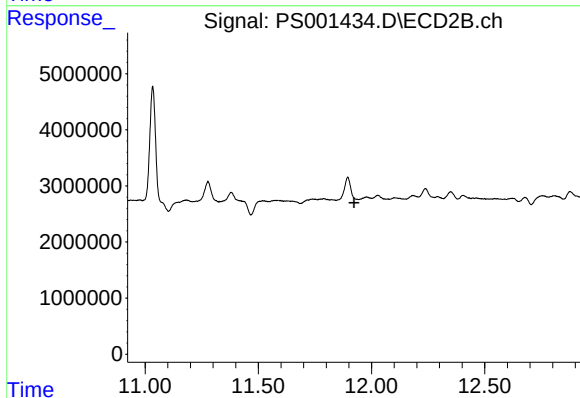


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

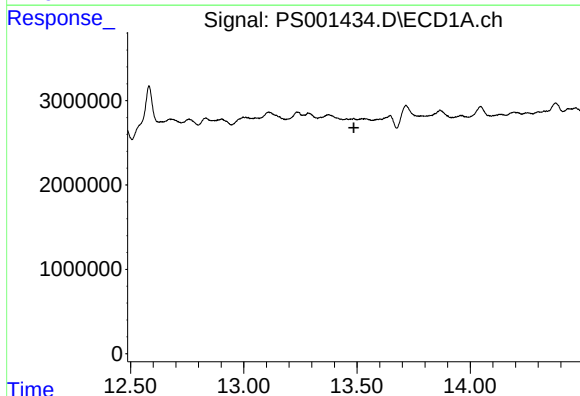


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.486 min
Response: 0
Conc: N.D.

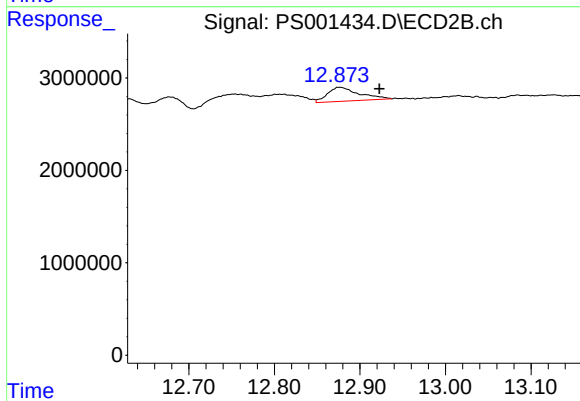

#9 2,4-D


R.T.: 12.877 min
Delta R.T.: -0.046 min
Response: 3865824
Conc: 16.29 ng/ml

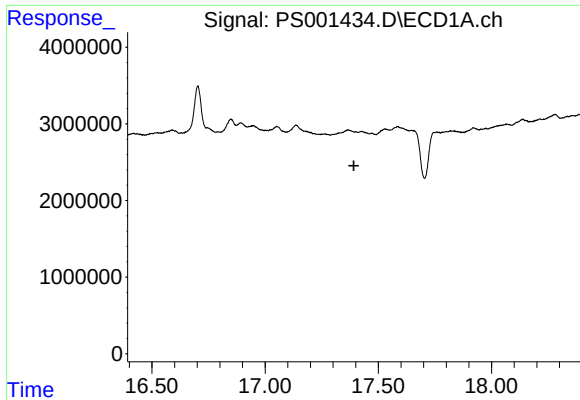

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

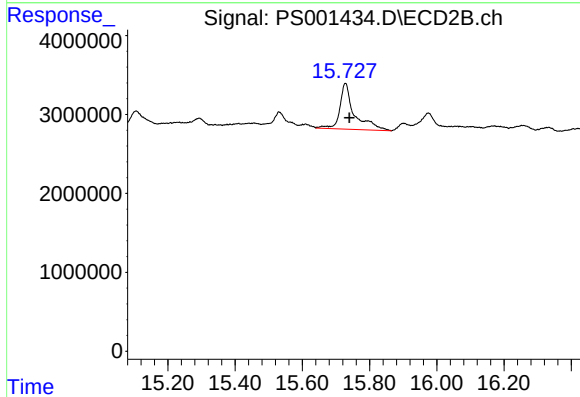


#14 DINOSEB

R.T.: 15.728 min
Delta R.T.: -0.011 min
Response: 17490615
Conc: 24.61 ng/ml

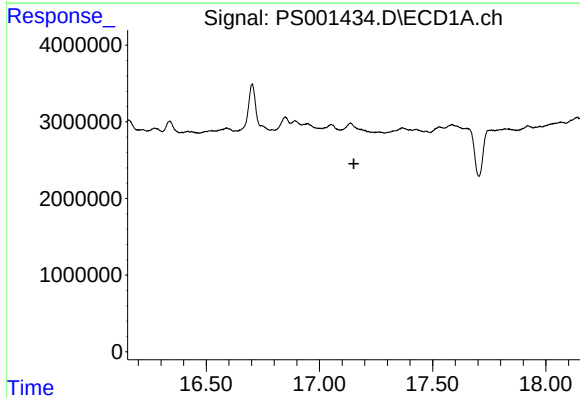


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

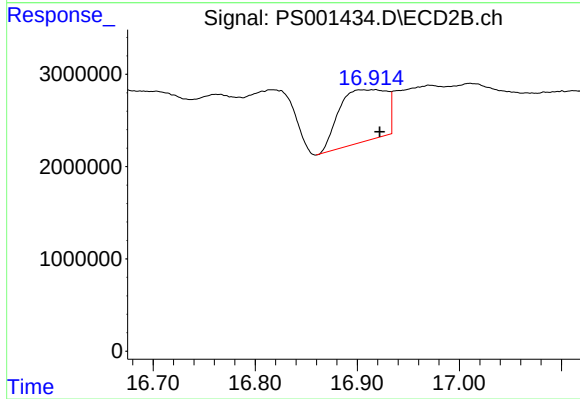

#15 Picloram


R.T.: 16.916 min
Delta R.T.: -0.006 min
Response: 18187743
Conc: 13.19 ng/ml

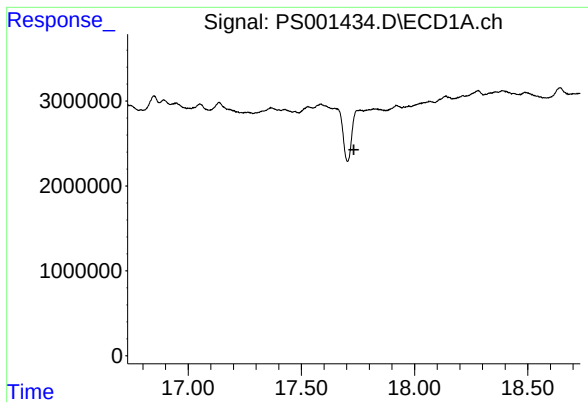

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

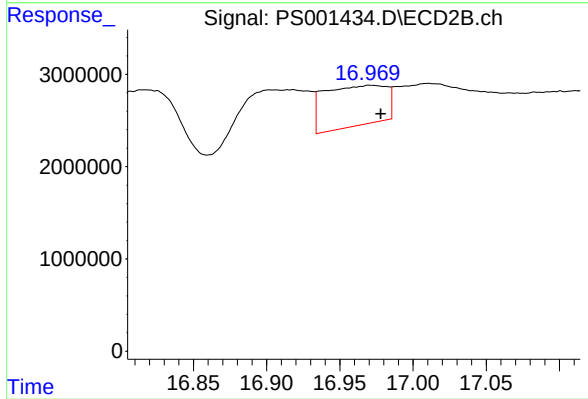

#16 DCPA

R.T.: 16.972 min
Delta R.T.: -0.006 min
Response: 12857709
Conc: 8.90 ng/ml