

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081018\
 Data File : PS001440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2018 23:52
 Operator : UA
 Sample : J4398-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 06:39:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.614	11.034	36269795	34250098	195.472	188.317
Target Compounds							
1) T	Dalapon	2.961	2.401	5235937	4247765	22.081	18.641
5) T	DICAMBA	0.000	11.279	0	5930328	N.D.	8.653 #
6) T	MCPD	12.305	0.000	10235547	0	20.365	N.D. #
7) T	MCPA	12.583	0.000	10071285	0	12.771	N.D. #
9) T	2,4-D	0.000	12.871	0	3892335	N.D.	16.403 #
12) T	2,4,5-T	0.000	14.704	0	92957095	N.D.	100.633 #
14) T	DINOSEB	0.000	15.729	0	25078141	N.D.	35.281 #
15) T	Picloram	0.000	16.981	0	83498213	N.D.	60.571 #
16) T	DCPA	0.000	16.981	0	83498213	N.D.	57.813 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081018\
Data File : PS001440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2018 23:52
Operator : UA
Sample : J4398-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 06:39:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

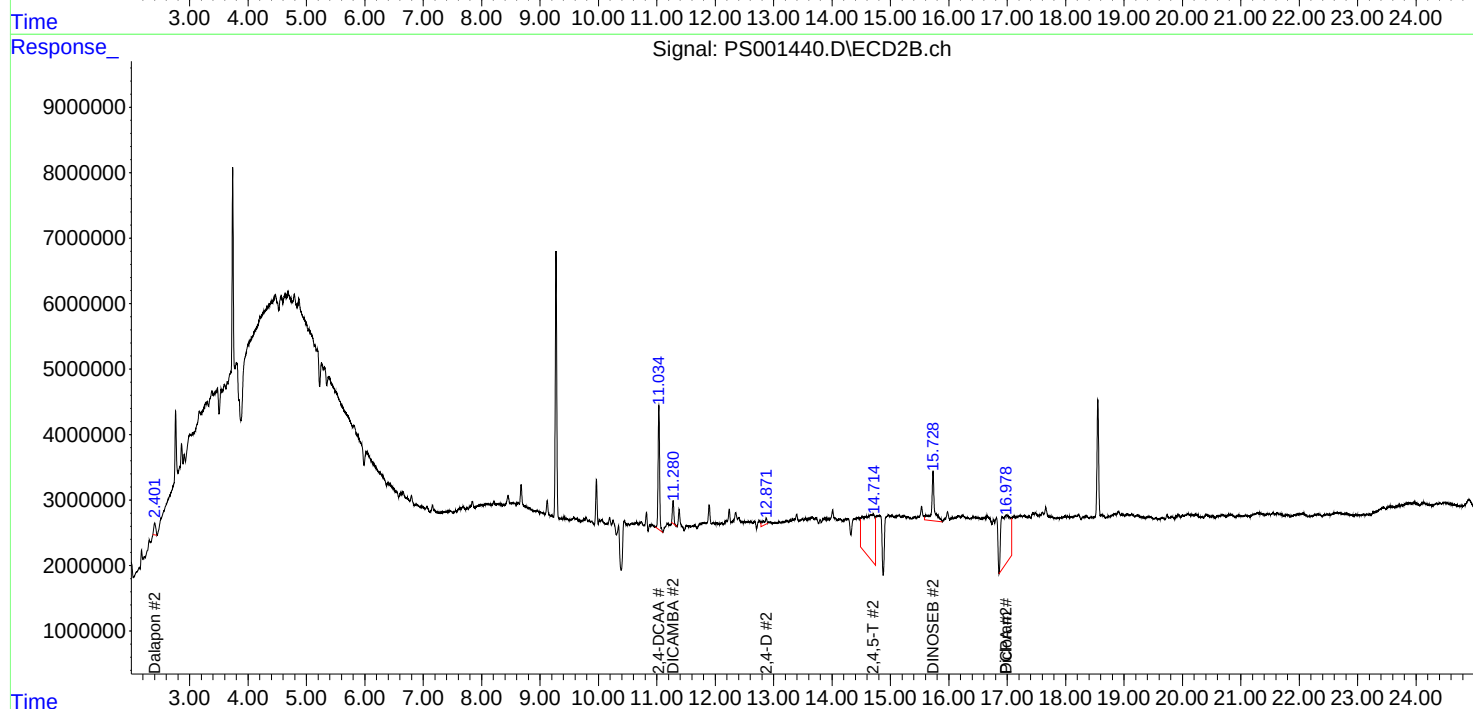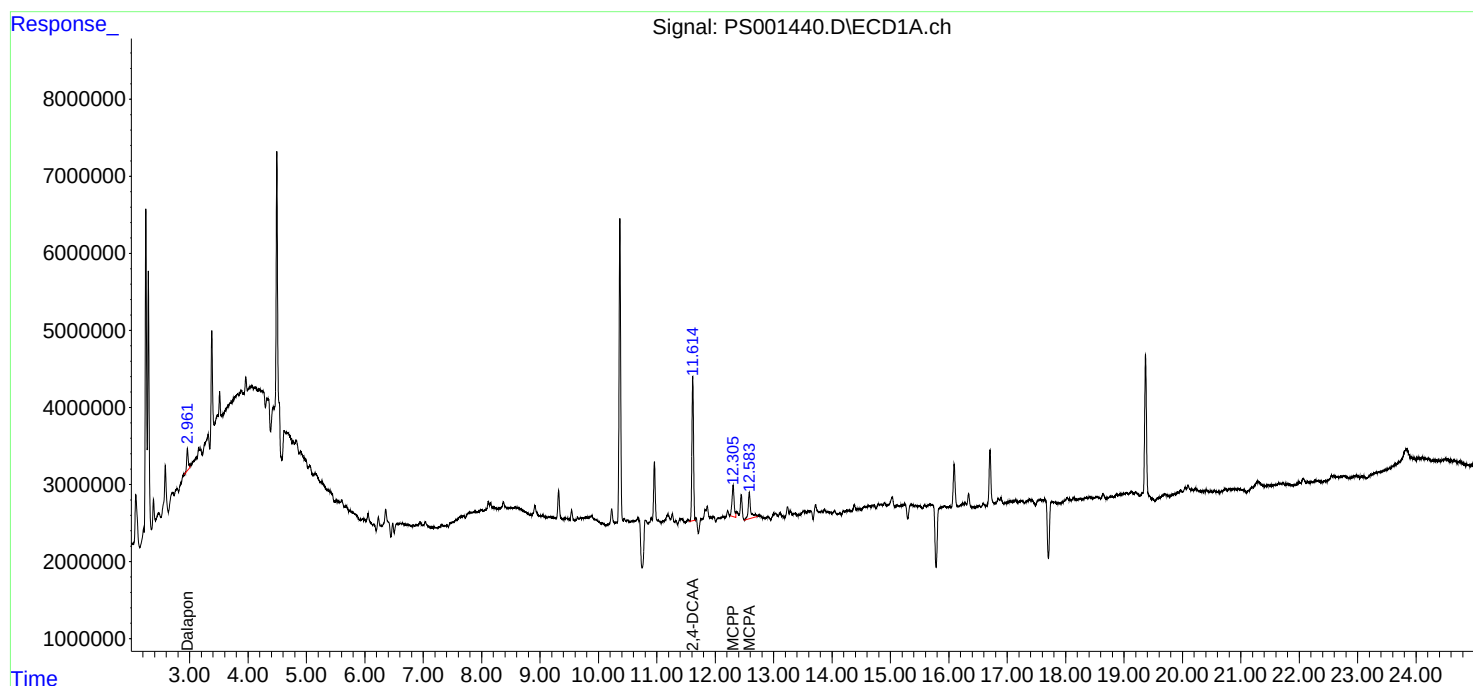


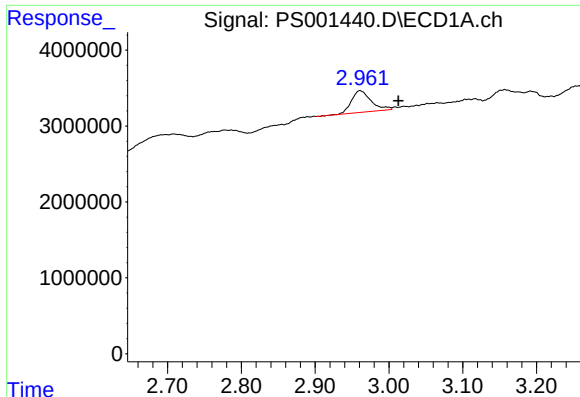

#1 Dalapon


R.T.: 2.961 min
Delta R.T.: -0.052 min
Response: 5235937
Conc: 22.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

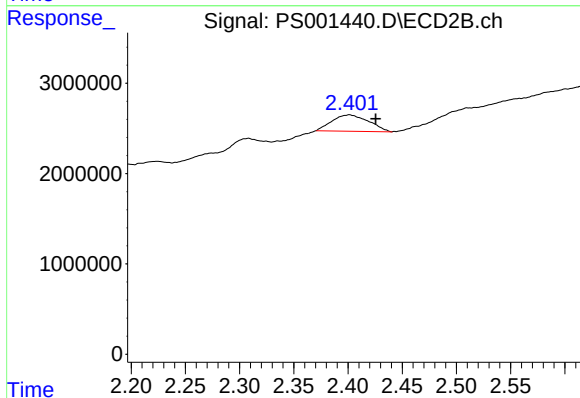


#1 Dalapon

R.T.: 2.401 min
Delta R.T.: -0.024 min
Response: 4247765
Conc: 18.64 ng/ml

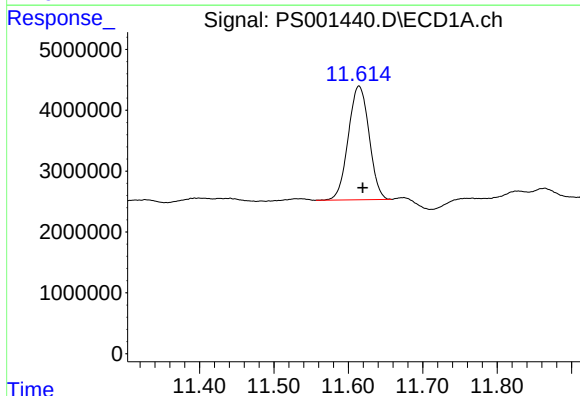


#4 2,4-DCAA

R.T.: 11.614 min
Delta R.T.: -0.005 min
Response: 36269795
Conc: 195.47 ng/ml

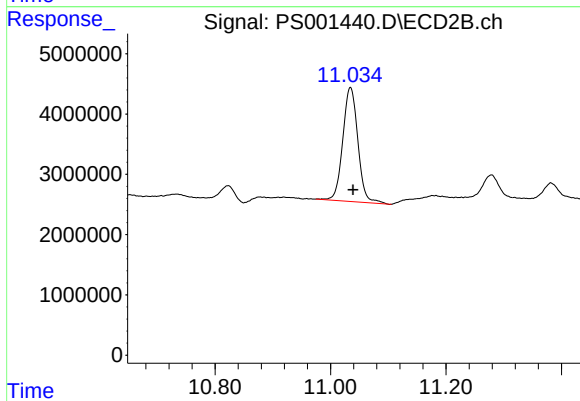

#4 2,4-DCAA


R.T.: 11.034 min
Delta R.T.: -0.004 min
Response: 34250098
Conc: 188.32 ng/ml

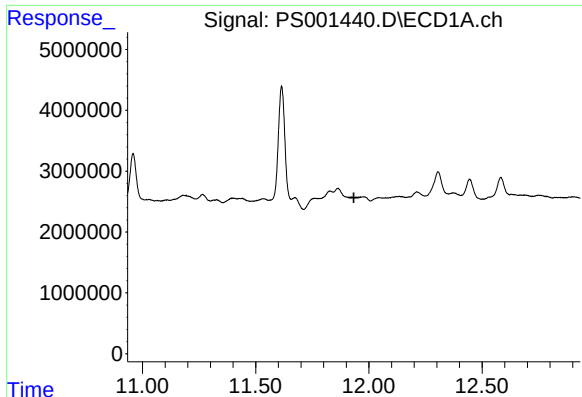

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

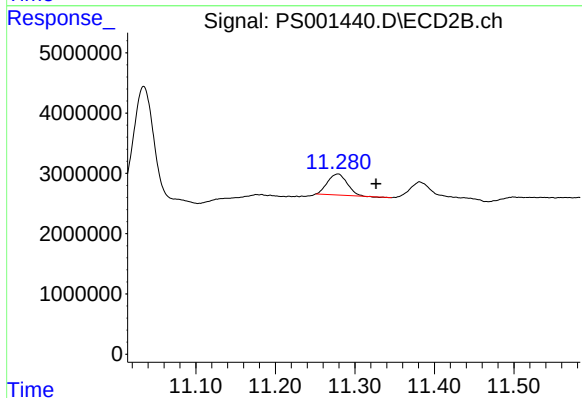


#5 DICAMBA

R.T.: 11.279 min
Delta R.T.: -0.048 min
Response: 5930328
Conc: 8.65 ng/ml

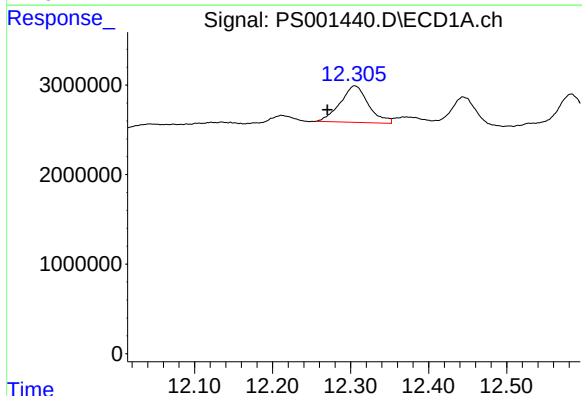


#6 MCP

R.T.: 12.305 min
Delta R.T.: 0.035 min
Response: 10235547
Conc: 20.36 ug/ml

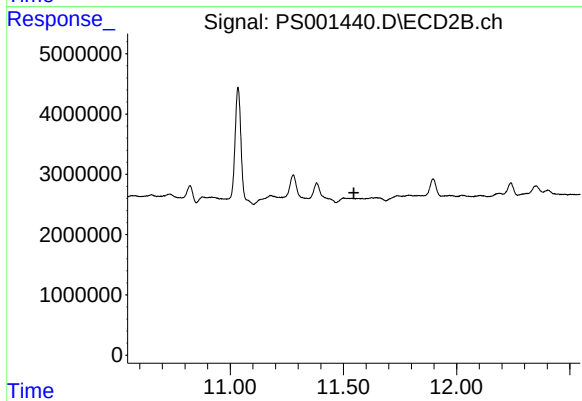

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

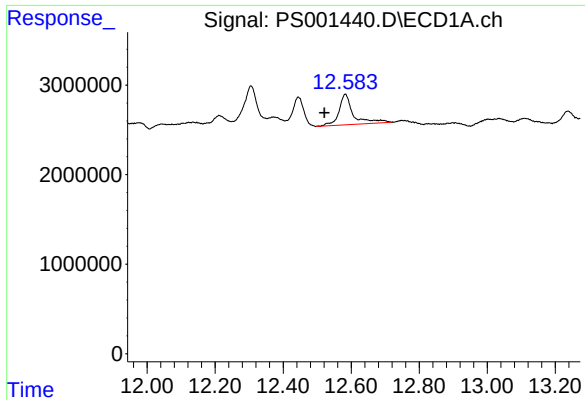

#7 MCPA


R.T.: 12.583 min
Delta R.T.: 0.061 min
Response: 10071285
Conc: 12.77 ug/ml

Instrument :
ECD_S
ClientSampleId :

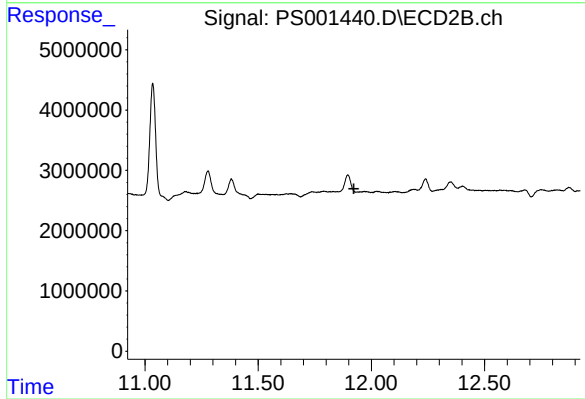


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

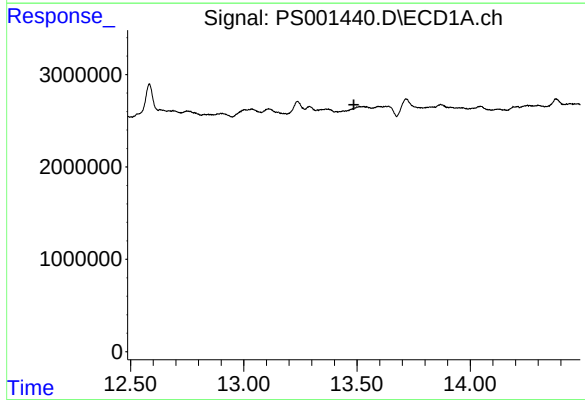


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.486 min
Response: 0
Conc: N.D.

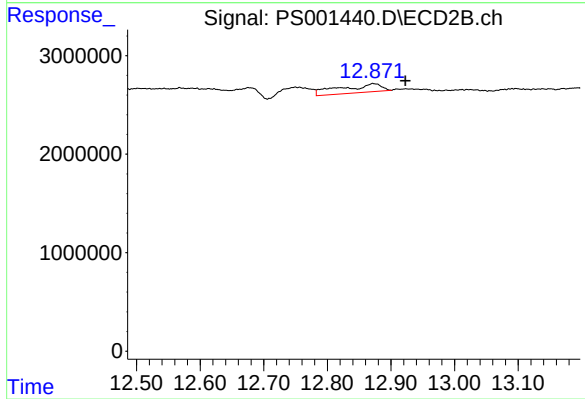

#9 2,4-D


R.T.: 12.871 min
Delta R.T.: -0.051 min
Response: 3892335
Conc: 16.40 ng/ml

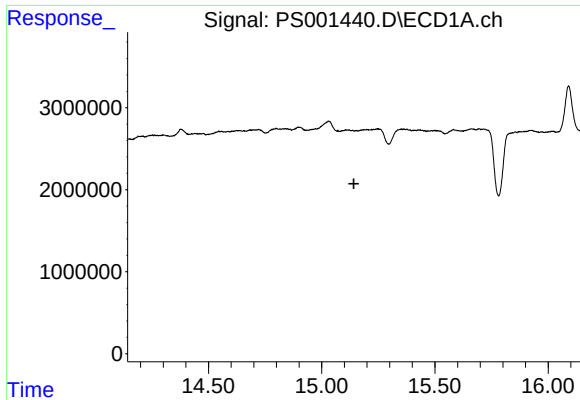

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

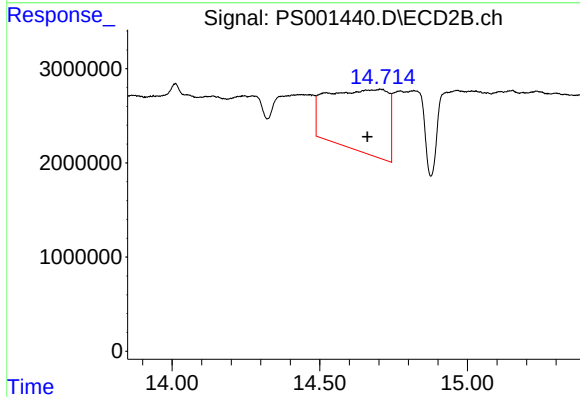


#12 2,4,5-T

R.T.: 14.704 min
Delta R.T.: 0.043 min
Response: 92957095
Conc: 100.63 ng/ml

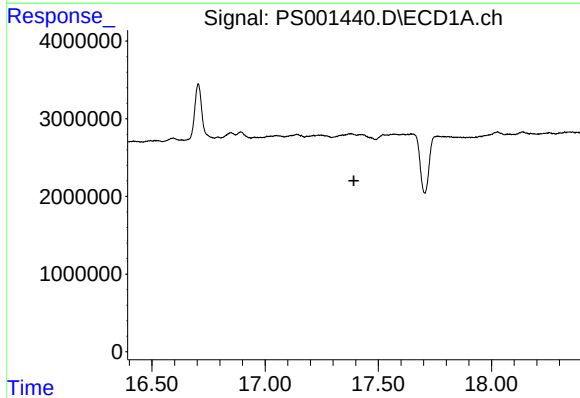


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.392 min
Response: 0
Conc: N.D.

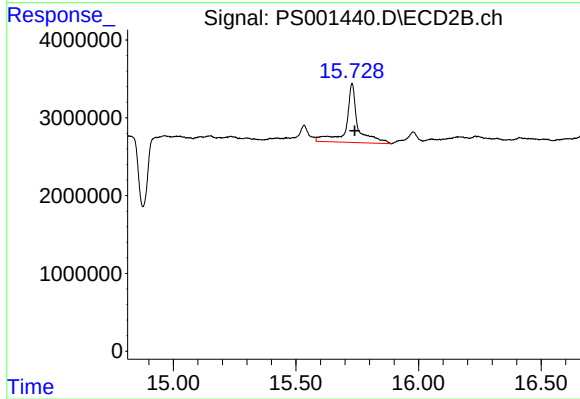

#14 DINOSEB


R.T.: 15.729 min
Delta R.T.: -0.011 min
Response: 25078141
Conc: 35.28 ng/ml

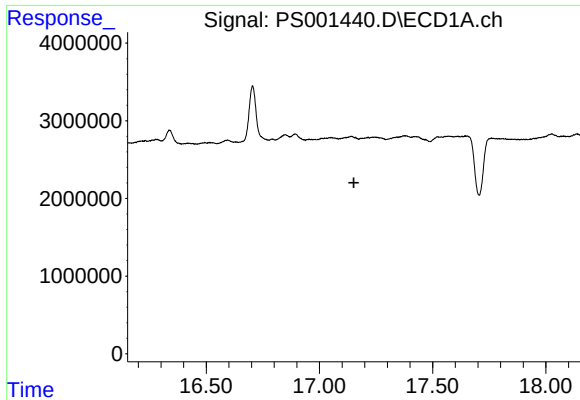

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

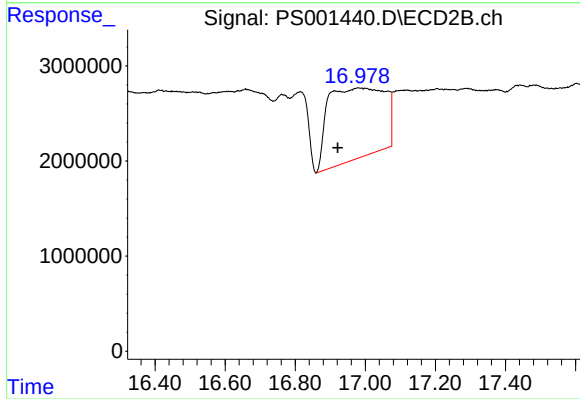


#15 Picloram

R.T.: 16.981 min
Delta R.T.: 0.059 min
Response: 83498213
Conc: 60.57 ng/ml

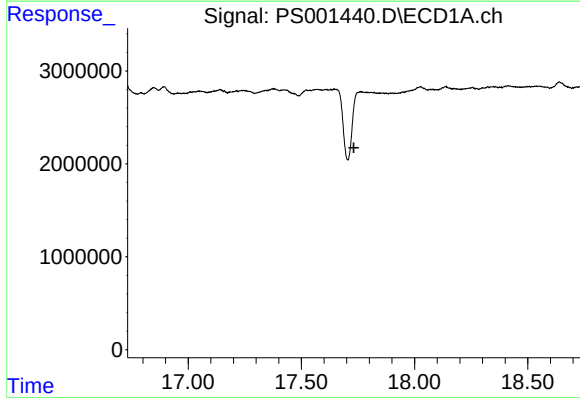

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

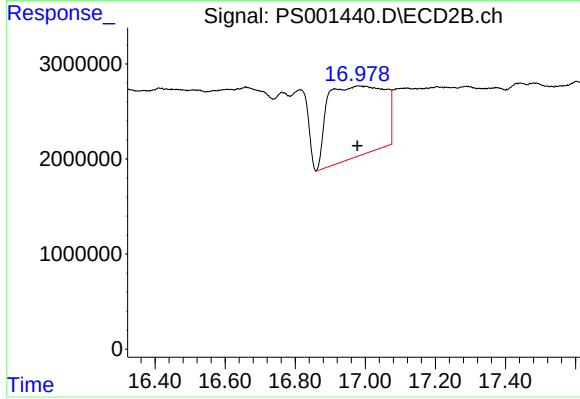

#16 DCPA

R.T.: 16.981 min
Delta R.T.: 0.003 min
Response: 83498213
Conc: 57.81 ng/ml