

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081018\
 Data File : PS001448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2018 04:01
 Operator : UA
 Sample : J4409-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 06:42:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.608	11.029	57513438	61616491	309.962	338.785
Target Compounds							
1) T	Dalapon	2.957	2.396	4755131	3555411	20.053	15.603
5) T	DICAMBA	0.000	11.376	0	9878061	N.D.	14.412 #
6) T	MCPD	12.299	11.506	6001090	2163523	11.940	4.986 #
7) T	MCPA	12.577	11.890	14111744	-6055687	17.894	N.D. #
9) T	2,4-D	0.000	12.868	0	5813317	N.D.	24.498 #
10) T	Pentachlo...	13.864	0.000	4196241	0	1.490	N.D. #
12) T	2,4,5-T	0.000	14.709	0	26075841	N.D.	28.229 #
14) T	DINOSEB	0.000	15.723	0	6200365	N.D.	8.723 #
15) T	Picloram	0.000	16.906	0	17362234	N.D.	12.595 #
16) T	DCPA	0.000	16.986	0	17683075	N.D.	12.243 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081018\
Data File : PS001448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2018 04:01
Operator : UA
Sample : J4409-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 06:42:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

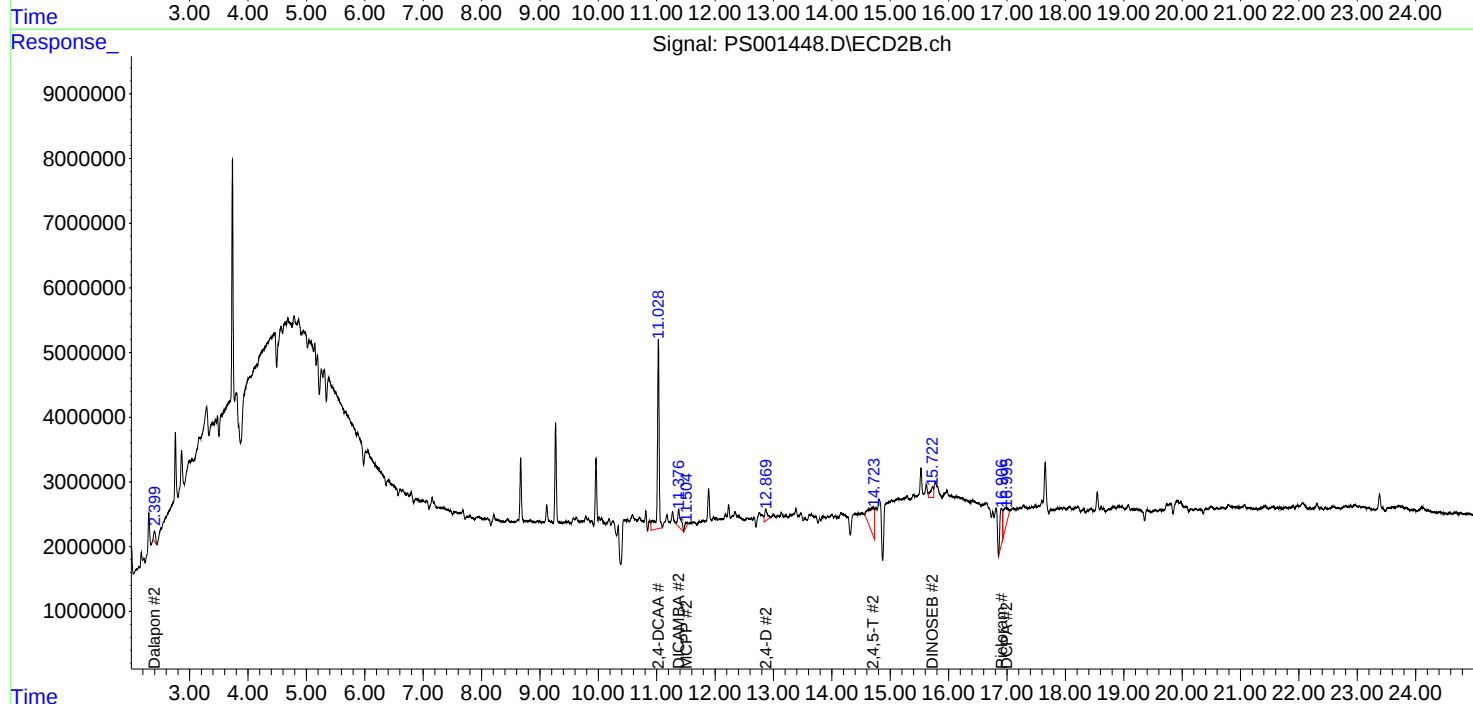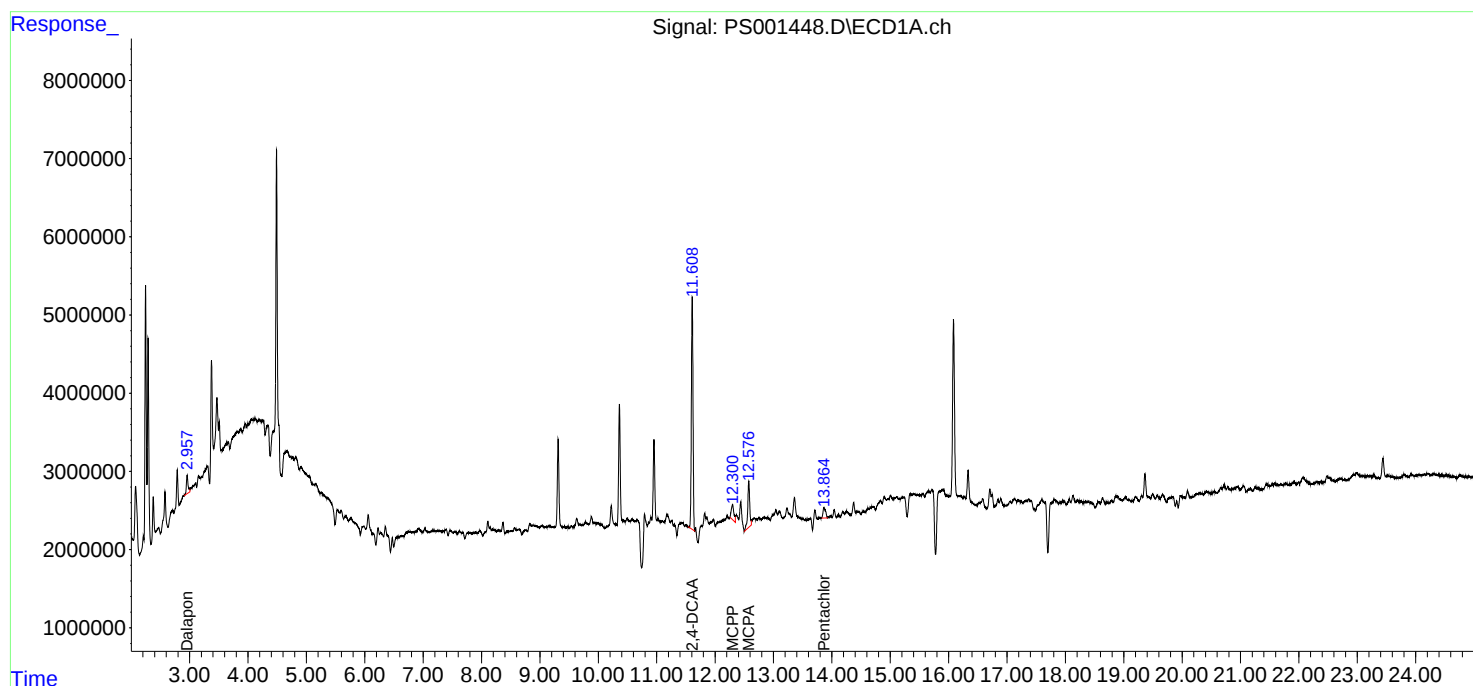


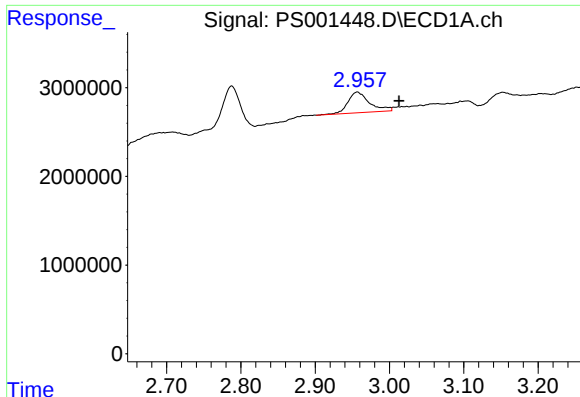

#1 Dalapon


R.T.: 2.957 min
Delta R.T.: -0.056 min
Response: 4755131
Conc: 20.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

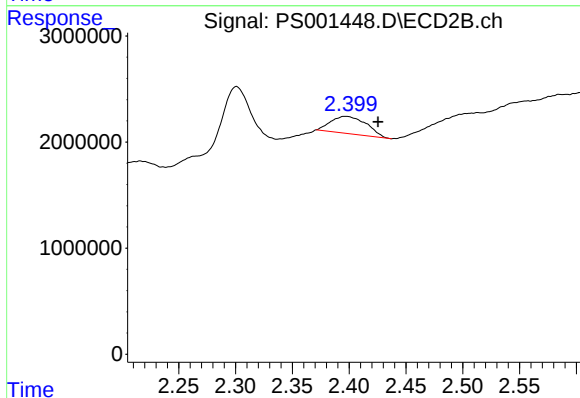


#1 Dalapon

R.T.: 2.396 min
Delta R.T.: -0.030 min
Response: 3555411
Conc: 15.60 ng/ml

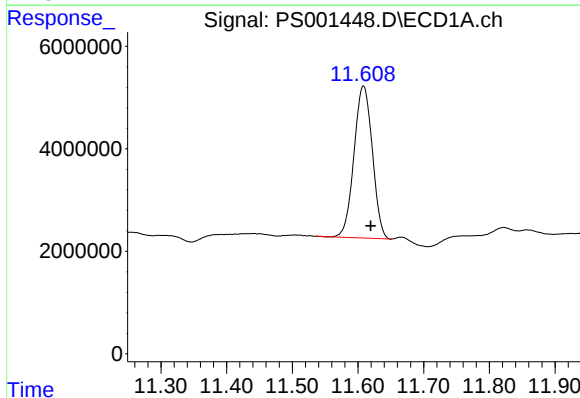


#4 2,4-DCAA

R.T.: 11.608 min
Delta R.T.: -0.011 min
Response: 57513438
Conc: 309.96 ng/ml

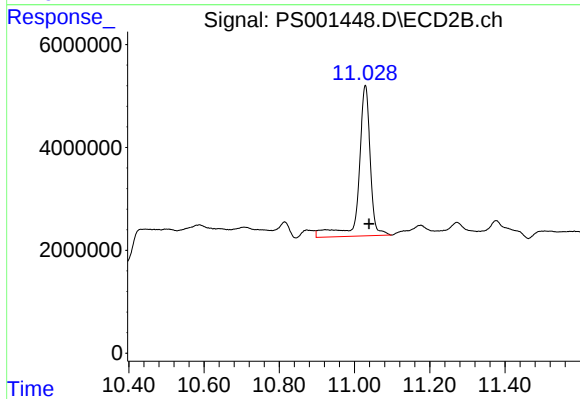

#4 2,4-DCAA


R.T.: 11.029 min
Delta R.T.: -0.010 min
Response: 61616491
Conc: 338.79 ng/ml

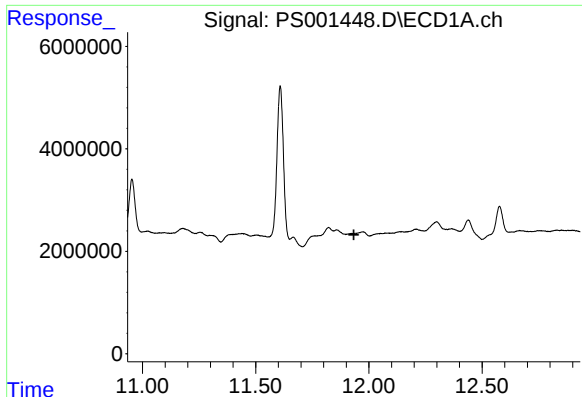

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

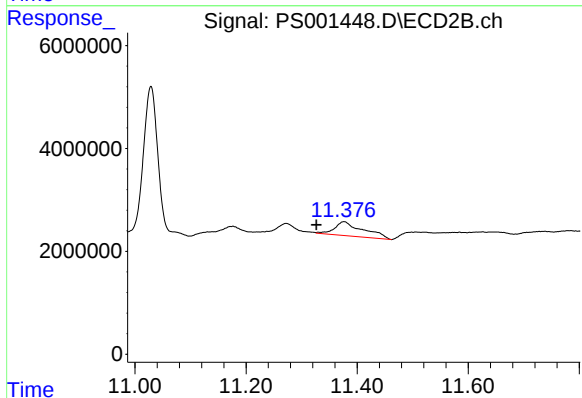


#5 DICAMBA

R.T.: 11.376 min
Delta R.T.: 0.050 min
Response: 9878061
Conc: 14.41 ng/ml

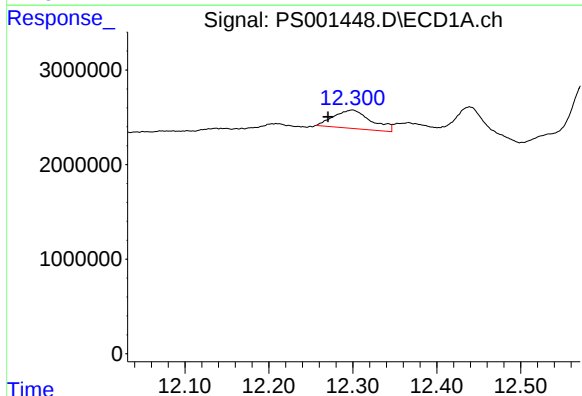


#6 MCP

R.T.: 12.299 min
Delta R.T.: 0.029 min
Response: 6001090
Conc: 11.94 ug/ml

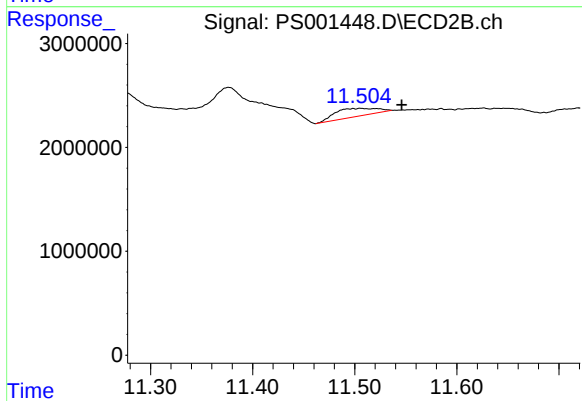

#6 MCP


R.T.: 11.506 min
Delta R.T.: -0.040 min
Response: 2163523
Conc: 4.99 ug/ml

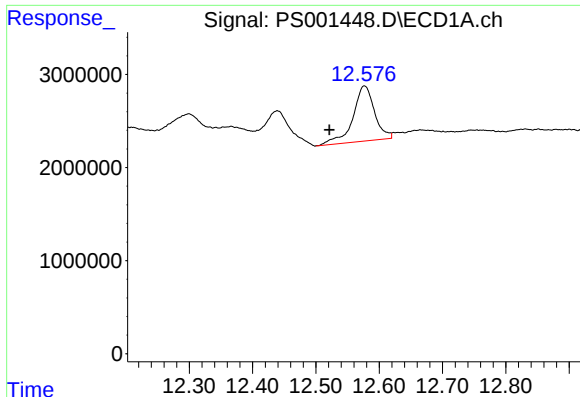

#7 MCPA


R.T.: 12.577 min
Delta R.T.: 0.056 min
Response: 14111744
Conc: 17.89 ug/ml

Instrument :
ECD_S
ClientSampleId :

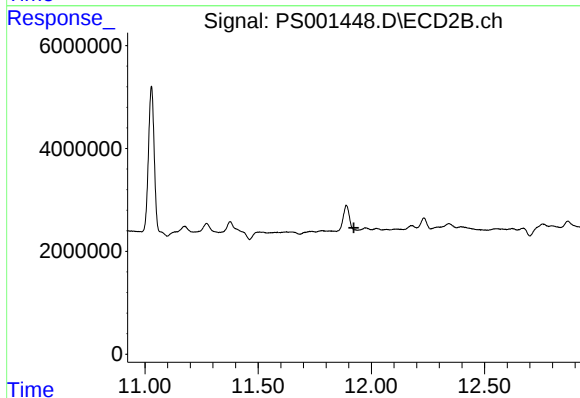


#7 MCPA

R.T.: 11.890 min
Delta R.T.: -0.033 min
Response: -6055687
Conc: N.D.

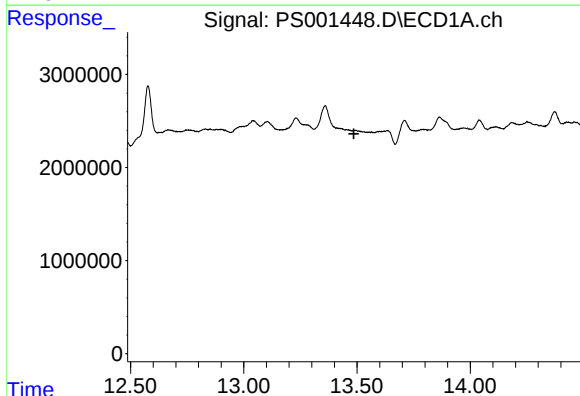


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.486 min
Response: 0
Conc: N.D.

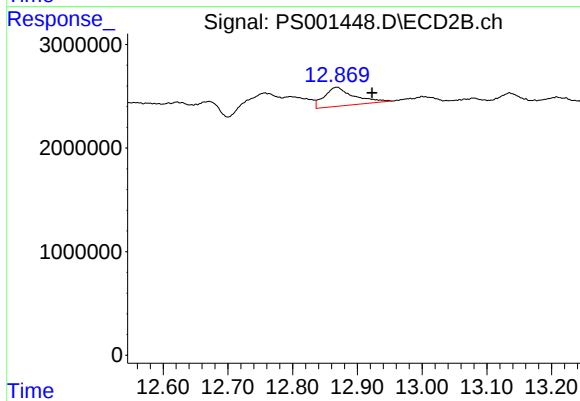

#9 2,4-D


R.T.: 12.868 min
Delta R.T.: -0.055 min
Response: 5813317
Conc: 24.50 ng/ml

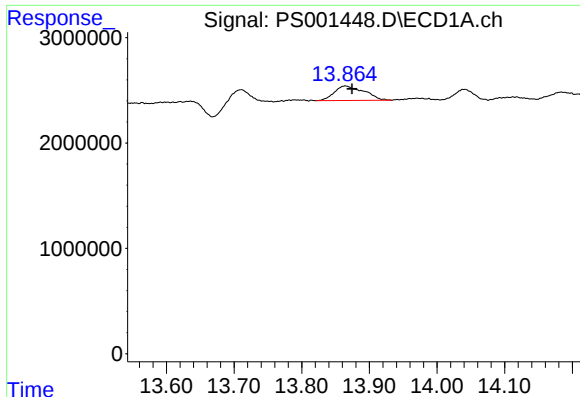

#10 Pentachlorophenol


R.T.: 13.864 min
Delta R.T.: -0.010 min
Response: 4196241
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

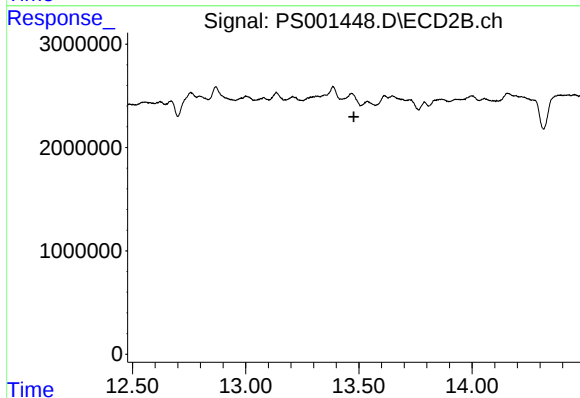


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.478 min
Response: 0
Conc: N.D.

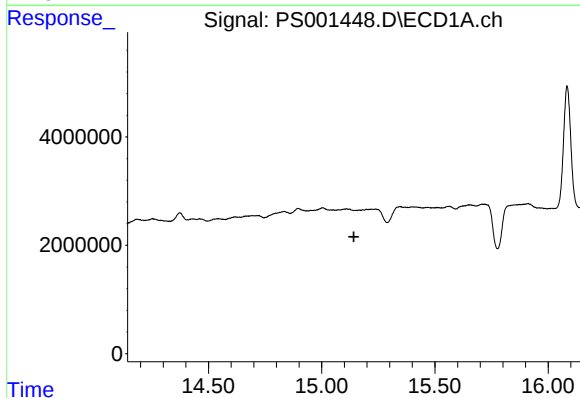


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.142 min
Response: 0
Conc: N.D.

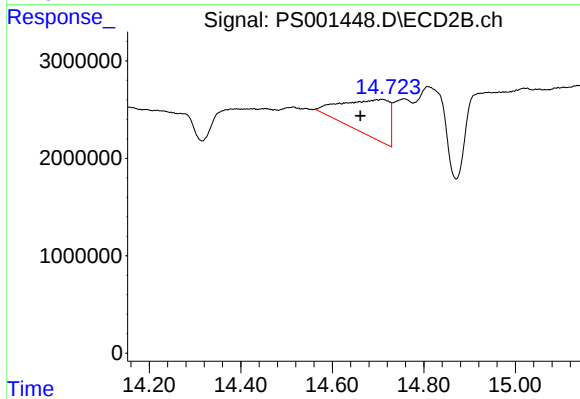

#12 2,4,5-T


R.T.: 14.709 min
Delta R.T.: 0.047 min
Response: 26075841
Conc: 28.23 ng/ml

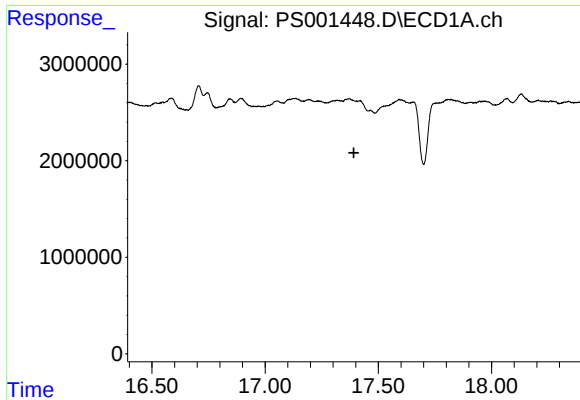

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

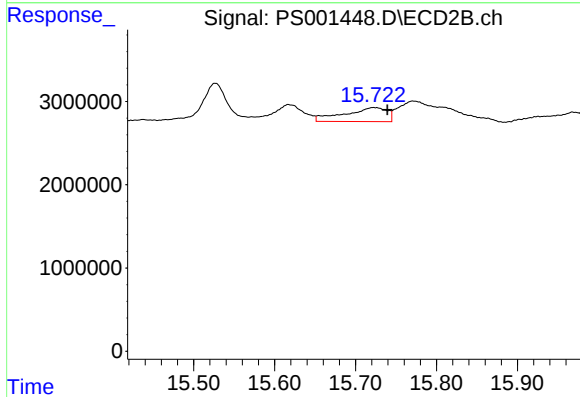


#14 DINOSEB

R.T.: 15.723 min
Delta R.T.: -0.016 min
Response: 6200365
Conc: 8.72 ng/ml

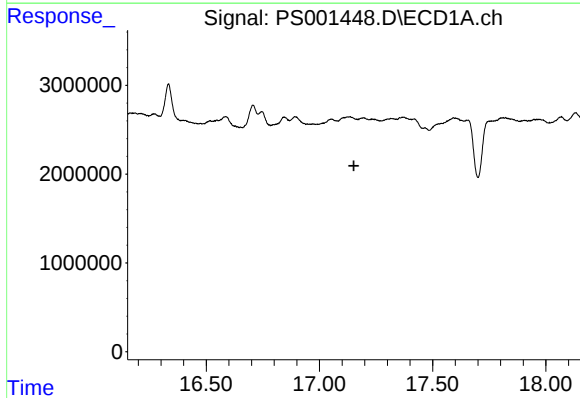


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

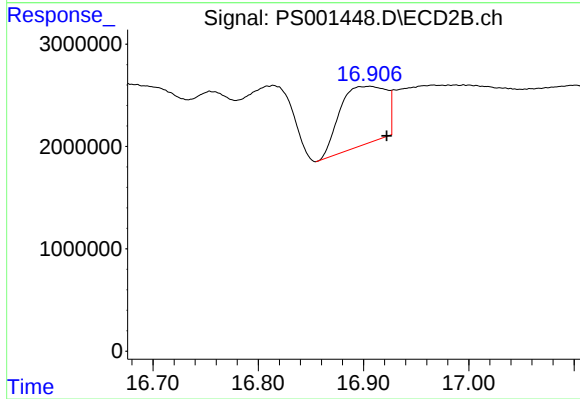

#15 Picloram


R.T.: 16.906 min
Delta R.T.: -0.016 min
Response: 17362234
Conc: 12.59 ng/ml

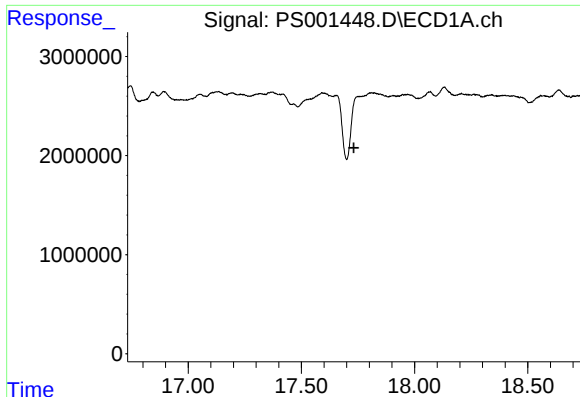

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

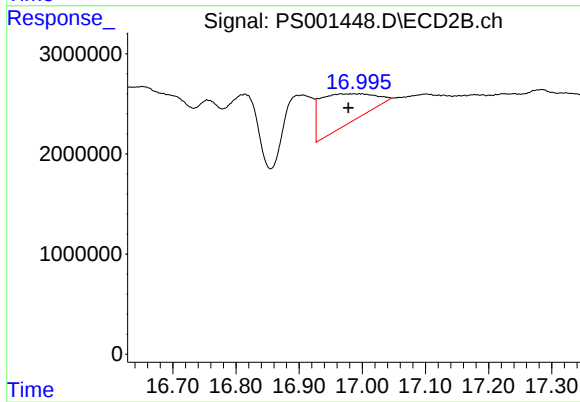

#16 DCPA

R.T.: 16.986 min
Delta R.T.: 0.008 min
Response: 17683075
Conc: 12.24 ng/ml