

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081021\
 Data File : PS016332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 09:04
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 15:57:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.765	600.2E6	249.6E6	408.009	478.428
Target Compounds							
12) T	2,4,5-T	9.377f	9.071f	17739199	13000340	2.327	4.488 #
15) T	Picloram	11.002	10.830	95340507	48635791	9.552	12.079 #
16) T	DCPA	0.000	10.830f	0	48635791	N.D.	10.820



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081021\
Data File : PS016332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 09:04
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 15:57:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

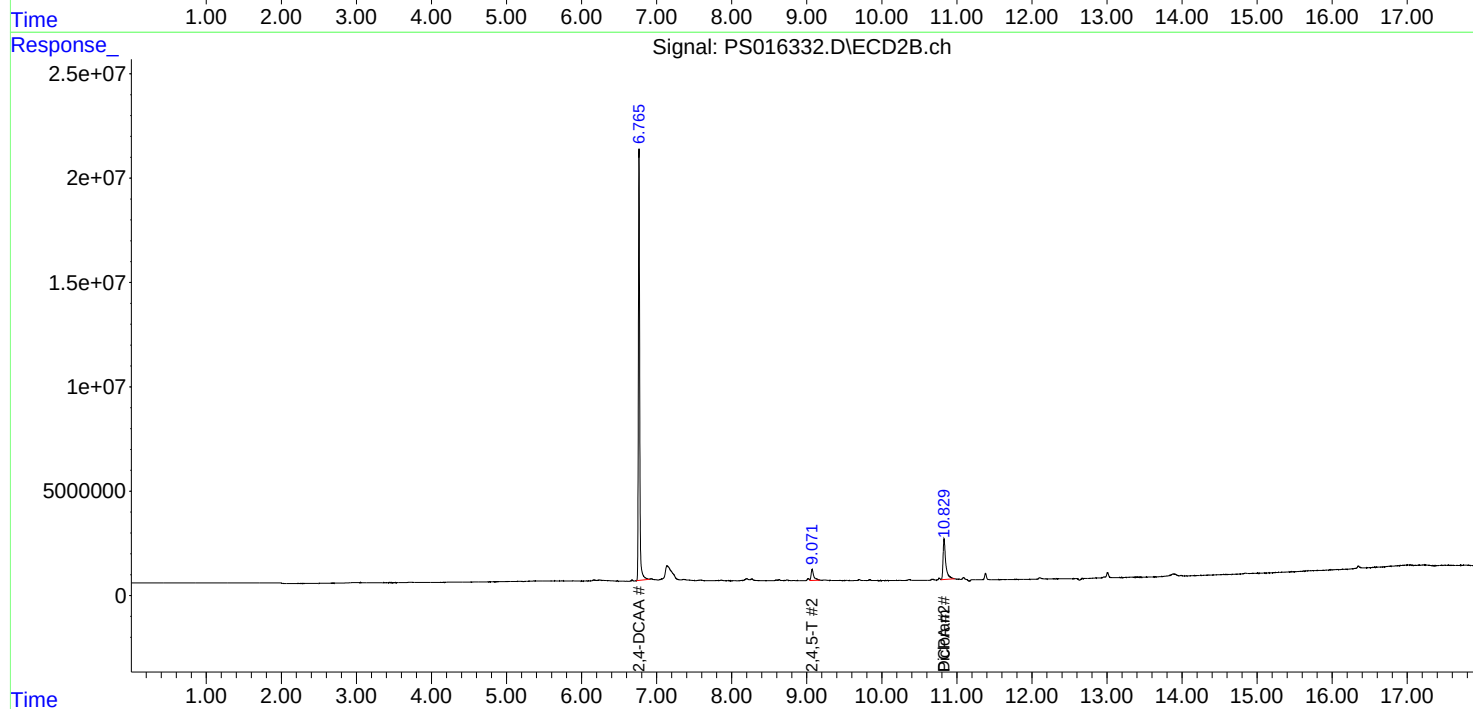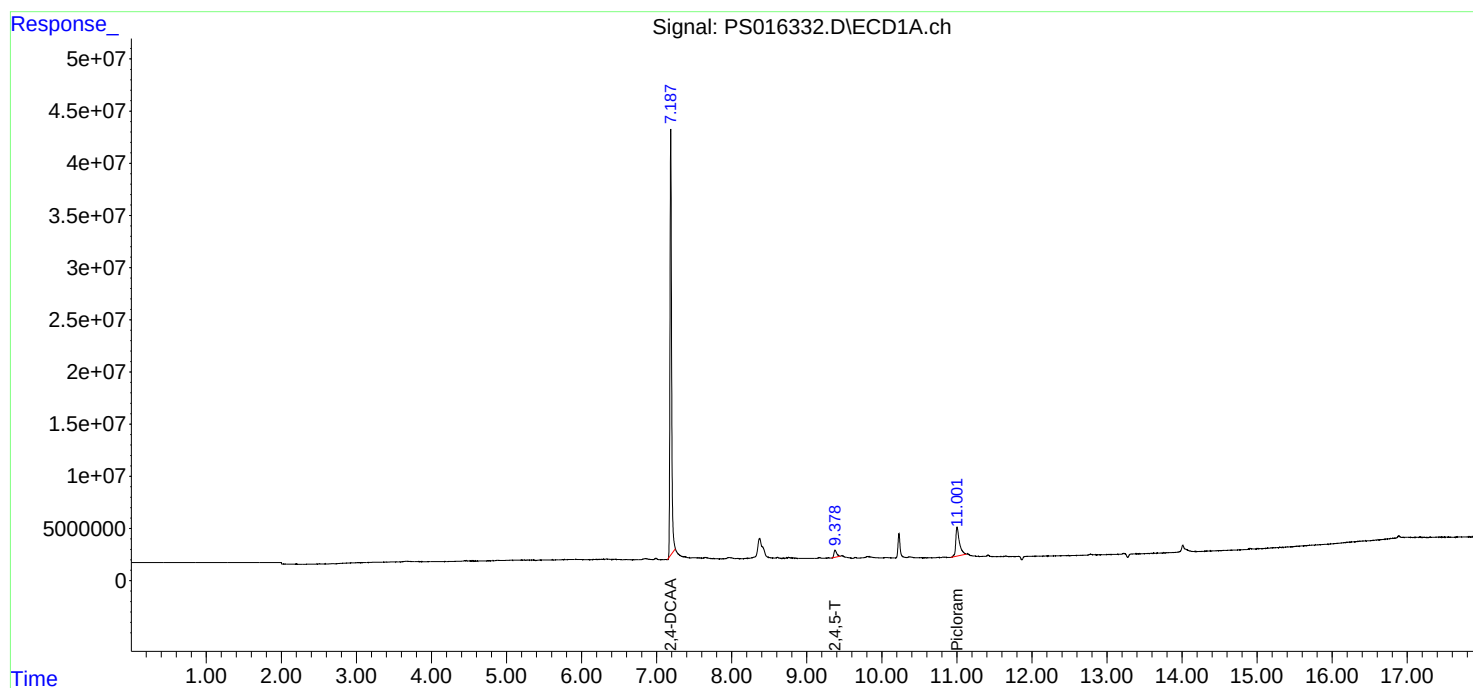


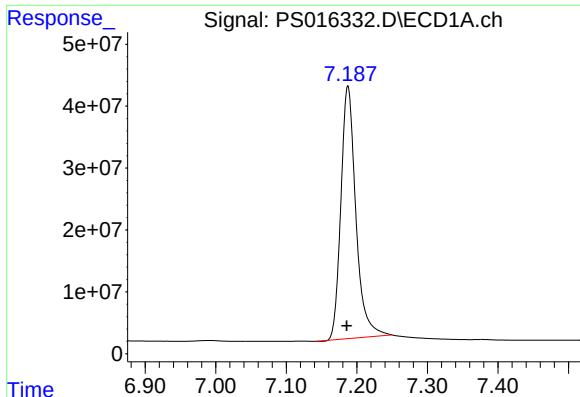

#4 2,4-DCAA


R.T.: 7.187 min
Delta R.T.: 0.002 min
Response: 600224444
Conc: 408.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

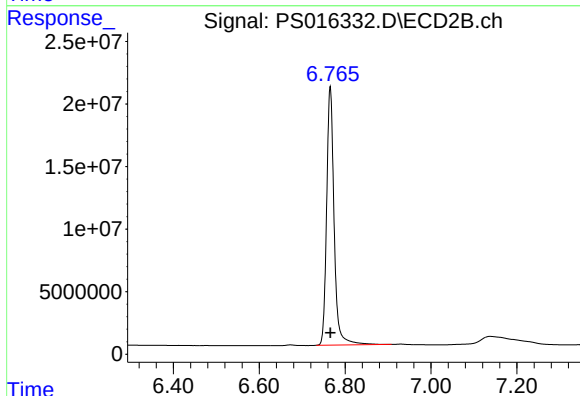


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: 0.000 min
Response: 249560018
Conc: 478.43 ng/ml

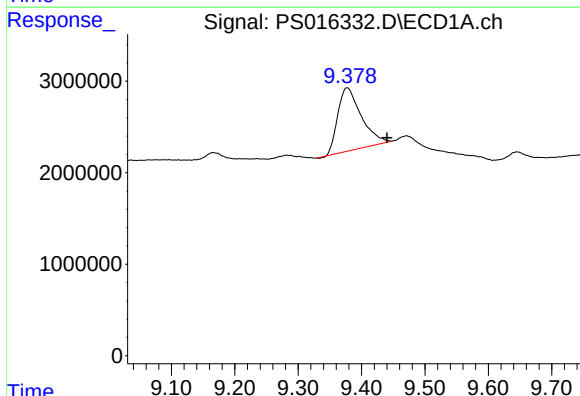


#12 2,4,5-T

R.T.: 9.377 min
Delta R.T.: -0.063 min
Response: 17739199
Conc: 2.33 ng/ml

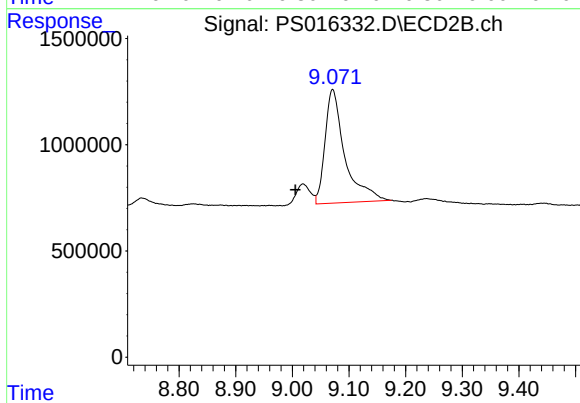

#12 2,4,5-T


R.T.: 9.071 min
Delta R.T.: 0.066 min
Response: 13000340
Conc: 4.49 ng/ml

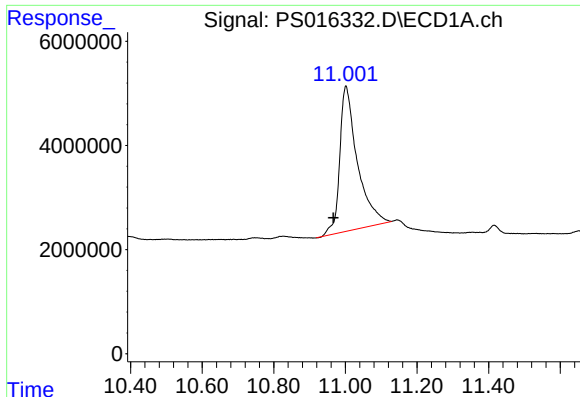

#15 Picloram


R.T.: 11.002 min
Delta R.T.: 0.035 min
Response: 95340507
Conc: 9.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

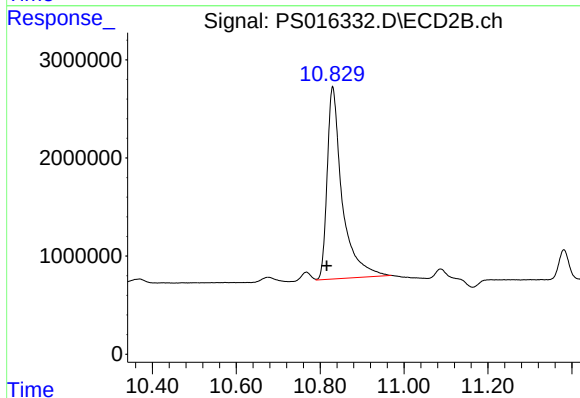


#15 Picloram

R.T.: 10.830 min
Delta R.T.: 0.014 min
Response: 48635791
Conc: 12.08 ng/ml

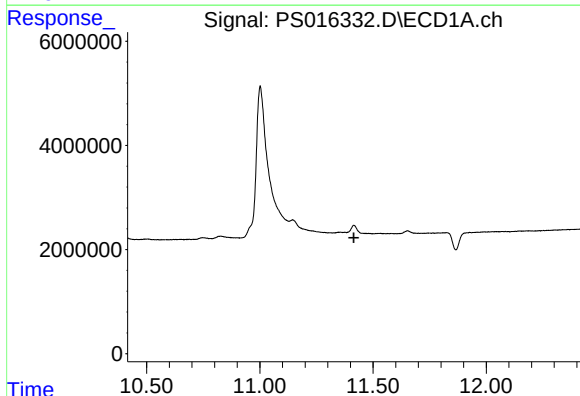

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.415 min
Response: 0
Conc: N.D.

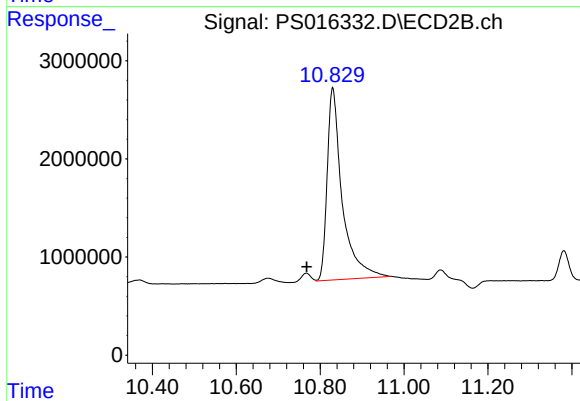

#16 DCPA

R.T.: 10.830 min
Delta R.T.: 0.062 min
Response: 48635791
Conc: 10.82 ng/ml