

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081021\
 Data File : PS016338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 12:35
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 15:59:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.763	608.0E6	244.4E6	413.321	468.462
Target Compounds							
5) T	DICAMBA	0.000	6.869f	0	3369201	N.D.	1.546
6) T	MCPD	0.000	7.044	0	1925992	N.D.	1.115
10) T	Pentachlo...	8.610	8.265	7396518	3267906	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.627	0	1907448	N.D.	<MDL
12) T	2,4,5-T	0.000	9.012	0	2989607	N.D.	1.032
14) T	DINOSEB	0.000	9.837	0	1714387	N.D.	<MDL
15) T	Picloram	10.998	10.828	13175732	8729900	1.320	2.168 #
16) T	DCPA	0.000	10.765	0	3221182	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081021\
Data File : PS016338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 12:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 15:59:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

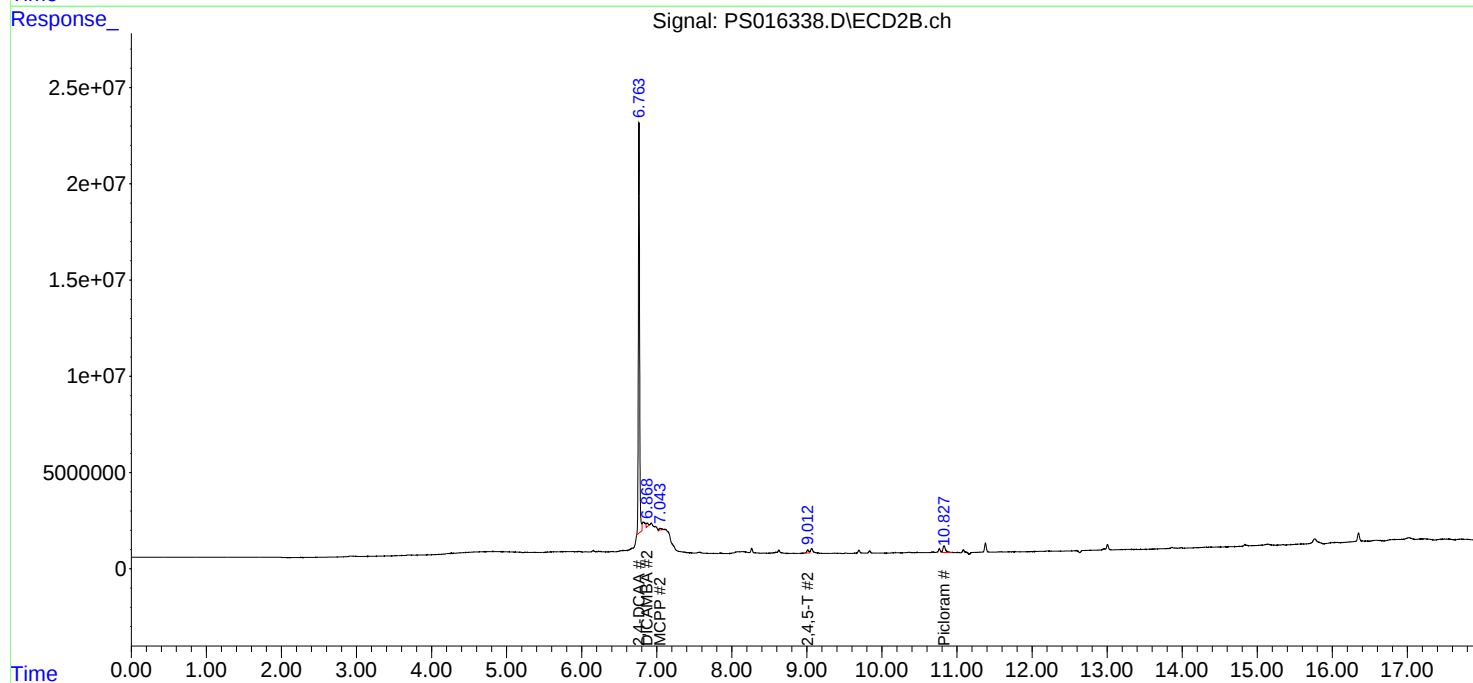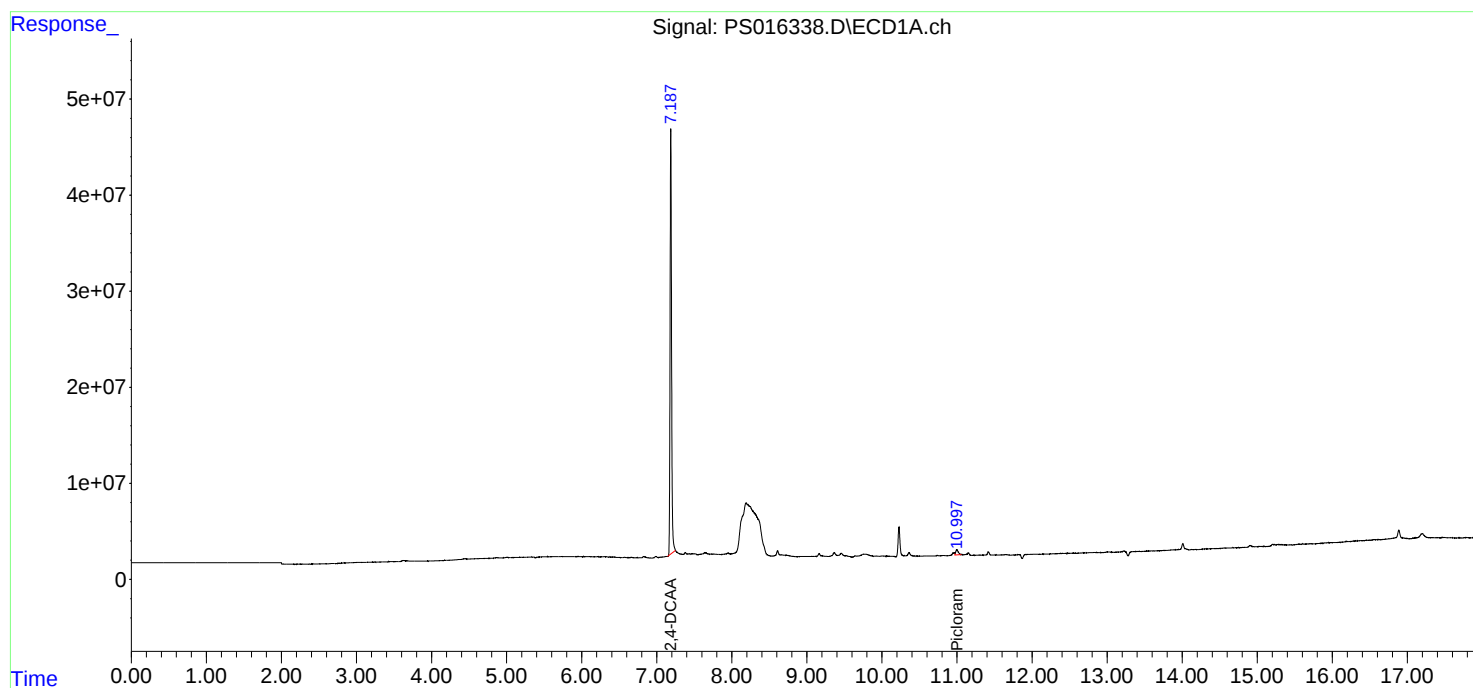


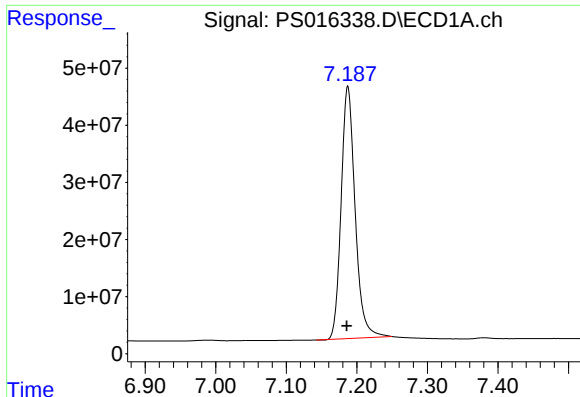

#4 2,4-DCAA


R.T.: 7.187 min
Delta R.T.: 0.002 min
Response: 608038954
Conc: 413.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

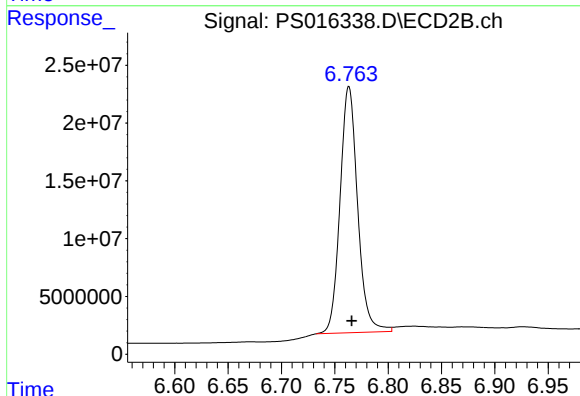


#4 2,4-DCAA

R.T.: 6.763 min
Delta R.T.: -0.003 min
Response: 244361204
Conc: 468.46 ng/ml

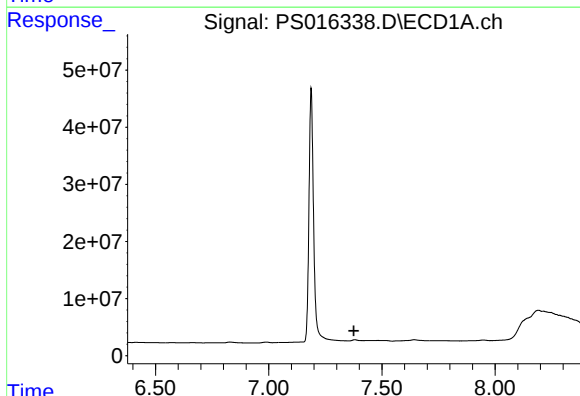


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

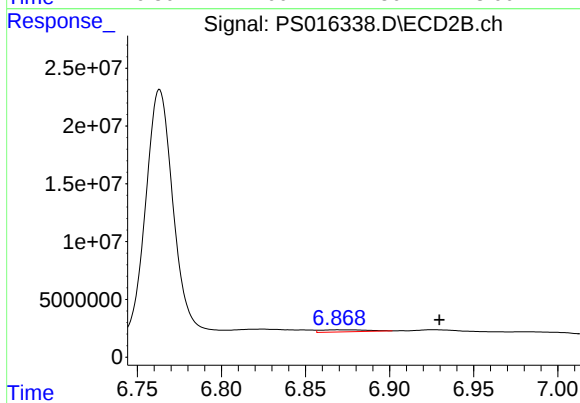

#5 DICAMBA


R.T.: 6.869 min
Delta R.T.: -0.060 min
Response: 3369201
Conc: 1.55 ng/ml

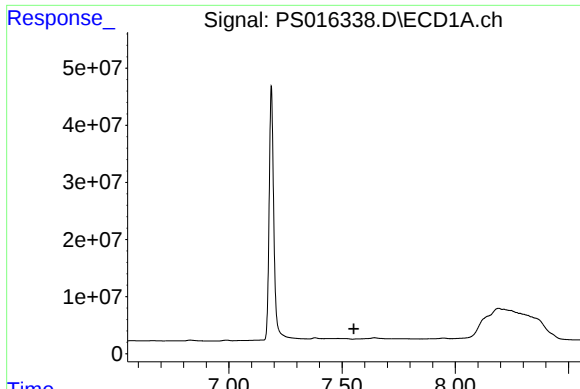

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

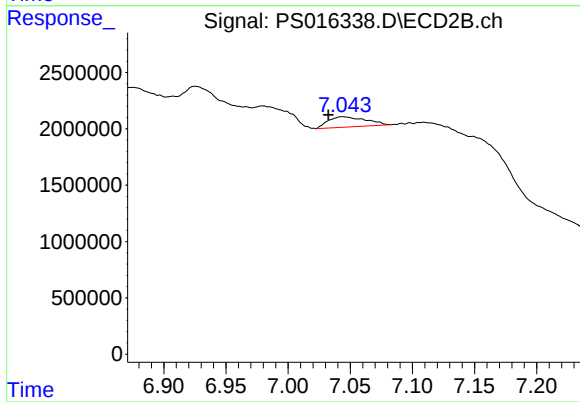


#6 MCP

R.T.: 7.044 min
Delta R.T.: 0.011 min
Response: 1925992
Conc: 1.11 ug/ml

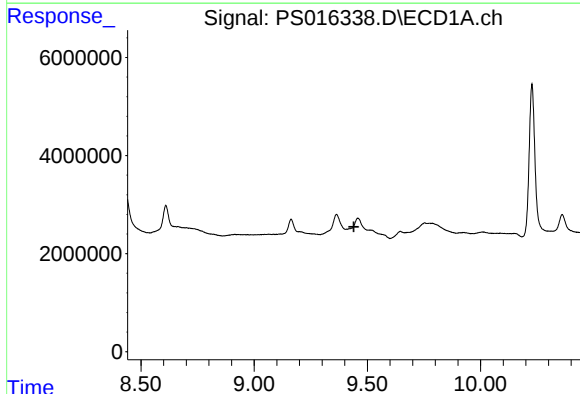


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.440 min
Response: 0
Conc: N.D.

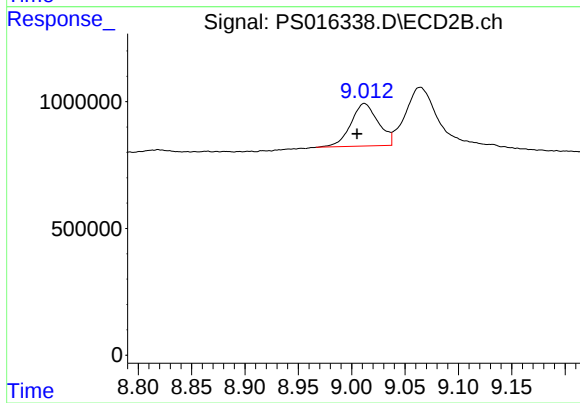

#12 2,4,5-T


R.T.: 9.012 min
Delta R.T.: 0.007 min
Response: 2989607
Conc: 1.03 ng/ml

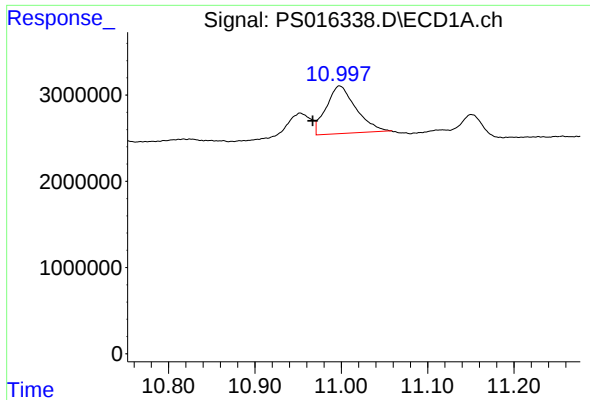

#15 Picloram

R.T.: 10.998 min
Delta R.T.: 0.031 min
Response: 13175732
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

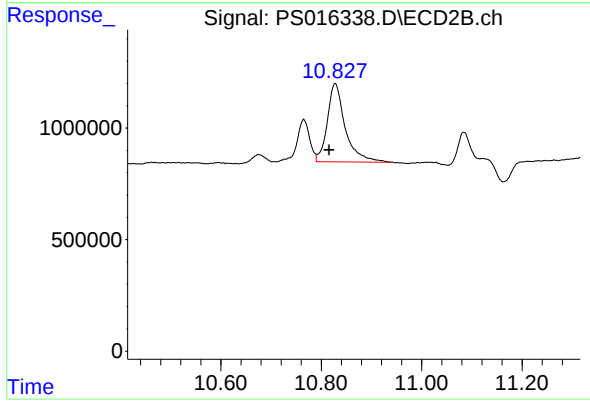

#15 Picloram

R.T.: 10.828 min
Delta R.T.: 0.012 min
Response: 8729900
Conc: 2.17 ng/ml