

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081023\
 Data File : PS024030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 20:12
 Operator : AR\AJ
 Sample : 03954-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:37:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.367	6.797	735.8E6	208.6E6	371.505	310.098
Target Compounds							
1) T	Dalapon	2.457	2.531	45247289	12680633	20.621	11.597 #
2) T	3,5-DICHL...	5.735	5.987	6869981	4384287	2.266	4.184 #
3) T	4-Nitroph...	6.182	6.438	53417606	5745549	48.262	14.516 #
5) T	DICAMBA	6.532	6.945	700603	1110867	<MDL	<MDL #
6) T	MCP	6.684	7.116f	20281457	-354070	3.252	N.D. #
7) T	MCPA	6.817	7.260	19769188	7458380	2.353	2.549
8) T	DICHLORPROP	7.050f	7.588	5825738	5880554	2.589	8.043 #
9) T	2,4-D	7.254f	7.864	15396602	1615546	6.213	1.896 #
10) T	Pentachlo...	7.521	8.279	16087711	1845127	<MDL	<MDL #
12) T	2,4,5-T	8.331	9.024	66030987	7469964	5.894	1.977 #
13) T	2,4-DB	8.802	9.516	39824712	2975970	22.378	6.529 #
14) T	DINOSEB	9.851	9.835	1133951	1239025	<MDL	<MDL #
15) T	Picloram	9.690	10.807	11192824	13095399	<MDL	2.628 #
16) T	DCPA	10.128	10.807	71062558	13095399	4.517	2.547 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081023\
Data File : PS024030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 20:12
Operator : AR\AJ
Sample : 03954-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:37:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

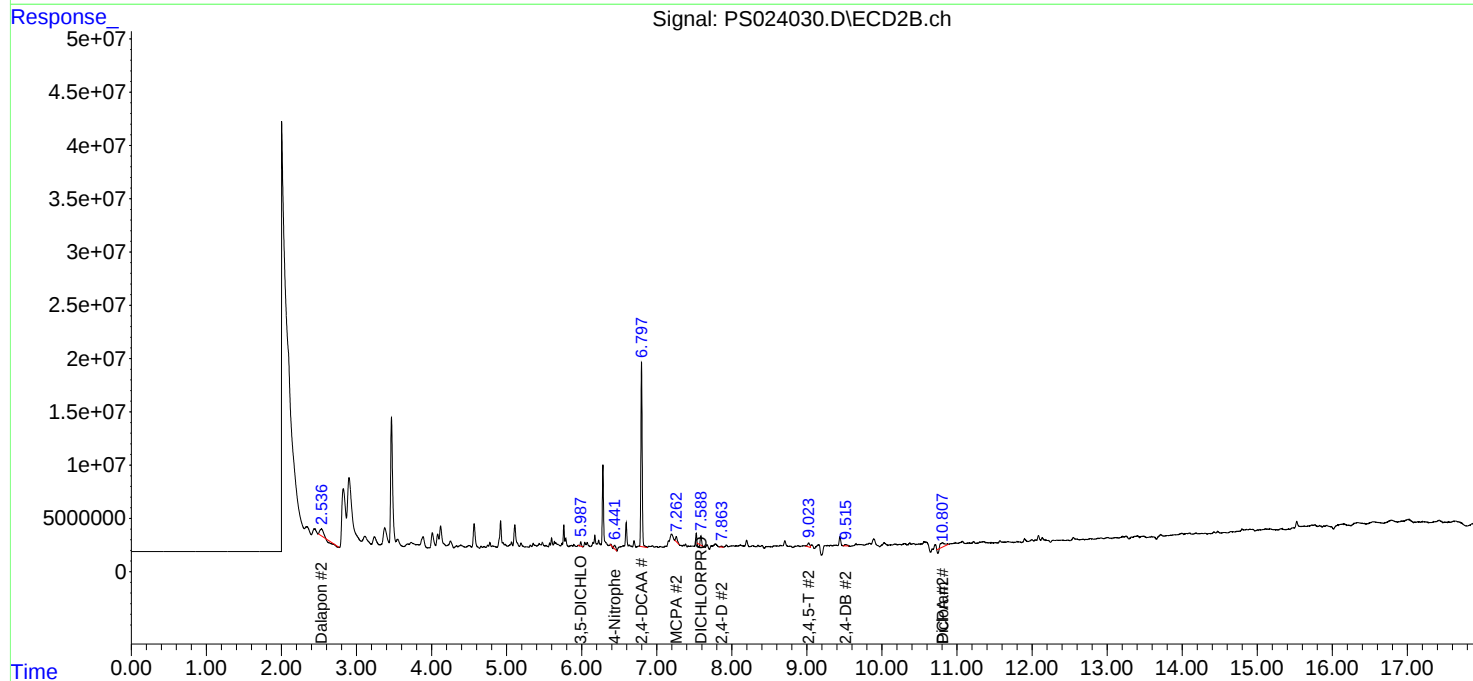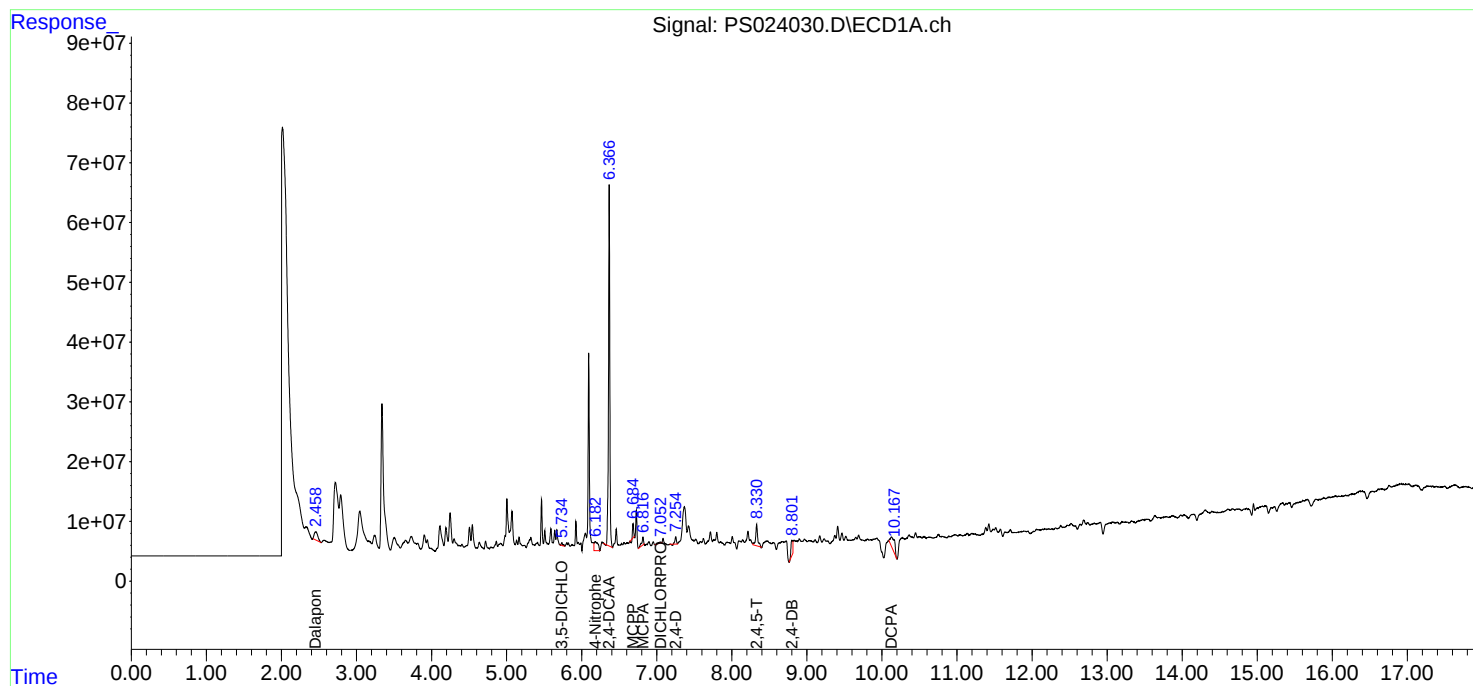


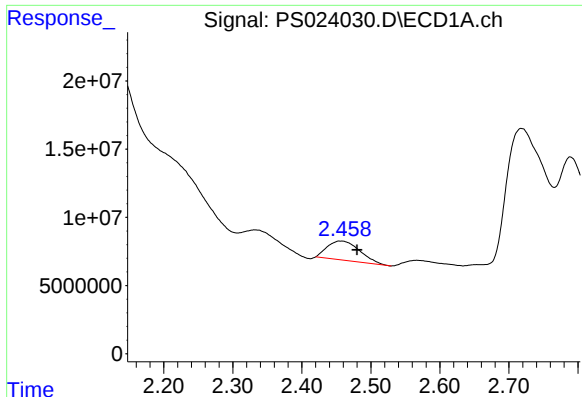

#1 Dalapon


R.T.: 2.457 min
Delta R.T.: -0.023 min
Response: 45247289
Conc: 20.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

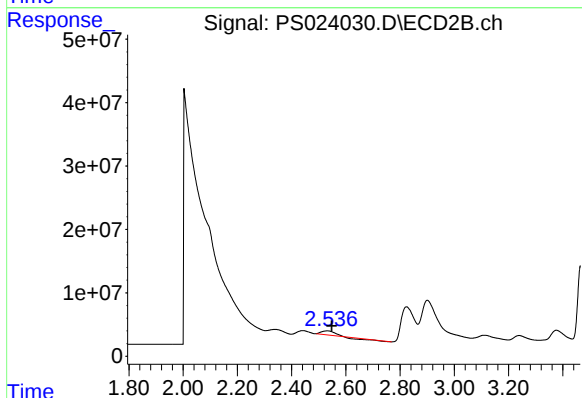


#1 Dalapon

R.T.: 2.531 min
Delta R.T.: -0.016 min
Response: 12680633
Conc: 11.60 ng/ml

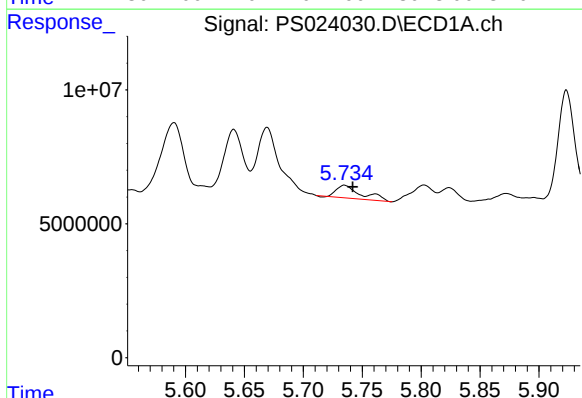


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.735 min
Delta R.T.: -0.007 min
Response: 6869981
Conc: 2.27 ng/ml

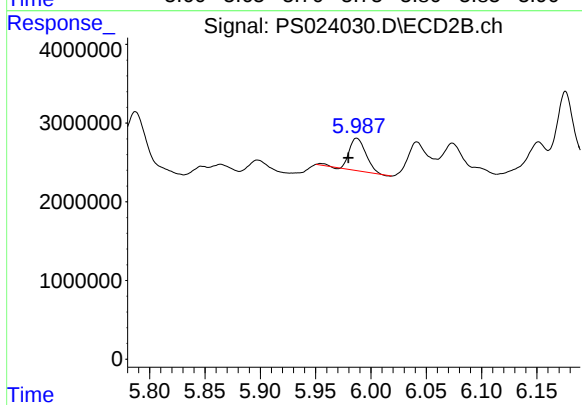

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.987 min
Delta R.T.: 0.008 min
Response: 4384287
Conc: 4.18 ng/ml

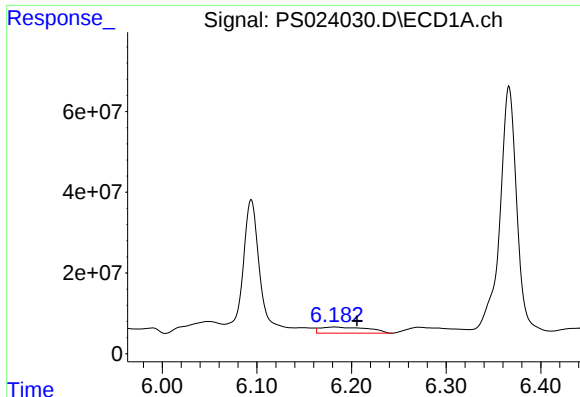

#3 4-Nitrophenol


R.T.: 6.182 min
Delta R.T.: -0.024 min
Response: 53417606
Conc: 48.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

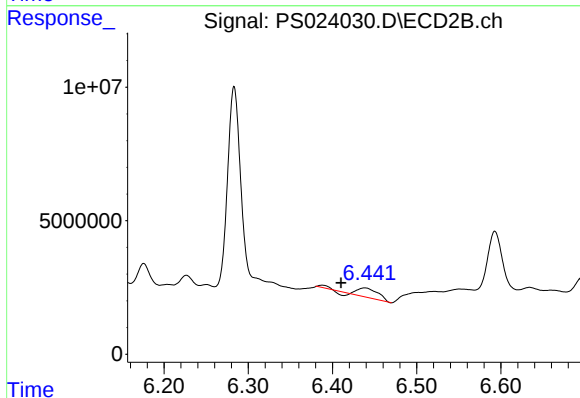


#3 4-Nitrophenol

R.T.: 6.438 min
Delta R.T.: 0.028 min
Response: 5745549
Conc: 14.52 ng/ml

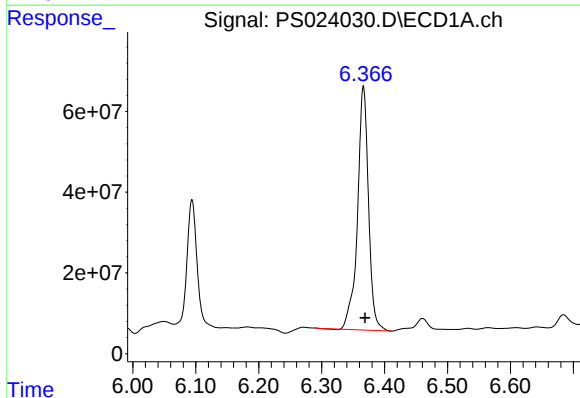


#4 2,4-DCAA

R.T.: 6.367 min
Delta R.T.: -0.003 min
Response: 735789335
Conc: 371.51 ng/ml

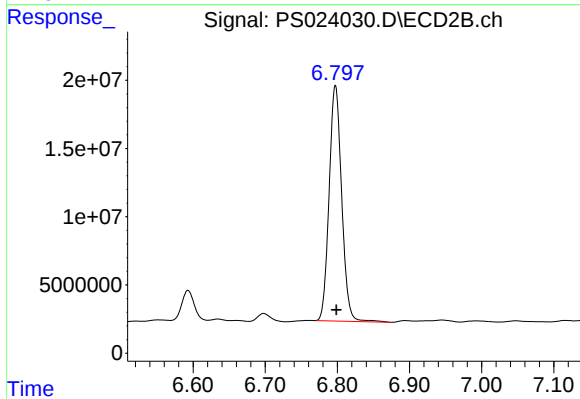

#4 2,4-DCAA


R.T.: 6.797 min
Delta R.T.: -0.001 min
Response: 208580703
Conc: 310.10 ng/ml

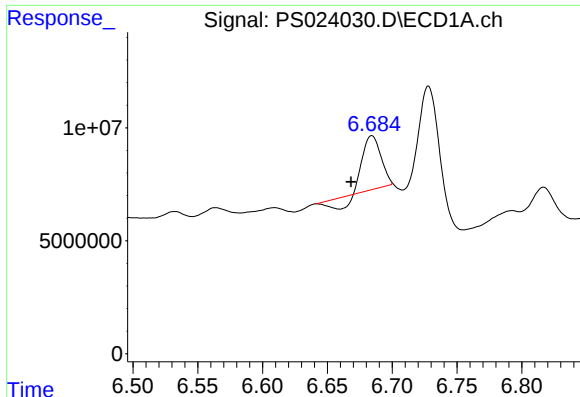

#6 MCPP


R.T.: 6.684 min
Delta R.T.: 0.016 min
Response: 20281457
Conc: 3.25 ug/ml

Instrument :
ECD_S
ClientSampleId :

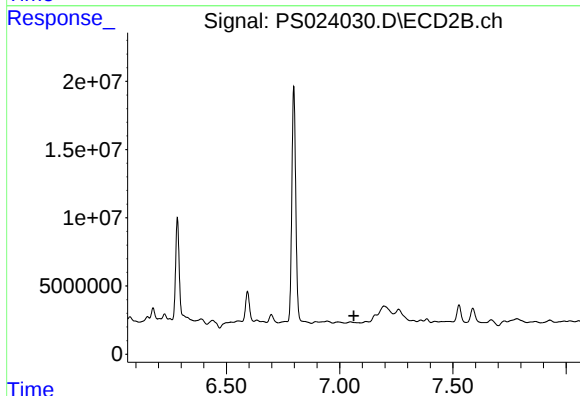


#6 MCPP

R.T.: 7.116 min
Delta R.T.: 0.053 min
Response: -354070
Conc: N.D.

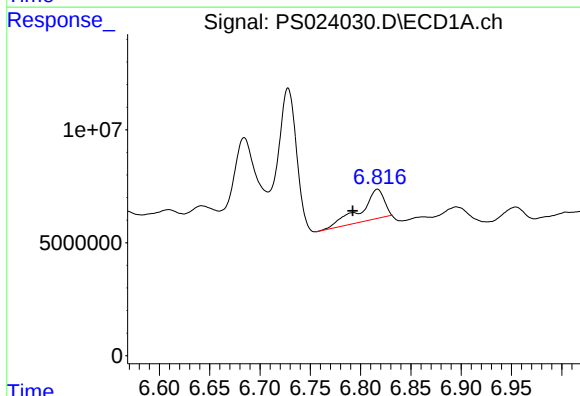


#7 MCPA

R.T.: 6.817 min
Delta R.T.: 0.025 min
Response: 19769188
Conc: 2.35 ug/ml

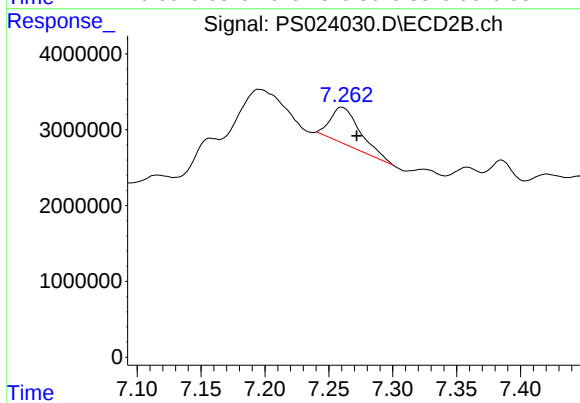

#7 MCPA


R.T.: 7.260 min
Delta R.T.: -0.011 min
Response: 7458380
Conc: 2.55 ug/ml

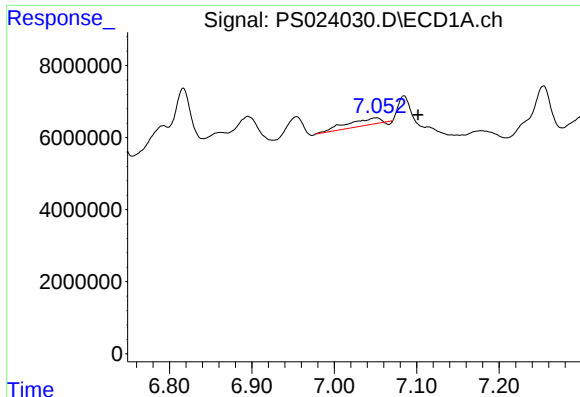

#8 DICHLORPROP


R.T.: 7.050 min
Delta R.T.: -0.052 min
Response: 5825738
Conc: 2.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

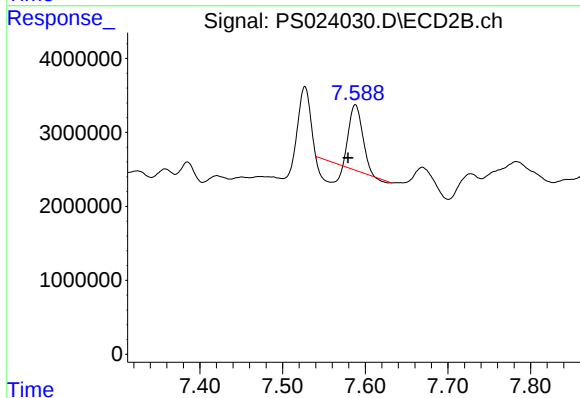


#8 DICHLORPROP

R.T.: 7.588 min
Delta R.T.: 0.009 min
Response: 5880554
Conc: 8.04 ng/ml

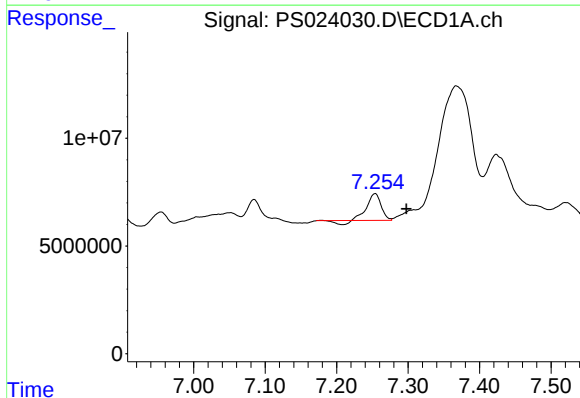


#9 2,4-D

R.T.: 7.254 min
Delta R.T.: -0.044 min
Response: 15396602
Conc: 6.21 ng/ml

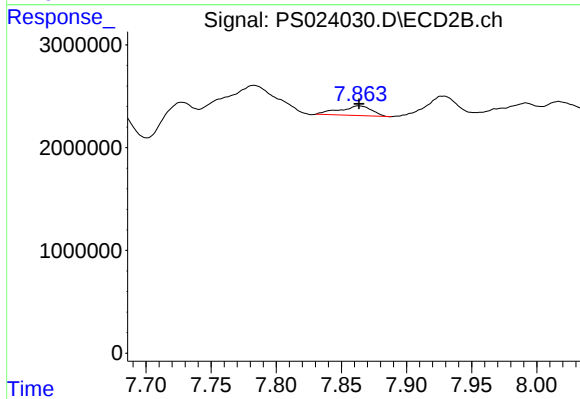

#9 2,4-D


R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 1615546
Conc: 1.90 ng/ml

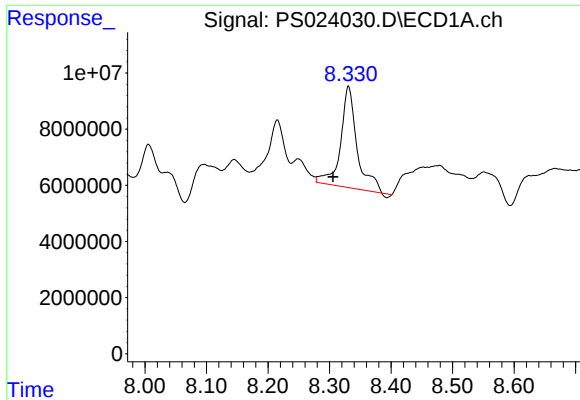

#12 2,4,5-T


R.T.: 8.331 min
Delta R.T.: 0.025 min
Response: 66030987
Conc: 5.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

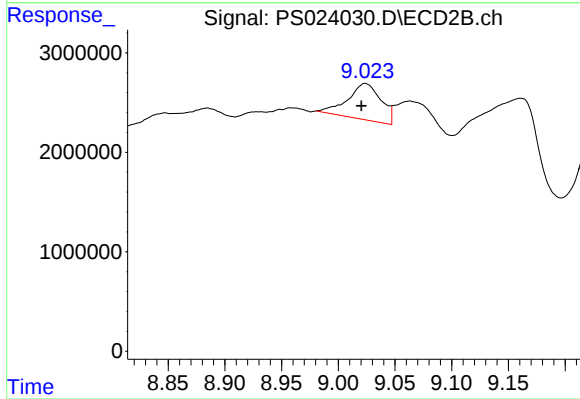


#12 2,4,5-T

R.T.: 9.024 min
Delta R.T.: 0.004 min
Response: 7469964
Conc: 1.98 ng/ml

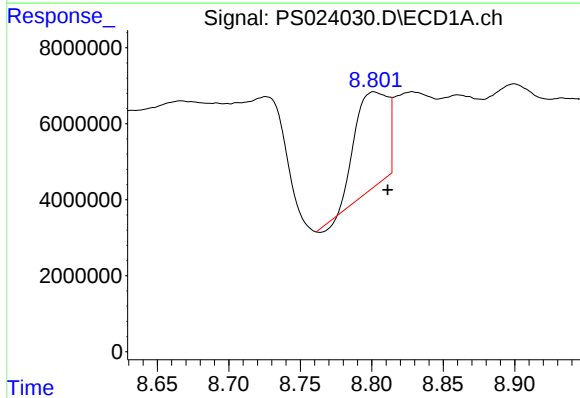


#13 2,4-DB

R.T.: 8.802 min
Delta R.T.: -0.009 min
Response: 39824712
Conc: 22.38 ng/ml

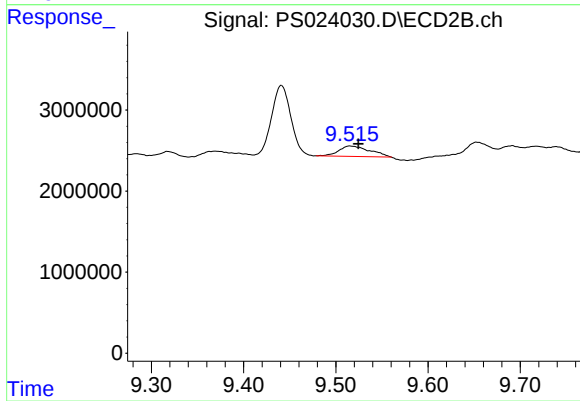

#13 2,4-DB


R.T.: 9.516 min
Delta R.T.: -0.008 min
Response: 2975970
Conc: 6.53 ng/ml

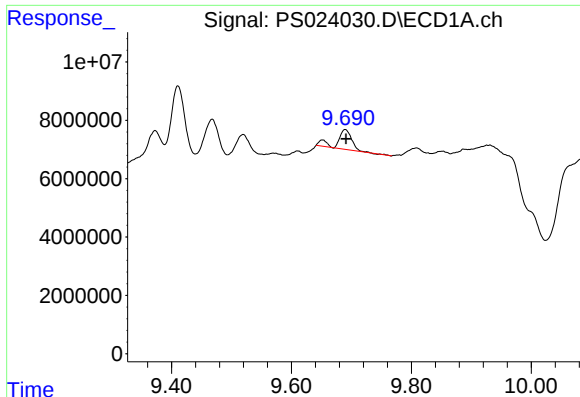

#15 Picloram


R.T.: 9.690 min
Delta R.T.: -0.001 min
Response: 11192824
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

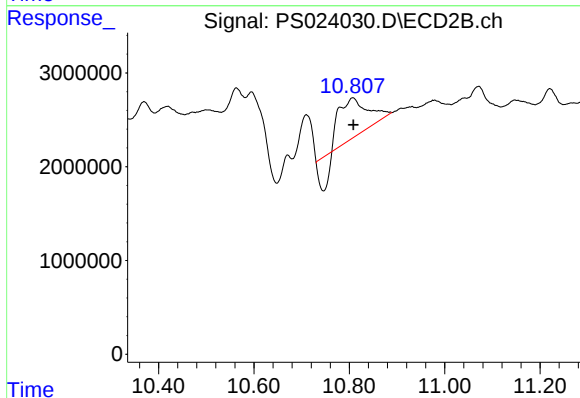


#15 Picloram

R.T.: 10.807 min
Delta R.T.: -0.002 min
Response: 13095399
Conc: 2.63 ng/ml

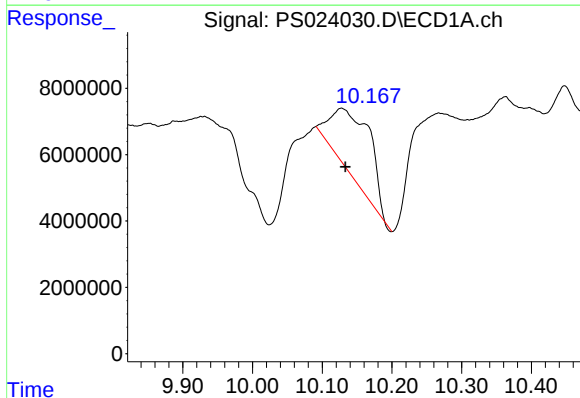

#16 DCPA

R.T.: 10.128 min
Delta R.T.: -0.005 min
Response: 71062558
Conc: 4.52 ng/ml

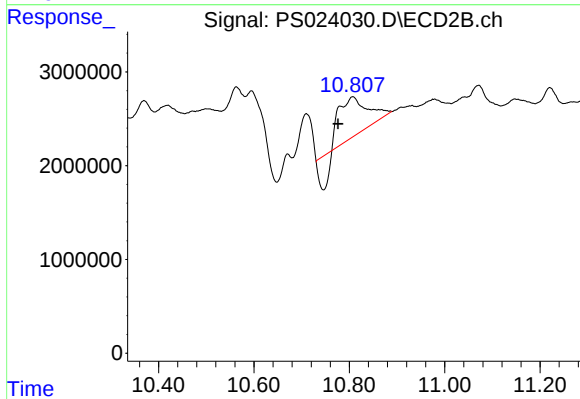

#16 DCPA

R.T.: 10.807 min
Delta R.T.: 0.031 min
Response: 13095399
Conc: 2.55 ng/ml