

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081023\
 Data File : PS024043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 02:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 06:59:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.367	6.797	1073.5E6	364.8E6	542.002	542.413
Target Compounds							
1) T	Dalapon	2.517	2.576	6682955	4803799	3.046	4.393 #
3) T	4-Nitroph...	6.207	6.390	9832643	897005	8.884	2.266 #
5) T	DICAMBA	6.498	7.005f	1595010	2221884	<MDL	<MDL #
6) T	MCP	6.686	7.005f	2400426	2221884	<MDL	1.148 #
7) T	MCPA	6.854f	7.270	1152617	3050386	<MDL	1.043 #
8) T	DICHLORPROP	7.149f	7.589	186323	1530455	<MDL	2.093 #
9) T	2,4-D	7.261	7.804f	4936631	736572	1.992	<MDL #
11) T	2,4,5-TP ...	8.049	8.645	944111	541688	<MDL	<MDL #
12) T	2,4,5-T	8.306	9.061f	1244571	583358	<MDL	<MDL #
13) T	2,4-DB	8.752f	0.000	803932	0	<MDL	N.D. #
14) T	DINOSEB	9.860	0.000	785612	0	<MDL	N.D. #
15) T	Picloram	9.666	10.807	13478895	6221843	1.042	1.249
16) T	DCPA	0.000	10.807	0	6221843	N.D.	1.210



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081023\
Data File : PS024043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 02:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 06:59:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

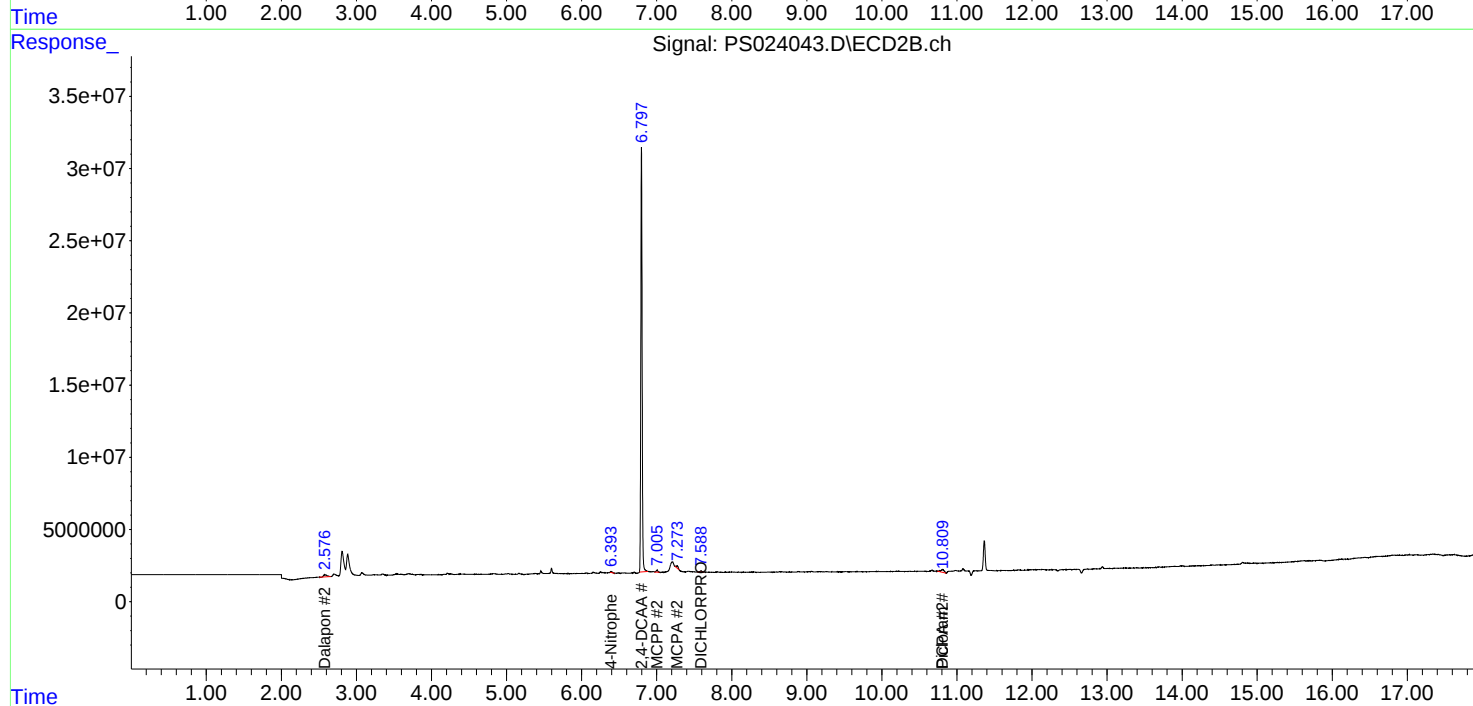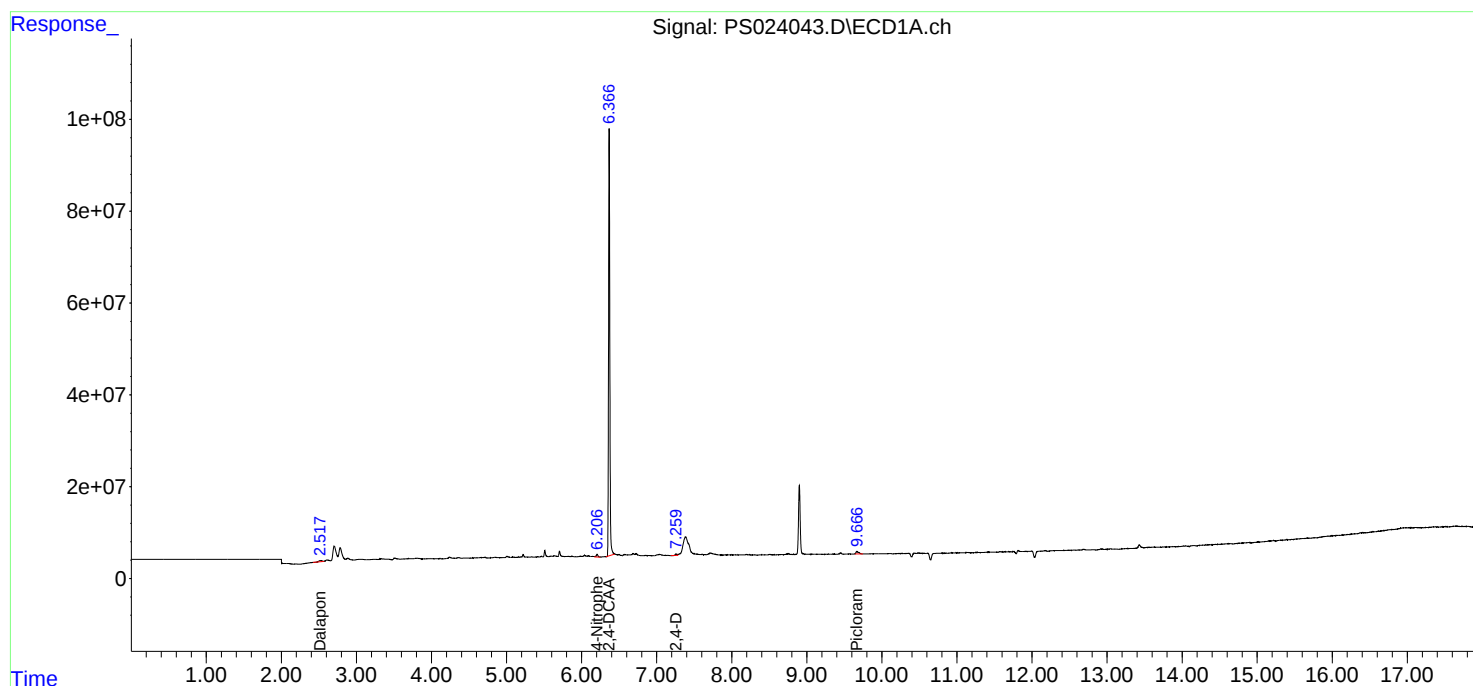


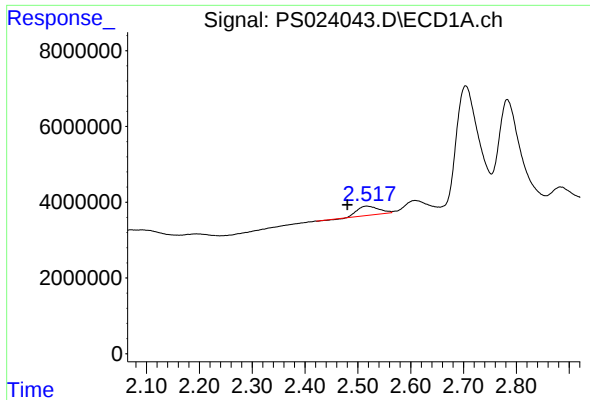

#1 Dalapon


R.T.: 2.517 min
Delta R.T.: 0.037 min
Response: 6682955
Conc: 3.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

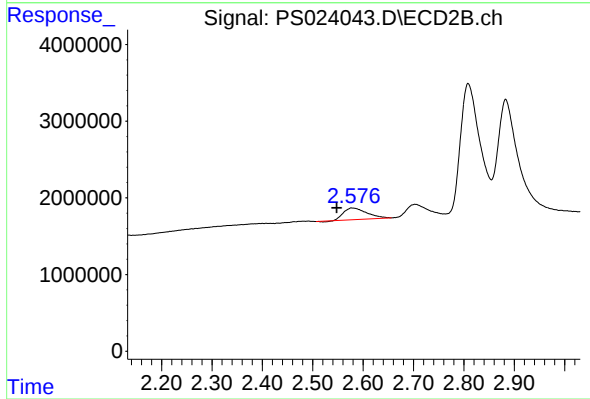


#1 Dalapon

R.T.: 2.576 min
Delta R.T.: 0.029 min
Response: 4803799
Conc: 4.39 ng/ml

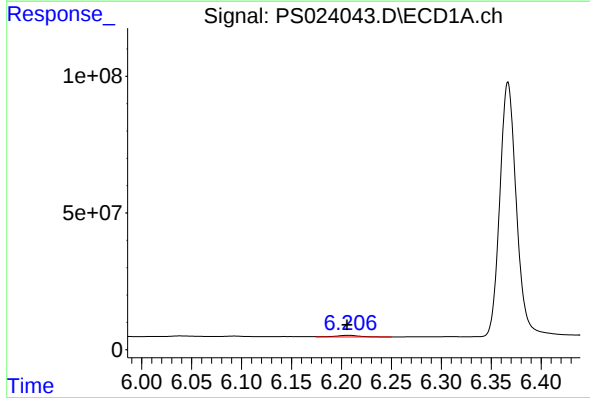


#3 4-Nitrophenol

R.T.: 6.207 min
Delta R.T.: 0.001 min
Response: 9832643
Conc: 8.88 ng/ml

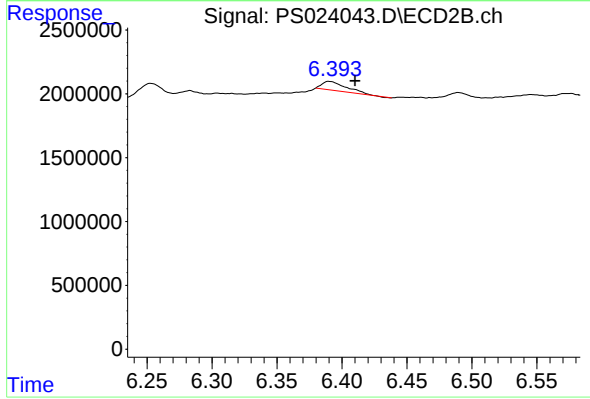

#3 4-Nitrophenol


R.T.: 6.390 min
Delta R.T.: -0.020 min
Response: 897005
Conc: 2.27 ng/ml

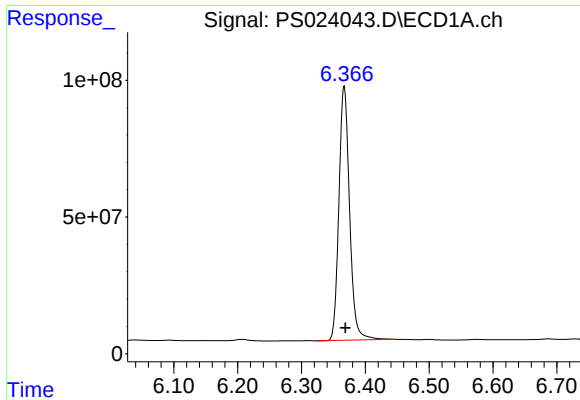

#4 2,4-DCAA


R.T.: 6.367 min
Delta R.T.: -0.002 min
Response: 1073469455
Conc: 542.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

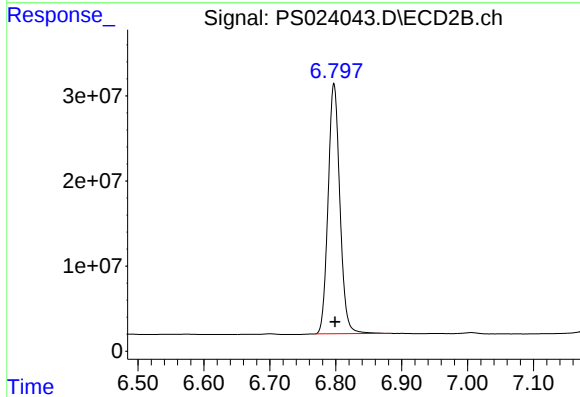


#4 2,4-DCAA

R.T.: 6.797 min
Delta R.T.: -0.001 min
Response: 364841922
Conc: 542.41 ng/ml

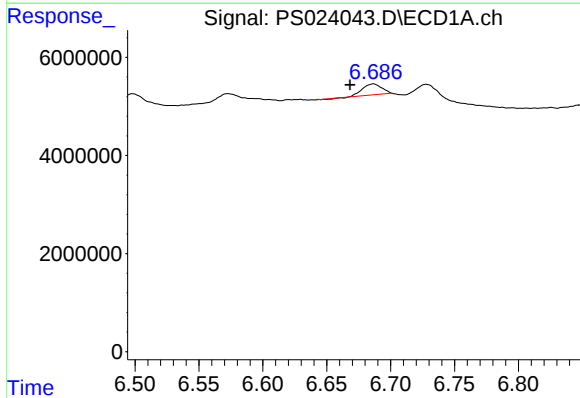


#6 MCP

R.T.: 6.686 min
Delta R.T.: 0.018 min
Response: 2400426
Conc: N.D.

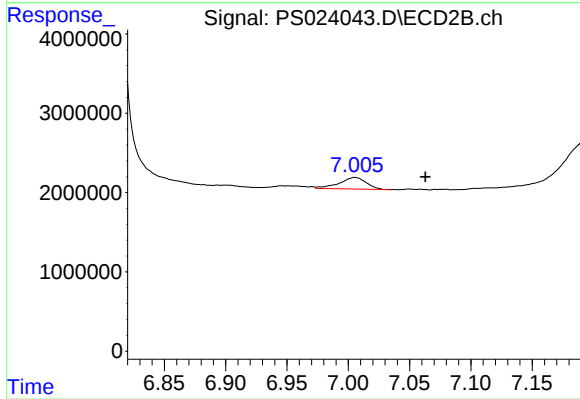

#6 MCP


R.T.: 7.005 min
Delta R.T.: -0.058 min
Response: 2221884
Conc: 1.15 ug/ml

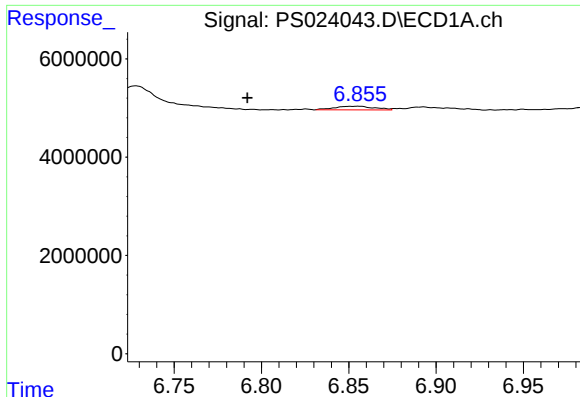

#7 MCPA


R.T.: 6.854 min
Delta R.T.: 0.062 min
Response: 1152617
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

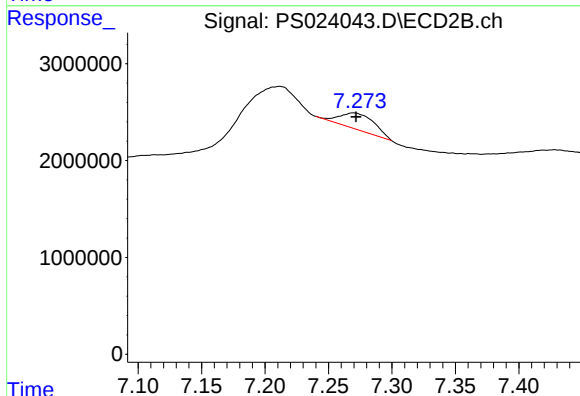


#7 MCPA

R.T.: 7.270 min
Delta R.T.: -0.002 min
Response: 3050386
Conc: 1.04 ug/ml

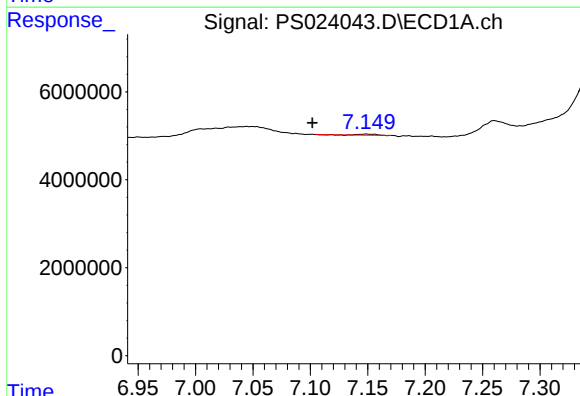


#8 DICHLORPROP

R.T.: 7.149 min
Delta R.T.: 0.047 min
Response: 186323
Conc: N.D.

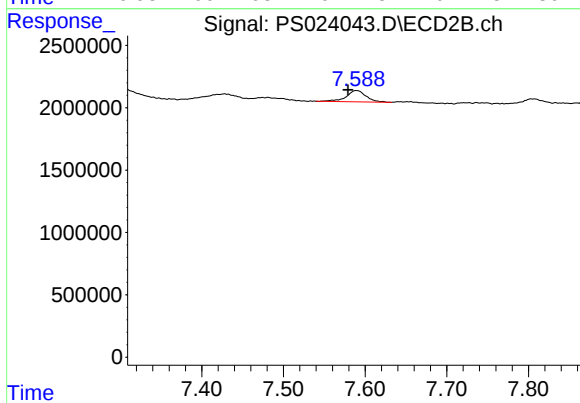

#8 DICHLORPROP


R.T.: 7.589 min
Delta R.T.: 0.010 min
Response: 1530455
Conc: 2.09 ng/ml

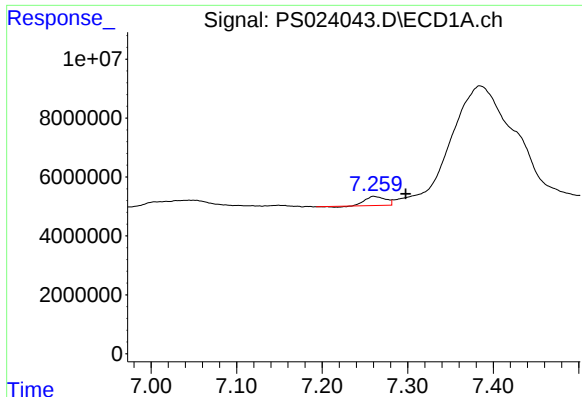

#9 2,4-D


R.T.: 7.261 min
Delta R.T.: -0.037 min
Response: 4936631
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

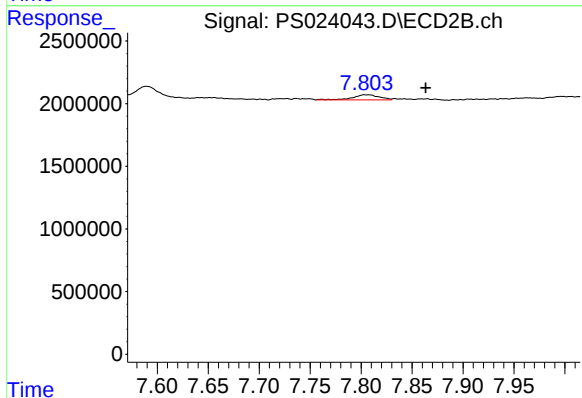


#9 2,4-D

R.T.: 7.804 min
Delta R.T.: -0.060 min
Response: 736572
Conc: N.D.

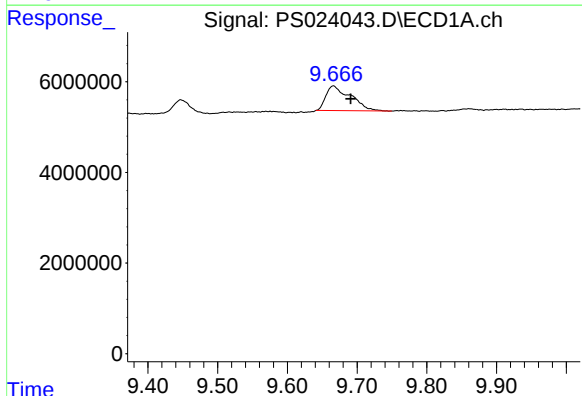


#15 Picloram

R.T.: 9.666 min
Delta R.T.: -0.025 min
Response: 13478895
Conc: 1.04 ng/ml

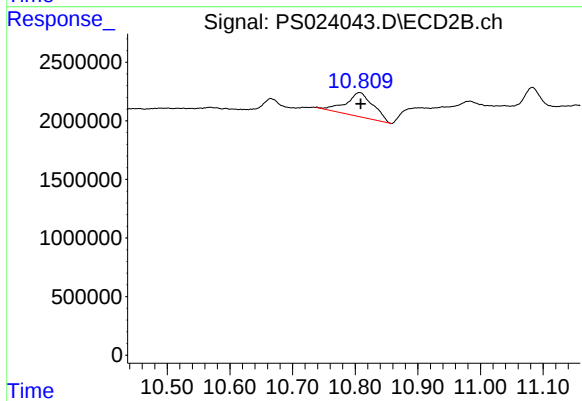

#15 Picloram


R.T.: 10.807 min
Delta R.T.: -0.002 min
Response: 6221843
Conc: 1.25 ng/ml

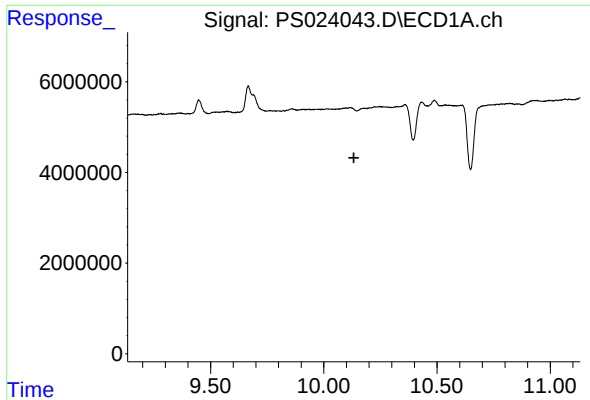

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

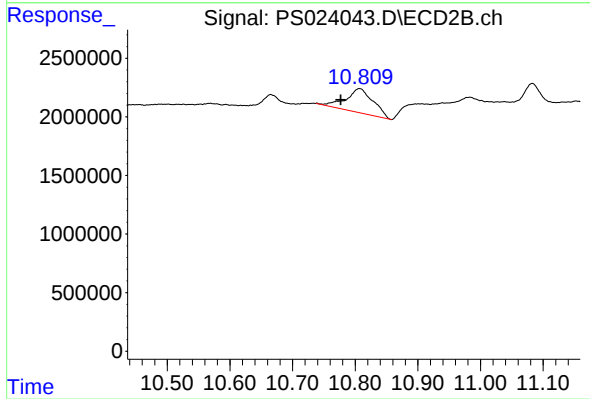

#16 DCPA

R.T.: 10.807 min
Delta R.T.: 0.030 min
Response: 6221843
Conc: 1.21 ng/ml