

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081120\
 Data File : PS011711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2020 14:20
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 15:38:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:09:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	819.6E6	401.0E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.035	2.623	851.2E6	516.3E6	682.500	682.500
2) T	3,5-DICHL...	6.434	6.066	1005.8E6	567.5E6	697.500	697.500
3) T	4-Nitroph...	7.050	6.522	386.1E6	238.4E6	682.500	682.500
5) T	DICAMBA	7.410	7.083	2916.3E6	1531.8E6	705.000	705.000
6) T	MCPD	7.580	7.180	229.3E6	125.6E6	70.500	70.500
7) T	MCPA	7.729	7.396	321.9E6	190.2E6	69.750	69.750
8) T	DICHLORPROP	8.102	7.709	711.9E6	398.4E6	705.000	705.000
9) T	2,4-D	8.332	8.003	798.3E6	517.8E6	705.000	705.000
10) T	Pentachlo...	8.642	8.433	10344.4E6	4819.5E6	712.500	712.500
11) T	2,4,5-TP ...	9.191	8.793	4198.6E6	2108.9E6	712.500	712.500
12) T	2,4,5-T	9.476	9.173	4264.7E6	2142.7E6	712.500	712.500
13) T	2,4-DB	10.029	9.679	573.9E6	298.5E6	712.500	712.500
14) T	DINOSEB	11.188	10.011	3395.3E6	1523.9E6	705.000	705.000
15) T	Picloram	11.011	10.996	5721.4E6	3299.6E6	712.500	712.500
16) T	DCPA	11.454	10.939	5563.4E6	2671.8E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081120\
Data File : PS011711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2020 14:20
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 15:38:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:09:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

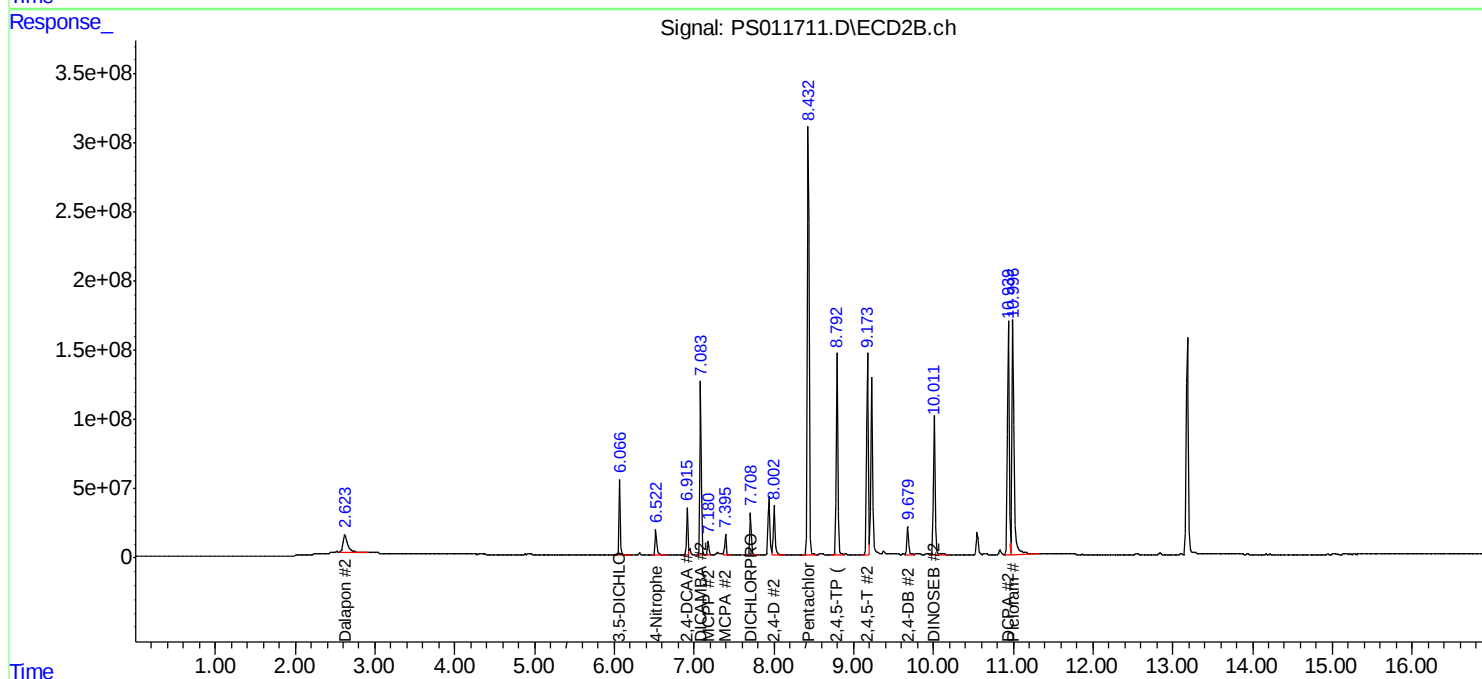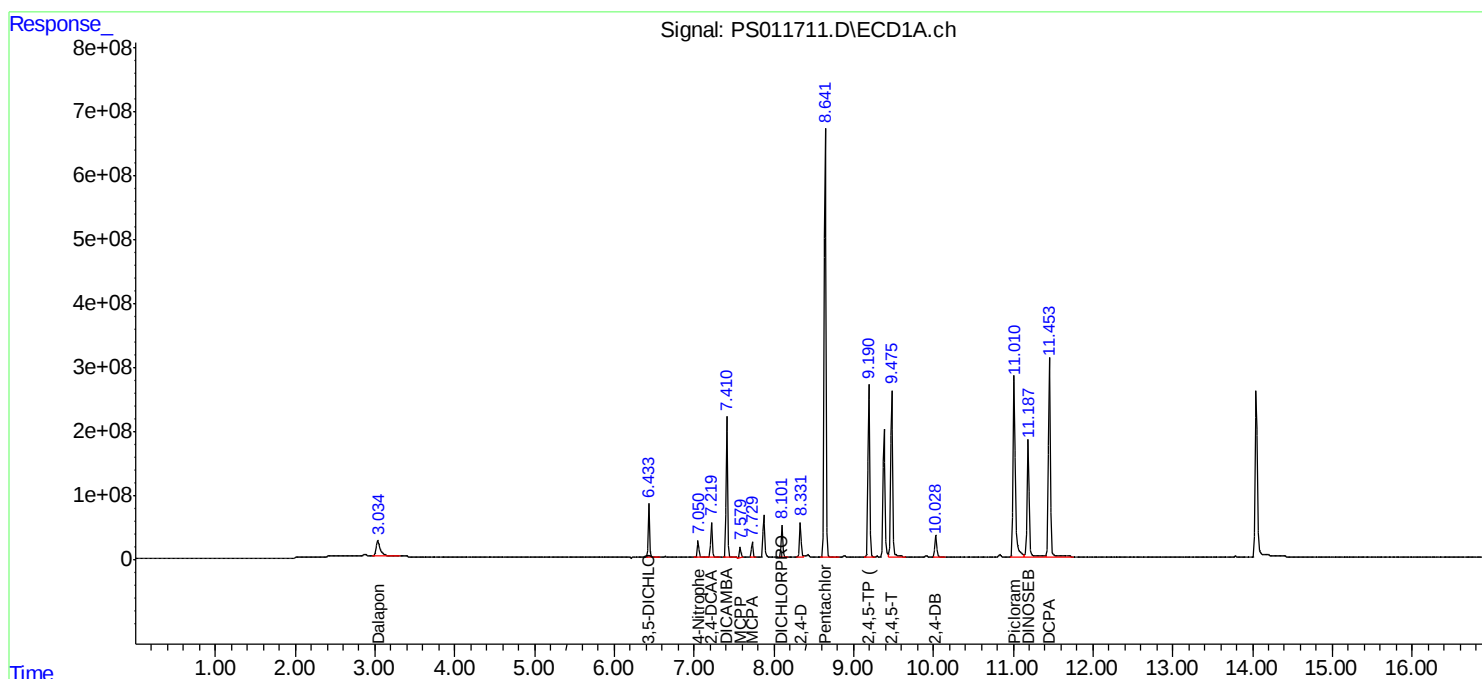


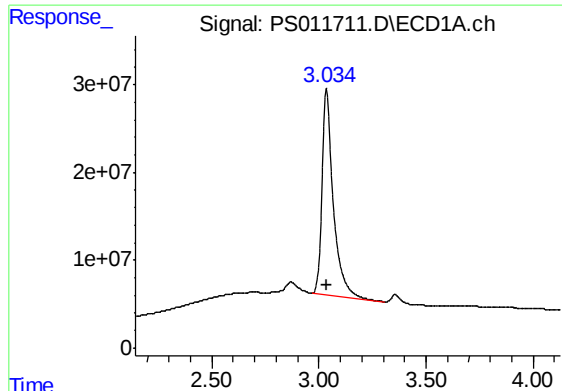

#1 Dalapon


R.T.: 3.035 min
Delta R.T.: 0.000 min
Response: 851247676
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

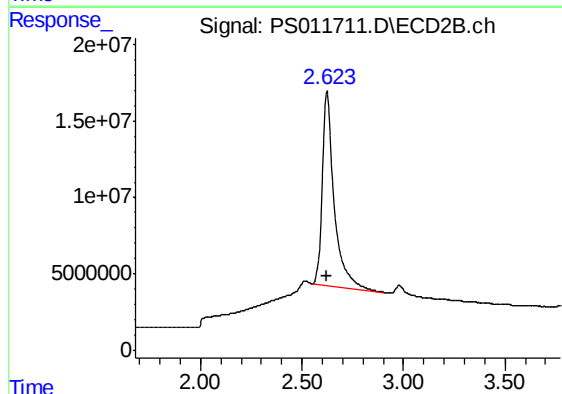


#1 Dalapon

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 516340222
Conc: 682.50 ng/ml

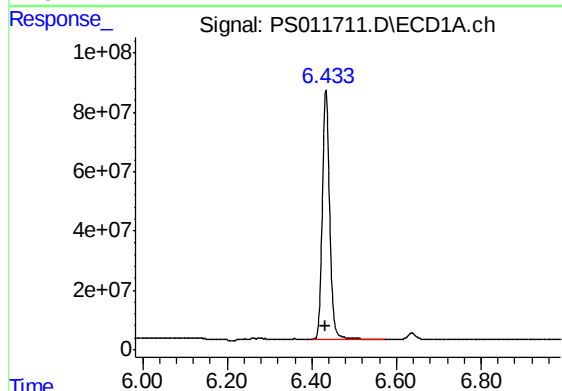


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 1005825060
Conc: 697.50 ng/ml

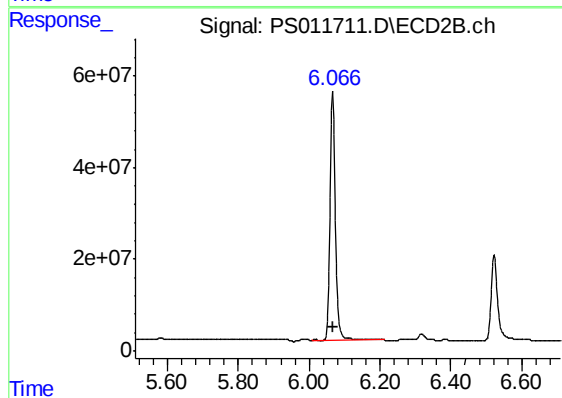

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 567456334
Conc: 697.50 ng/ml

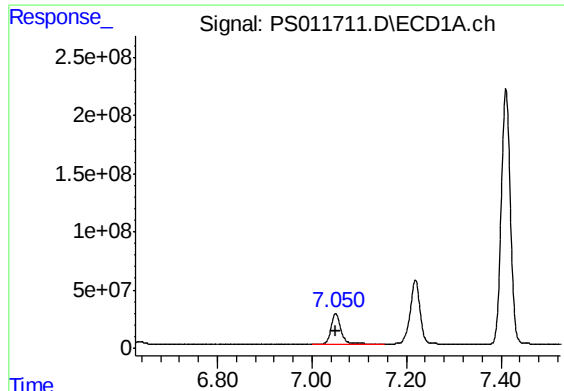

#3 4-Nitrophenol


R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 386109957
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

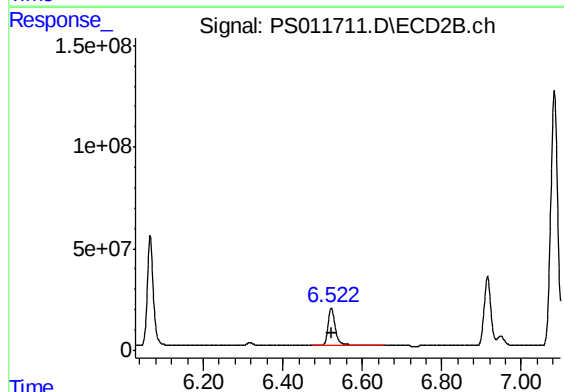


#3 4-Nitrophenol

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 238395575
Conc: 682.50 ng/ml

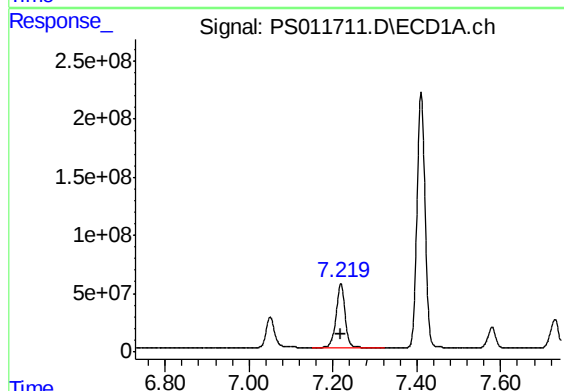


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 819594023
Conc: 750.00 ng/ml

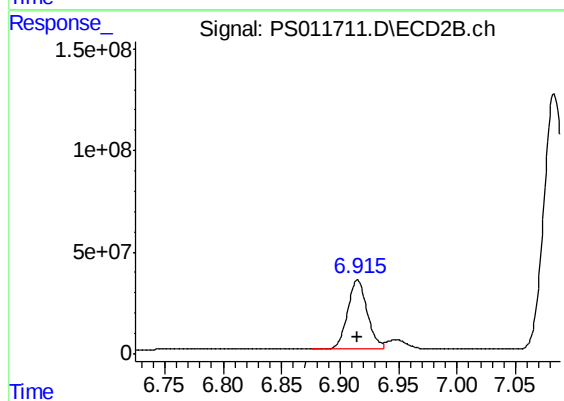

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 401045467
Conc: 750.00 ng/ml

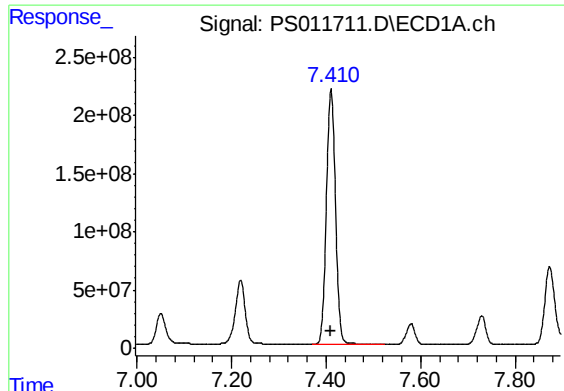

#5 DICAMBA


R.T.: 7.410 min
Delta R.T.: 0.000 min
Response: 2916271389
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

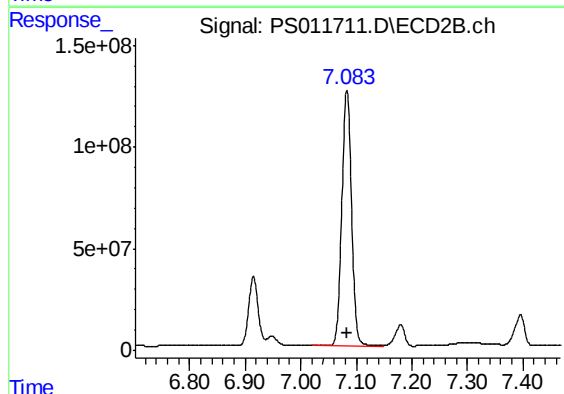


#5 DICAMBA

R.T.: 7.083 min
Delta R.T.: 0.000 min
Response: 1531778062
Conc: 705.00 ng/ml

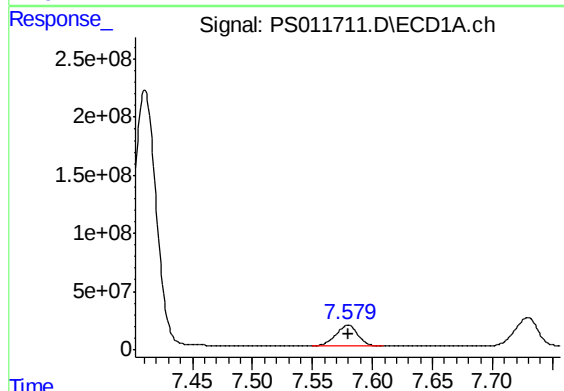


#6 MCPP

R.T.: 7.580 min
Delta R.T.: 0.000 min
Response: 229259474
Conc: 70.50 ug/ml

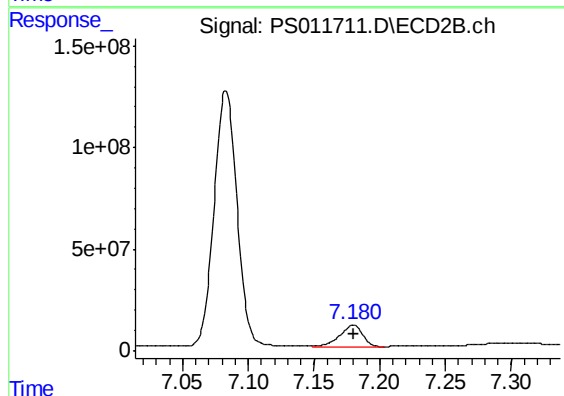

#6 MCPP


R.T.: 7.180 min
Delta R.T.: 0.000 min
Response: 125592712
Conc: 70.50 ug/ml

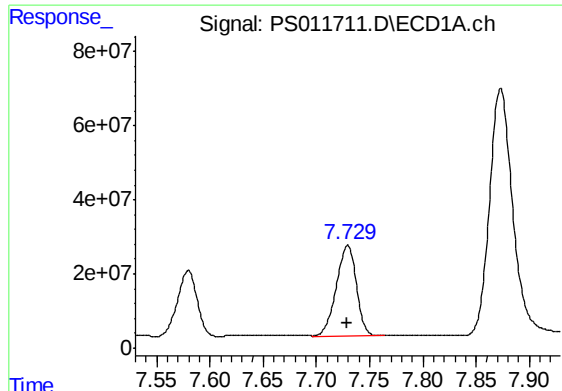

#7 MCPA


R.T.: 7.729 min
Delta R.T.: 0.000 min
Response: 321871967
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

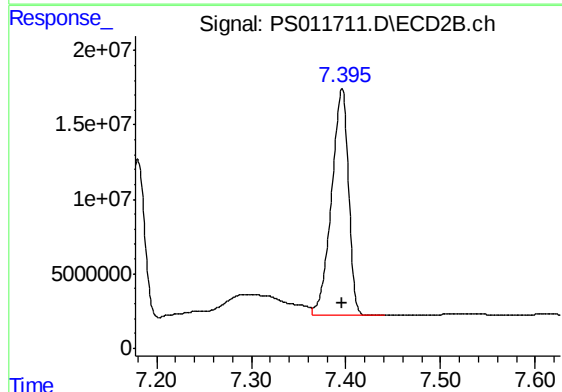


#7 MCPA

R.T.: 7.396 min
Delta R.T.: 0.000 min
Response: 190174359
Conc: 69.75 ug/ml

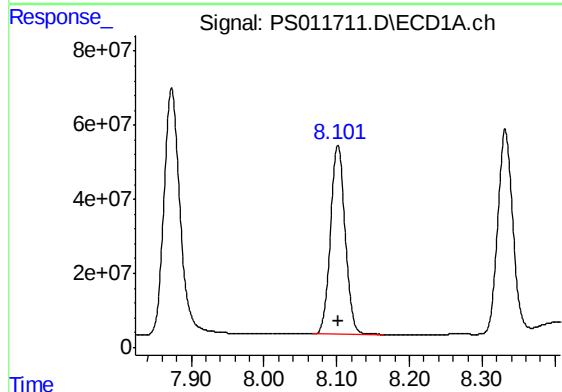


#8 DICHLORPROP

R.T.: 8.102 min
Delta R.T.: 0.000 min
Response: 711864374
Conc: 705.00 ng/ml

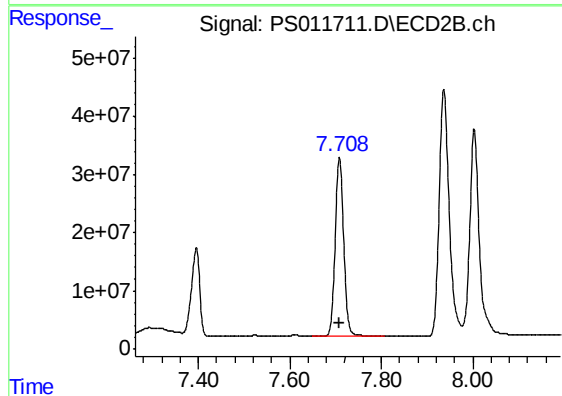

#8 DICHLORPROP


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 398415243
Conc: 705.00 ng/ml

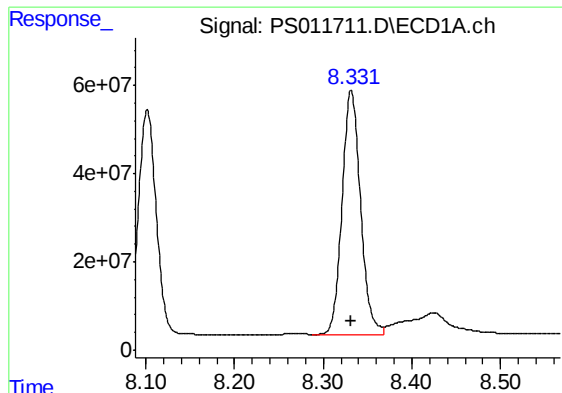

#9 2,4-D


R.T.: 8.332 min
Delta R.T.: 0.000 min
Response: 798258120
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

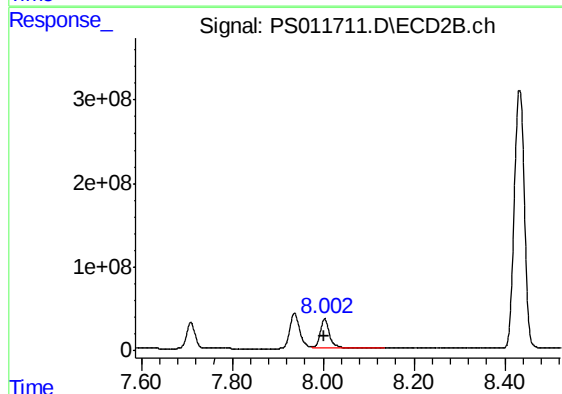


#9 2,4-D

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 517841818
Conc: 705.00 ng/ml

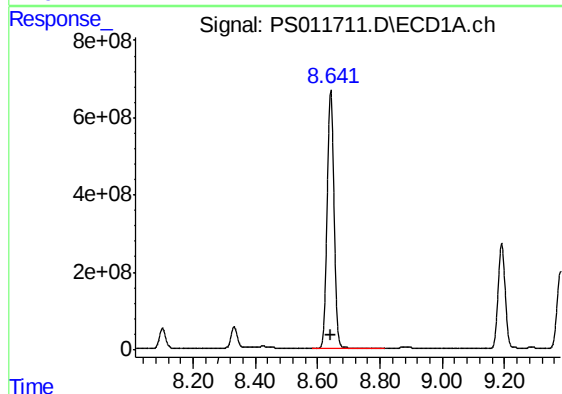


#10 Pentachlorophenol

R.T.: 8.642 min
Delta R.T.: 0.000 min
Response: 10344429883
Conc: 712.50 ng/ml

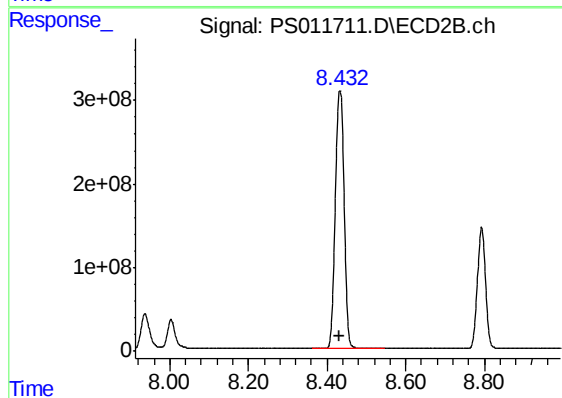

#10 Pentachlorophenol


R.T.: 8.433 min
Delta R.T.: 0.000 min
Response: 4819505836
Conc: 712.50 ng/ml

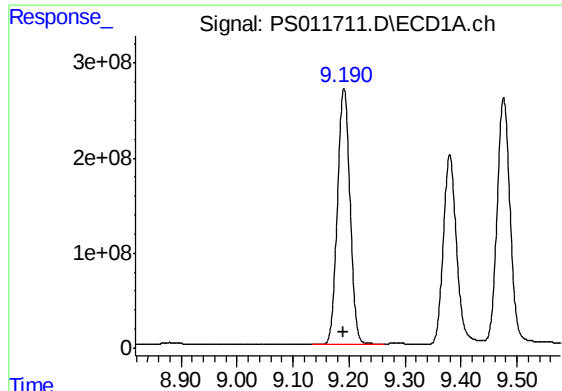

#11 2,4,5-TP (SILVEX)


R.T.: 9.191 min
Delta R.T.: 0.000 min
Response: 4198614840
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

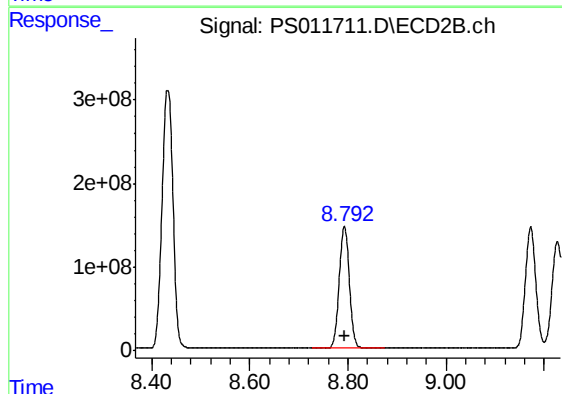


#11 2,4,5-TP (SILVEX)

R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 2108898443
Conc: 712.50 ng/ml

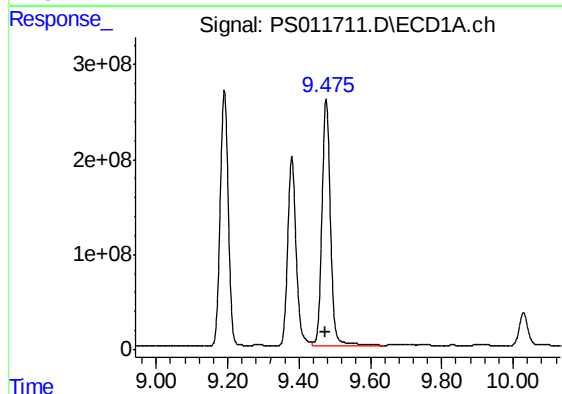


#12 2,4,5-T

R.T.: 9.476 min
Delta R.T.: 0.000 min
Response: 4264652717
Conc: 712.50 ng/ml

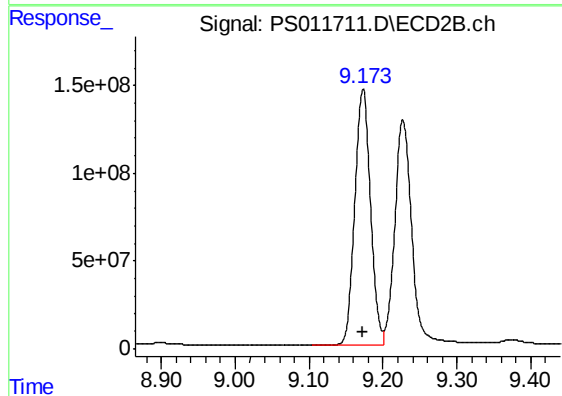

#12 2,4,5-T


R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 2142747621
Conc: 712.50 ng/ml

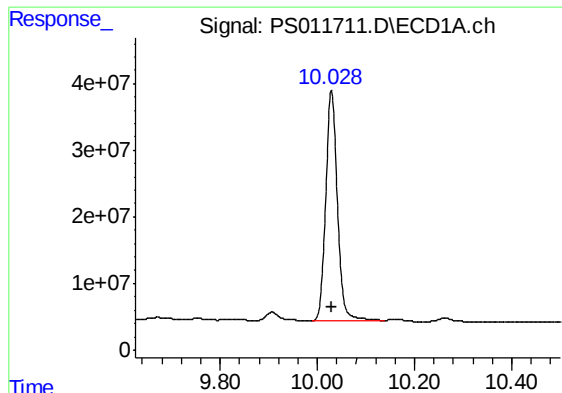

#13 2,4-DB


R.T.: 10.029 min
Delta R.T.: 0.000 min
Response: 573879657
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

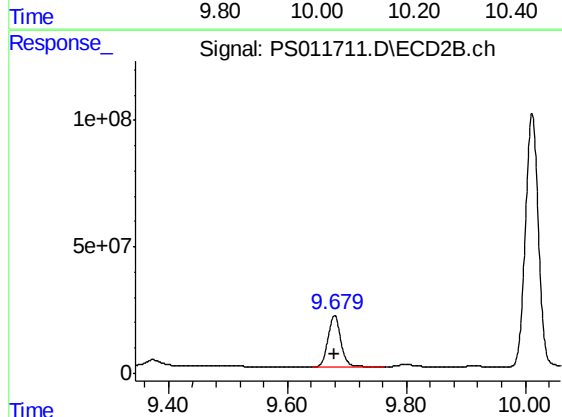


#13 2,4-DB

R.T.: 9.679 min
Delta R.T.: 0.000 min
Response: 298482488
Conc: 712.50 ng/ml

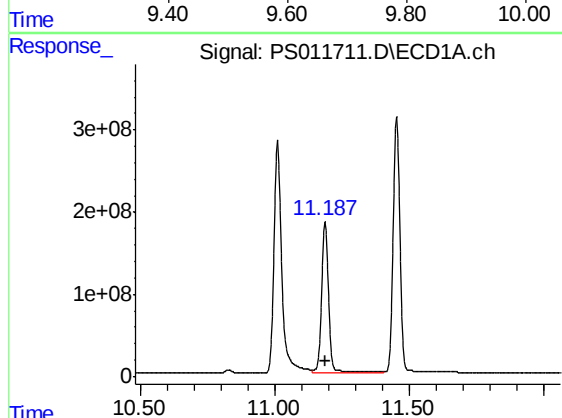


#14 DINOSEB

R.T.: 11.188 min
Delta R.T.: 0.000 min
Response: 3395340928
Conc: 705.00 ng/ml

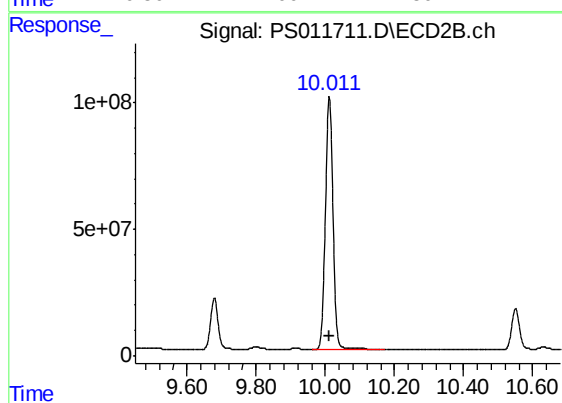

#14 DINOSEB


R.T.: 10.011 min
Delta R.T.: 0.000 min
Response: 1523899838
Conc: 705.00 ng/ml

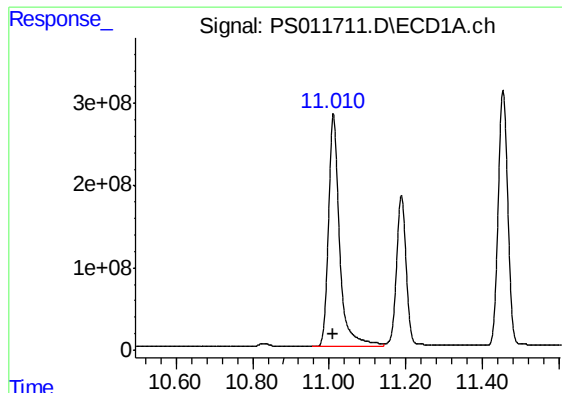

#15 Picloram


R.T.: 11.011 min
Delta R.T.: 0.000 min
Response: 5721446383
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

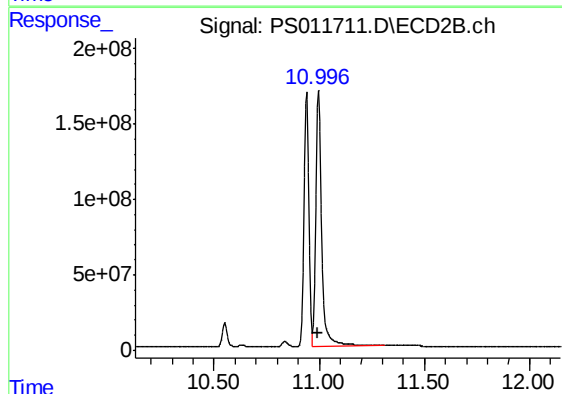


#15 Picloram

R.T.: 10.996 min
Delta R.T.: 0.000 min
Response: 3299576551
Conc: 712.50 ng/ml

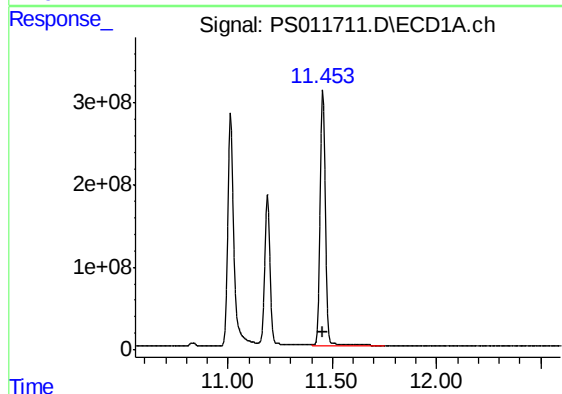

#16 DCPA

R.T.: 11.454 min
Delta R.T.: 0.000 min
Response: 5563365595
Conc: 720.00 ng/ml

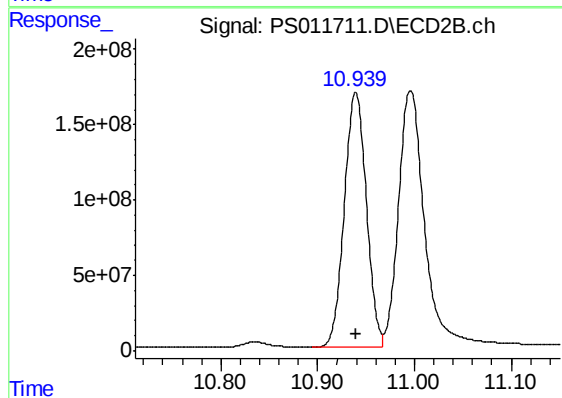

#16 DCPA

R.T.: 10.939 min
Delta R.T.: 0.000 min
Response: 2671848370
Conc: 720.00 ng/ml