

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081120\
 Data File : PS011715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2020 15:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 16:12:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.221	6.917	416.4E6	242.2E6	381.718	452.820
Target Compounds							
9) T	2,4-D	8.402	0.000	145.7E6	0	129.042	N.D. #
10) T	Pentachlo...	8.644	8.436	11056393	7119857	<MDL	1.048 #
15) T	Picloram	11.044	11.028	33550765	25075139	4.293	5.532 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081120\
Data File : PS011715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2020 15:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 16:12:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

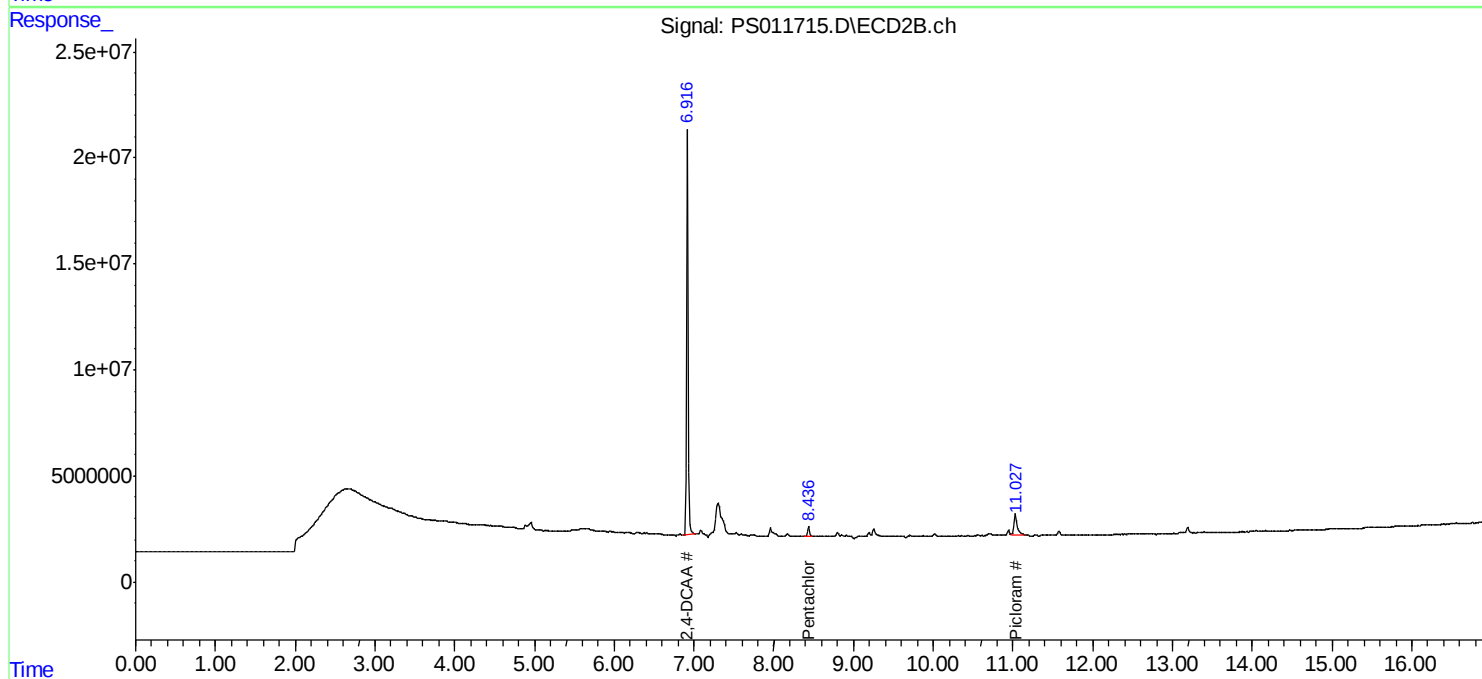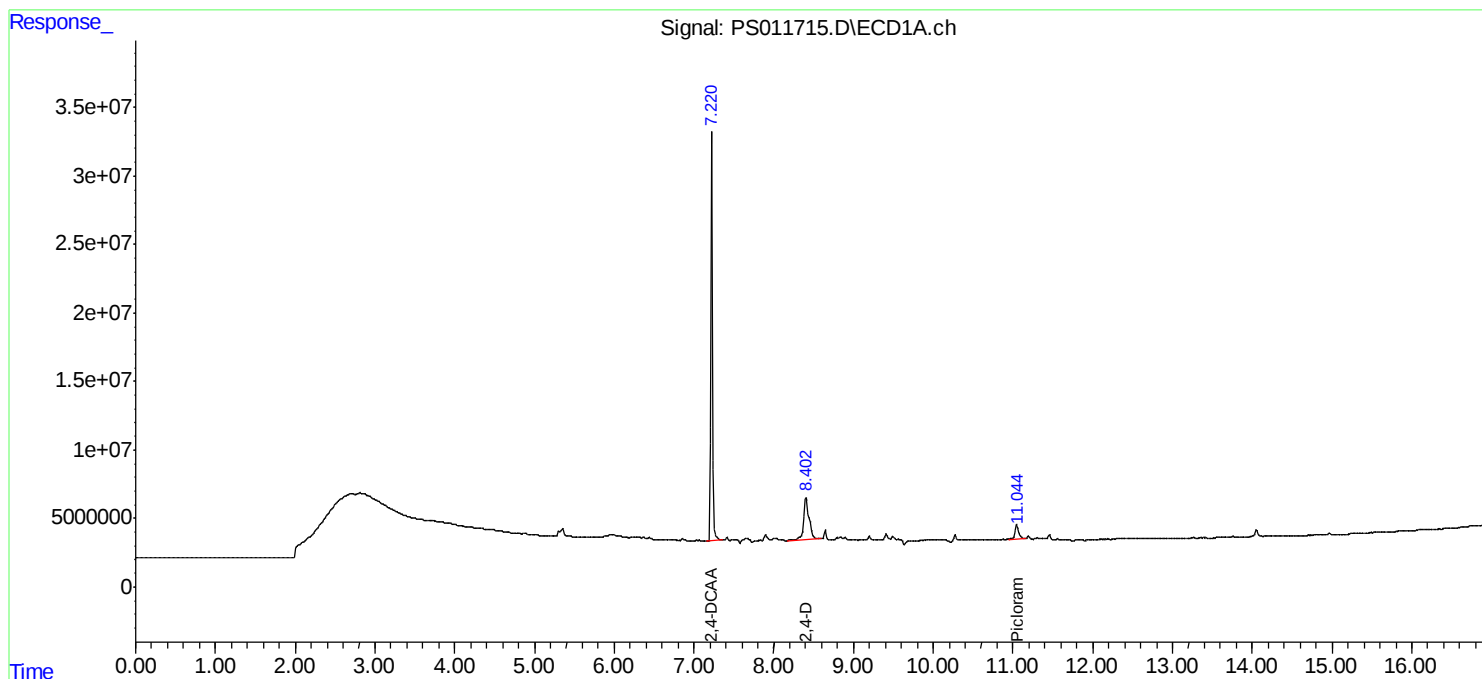


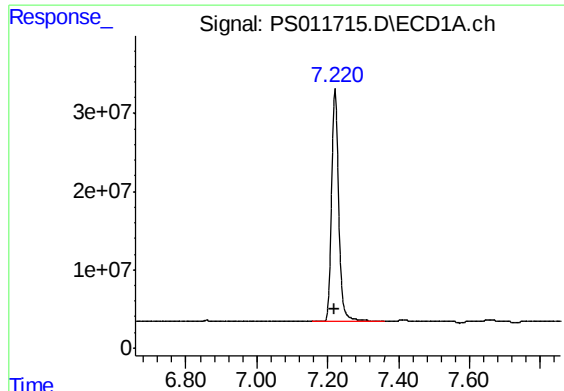

#4 2,4-DCAA


R.T.: 7.221 min
Delta R.T.: 0.000 min
Response: 416365963
Conc: 381.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

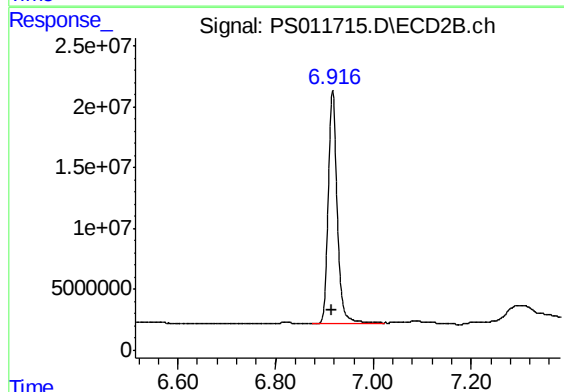


#4 2,4-DCAA

R.T.: 6.917 min
Delta R.T.: 0.001 min
Response: 242162294
Conc: 452.82 ng/ml

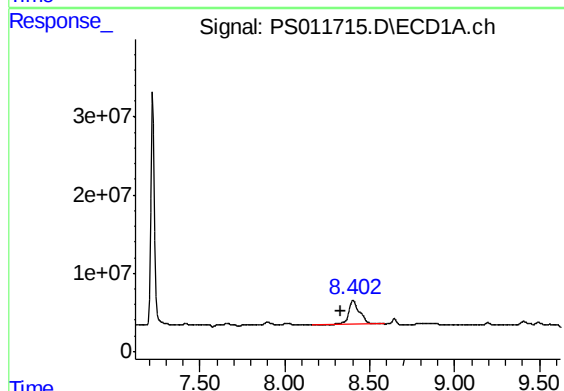


#9 2,4-D

R.T.: 8.402 min
Delta R.T.: 0.070 min
Response: 145700088
Conc: 129.04 ng/ml

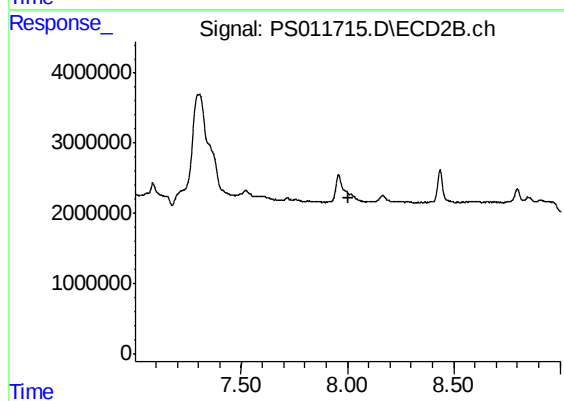

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

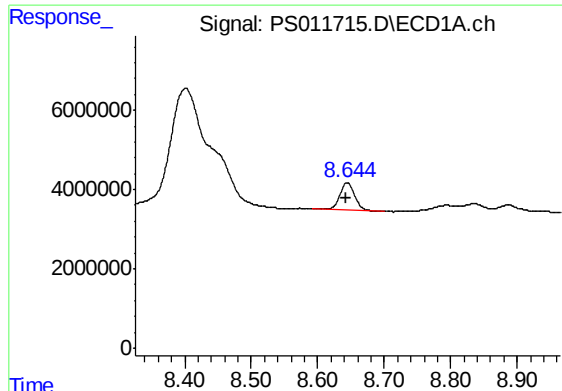

#10 Pentachlorophenol


R.T.: 8.644 min
Delta R.T.: 0.001 min
Response: 11056393
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

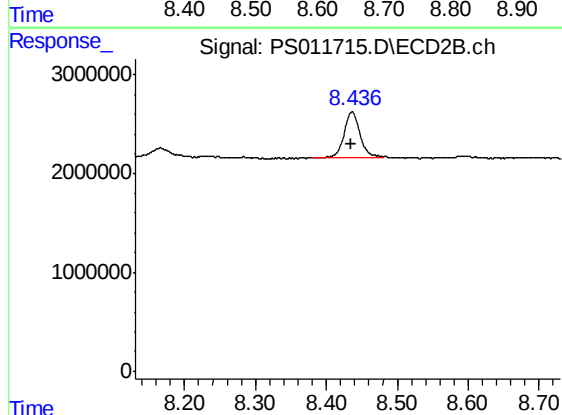


#10 Pentachlorophenol

R.T.: 8.436 min
Delta R.T.: 0.002 min
Response: 7119857
Conc: 1.05 ng/ml

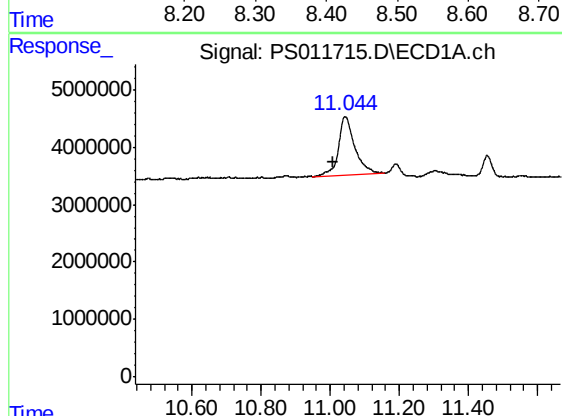

#15 Picloram

R.T.: 11.044 min
Delta R.T.: 0.034 min
Response: 33550765
Conc: 4.29 ng/ml

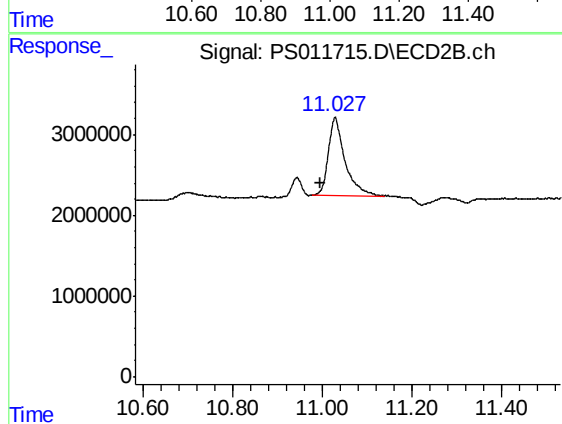

#15 Picloram

R.T.: 11.028 min
Delta R.T.: 0.032 min
Response: 25075139
Conc: 5.53 ng/ml