

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081121\
 Data File : PS016351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2021 11:15
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 05:13:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
1) T	Dalapon	0.000	2.526	0	17694878	N.D.	25.400
5) T	DICAMBA	0.000	6.926	0	3904393	N.D.	1.792
6) T	MCPD	0.000	7.064	0	1716935	N.D.	<MDL
8) T	DICHLORPROP	8.078	0.000	37977586	0	28.220	N.D. #
10) T	Pentachlo...	8.608	8.263	10329259	4588253	<MDL	<MDL #
11) T	2,4,5-TP ...	9.159	8.625	8772761	4418895	1.213	1.514
12) T	2,4,5-T	9.447	9.006	15280210	5792447	2.005	2.000
14) T	DINOSEB	11.149	9.835	11744333	3078358	2.227	1.511 #
15) T	Picloram	10.976	10.816	240.4E6	100.5E6	24.084	24.966
16) T	DCPA	11.416	10.765	14023702	7114335	1.327	1.583



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081121\
Data File : PS016351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2021 11:15
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 05:13:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

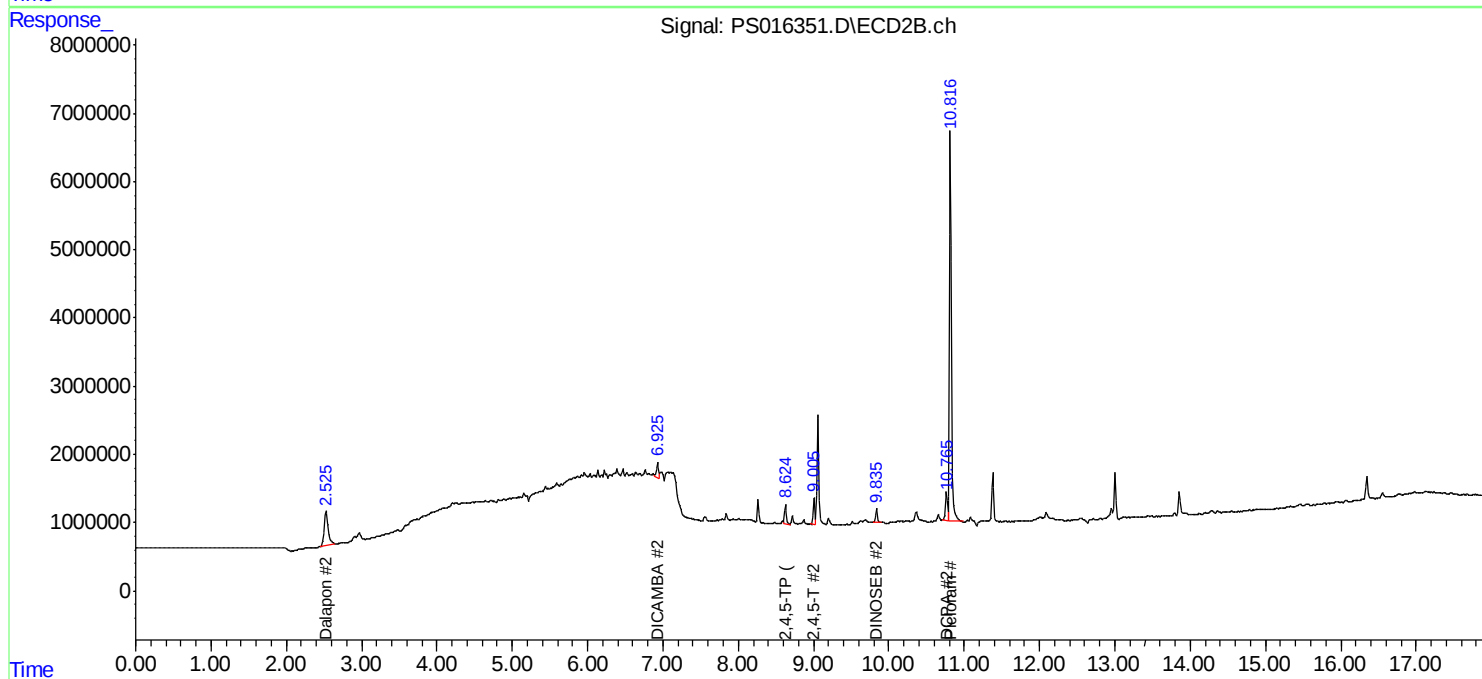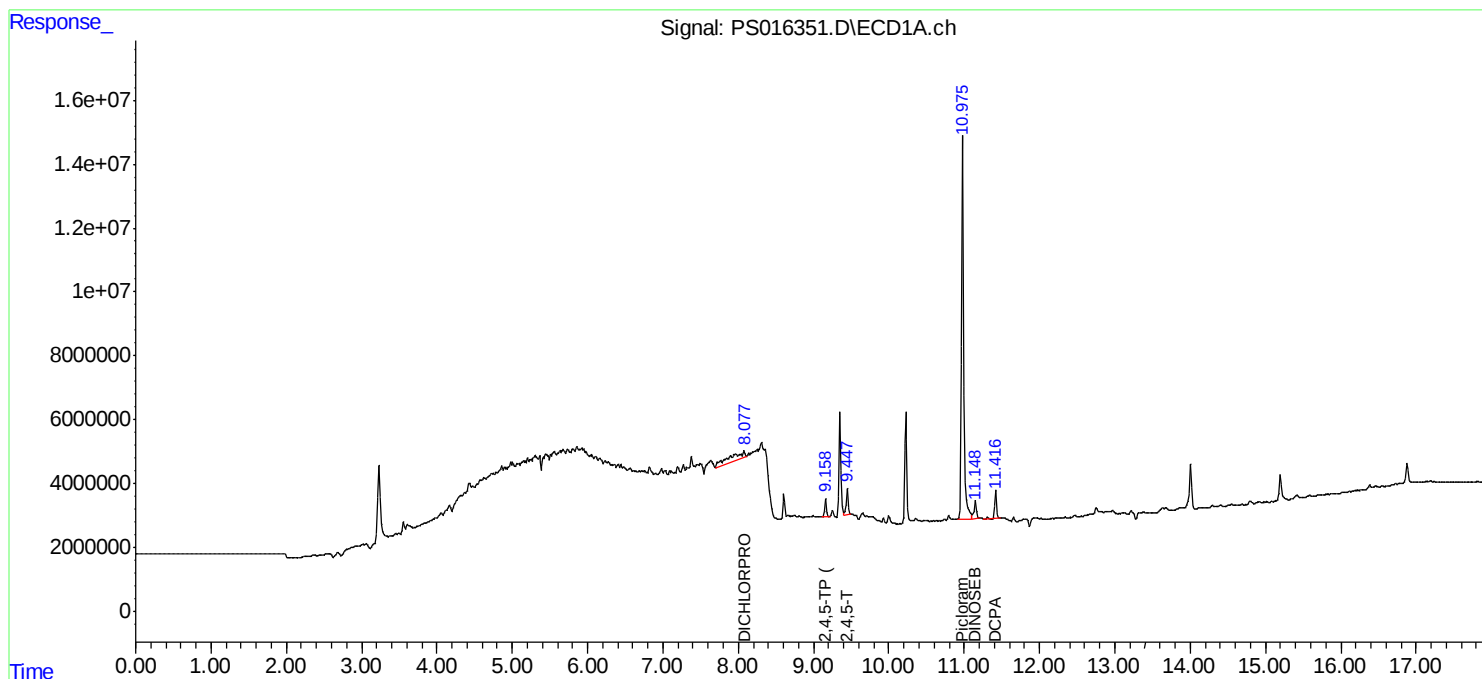


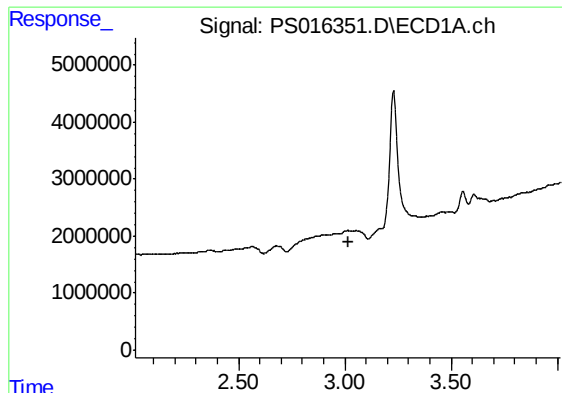

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

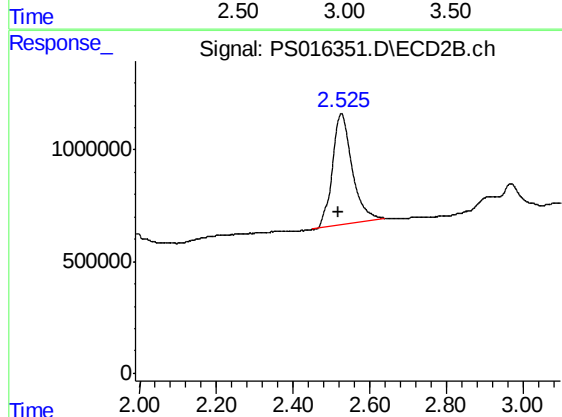


#1 Dalapon

R.T.: 2.526 min
Delta R.T.: 0.008 min
Response: 17694878
Conc: 25.40 ng/ml

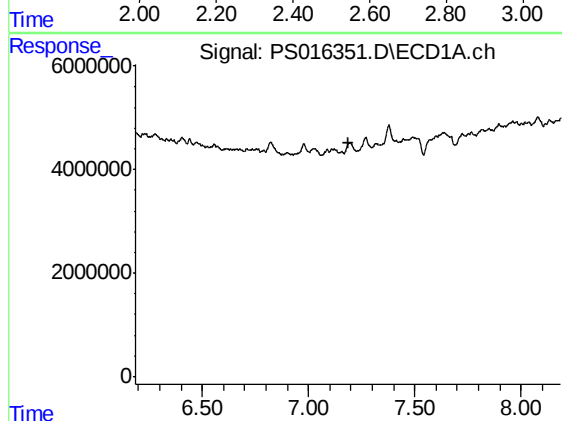


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

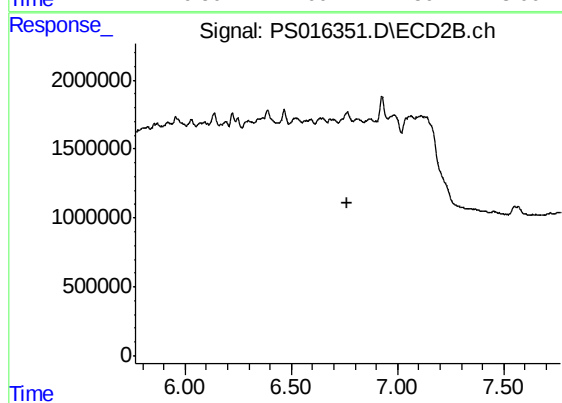

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.766 min
Response: 0
Conc: N.D.

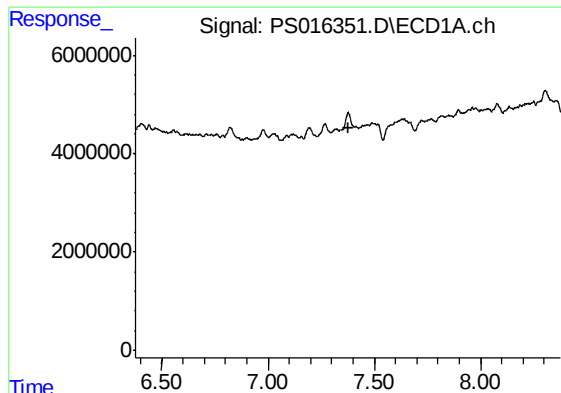

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

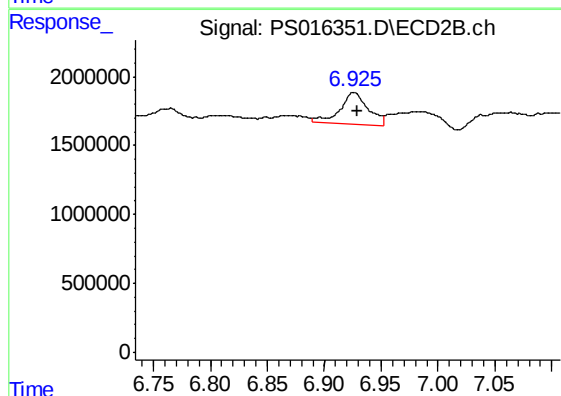


#5 DICAMBA

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 3904393
Conc: 1.79 ng/ml

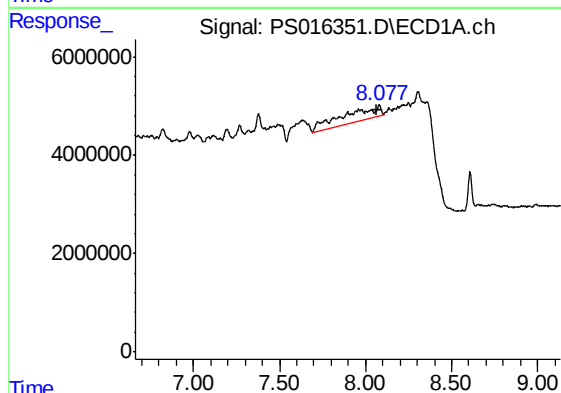


#8 DICHLORPROP

R.T.: 8.078 min
Delta R.T.: 0.009 min
Response: 37977586
Conc: 28.22 ng/ml

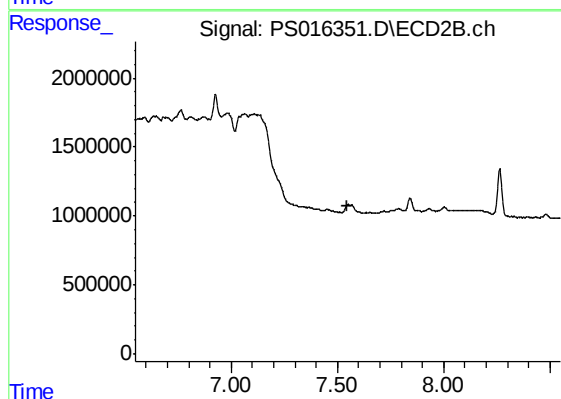

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.549 min
Response: 0
Conc: N.D.

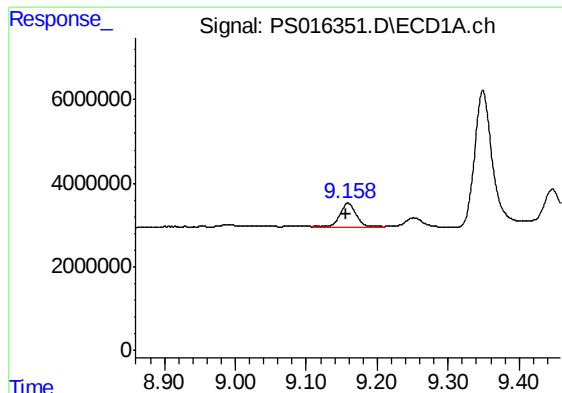

#11 2,4,5-TP (SILVEX)


R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 8772761
Conc: 1.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

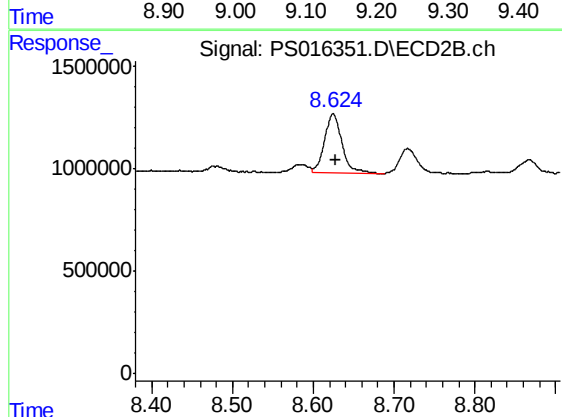


#11 2,4,5-TP (SILVEX)

R.T.: 8.625 min
Delta R.T.: -0.004 min
Response: 4418895
Conc: 1.51 ng/ml

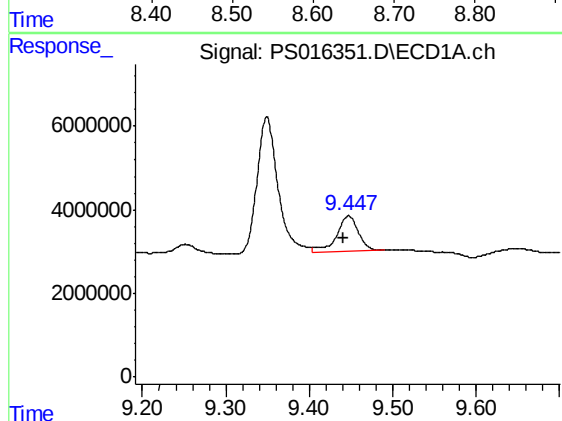


#12 2,4,5-T

R.T.: 9.447 min
Delta R.T.: 0.007 min
Response: 15280210
Conc: 2.00 ng/ml

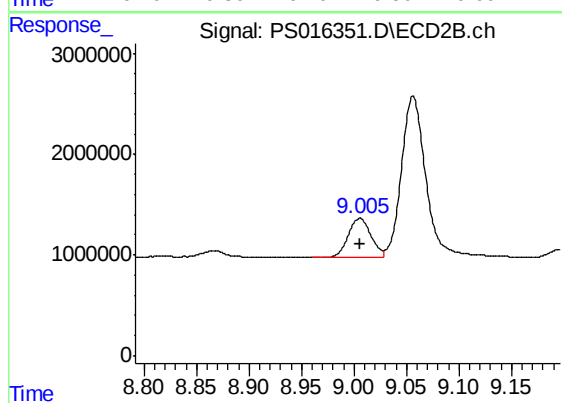

#12 2,4,5-T


R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 5792447
Conc: 2.00 ng/ml

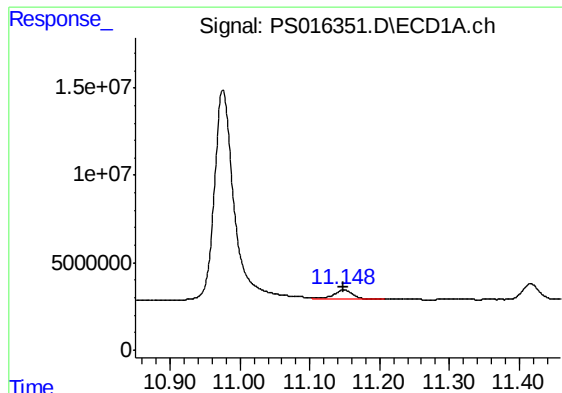

#14 DINOSEB


R.T.: 11.149 min
Delta R.T.: 0.000 min
Response: 11744333
Conc: 2.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

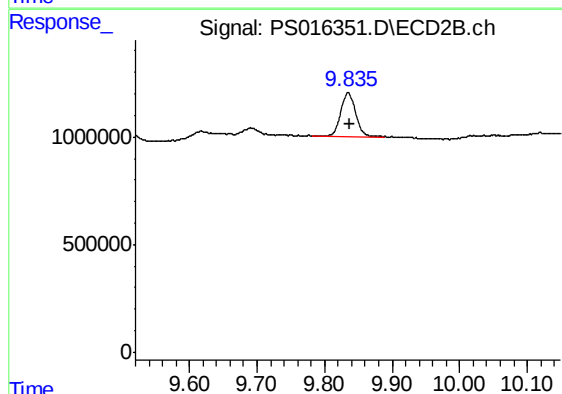


#14 DINOSEB

R.T.: 9.835 min
Delta R.T.: -0.003 min
Response: 3078358
Conc: 1.51 ng/ml

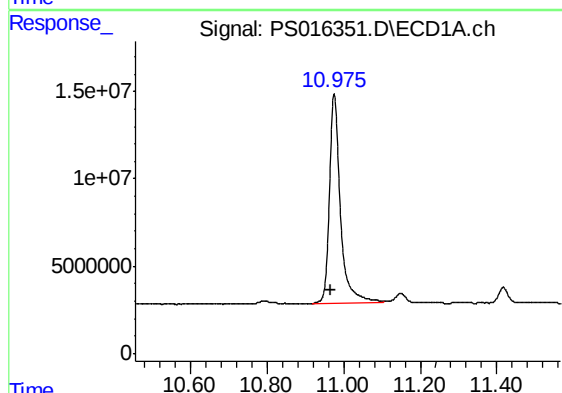


#15 Picloram

R.T.: 10.976 min
Delta R.T.: 0.009 min
Response: 240380332
Conc: 24.08 ng/ml

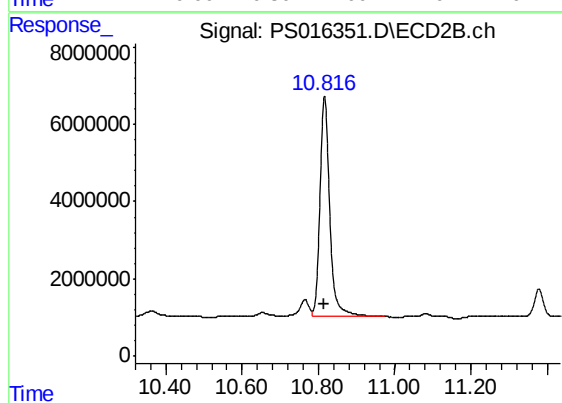

#15 Picloram


R.T.: 10.816 min
Delta R.T.: 0.000 min
Response: 100528563
Conc: 24.97 ng/ml

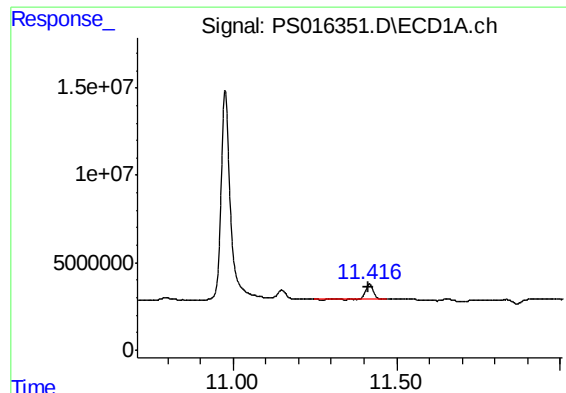

#16 DCPA

R.T.: 11.416 min
Delta R.T.: 0.001 min
Response: 14023702
Conc: 1.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

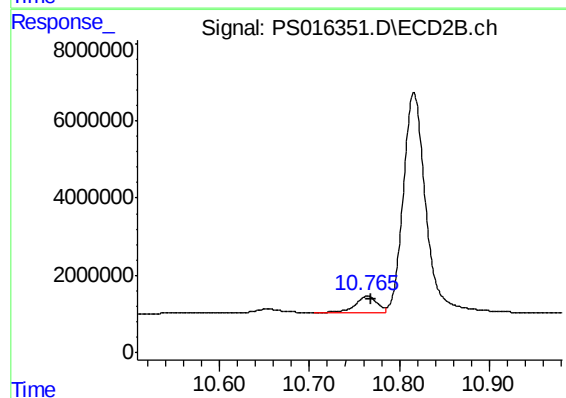

#16 DCPA

R.T.: 10.765 min
Delta R.T.: -0.003 min
Response: 7114335
Conc: 1.58 ng/ml