

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081121\
 Data File : PS016352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2021 11:39
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 05:13:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.766	616.7E6	256.5E6	419.211	491.767
Target Compounds							
12) T	2,4,5-T	9.372f	9.069f	8155300	8045377	1.070	2.778 #
15) T	Picloram	10.998	10.828	113.7E6	47060011	11.387	11.687
16) T	DCPA	0.000	10.828f	0	47060011	N.D.	10.469



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081121\
Data File : PS016352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2021 11:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 05:13:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

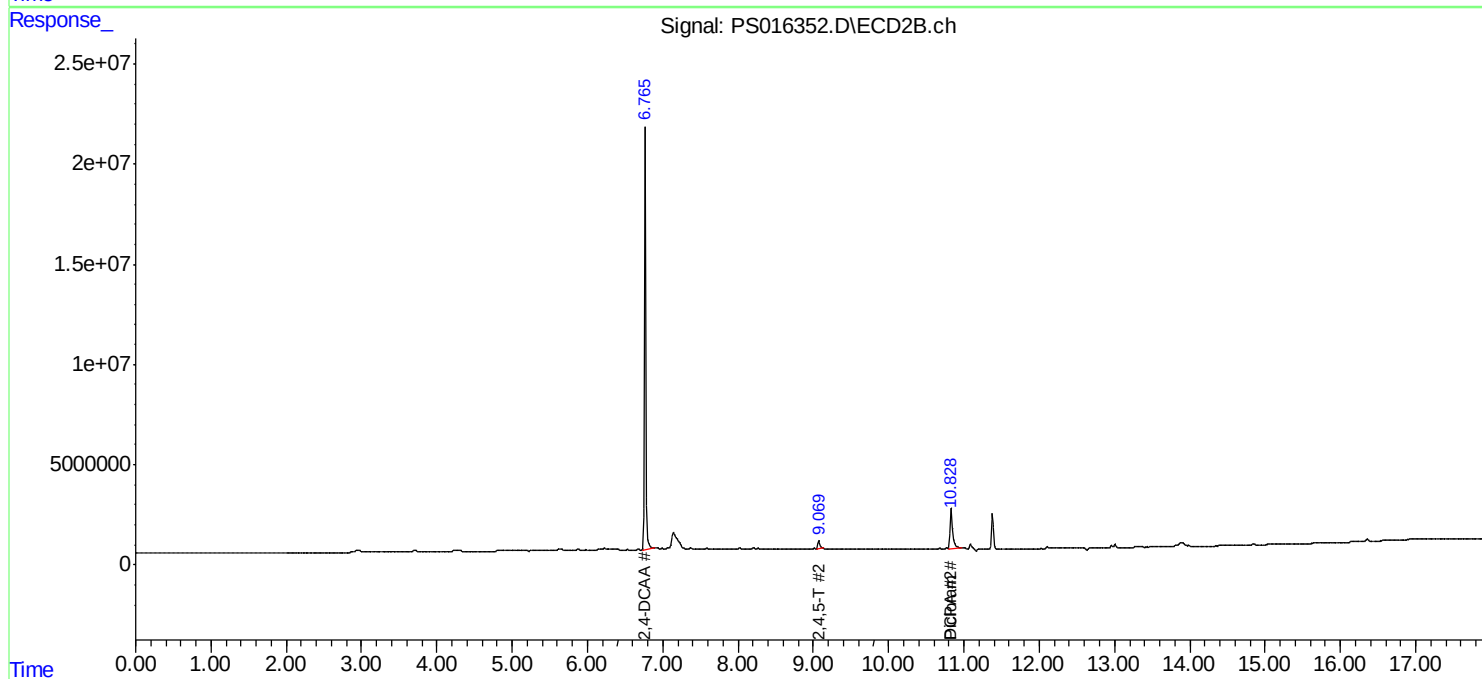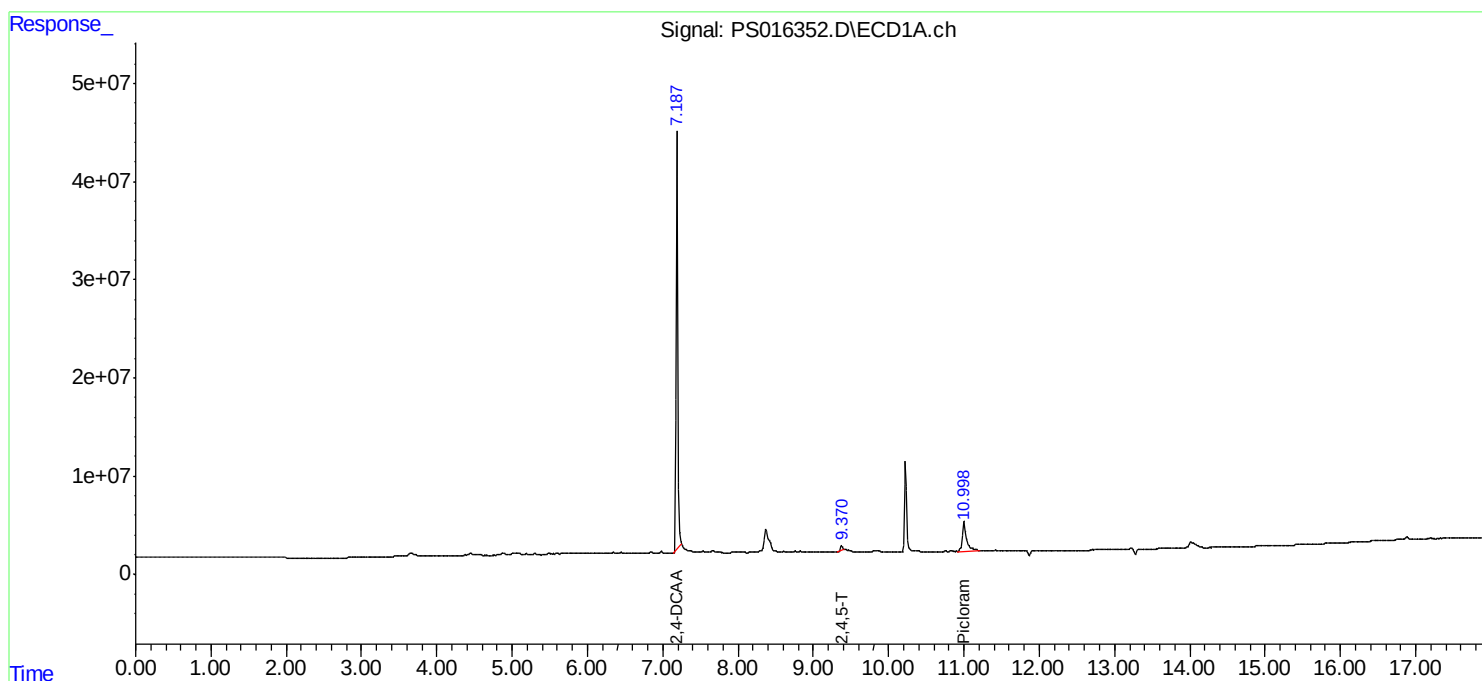


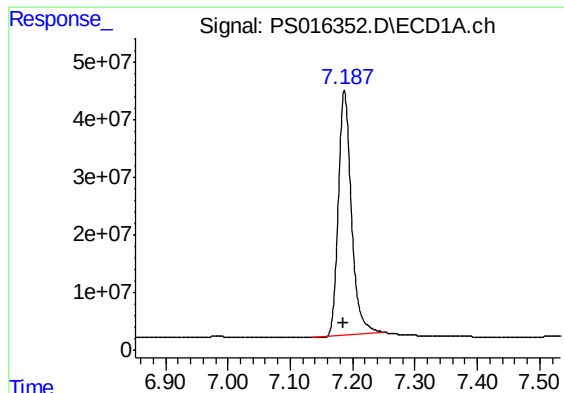

#4 2,4-DCAA


R.T.: 7.187 min
Delta R.T.: 0.001 min
Response: 616703977
Conc: 419.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

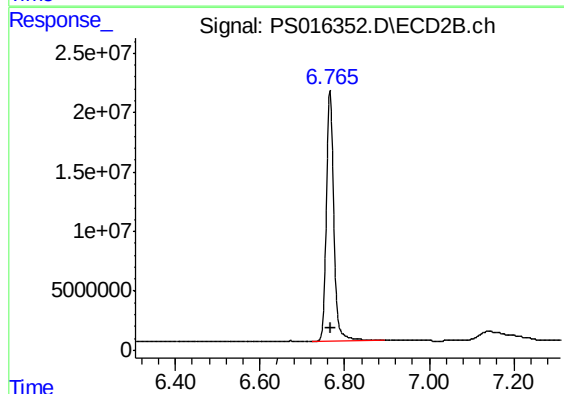


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: 0.000 min
Response: 256517868
Conc: 491.77 ng/ml

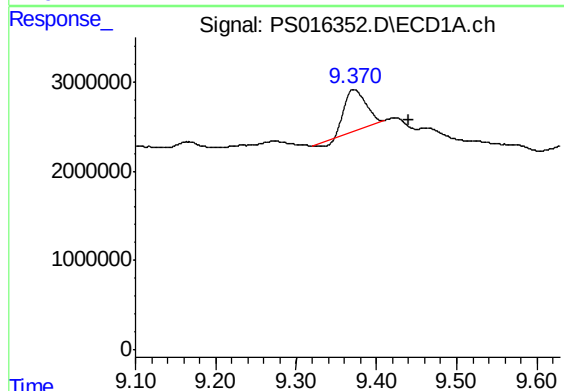


#12 2,4,5-T

R.T.: 9.372 min
Delta R.T.: -0.069 min
Response: 8155300
Conc: 1.07 ng/ml

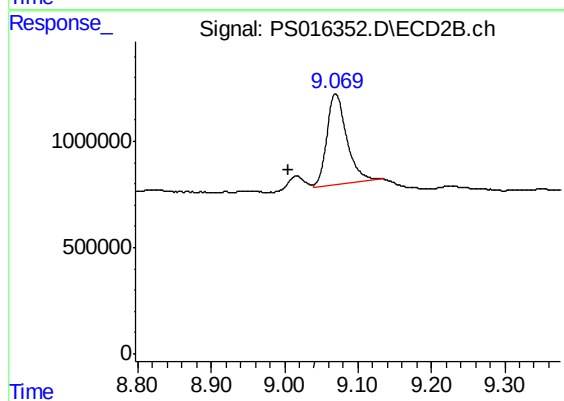

#12 2,4,5-T


R.T.: 9.069 min
Delta R.T.: 0.064 min
Response: 8045377
Conc: 2.78 ng/ml

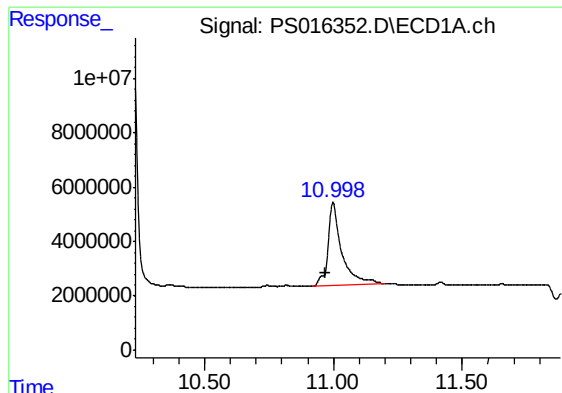

#15 Picloram


R.T.: 10.998 min
Delta R.T.: 0.031 min
Response: 113651371
Conc: 11.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

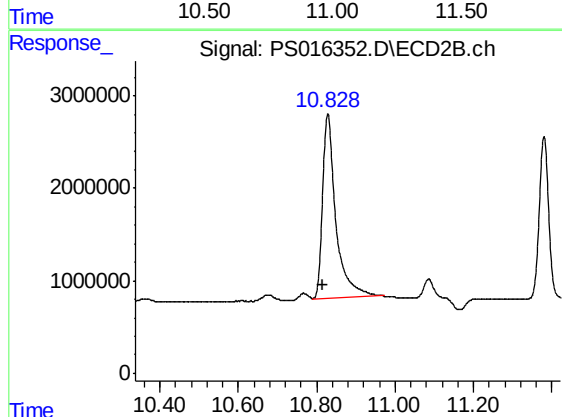


#15 Picloram

R.T.: 10.828 min
Delta R.T.: 0.013 min
Response: 47060011
Conc: 11.69 ng/ml

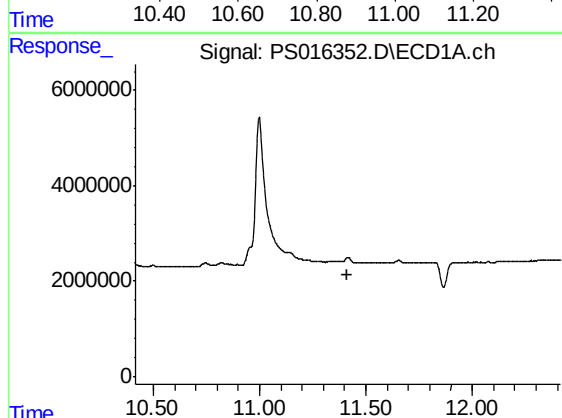

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.415 min
Response: 0
Conc: N.D.

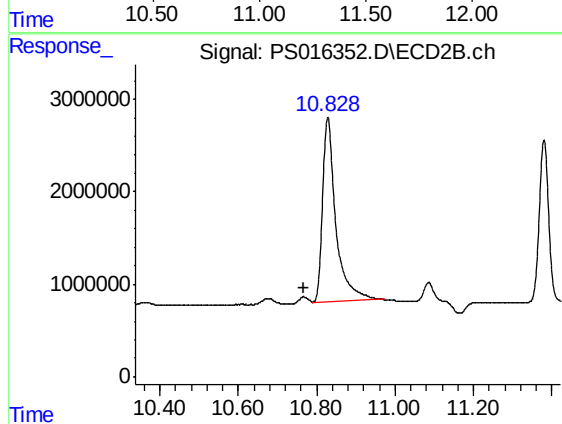

#16 DCPA

R.T.: 10.828 min
Delta R.T.: 0.060 min
Response: 47060011
Conc: 10.47 ng/ml