

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081122\
 Data File : PS020260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2022 20:03
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 22:16:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.179	6.758	1406.0E6	457.2E6	476.823	560.983
Target Compounds							
1) T	Dalapon	3.040	0.000	1102147	0	<MDL	N.D. #
6) T	MCP	7.556	0.000	1693269	0	<MDL	N.D. #
7) T	MCPA	7.636f	0.000	6518038	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.582	0	2029091	N.D.	2.170
10) T	Pentachlo...	8.605	0.000	173254	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.203f	8.657	33016119	1933222	1.938	<MDL #
12) T	2,4,5-T	9.505f	0.000	31499670	0	1.735	N.D. #
13) T	2,4-DB	10.018	0.000	3662691	0	1.004	N.D. #
14) T	DINOSEB	11.099	9.766f	26291305	1240488	1.653	<MDL #
15) T	Picloram	10.994	10.822	25494680	9383841	<MDL	1.244 #
16) T	DCPA	11.408	0.000	5983209	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081122\
Data File : PS020260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2022 20:03
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 22:16:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

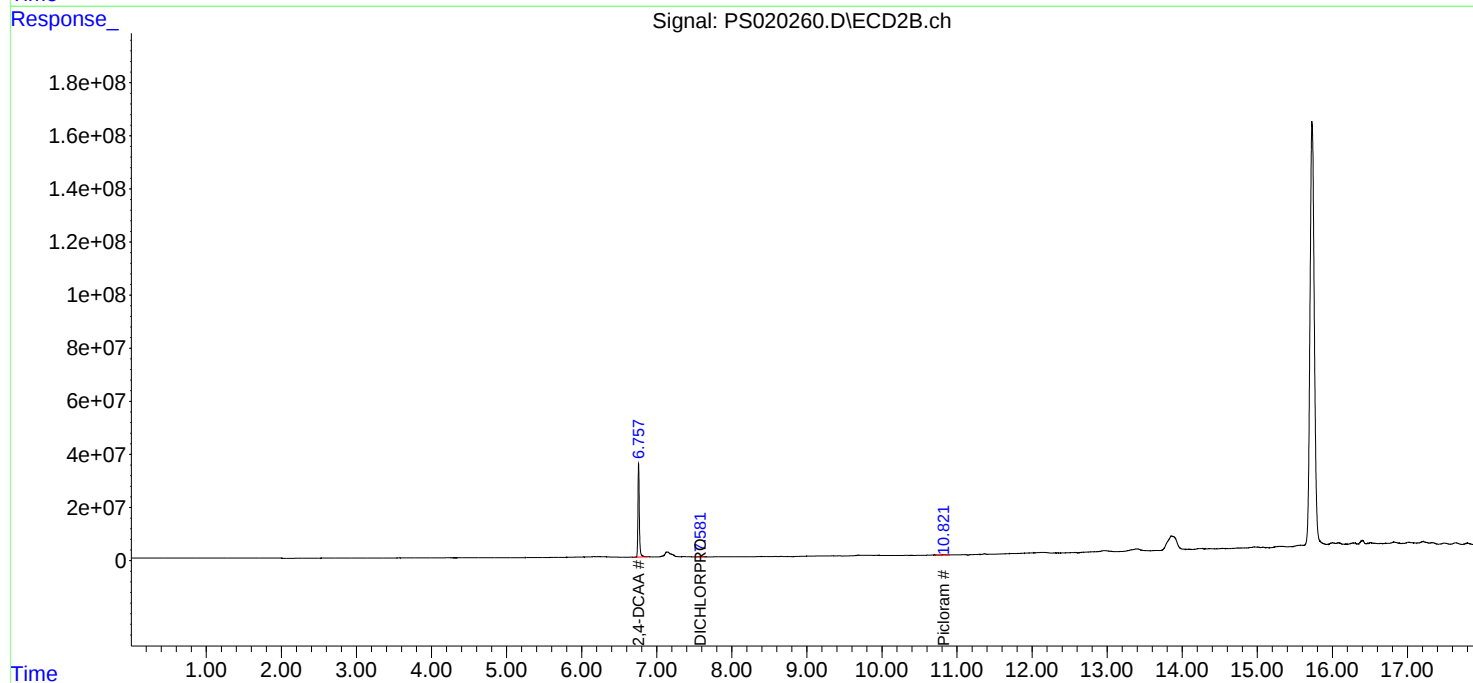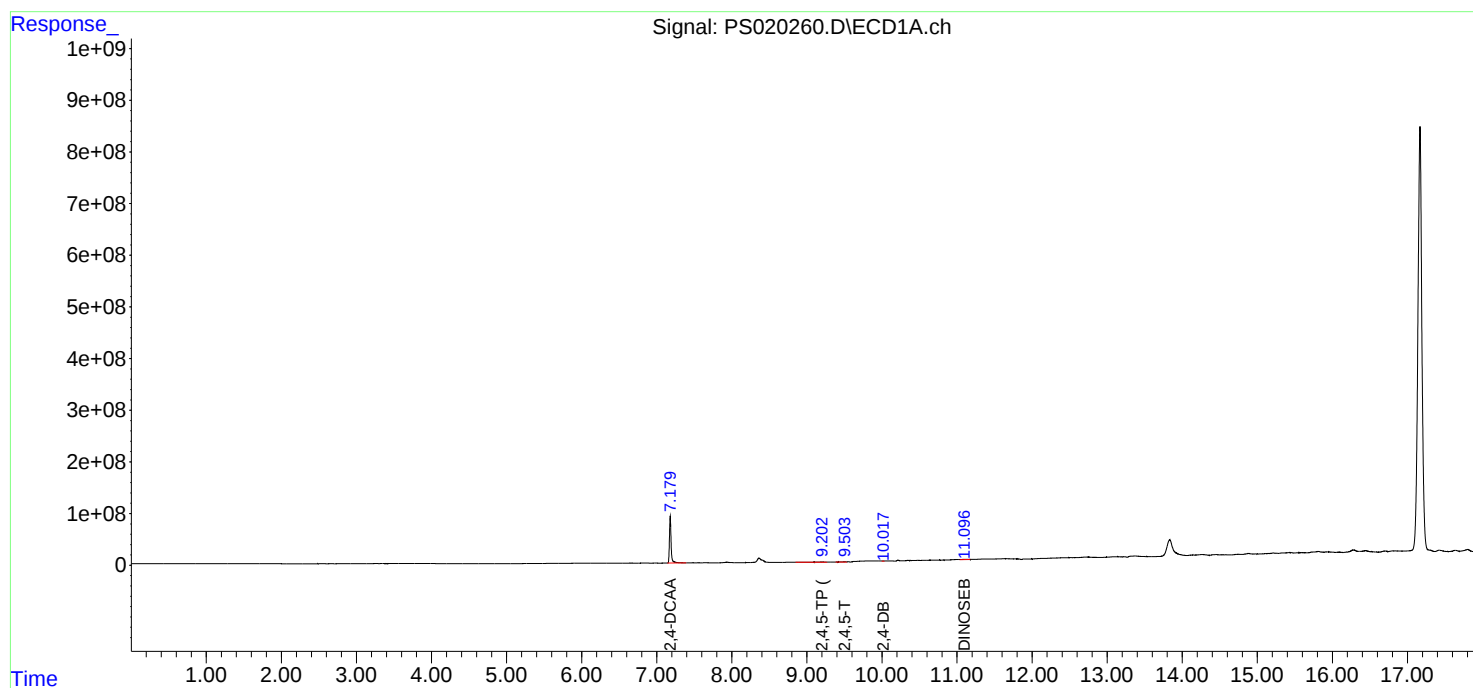


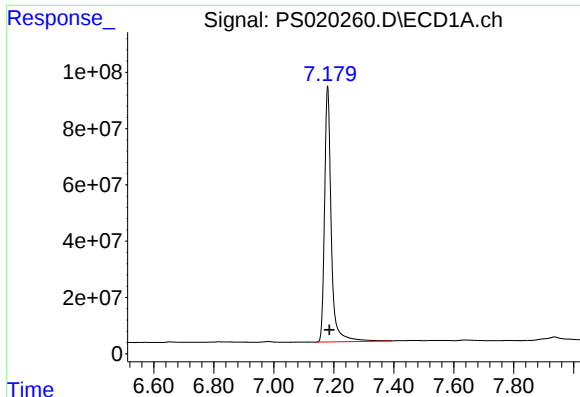

#4 2,4-DCAA


R.T.: 7.179 min
Delta R.T.: -0.006 min
Response: 1406018969
Conc: 476.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

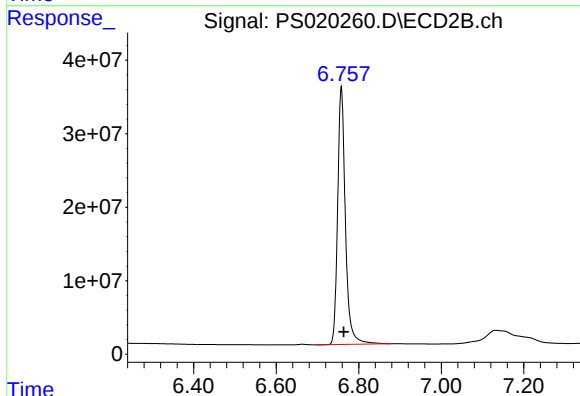


#4 2,4-DCAA

R.T.: 6.758 min
Delta R.T.: -0.006 min
Response: 457176148
Conc: 560.98 ng/ml

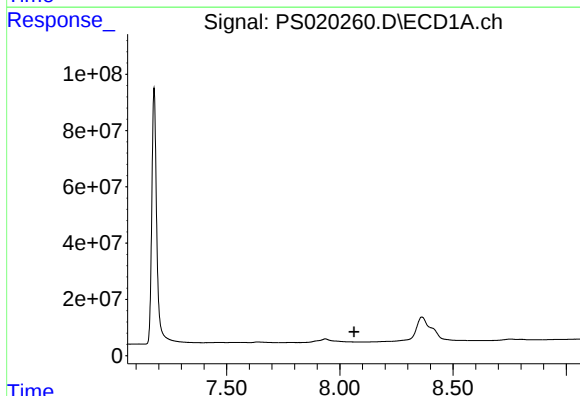


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.062 min
Response: 0
Conc: N.D.

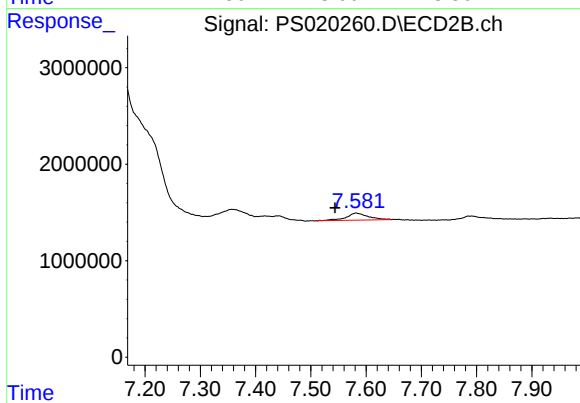

#8 DICHLORPROP


R.T.: 7.582 min
Delta R.T.: 0.038 min
Response: 2029091
Conc: 2.17 ng/ml

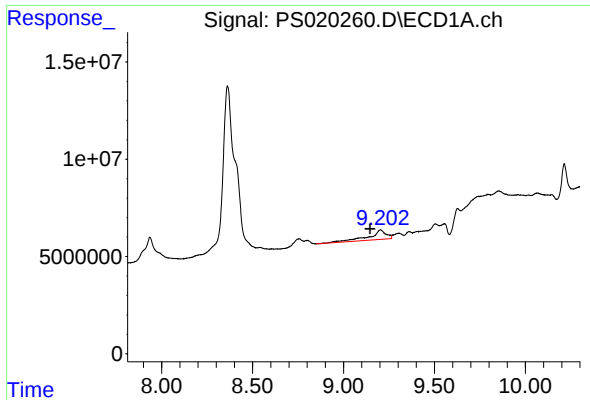

#11 2,4,5-TP (SILVEX)


R.T.: 9.203 min
Delta R.T.: 0.056 min
Response: 33016119
Conc: 1.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

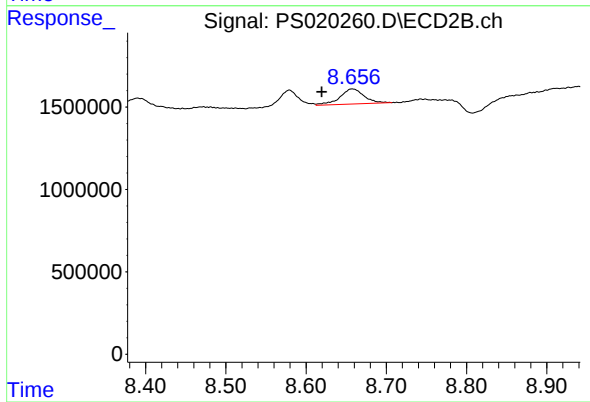


#11 2,4,5-TP (SILVEX)

R.T.: 8.657 min
Delta R.T.: 0.038 min
Response: 1933222
Conc: N.D.

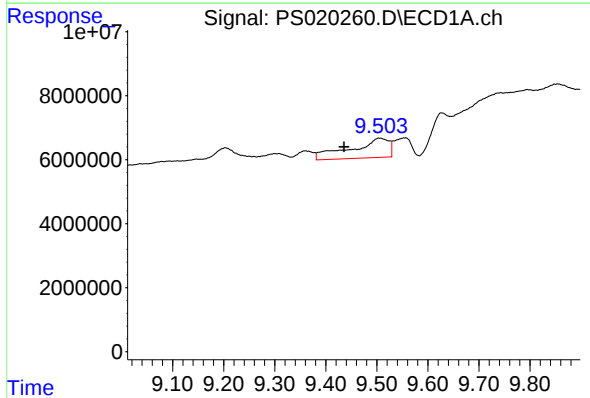


#12 2,4,5-T

R.T.: 9.505 min
Delta R.T.: 0.069 min
Response: 31499670
Conc: 1.74 ng/ml

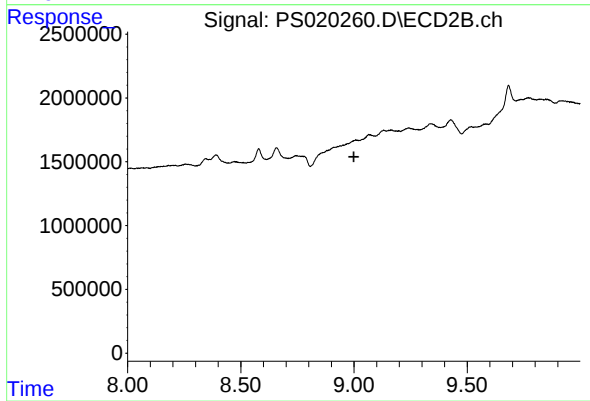

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.999 min
Response: 0
Conc: N.D.

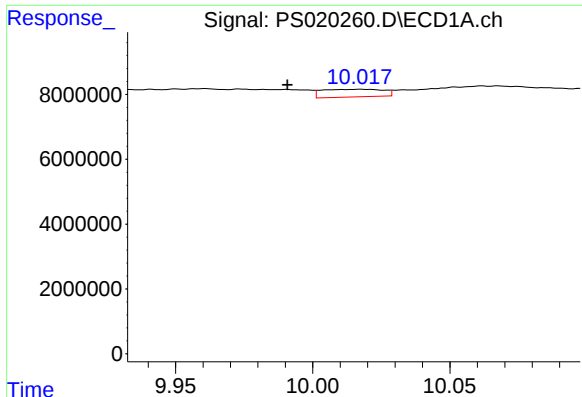

#13 2,4-DB


R.T.: 10.018 min
Delta R.T.: 0.027 min
Response: 3662691
Conc: 1.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

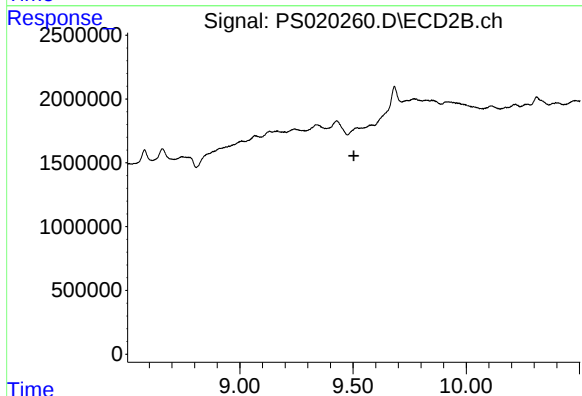


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.503 min
Response: 0
Conc: N.D.

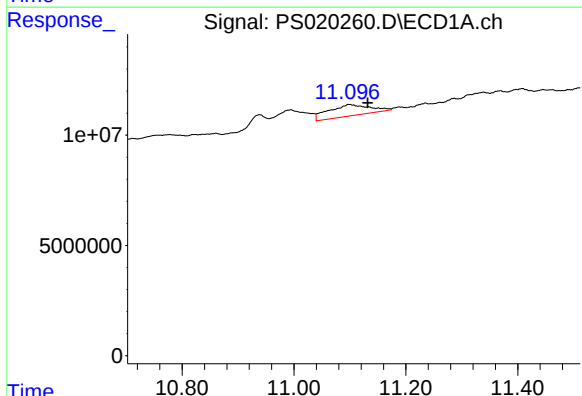


#14 DINOSEB

R.T.: 11.099 min
Delta R.T.: -0.033 min
Response: 26291305
Conc: 1.65 ng/ml

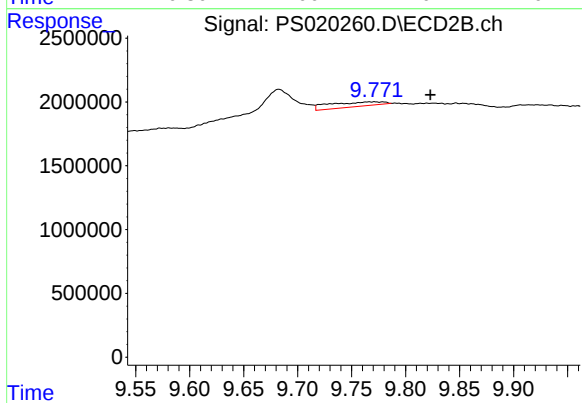

#14 DINOSEB


R.T.: 9.766 min
Delta R.T.: -0.057 min
Response: 1240488
Conc: N.D.

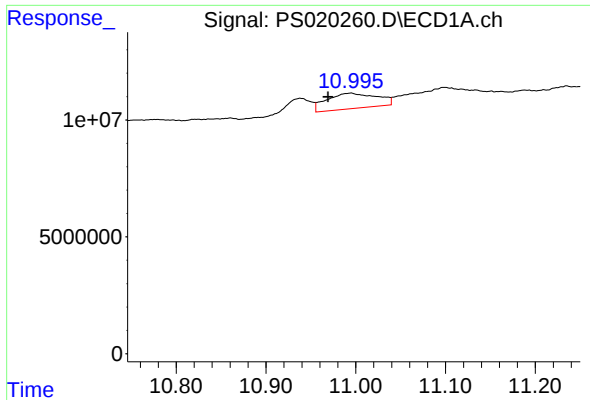

#15 Picloram

R.T.: 10.994 min
Delta R.T.: 0.025 min
Response: 25494680
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

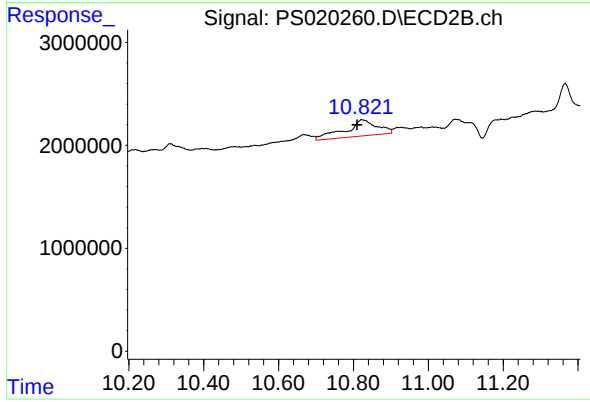

#15 Picloram

R.T.: 10.822 min
Delta R.T.: 0.012 min
Response: 9383841
Conc: 1.24 ng/ml