

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081123\
 Data File : PS024053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 08:23
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:03:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	0.000	2696378	0	1.361	N.D. #
Target Compounds							
1) T	Dalapon	2.516	2.578	7426119	5241941	3.384	4.794 #
3) T	4-Nitroph...	6.203	6.392	11093497	890331	10.023	2.249 #
5) T	DICAMBA	6.504	6.960	3316679	607119	<MDL	<MDL #
6) T	MCP	6.687	7.078	4207888	65179	<MDL	<MDL #
7) T	MCPA	6.823	7.211f	-630877	8301882	N.D.	2.838
8) T	DICHLORPROP	7.092	7.587	958020	4530084	<MDL	6.196 #
9) T	2,4-D	7.332	7.863	96269063	396886	38.849	<MDL #
10) T	Pentachlo...	7.528	8.285	11834335	1828558	<MDL	<MDL #
11) T	2,4,5-TP ...	8.050	8.645	3152845	1682452	<MDL	<MDL #
12) T	2,4,5-T	8.306	9.018	5165495	1677550	<MDL	<MDL #
13) T	2,4-DB	8.801	9.517	-282521	842716	N.D.	1.849
14) T	DINOSEB	9.864	9.848	2596564	600236	<MDL	<MDL #
15) T	Picloram	9.692	10.805	86904702	35304996	6.721	7.085
16) T	DCPA	10.124	10.805	4593109	35304996	<MDL	6.867 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081123\
Data File : PS024053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 08:23
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:03:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

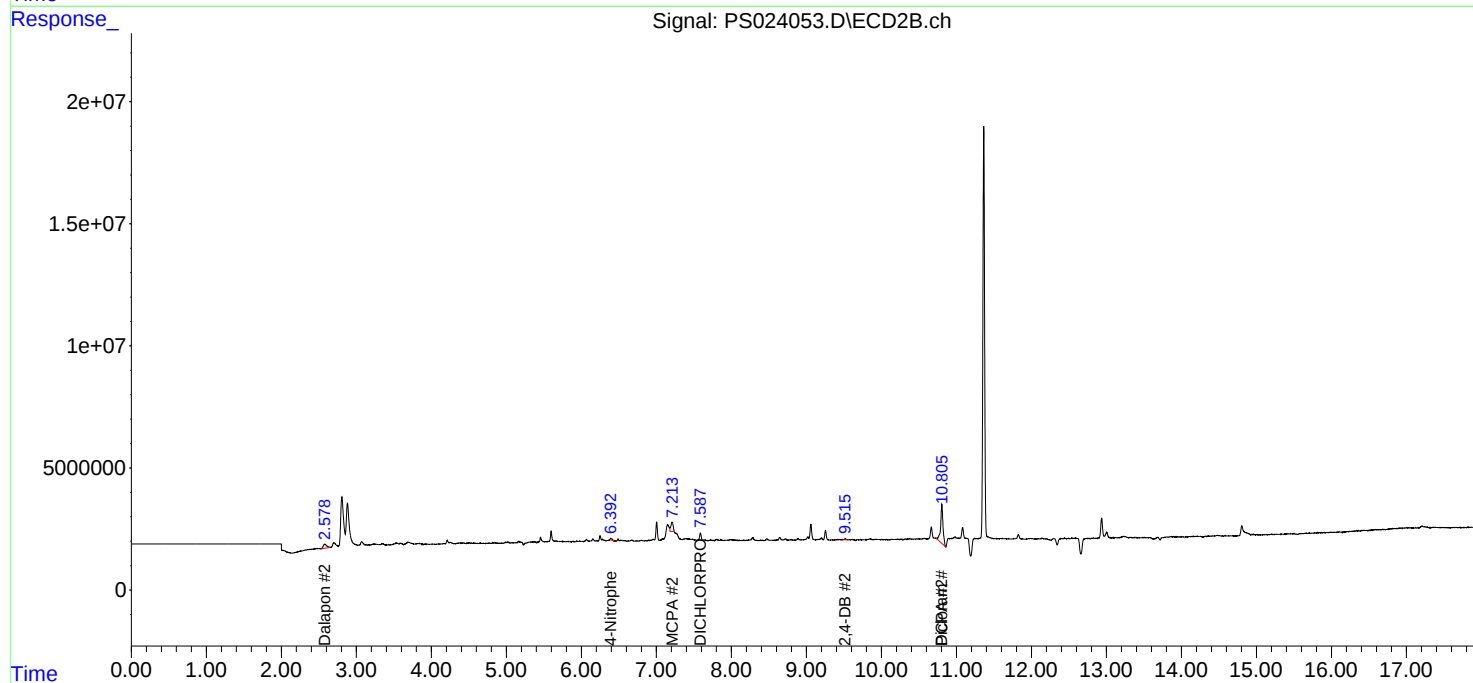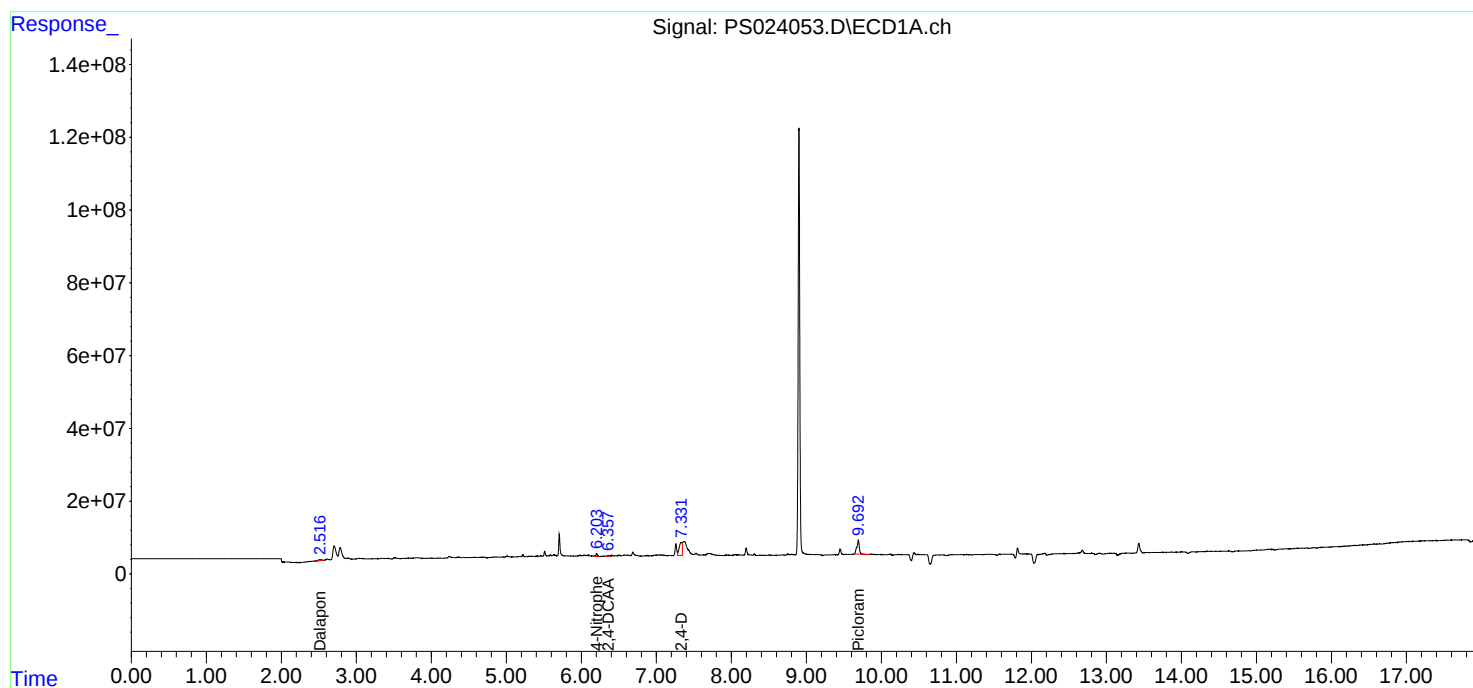


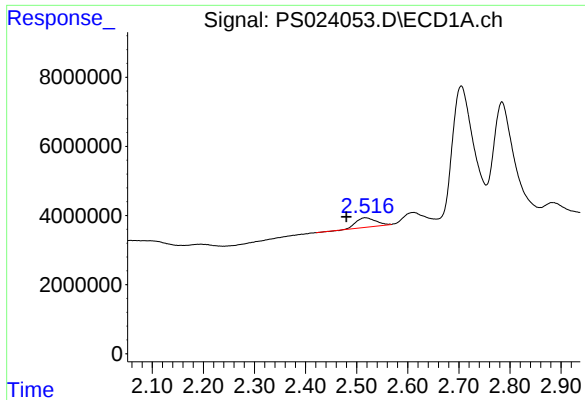

#1 Dalapon


R.T.: 2.516 min
Delta R.T.: 0.036 min
Response: 7426119
Conc: 3.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

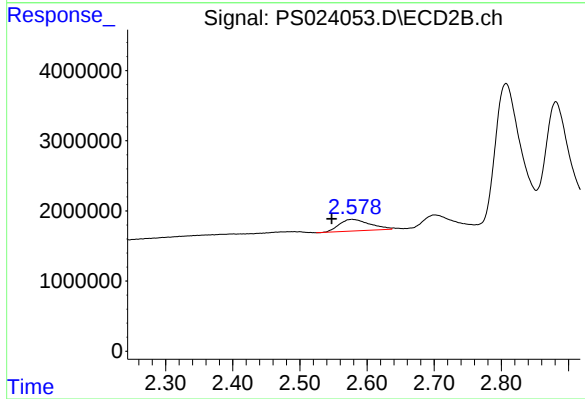


#1 Dalapon

R.T.: 2.578 min
Delta R.T.: 0.031 min
Response: 5241941
Conc: 4.79 ng/ml

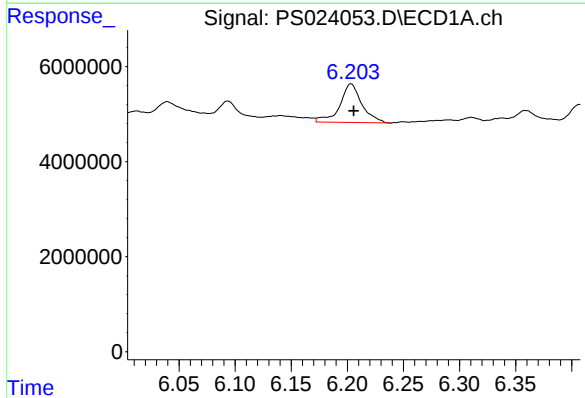


#3 4-Nitrophenol

R.T.: 6.203 min
Delta R.T.: -0.002 min
Response: 11093497
Conc: 10.02 ng/ml

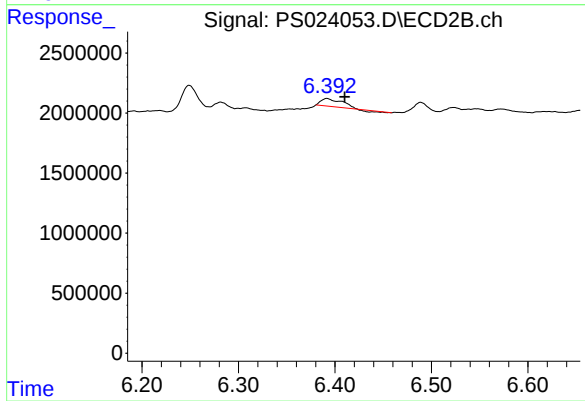

#3 4-Nitrophenol


R.T.: 6.392 min
Delta R.T.: -0.018 min
Response: 890331
Conc: 2.25 ng/ml

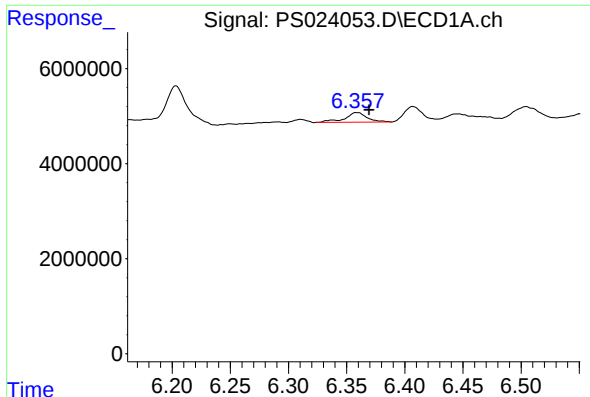

#4 2,4-DCAA


R.T.: 6.359 min
Delta R.T.: -0.010 min
Response: 2696378
Conc: 1.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

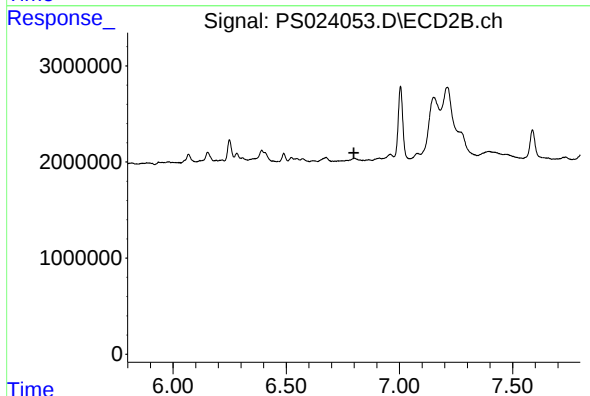


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

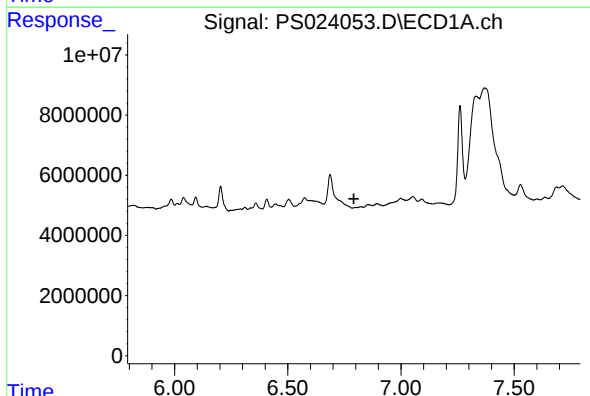


#7 MCPA

R.T.: 6.823 min
Delta R.T.: 0.031 min
Response: -630877
Conc: N.D.

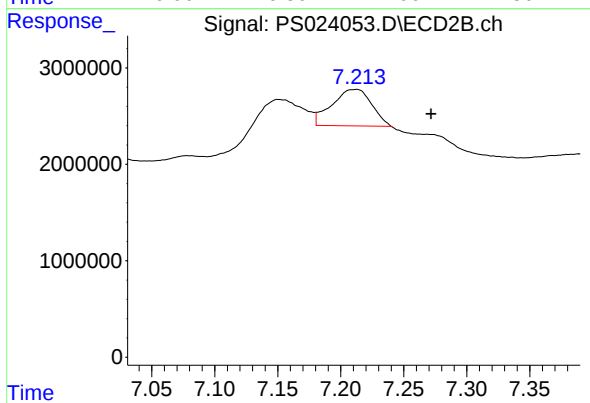

#7 MCPA


R.T.: 7.211 min
Delta R.T.: -0.061 min
Response: 8301882
Conc: 2.84 ug/ml

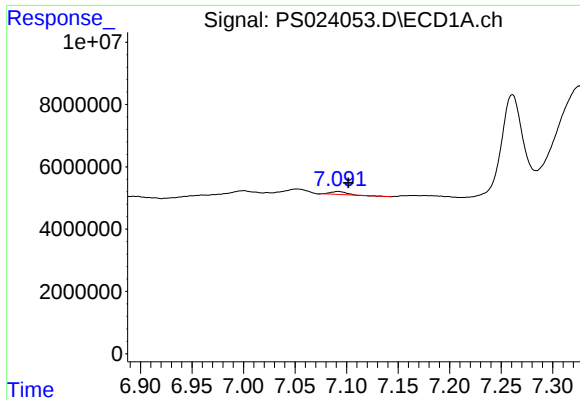

#8 DICHLORPROP


R.T.: 7.092 min
Delta R.T.: -0.010 min
Response: 958020
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

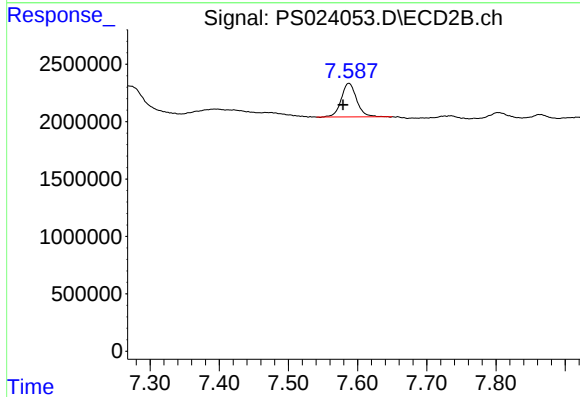


#8 DICHLORPROP

R.T.: 7.587 min
Delta R.T.: 0.008 min
Response: 4530084
Conc: 6.20 ng/ml

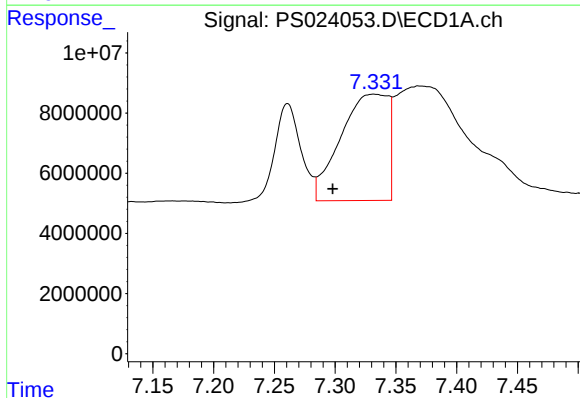


#9 2,4-D

R.T.: 7.332 min
Delta R.T.: 0.034 min
Response: 96269063
Conc: 38.85 ng/ml

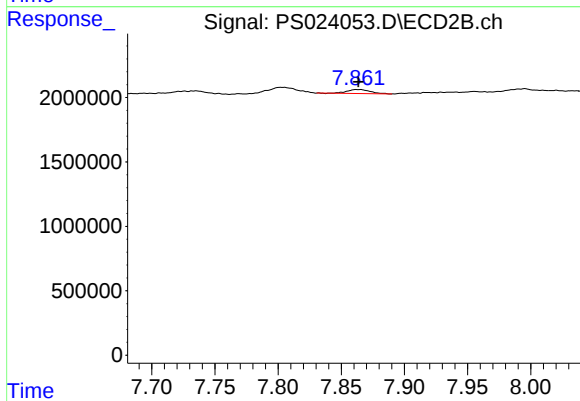

#9 2,4-D


R.T.: 7.863 min
Delta R.T.: 0.000 min
Response: 396886
Conc: N.D.

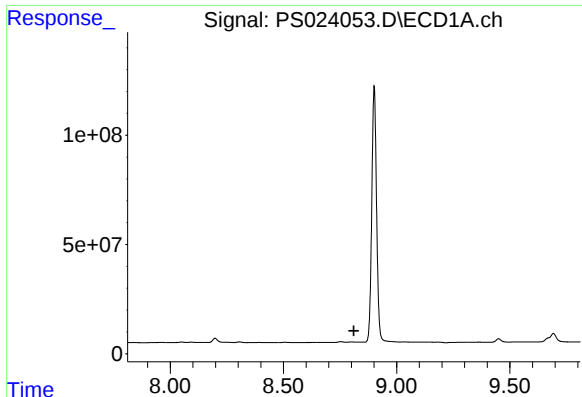

#13 2,4-DB


R.T.: 8.801 min
Delta R.T.: -0.010 min
Response: -282521
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

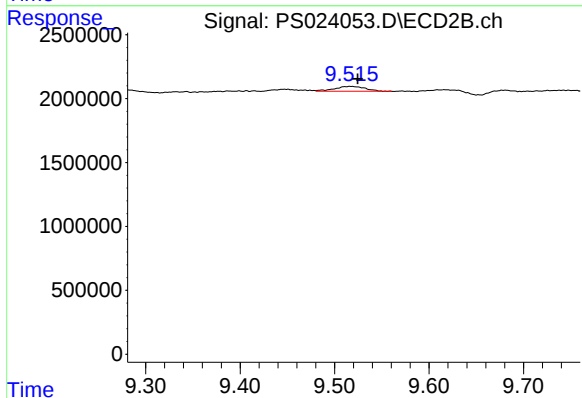


#13 2,4-DB

R.T.: 9.517 min
Delta R.T.: -0.008 min
Response: 842716
Conc: 1.85 ng/ml

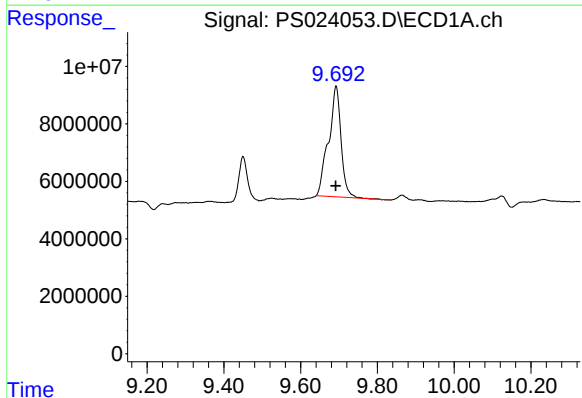


#15 Picloram

R.T.: 9.692 min
Delta R.T.: 0.001 min
Response: 86904702
Conc: 6.72 ng/ml

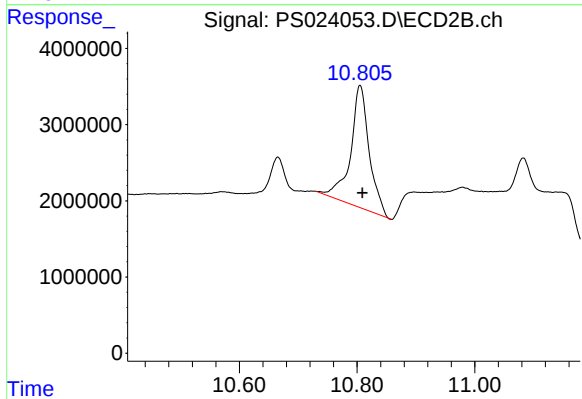

#15 Picloram


R.T.: 10.805 min
Delta R.T.: -0.004 min
Response: 35304996
Conc: 7.09 ng/ml

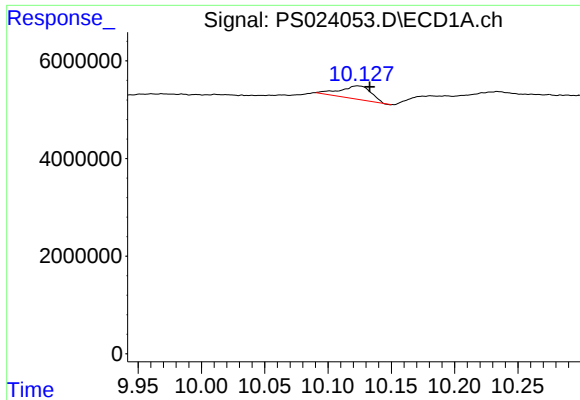

#16 DCPA

R.T.: 10.124 min
Delta R.T.: -0.009 min
Response: 4593109
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

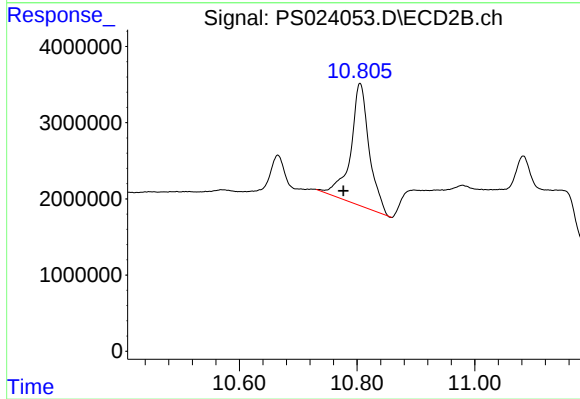

#16 DCPA

R.T.: 10.805 min
Delta R.T.: 0.028 min
Response: 35304996
Conc: 6.87 ng/ml