

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081123\
 Data File : PS024054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 08:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:04:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.366	6.797	1009.4E6	341.8E6	509.651	508.115
Target Compounds							
1) T	Dalapon	2.514	2.581	6600266	5295149	3.008	4.843 #
2) T	3,5-DICHL...	5.737	0.000	183349	0	<MDL	N.D. #
3) T	4-Nitroph...	6.207	0.000	7657341	0	6.918	N.D. #
5) T	DICAMBA	6.498	0.000	2054597	0	<MDL	N.D. #
6) T	MCP	6.689	0.000	479553	0	<MDL	N.D. #
7) T	MCPA	6.851f	7.203f	448578	13687174	<MDL	4.679 #
8) T	DICHLORPROP	7.149f	7.588	391178	812826	<MDL	1.112 #
9) T	2,4-D	0.000	7.807f	0	593815	N.D.	<MDL
10) T	Pentachlo...	7.522	8.287	4623647	789517	<MDL	<MDL #
11) T	2,4,5-TP ...	8.047	8.645	1240928	712986	<MDL	<MDL #
12) T	2,4,5-T	8.304	9.017	2314096	528928	<MDL	<MDL #
14) T	DINOSEB	9.861	0.000	1451742	0	<MDL	N.D. #
15) T	Picloram	9.692	10.805	33162928	12317633	2.565	2.472
16) T	DCPA	10.126	10.805	1618560	12317633	<MDL	2.396 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081123\
Data File : PS024054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 08:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:04:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

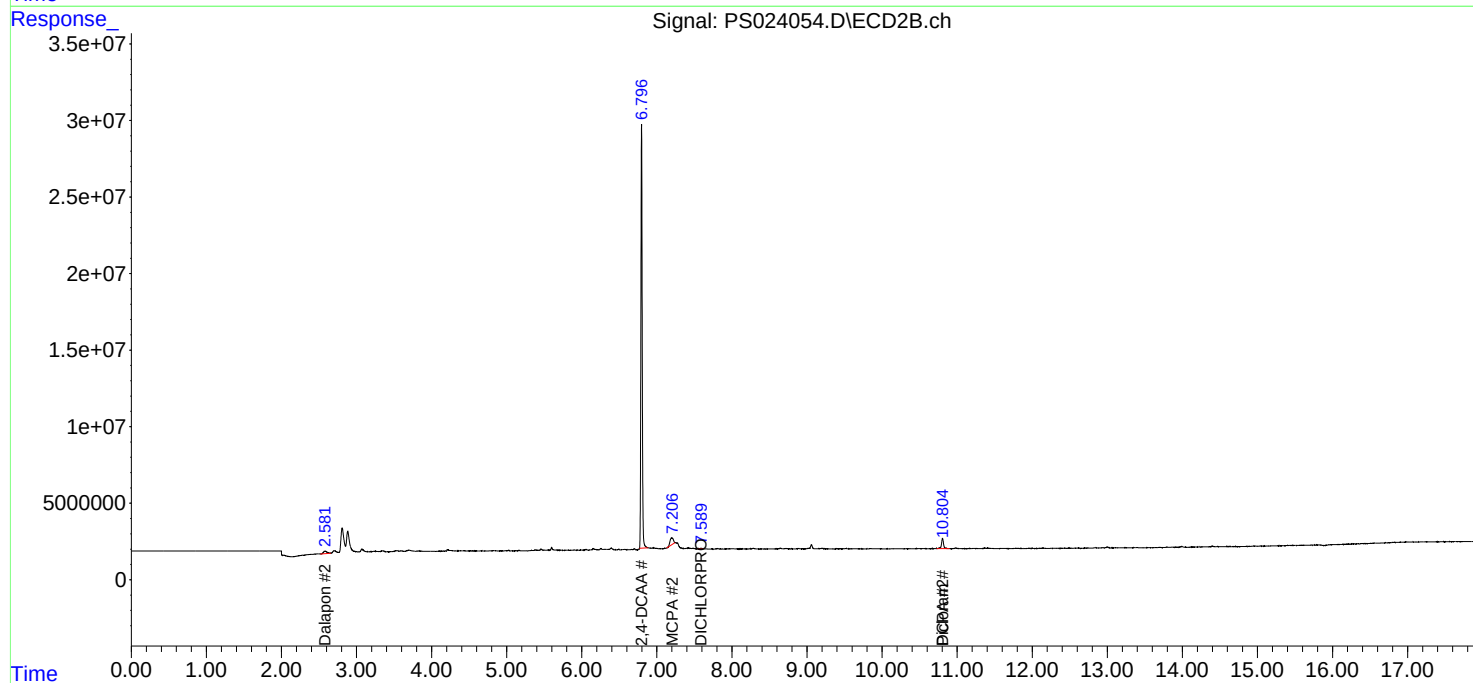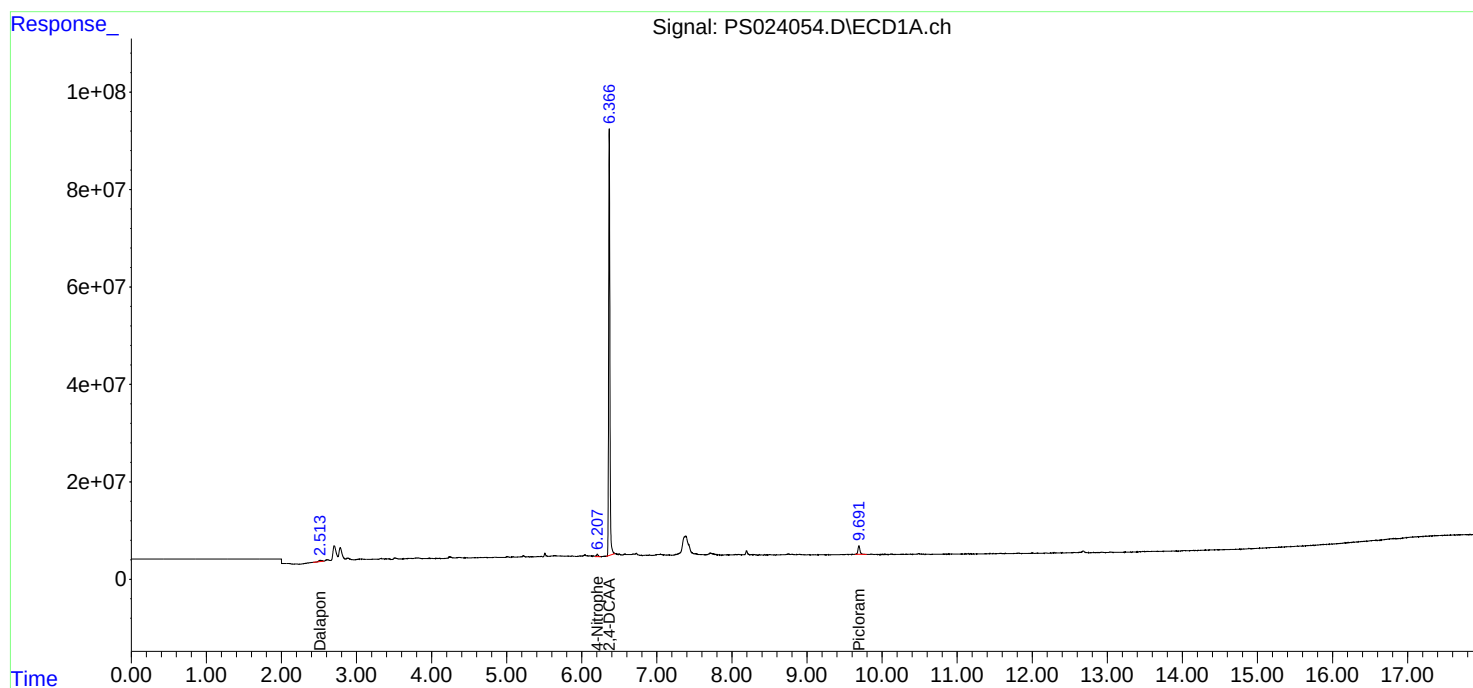


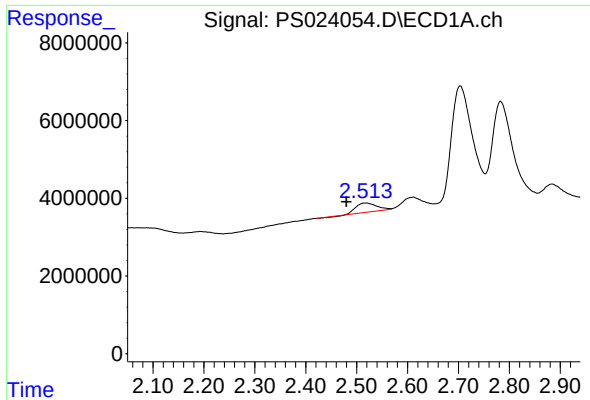

#1 Dalapon


R.T.: 2.514 min
Delta R.T.: 0.034 min
Response: 6600266
Conc: 3.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

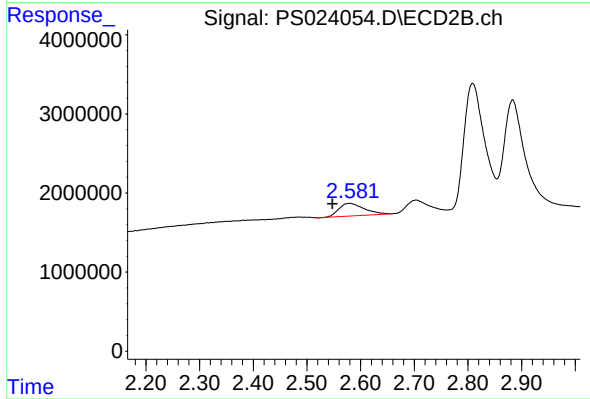


#1 Dalapon

R.T.: 2.581 min
Delta R.T.: 0.034 min
Response: 5295149
Conc: 4.84 ng/ml

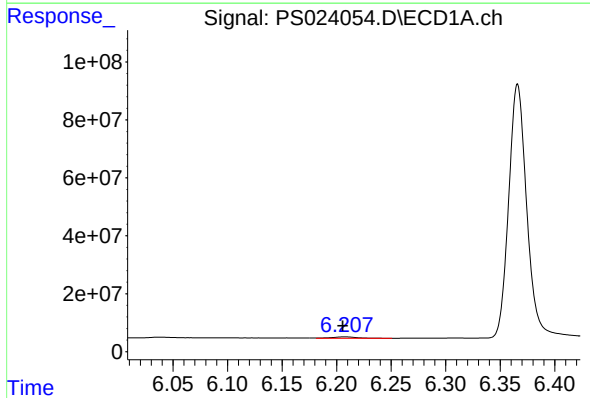


#3 4-Nitrophenol

R.T.: 6.207 min
Delta R.T.: 0.002 min
Response: 7657341
Conc: 6.92 ng/ml

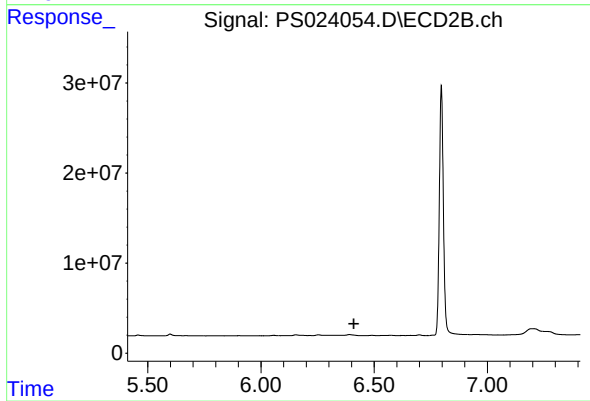

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

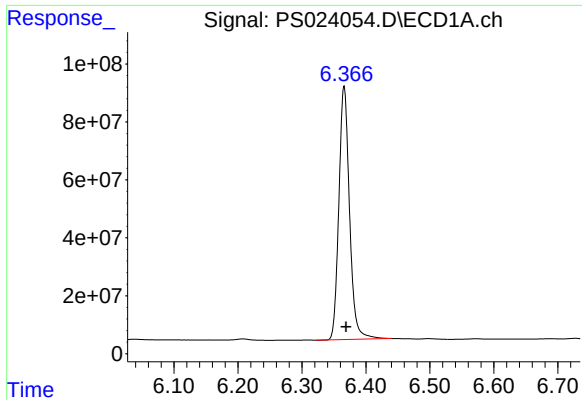

#4 2,4-DCAA


R.T.: 6.366 min
Delta R.T.: -0.003 min
Response: 1009396246
Conc: 509.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

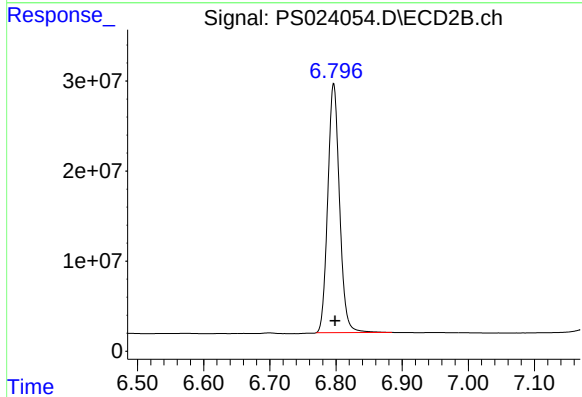


#4 2,4-DCAA

R.T.: 6.797 min
Delta R.T.: -0.002 min
Response: 341772324
Conc: 508.12 ng/ml

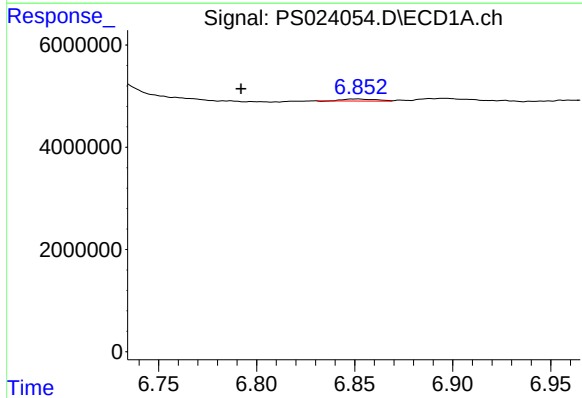


#7 MCPA

R.T.: 6.851 min
Delta R.T.: 0.059 min
Response: 448578
Conc: N.D.

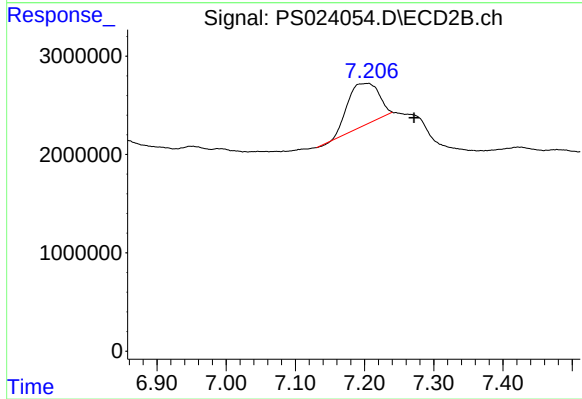

#7 MCPA


R.T.: 7.203 min
Delta R.T.: -0.068 min
Response: 13687174
Conc: 4.68 ug/ml

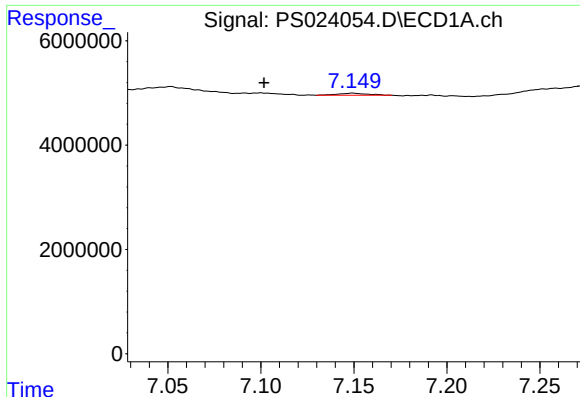

#8 DICHLORPROP


R.T.: 7.149 min
Delta R.T.: 0.048 min
Response: 391178
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

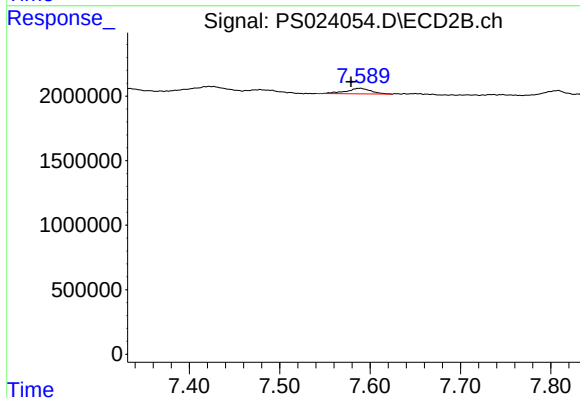


#8 DICHLORPROP

R.T.: 7.588 min
Delta R.T.: 0.009 min
Response: 812826
Conc: 1.11 ng/ml

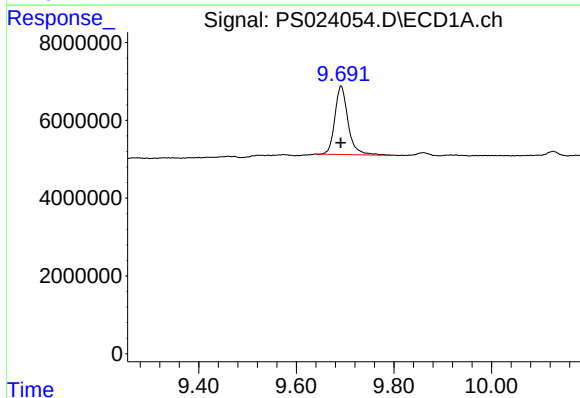


#15 Picloram

R.T.: 9.692 min
Delta R.T.: 0.000 min
Response: 33162928
Conc: 2.56 ng/ml

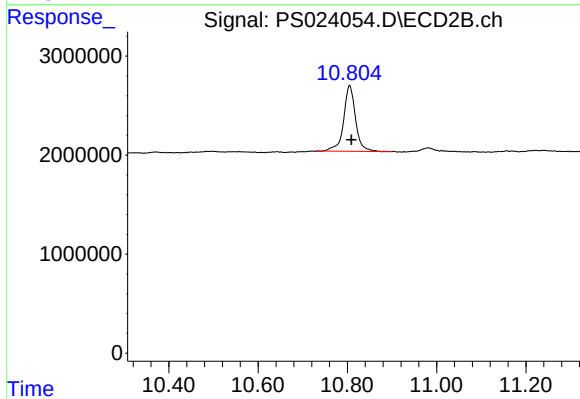

#15 Picloram


R.T.: 10.805 min
Delta R.T.: -0.004 min
Response: 12317633
Conc: 2.47 ng/ml

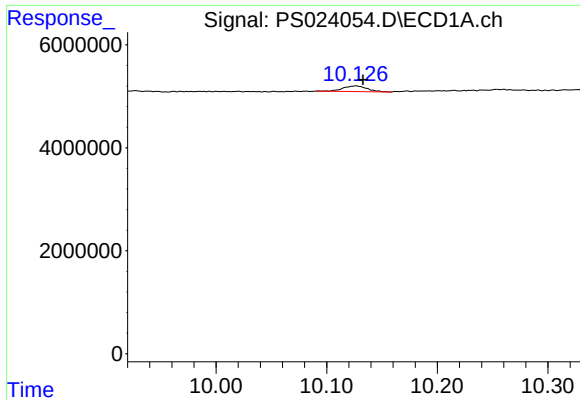

#16 DCPA

R.T.: 10.126 min
Delta R.T.: -0.007 min
Response: 1618560
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

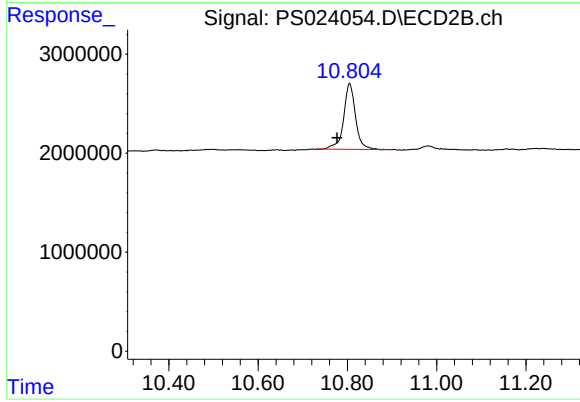

#16 DCPA

R.T.: 10.805 min
Delta R.T.: 0.028 min
Response: 12317633
Conc: 2.40 ng/ml