

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS005997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 15:31
 Operator : SM\AJ
 Sample : PB122129TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB122129TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:08:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.574	5.294	715.6E6	488.0E6	493.261	490.561
Target Compounds							
2) T	3,5-DICHL...	0.000	4.614	0	153.0E6	N.D.	117.940
7) T	MCPA	0.000	5.692	0	29123260	N.D.	6.919
10) T	Pentachlo...	0.000	6.553	0	18202751	N.D.	1.402
11) T	2,4,5-TP ...	0.000	6.943	0	41422489	N.D.	7.985
12) T	2,4,5-T	7.587	0.000	102.4E6	0	12.266	N.D. #
15) T	Picloram	0.000	9.127	0	23795403	N.D.	3.168



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS005997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 15:31
Operator : SM\AJ
Sample : PB122129TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB122129TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:08:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

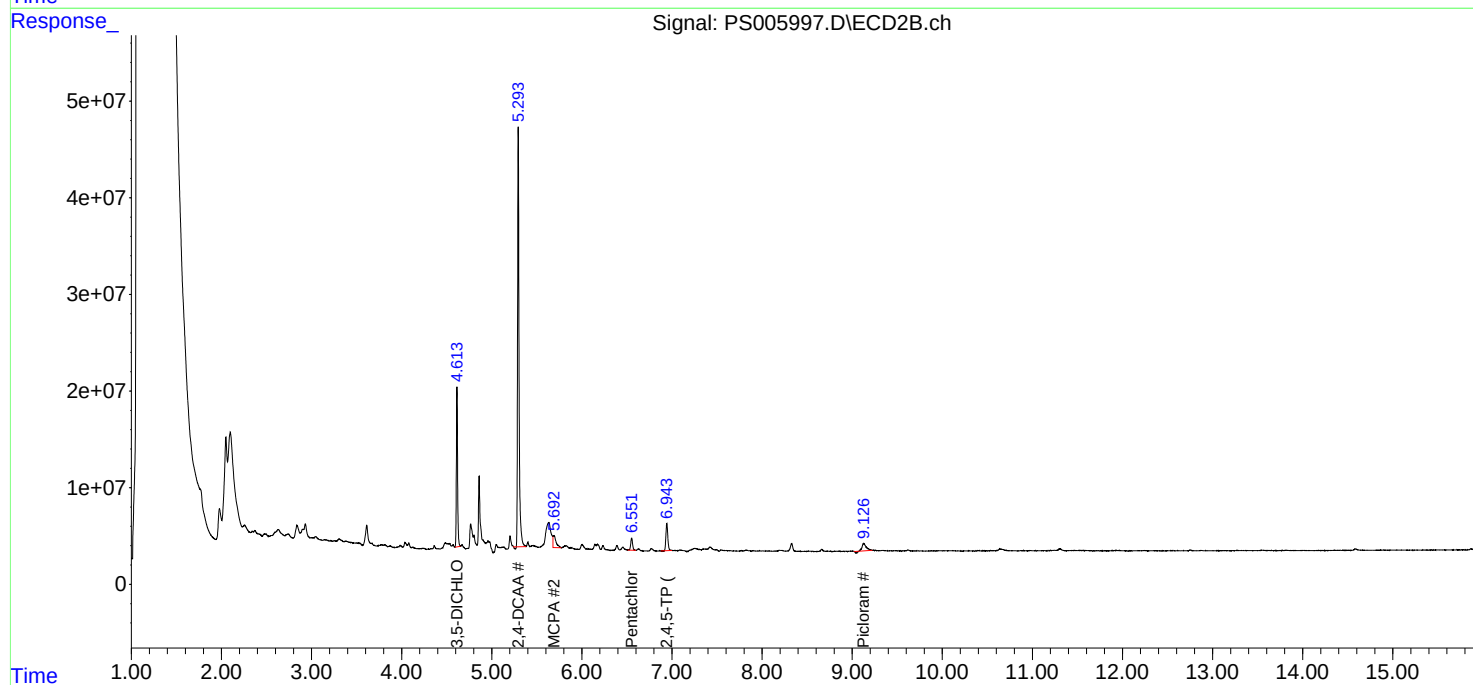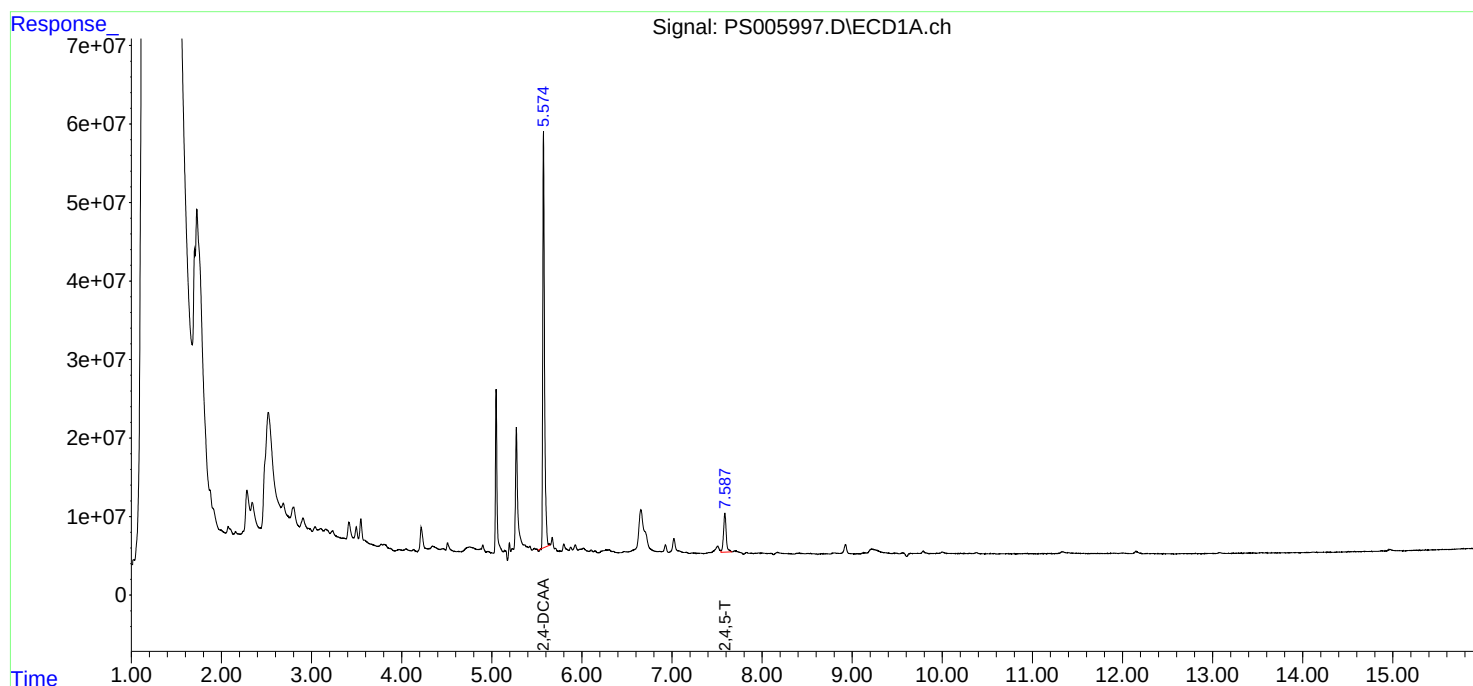


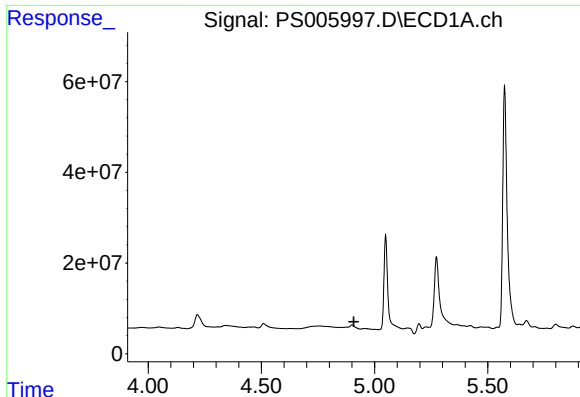

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB122129TB

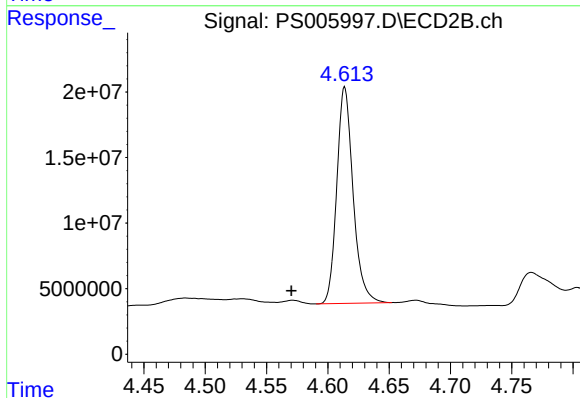


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.614 min
Delta R.T.: 0.044 min
Response: 153005815
Conc: 117.94 ng/ml

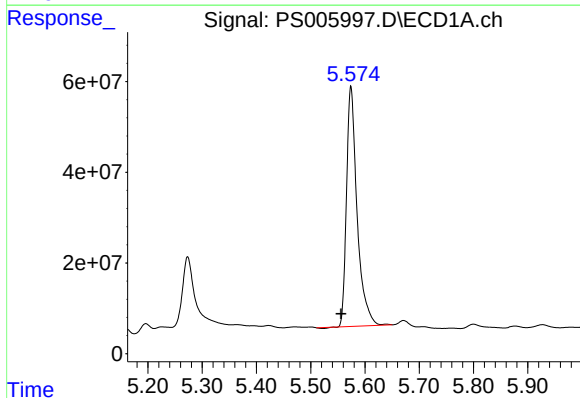


#4 2,4-DCAA

R.T.: 5.574 min
Delta R.T.: 0.018 min
Response: 715631492
Conc: 493.26 ng/ml

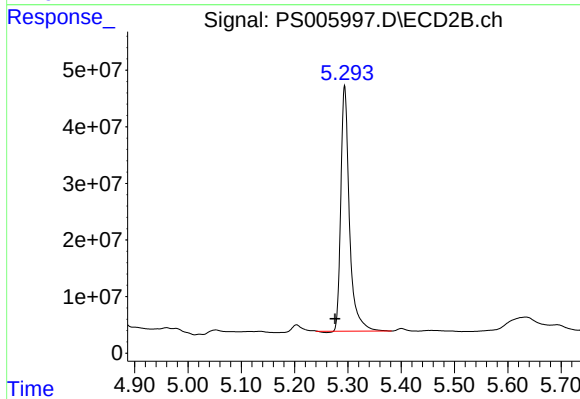

#4 2,4-DCAA


R.T.: 5.294 min
Delta R.T.: 0.018 min
Response: 487950387
Conc: 490.56 ng/ml

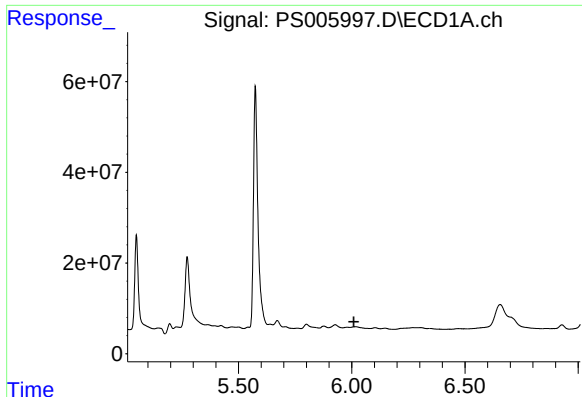

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB122129TB

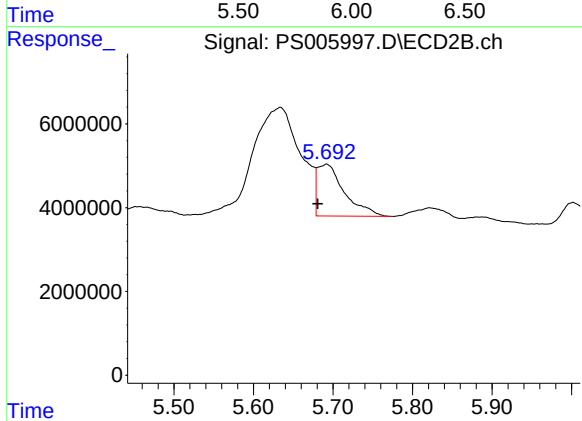


#7 MCPA

R.T.: 5.692 min
Delta R.T.: 0.011 min
Response: 29123260
Conc: 6.92 ug/ml

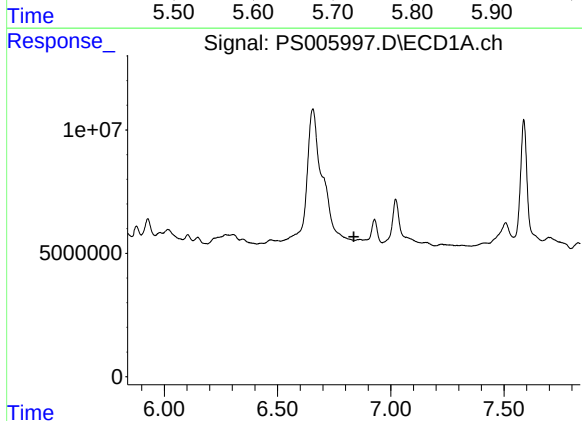


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

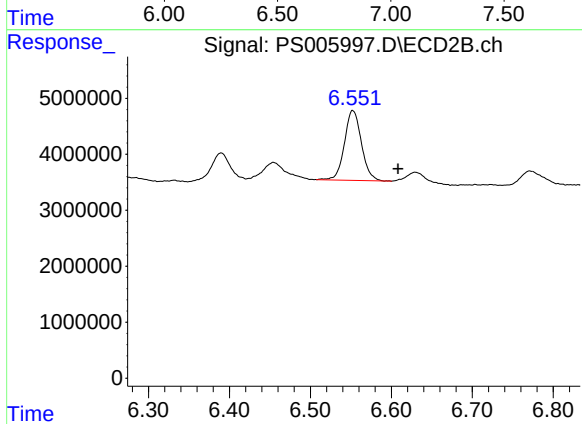

#10 Pentachlorophenol


R.T.: 6.553 min
Delta R.T.: -0.056 min
Response: 18202751
Conc: 1.40 ng/ml

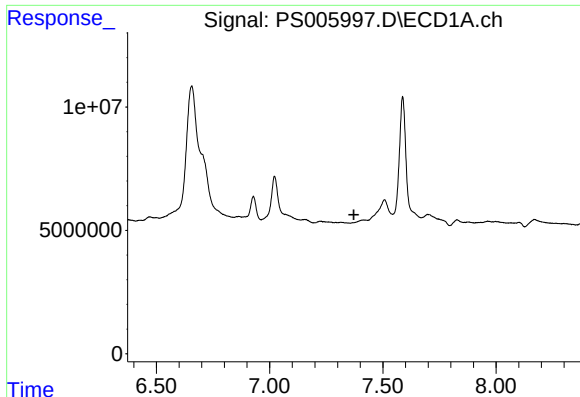

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB122129TB

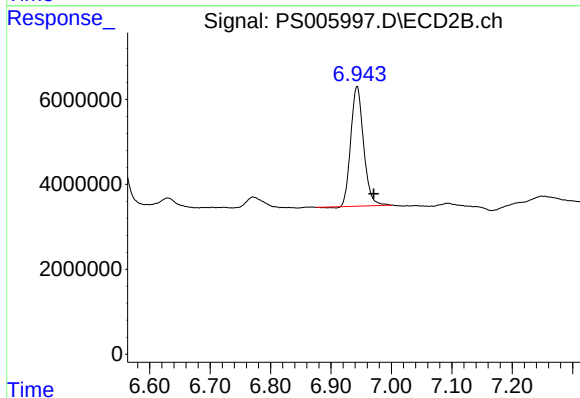


#11 2,4,5-TP (SILVEX)

R.T.: 6.943 min
Delta R.T.: -0.028 min
Response: 41422489
Conc: 7.99 ng/ml

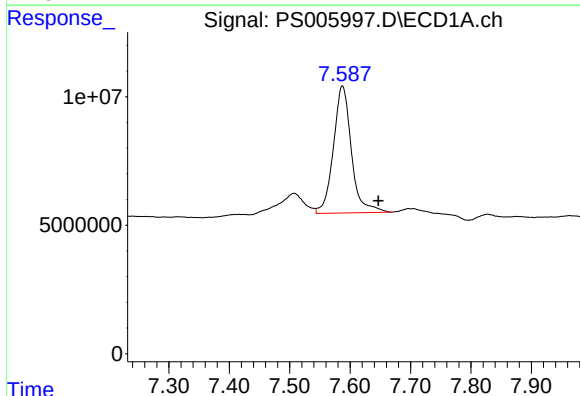


#12 2,4,5-T

R.T.: 7.587 min
Delta R.T.: -0.059 min
Response: 102382924
Conc: 12.27 ng/ml

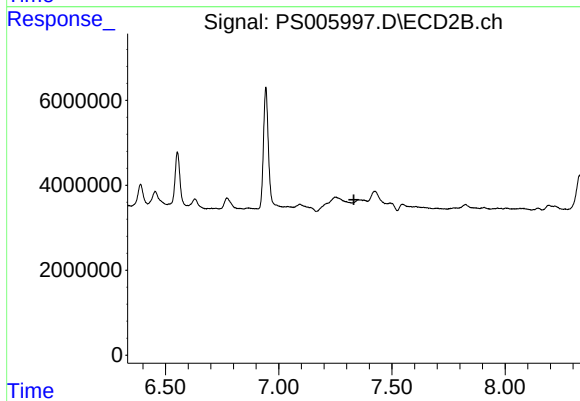

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.

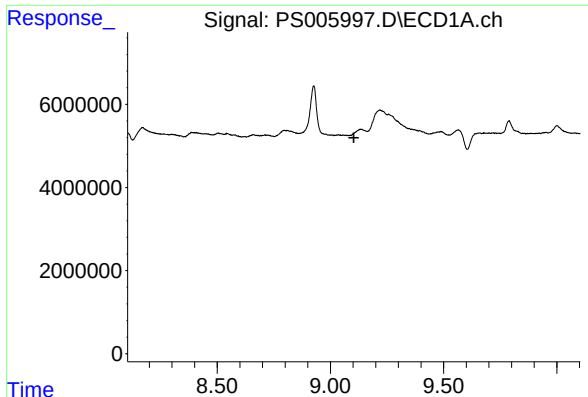

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB122129TB

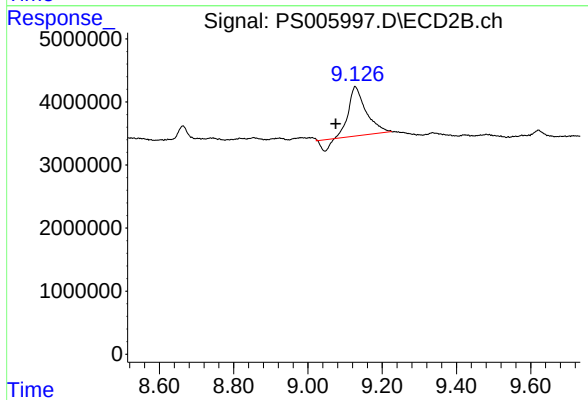

#15 Picloram

R.T.: 9.127 min
Delta R.T.: 0.052 min
Response: 23795403
Conc: 3.17 ng/ml