

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 18:50
 Operator : SM\AJ
 Sample : K4227-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 1S-Q-(0-1)-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:11:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.547	5.267	656.6E6	443.6E6	452.555	445.965
Target Compounds							
1) T	Dalapon	2.047	0.000	20200298	0	10.900	N.D. #
2) T	3,5-DICHL...	0.000	4.586	0	155.9E6	N.D.	120.163
5) T	DICAMBA	5.772	0.000	15747889	0	2.637	N.D. #
9) T	2,4-D	6.627	0.000	252.4E6	0	168.401	N.D. #
10) T	Pentachlo...	6.900	0.000	14227247	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.915	0	43703855	N.D.	8.425
15) T	Picloram	0.000	9.097	0	14836185	N.D.	1.975
16) T	DCPA	0.000	9.097	0	14836185	N.D.	2.250



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 18:50
Operator : SM\AJ
Sample : K4227-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
1S-Q-(0-1)-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:11:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

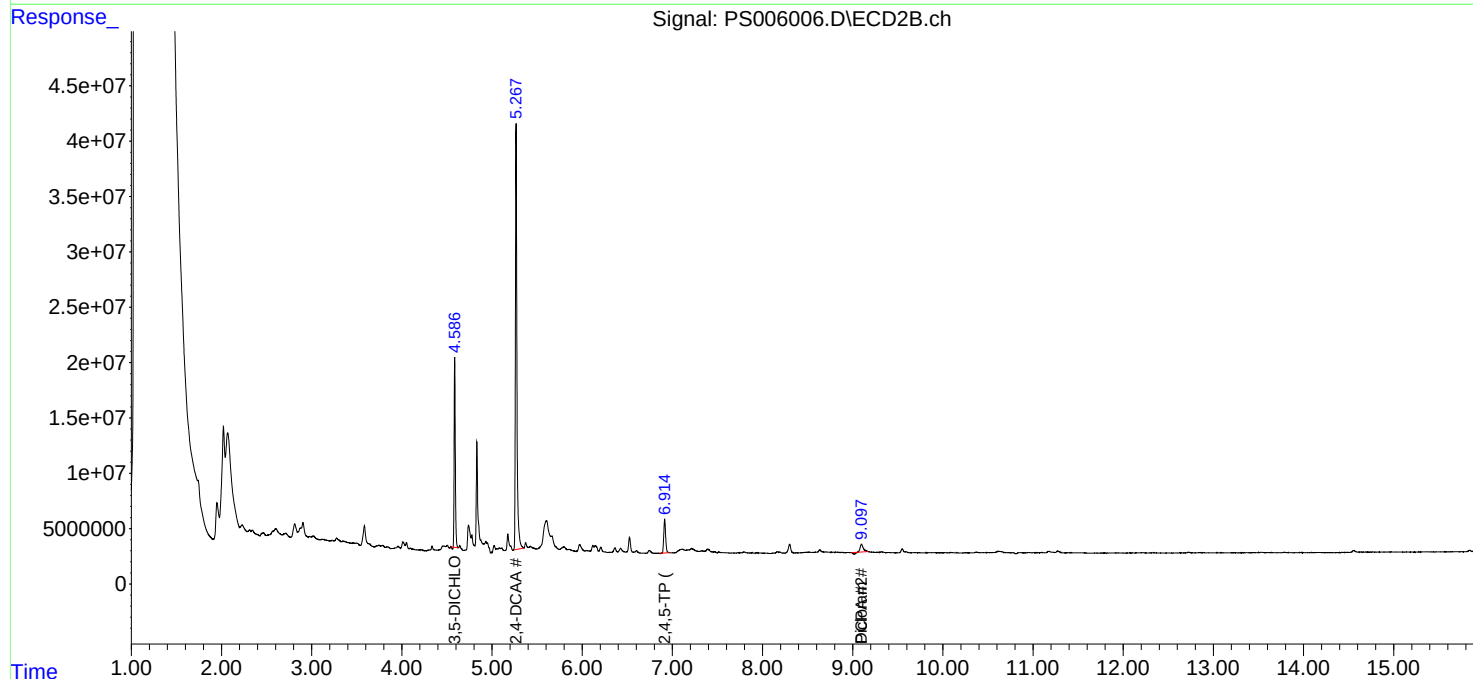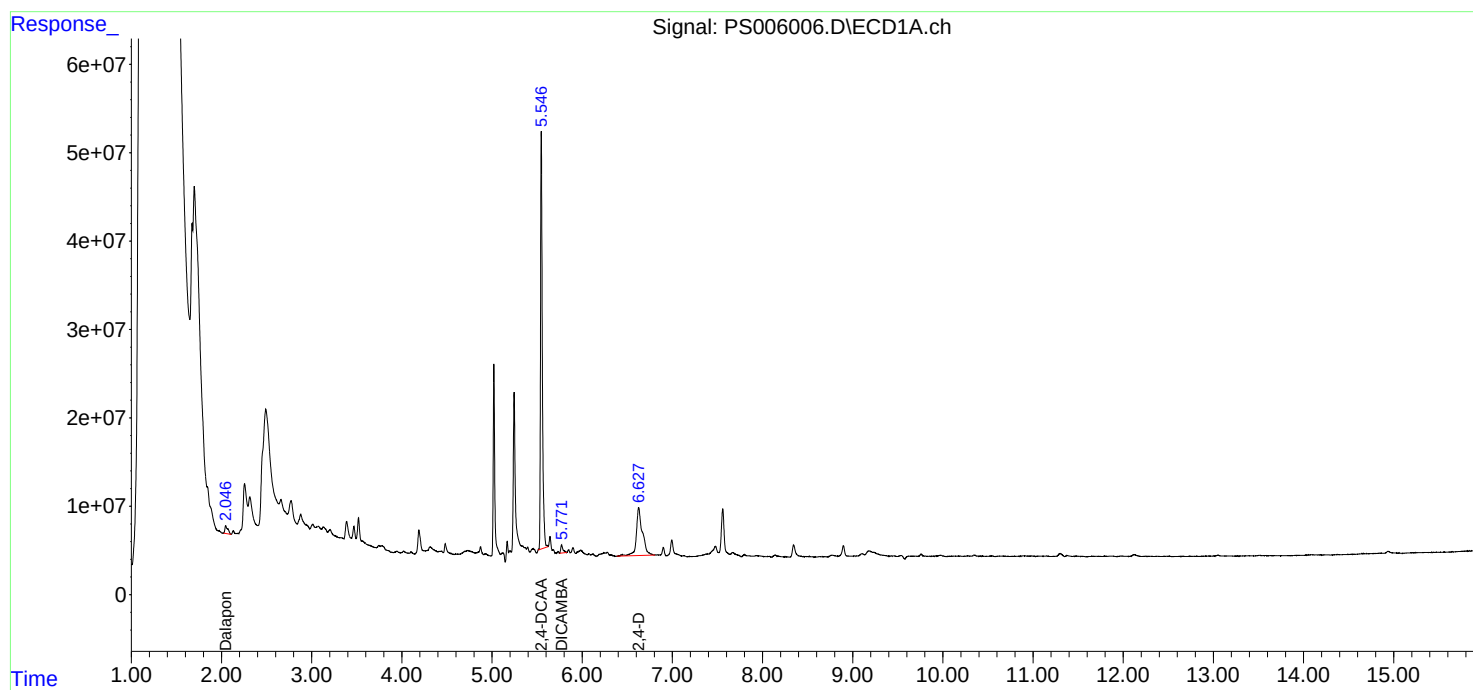


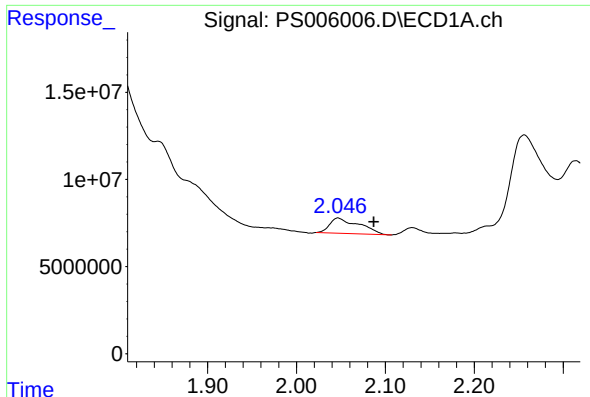

#1 Dalapon


R.T.: 2.047 min
Delta R.T.: -0.040 min
Response: 20200298
Conc: 10.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
1S-Q-(0-1)-COMP

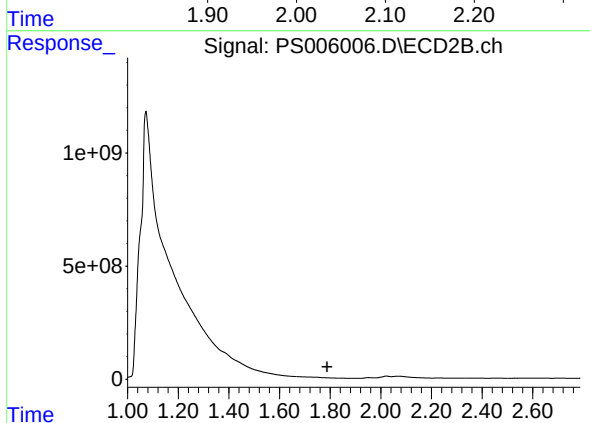


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

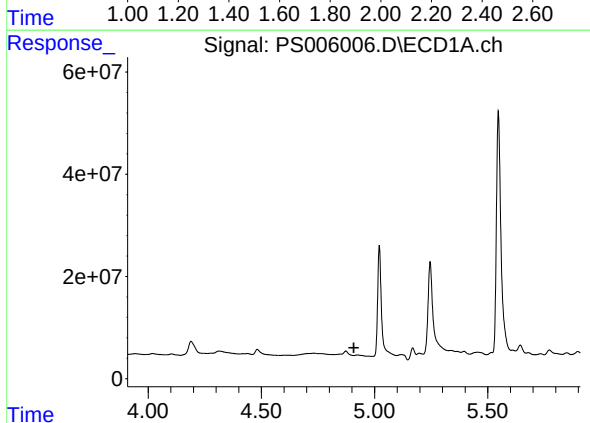


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

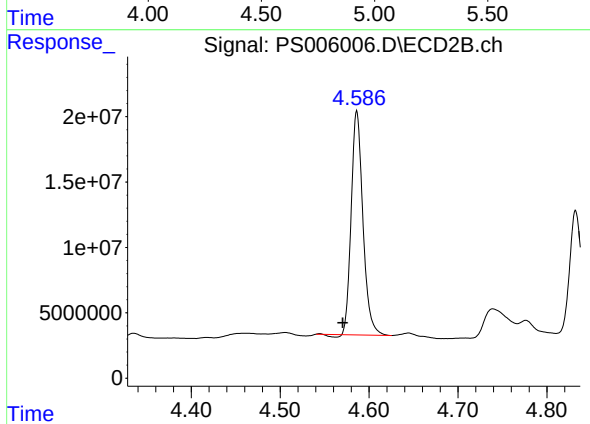

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.586 min
Delta R.T.: 0.016 min
Response: 155889378
Conc: 120.16 ng/ml

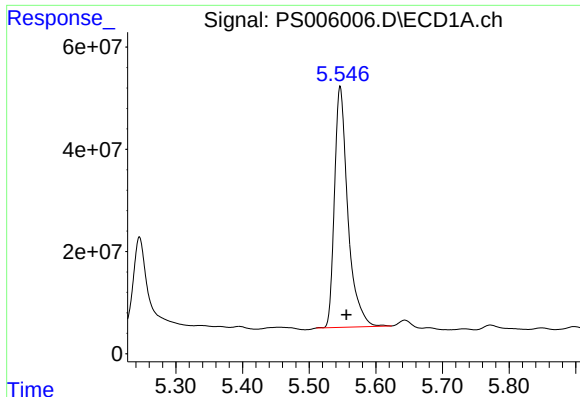

#4 2,4-DCAA


R.T.: 5.547 min
Delta R.T.: -0.009 min
Response: 656574883
Conc: 452.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
1S-Q-(0-1)-COMP

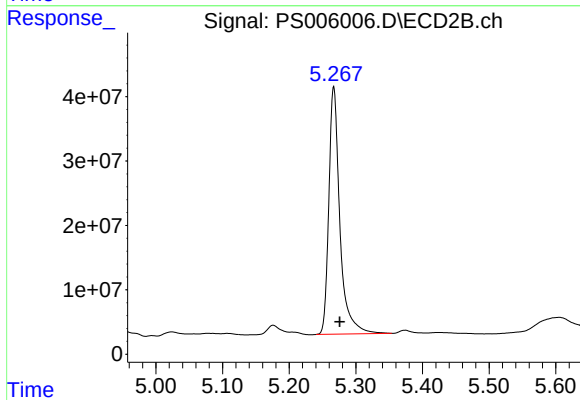


#4 2,4-DCAA

R.T.: 5.267 min
Delta R.T.: -0.009 min
Response: 443591559
Conc: 445.96 ng/ml

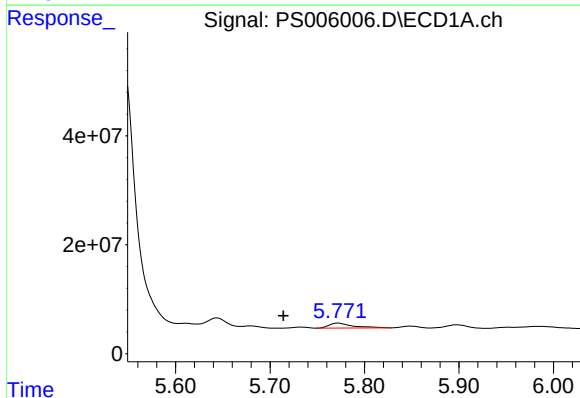


#5 DICAMBA

R.T.: 5.772 min
Delta R.T.: 0.058 min
Response: 15747889
Conc: 2.64 ng/ml

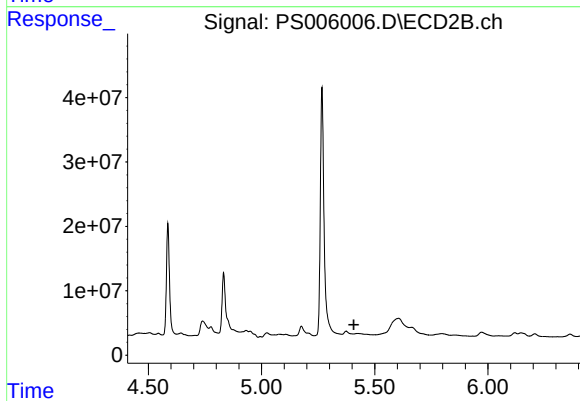

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

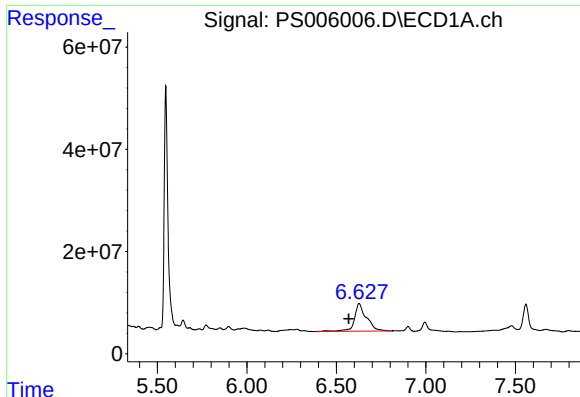

#9 2,4-D


R.T.: 6.627 min
Delta R.T.: 0.058 min
Response: 252376676
Conc: 168.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
1S-Q-(0-1)-COMP

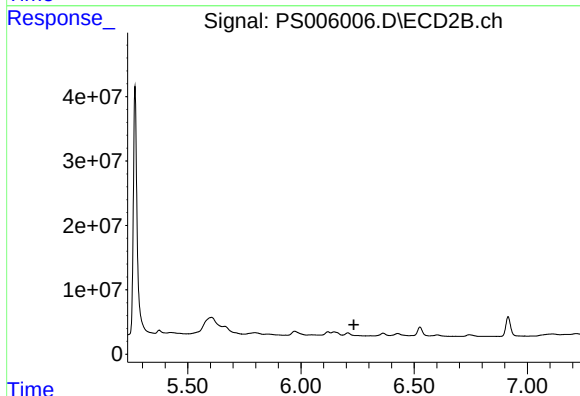


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

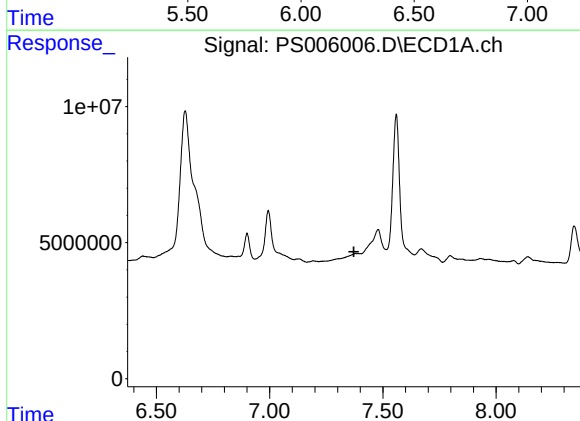


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.372 min
Response: 0
Conc: N.D.

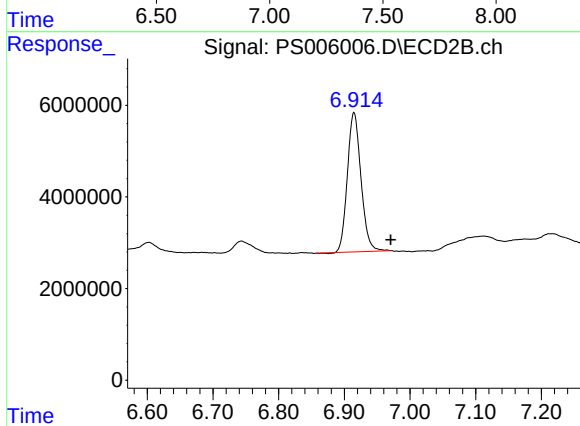

#11 2,4,5-TP (SILVEX)


R.T.: 6.915 min
Delta R.T.: -0.056 min
Response: 43703855
Conc: 8.43 ng/ml

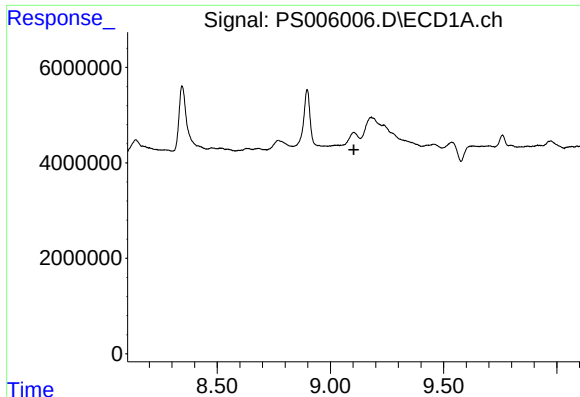

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
1S-Q-(0-1)-COMP

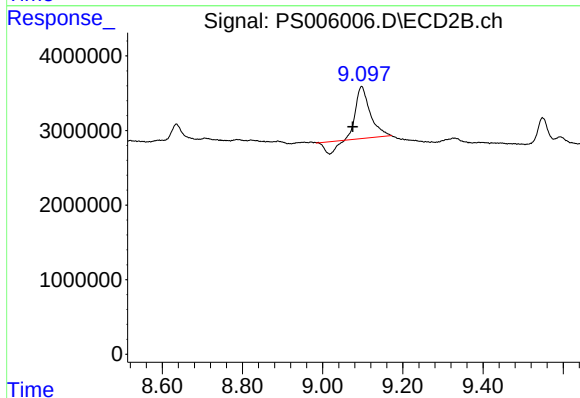


#15 Picloram

R.T.: 9.097 min
Delta R.T.: 0.022 min
Response: 14836185
Conc: 1.97 ng/ml

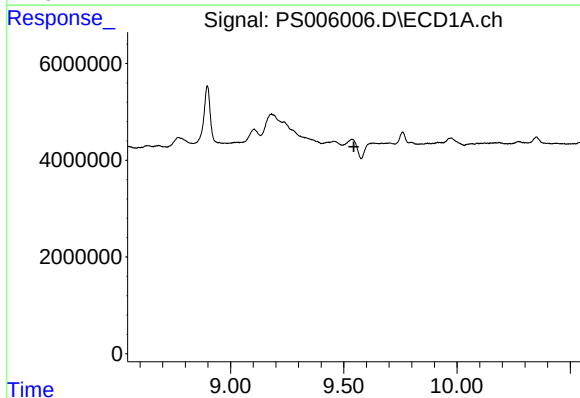

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.545 min
Response: 0
Conc: N.D.

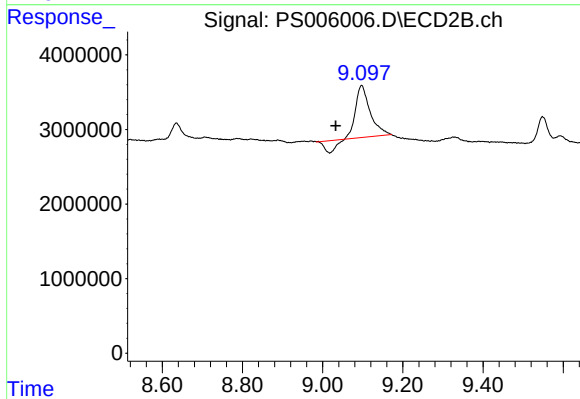

#16 DCPA

R.T.: 9.097 min
Delta R.T.: 0.064 min
Response: 14836185
Conc: 2.25 ng/ml