

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 20:19
 Operator : SM\AJ
 Sample : K4228-27
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 2S-F1-F4-COMP-(1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:13:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.561	5.281	933.2E6	610.5E6	643.199	613.797
Target Compounds							
2) T	3,5-DICHL...	0.000	4.601	0	191.6E6	N.D.	147.673
5) T	DICAMBA	0.000	5.388	0	9700061	N.D.	2.598
7) T	MCPA	0.000	5.620	0	113.6E6	N.D.	26.979
10) T	Pentachlo...	0.000	6.540	0	22642705	N.D.	1.744
11) T	2,4,5-TP ...	0.000	6.929	0	57186346	N.D.	11.024



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 20:19
Operator : SM\AJ
Sample : K4228-27
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:13:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

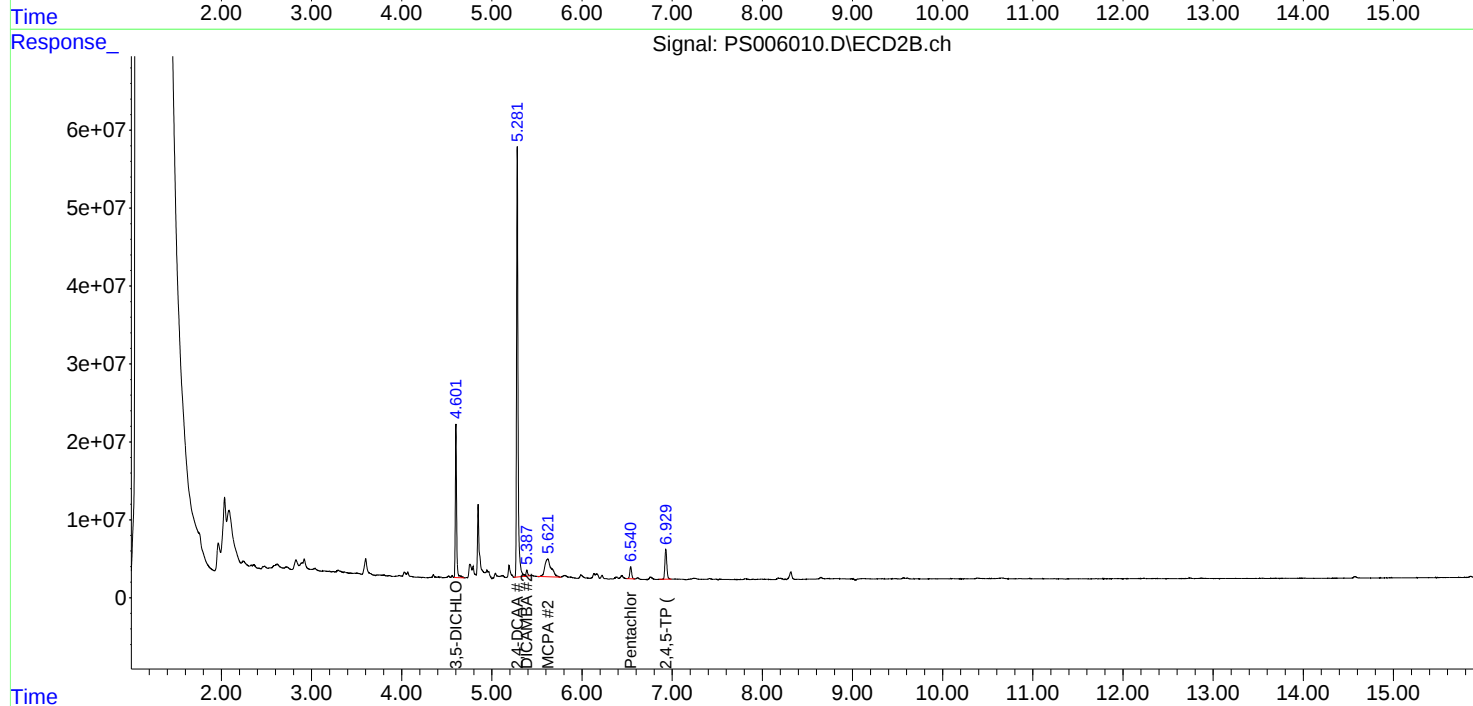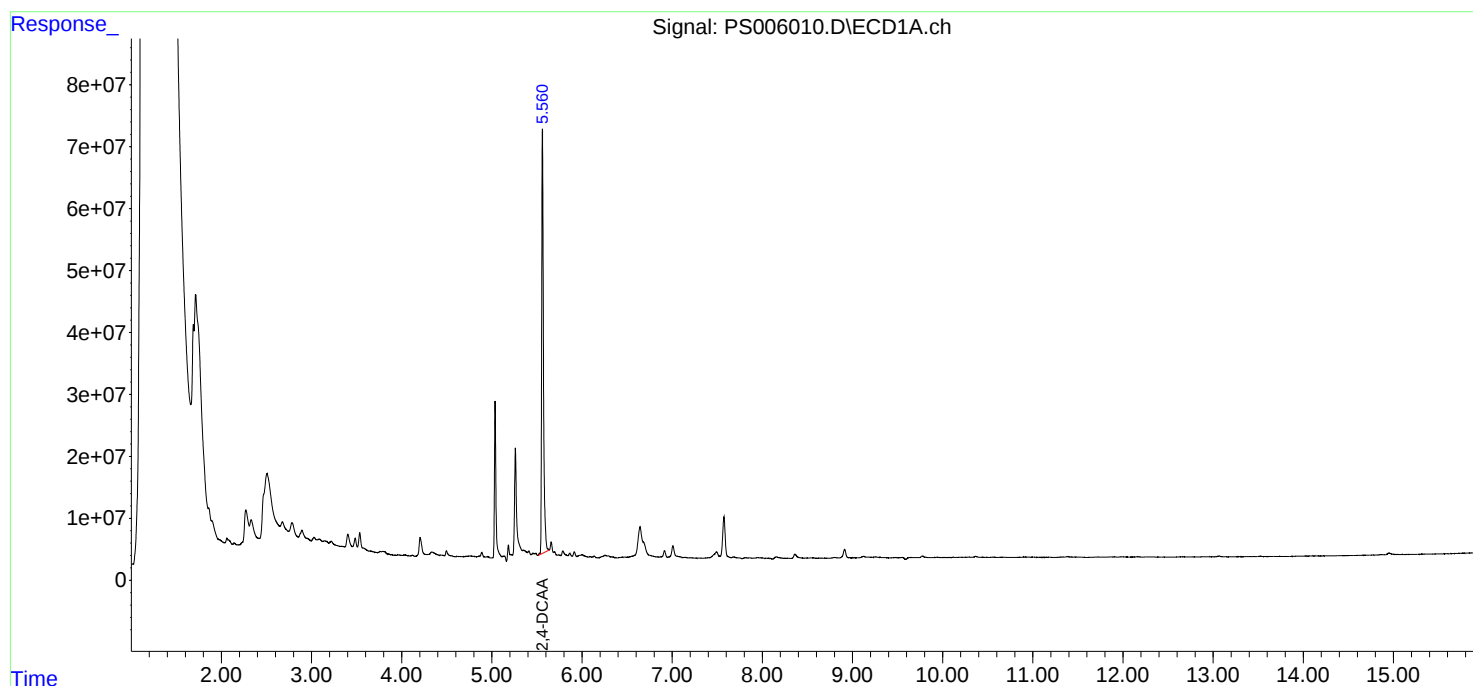


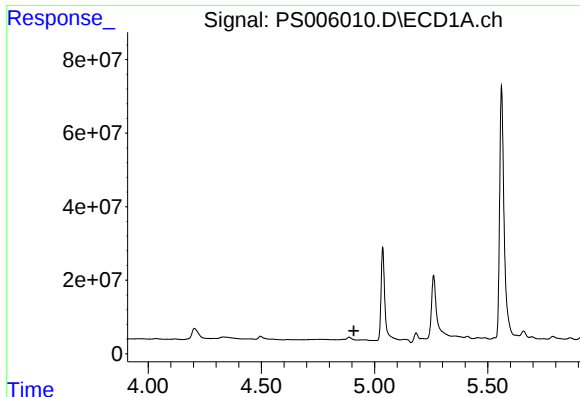

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(1)

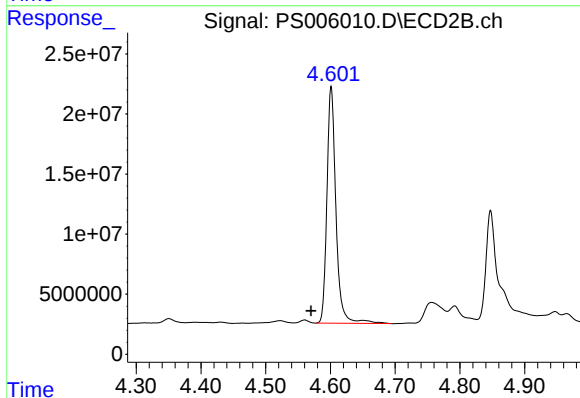


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.601 min
Delta R.T.: 0.031 min
Response: 191578545
Conc: 147.67 ng/ml

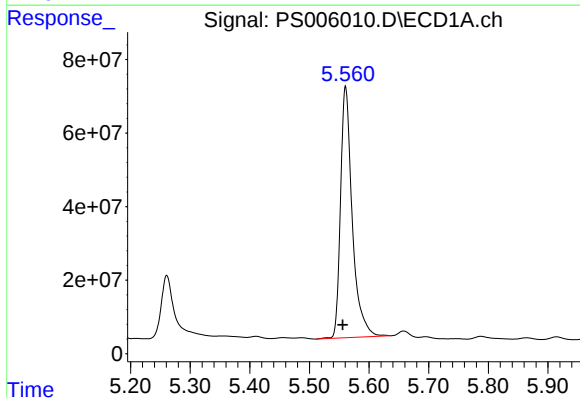


#4 2,4-DCAA

R.T.: 5.561 min
Delta R.T.: 0.005 min
Response: 933165250
Conc: 643.20 ng/ml

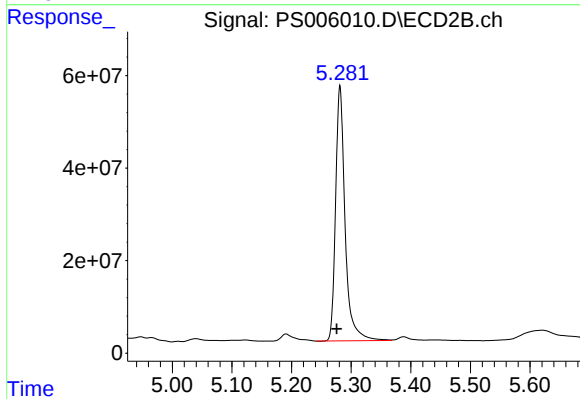

#4 2,4-DCAA


R.T.: 5.281 min
Delta R.T.: 0.006 min
Response: 610530950
Conc: 613.80 ng/ml

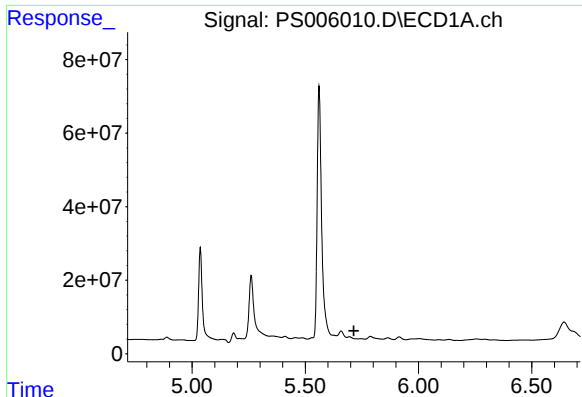

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.714 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(1)

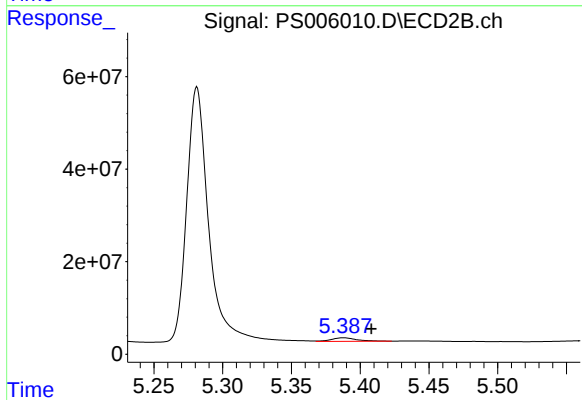


#5 DICAMBA

R.T.: 5.388 min
Delta R.T.: -0.020 min
Response: 9700061
Conc: 2.60 ng/ml

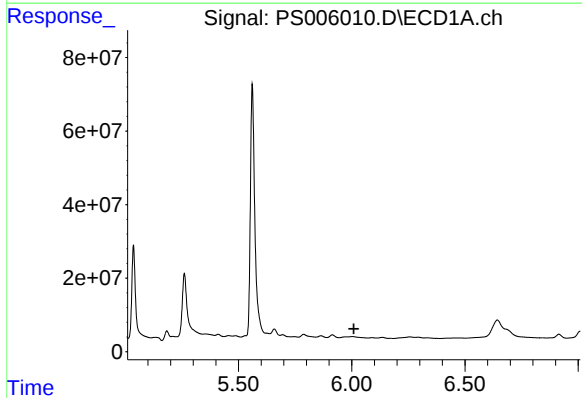


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

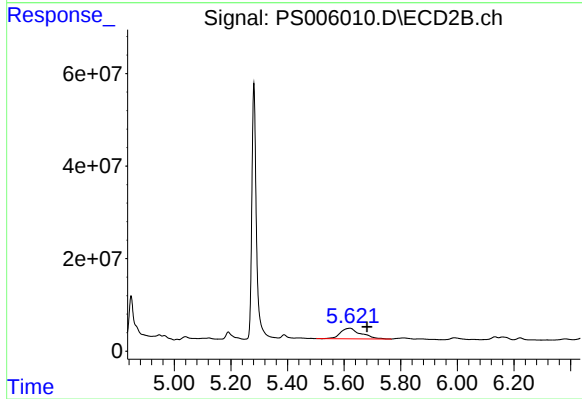

#7 MCPA


R.T.: 5.620 min
Delta R.T.: -0.061 min
Response: 113556122
Conc: 26.98 ug/ml

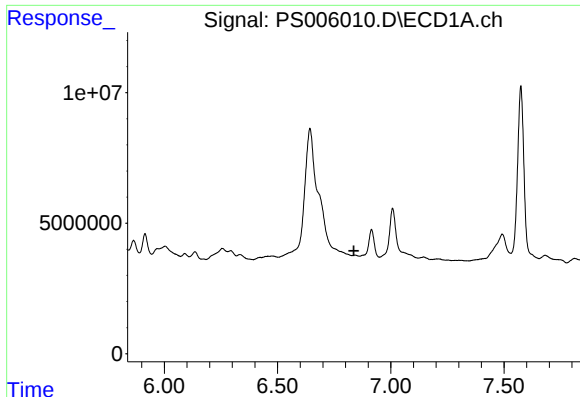

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(1)

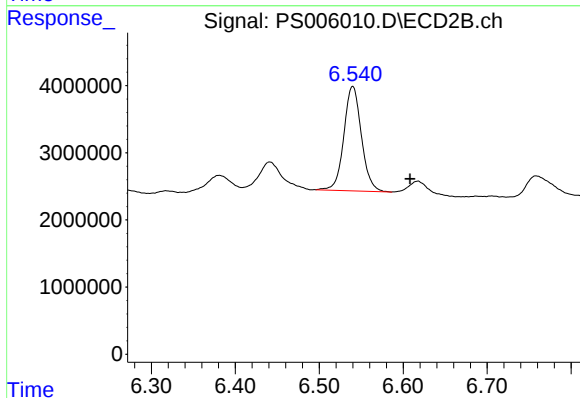


#10 Pentachlorophenol

R.T.: 6.540 min
Delta R.T.: -0.069 min
Response: 22642705
Conc: 1.74 ng/ml

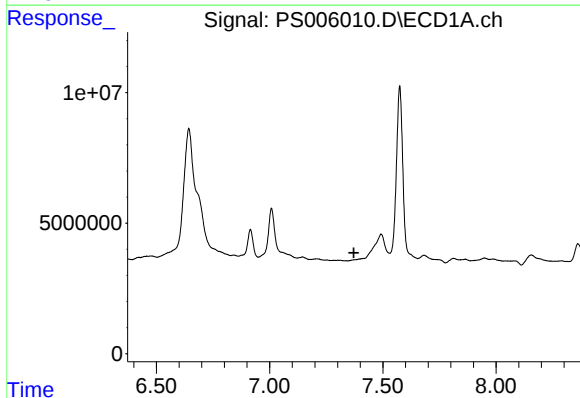

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

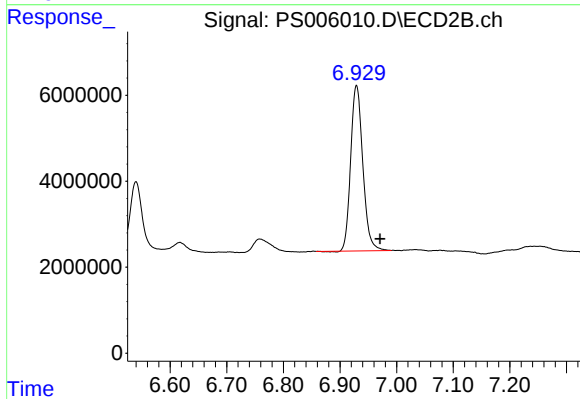

#11 2,4,5-TP (SILVEX)

R.T.: 6.929 min
Delta R.T.: -0.041 min
Response: 57186346
Conc: 11.02 ng/ml