

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 20:41
 Operator : SM\AJ
 Sample : K4228-32
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 2S-I1-I4-COMP-(0-1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:14:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.598	5.318	877.3E6	584.1E6	604.725	587.221
Target Compounds							
1) T	Dalapon	2.099	0.000	25270397	0	13.635	N.D. #
2) T	3,5-DICHL...	0.000	4.638	0	126.0E6	N.D.	97.155
3) T	4-Nitroph...	0.000	4.884	0	104.2E6	N.D.	210.364
5) T	DICAMBA	5.695	0.000	17483937	0	2.927	N.D. #
7) T	MCPA	0.000	5.656	0	111.7E6	N.D.	26.528
9) T	2,4-D	0.000	6.170	0	1040260	N.D.	<MDL
10) T	Pentachlo...	0.000	6.577	0	21287344	N.D.	1.640
11) T	2,4,5-TP ...	0.000	6.966	0	39683786	N.D.	7.650
12) T	2,4,5-T	7.610	0.000	101.0E6	0	12.101	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 20:41
Operator : SM\AJ
Sample : K4228-32
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(0-1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:14:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

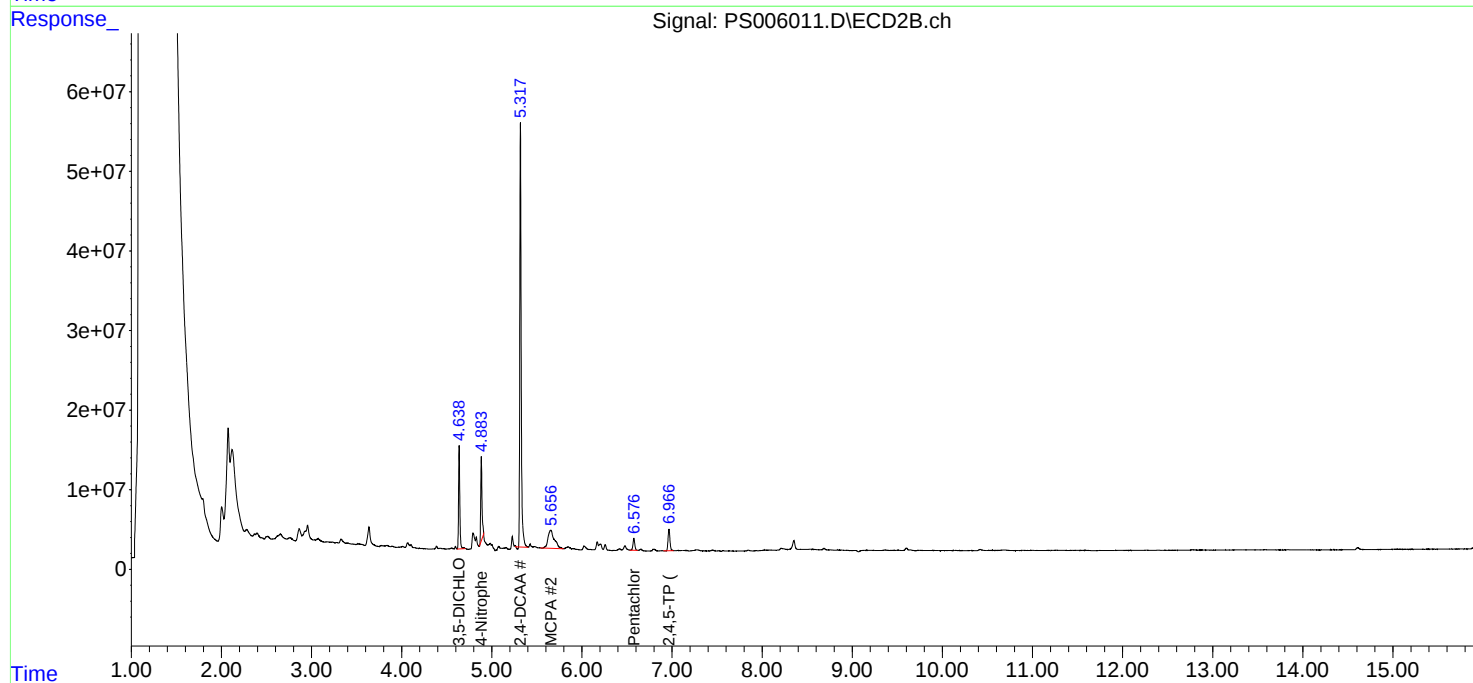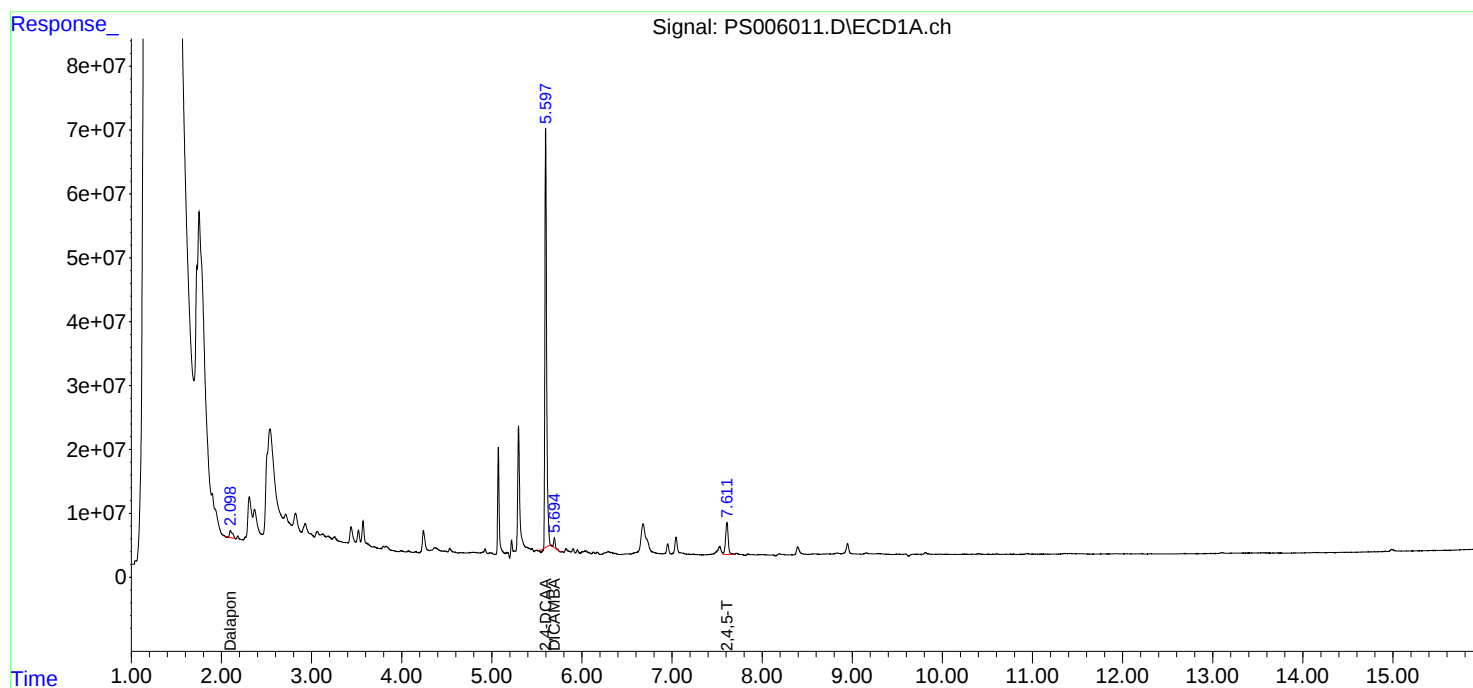


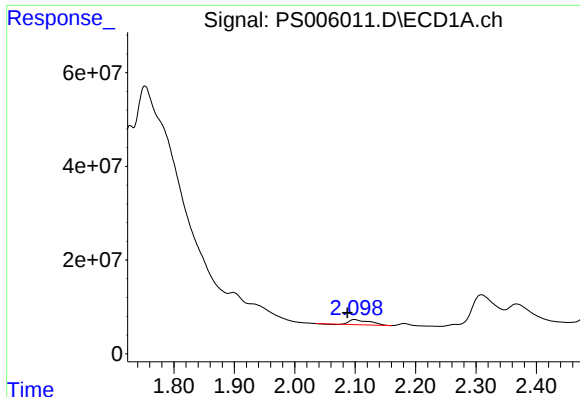

#1 Dalapon


R.T.: 2.099 min
Delta R.T.: 0.012 min
Response: 25270397
Conc: 13.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(0-1)

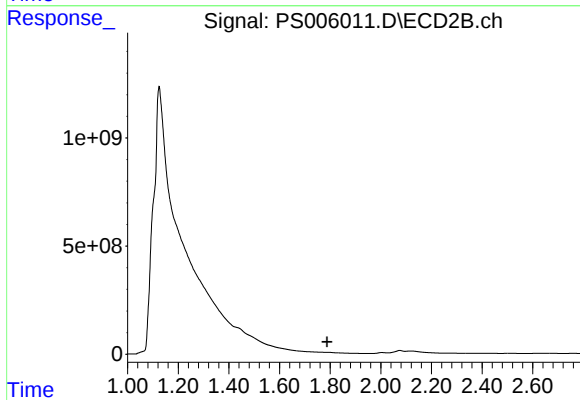


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

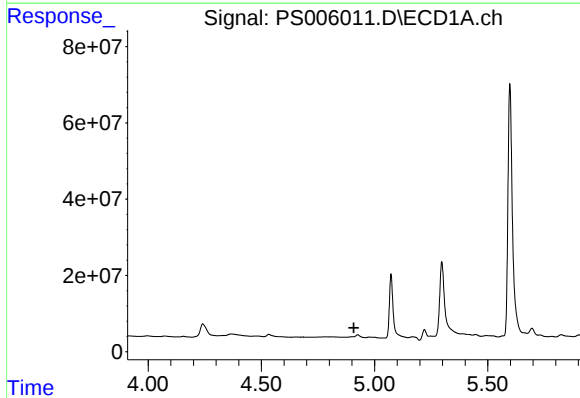


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

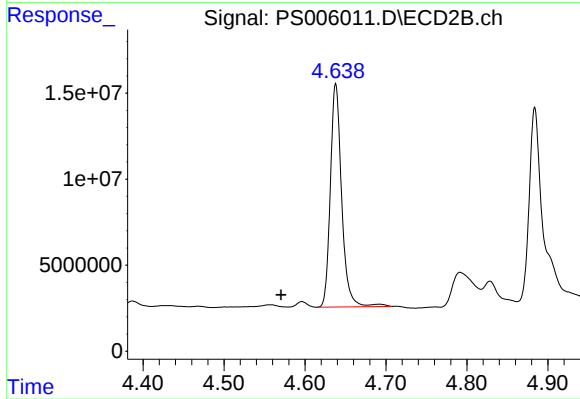

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.638 min
Delta R.T.: 0.068 min
Response: 126040558
Conc: 97.15 ng/ml

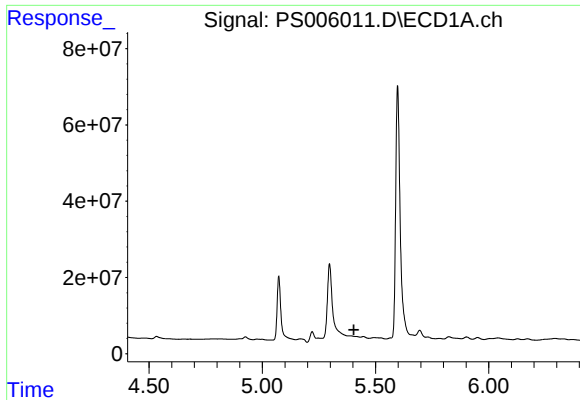

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(0-1)

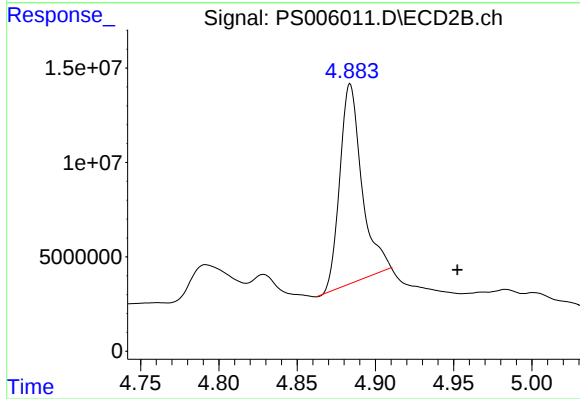


#3 4-Nitrophenol

R.T.: 4.884 min
Delta R.T.: -0.068 min
Response: 104211017
Conc: 210.36 ng/ml

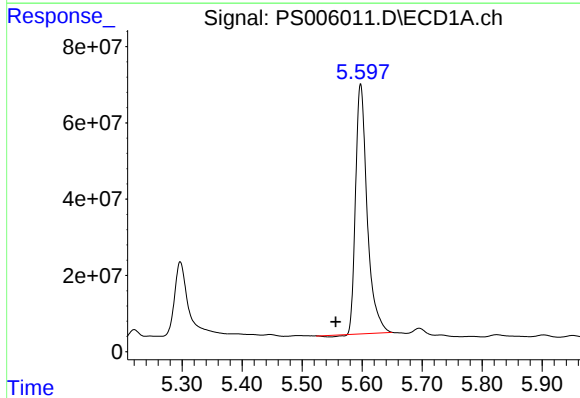


#4 2,4-DCAA

R.T.: 5.598 min
Delta R.T.: 0.042 min
Response: 877345872
Conc: 604.73 ng/ml

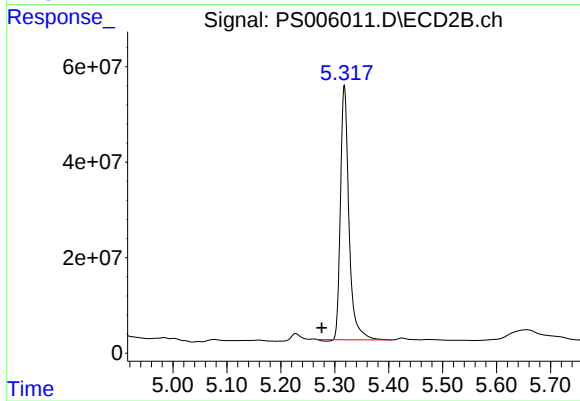

#4 2,4-DCAA


R.T.: 5.318 min
Delta R.T.: 0.042 min
Response: 584095717
Conc: 587.22 ng/ml

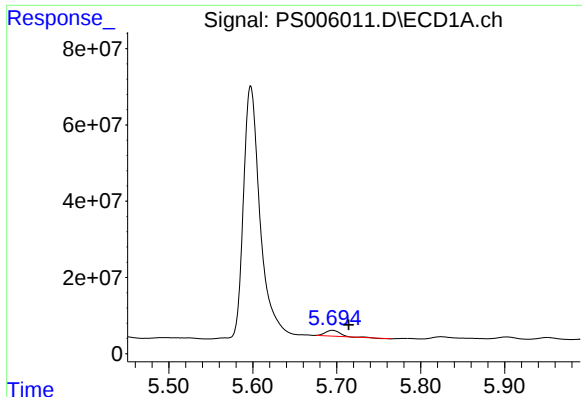

#5 DICAMBA


R.T.: 5.695 min
Delta R.T.: -0.019 min
Response: 17483937
Conc: 2.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(0-1)

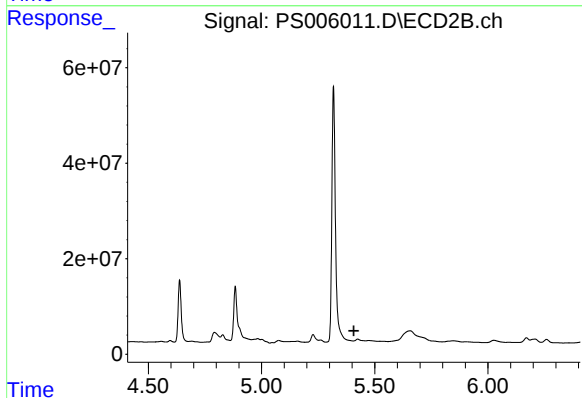


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

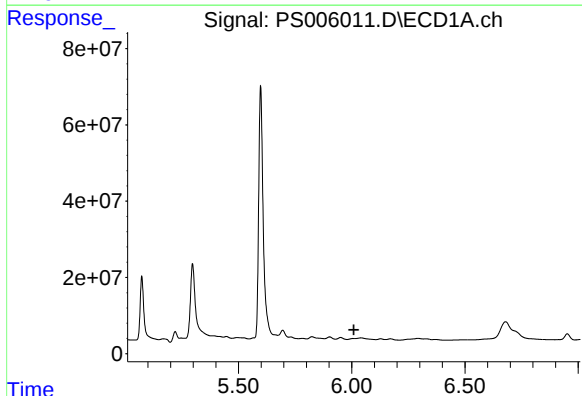


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

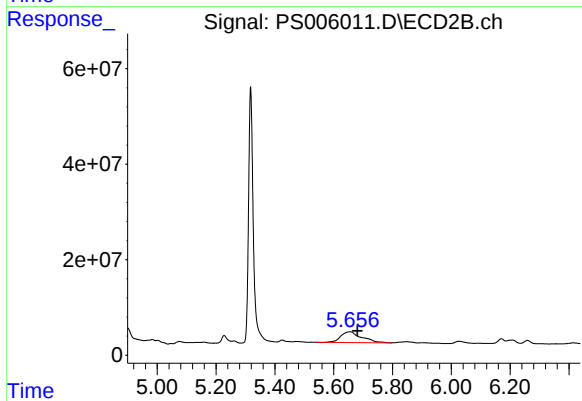

#7 MCPA


R.T.: 5.656 min
Delta R.T.: -0.025 min
Response: 111655143
Conc: 26.53 ug/ml

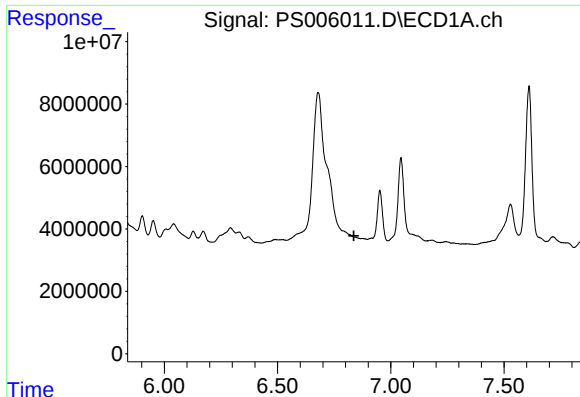

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(0-1)

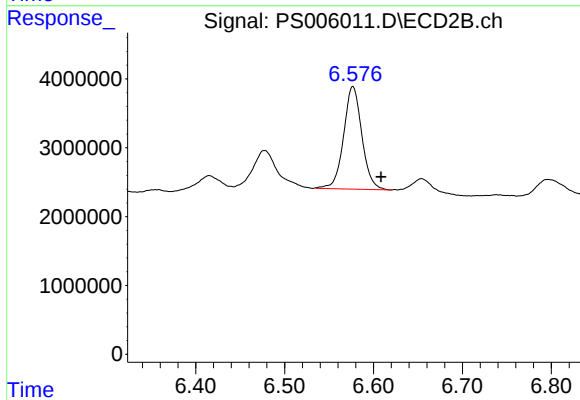


#10 Pentachlorophenol

R.T.: 6.577 min
Delta R.T.: -0.032 min
Response: 21287344
Conc: 1.64 ng/ml

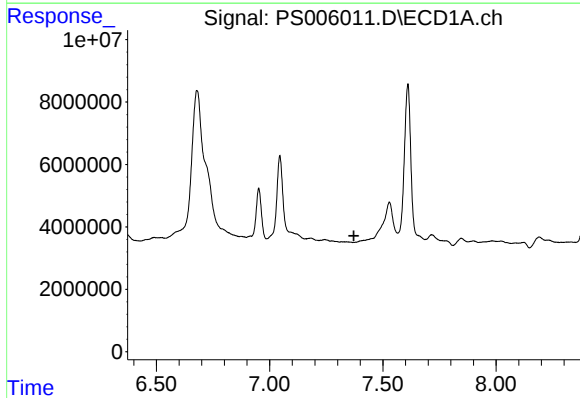


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

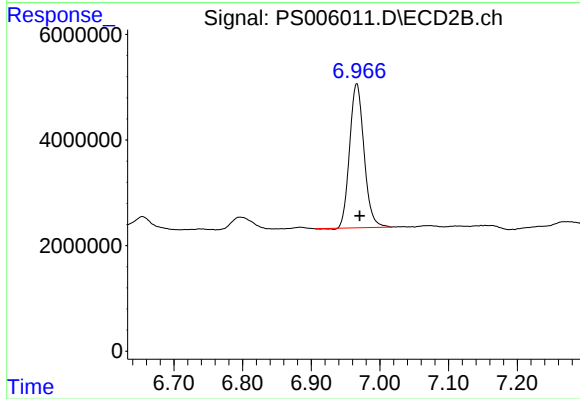

#11 2,4,5-TP (SILVEX)


R.T.: 6.966 min
Delta R.T.: -0.004 min
Response: 39683786
Conc: 7.65 ng/ml

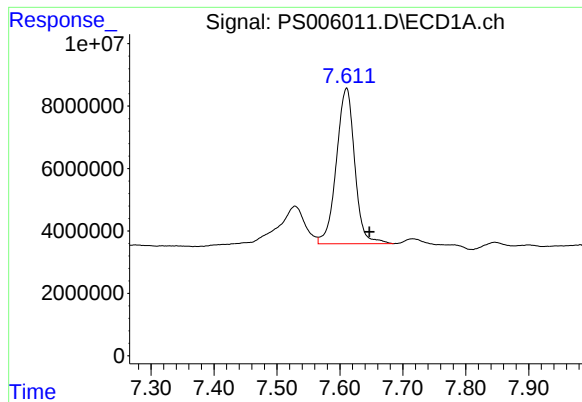

#12 2,4,5-T

R.T.: 7.610 min
Delta R.T.: -0.036 min
Response: 101000156
Conc: 12.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(0-1)

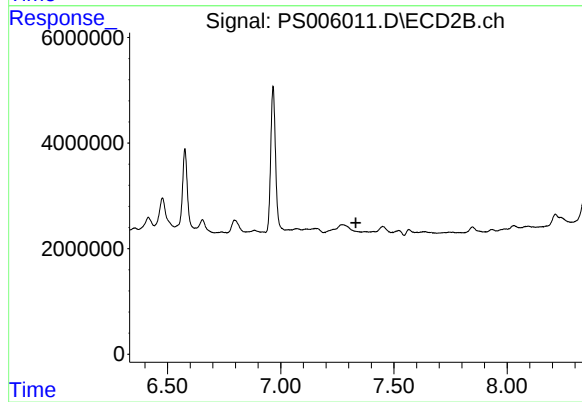

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.