

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 21:03
 Operator : SM\AJ
 Sample : K4228-37
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 2S-I1-I4-COMP-(1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:14:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.584	5.304	769.5E6	525.0E6	530.399	527.848
Target Compounds							
2) T	3,5-DICHL...	0.000	4.624	0	201.6E6	N.D.	155.362
7) T	MCPA	0.000	5.640	0	115.3E6	N.D.	27.387
10) T	Pentachlo...	0.000	6.562	0	17908160	N.D.	1.379
11) T	2,4,5-TP ...	0.000	6.952	0	54028171	N.D.	10.415
12) T	2,4,5-T	7.598	0.000	116.9E6	0	14.000	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 21:03
Operator : SM\AJ
Sample : K4228-37
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:14:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

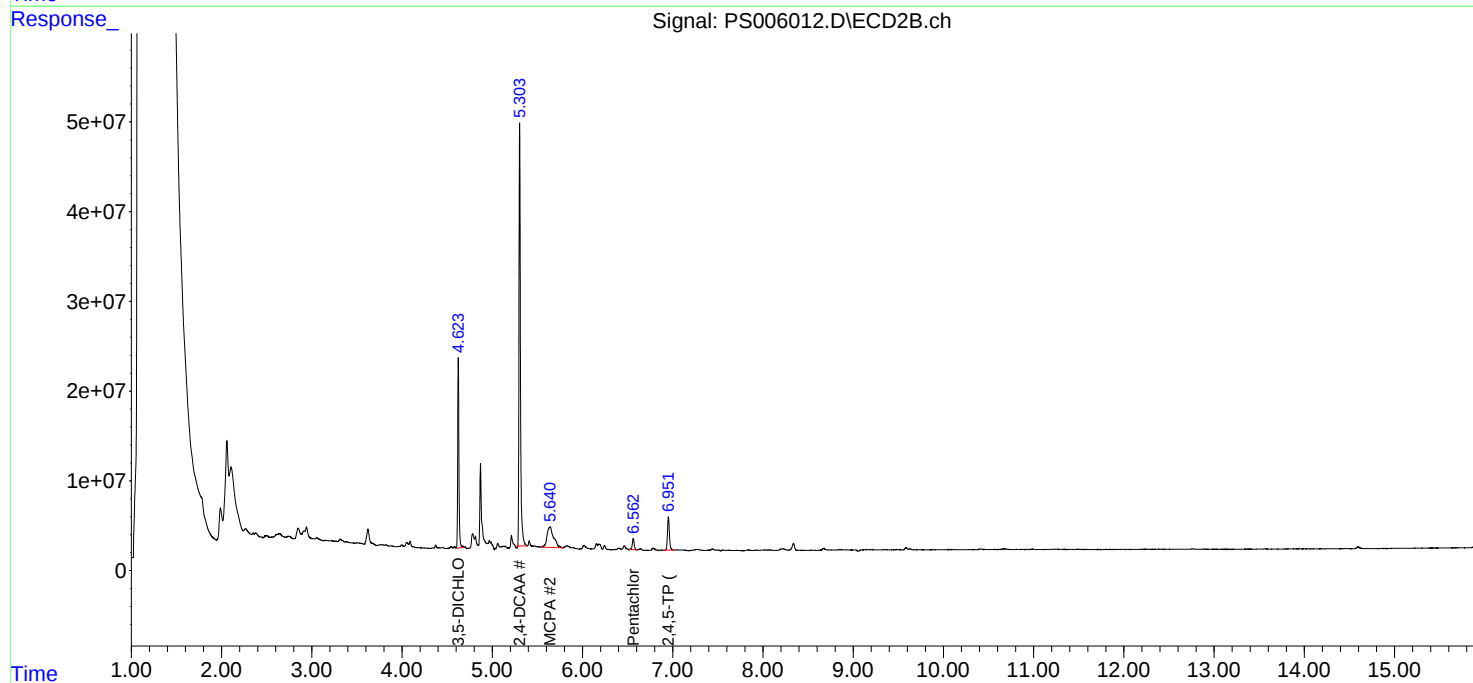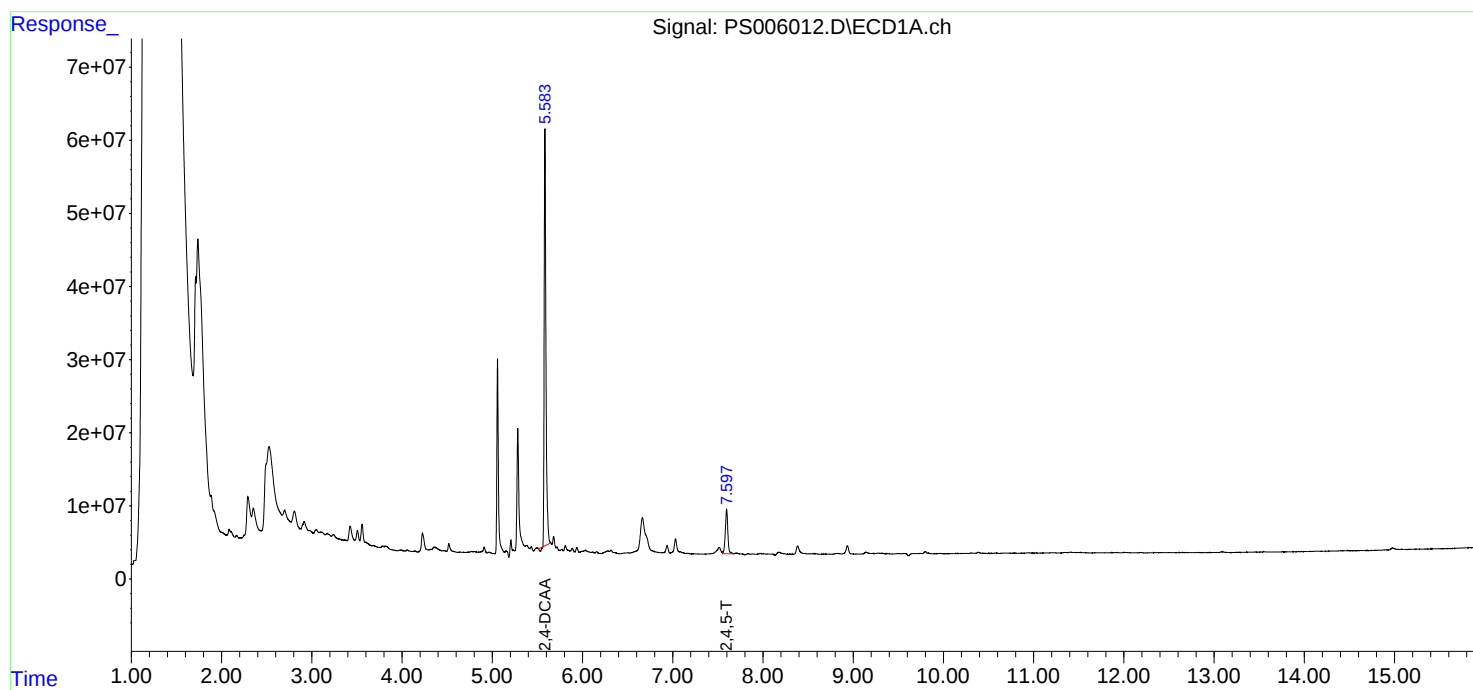


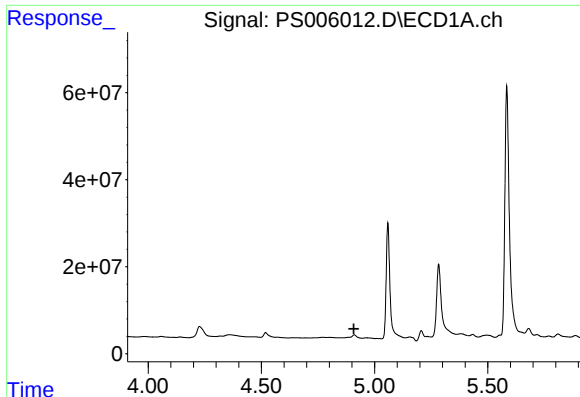

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(1)

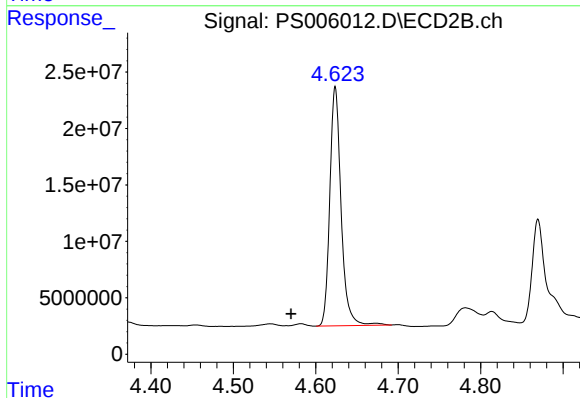


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.624 min
Delta R.T.: 0.054 min
Response: 201553678
Conc: 155.36 ng/ml

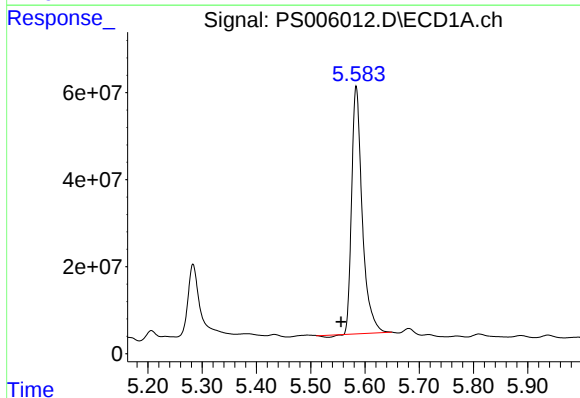


#4 2,4-DCAA

R.T.: 5.584 min
Delta R.T.: 0.028 min
Response: 769512163
Conc: 530.40 ng/ml

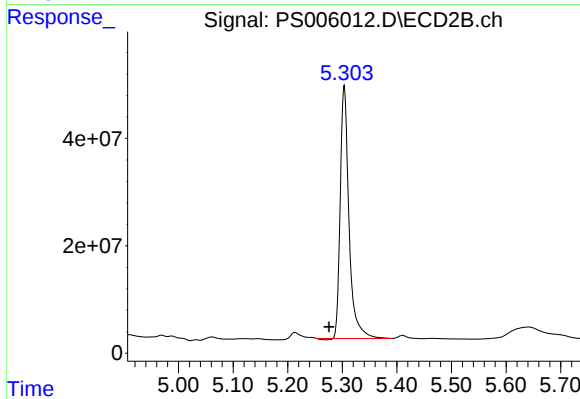

#4 2,4-DCAA


R.T.: 5.304 min
Delta R.T.: 0.028 min
Response: 525039281
Conc: 527.85 ng/ml

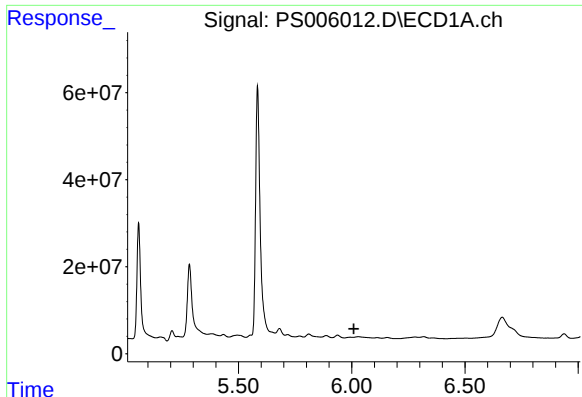

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(1)

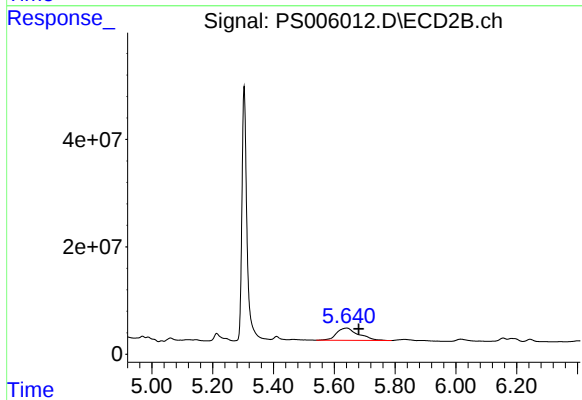


#7 MCPA

R.T.: 5.640 min
Delta R.T.: -0.040 min
Response: 115270585
Conc: 27.39 ug/ml

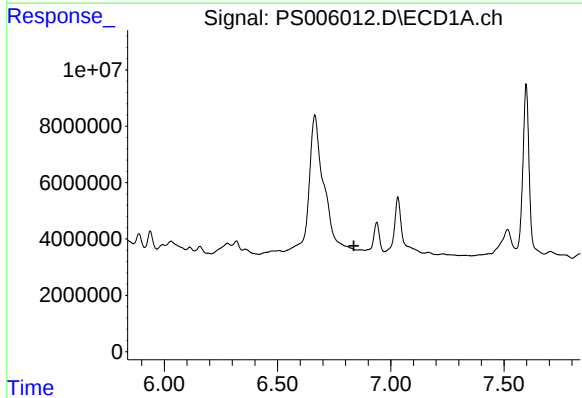


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

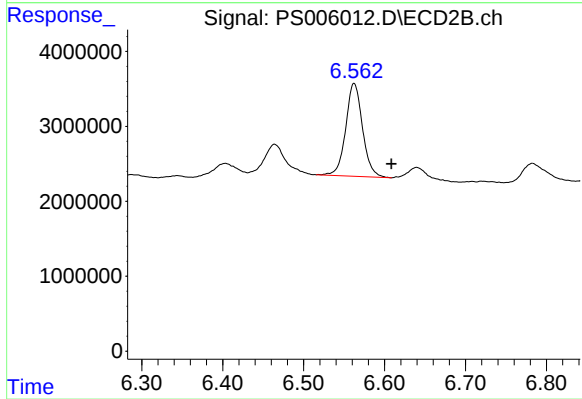

#10 Pentachlorophenol


R.T.: 6.562 min
Delta R.T.: -0.046 min
Response: 17908160
Conc: 1.38 ng/ml

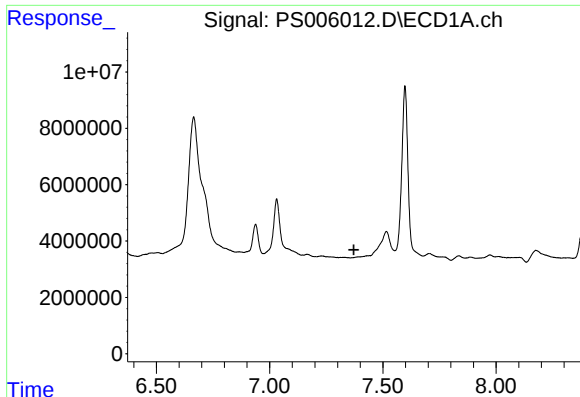

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-I1-I4-COMP-(1)

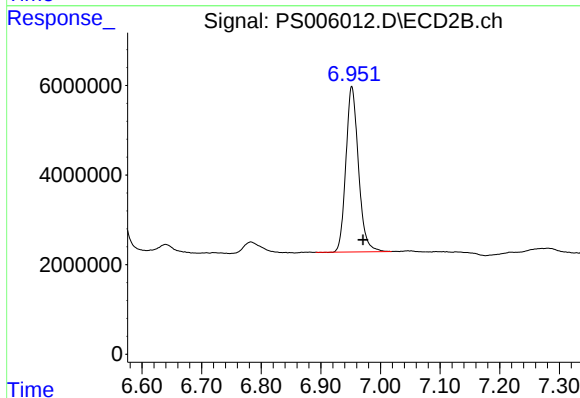


#11 2,4,5-TP (SILVEX)

R.T.: 6.952 min
Delta R.T.: -0.019 min
Response: 54028171
Conc: 10.42 ng/ml

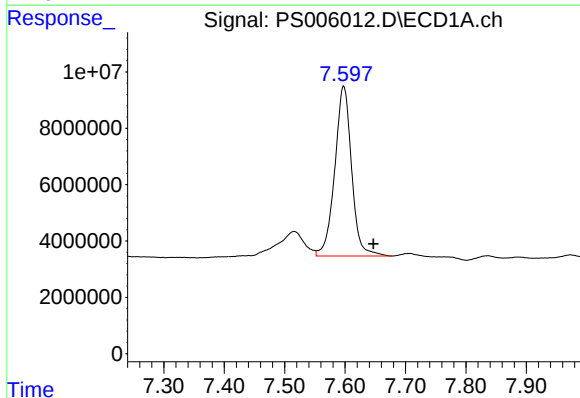

#12 2,4,5-T

R.T.: 7.598 min
Delta R.T.: -0.049 min
Response: 116852020
Conc: 14.00 ng/ml

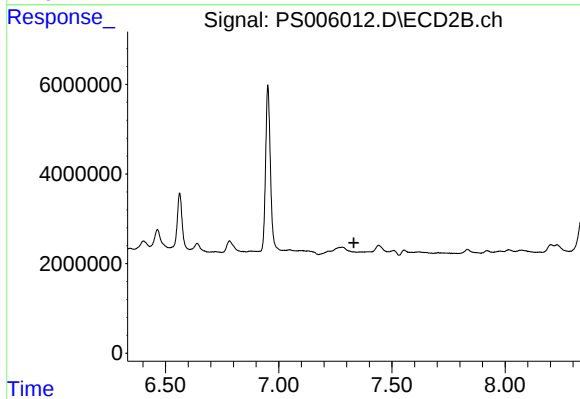

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.