

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 22:10
 Operator : SM\AJ
 Sample : K4245-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:15:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.597	5.317	934.6E6	665.7E6	644.162	669.231
Target Compounds							
2) T	3,5-DICHL...	0.000	4.637	0	230.7E6	N.D.	177.817
3) T	4-Nitroph...	0.000	4.883	0	187.2E6	N.D.	377.811
5) T	DICAMBA	5.695	5.423	22867491	8984749	3.829	2.407 #
7) T	MCPA	0.000	5.646	0	118.7E6	N.D.	28.209
8) T	DICHLORPROP	6.332	0.000	16772663	0	11.663	N.D. #
9) T	2,4-D	0.000	6.169	0	5268448	N.D.	4.904
10) T	Pentachlo...	0.000	6.576	0	23724335	N.D.	1.827
11) T	2,4,5-TP ...	0.000	6.965	0	73546992	N.D.	14.178
12) T	2,4,5-T	7.611	0.000	159.7E6	0	19.135	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 22:10
Operator : SM\AJ
Sample : K4245-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:15:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

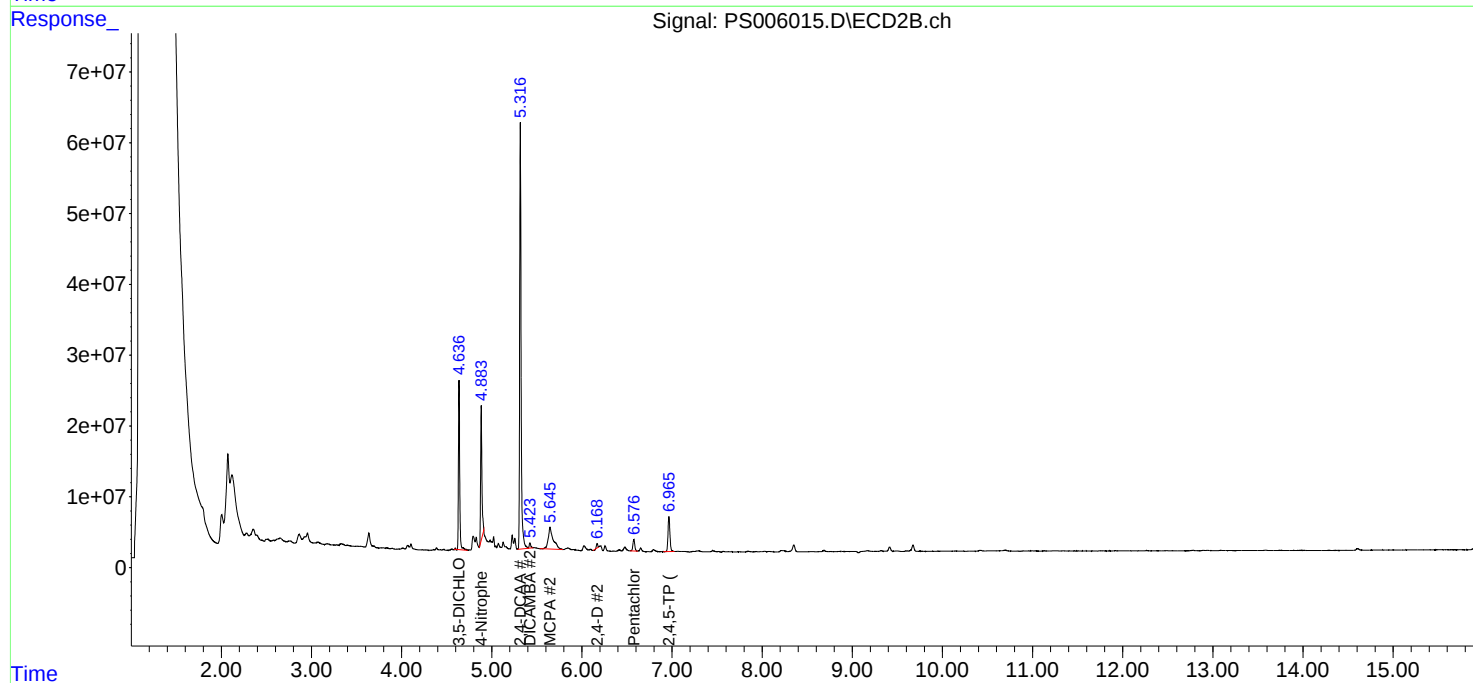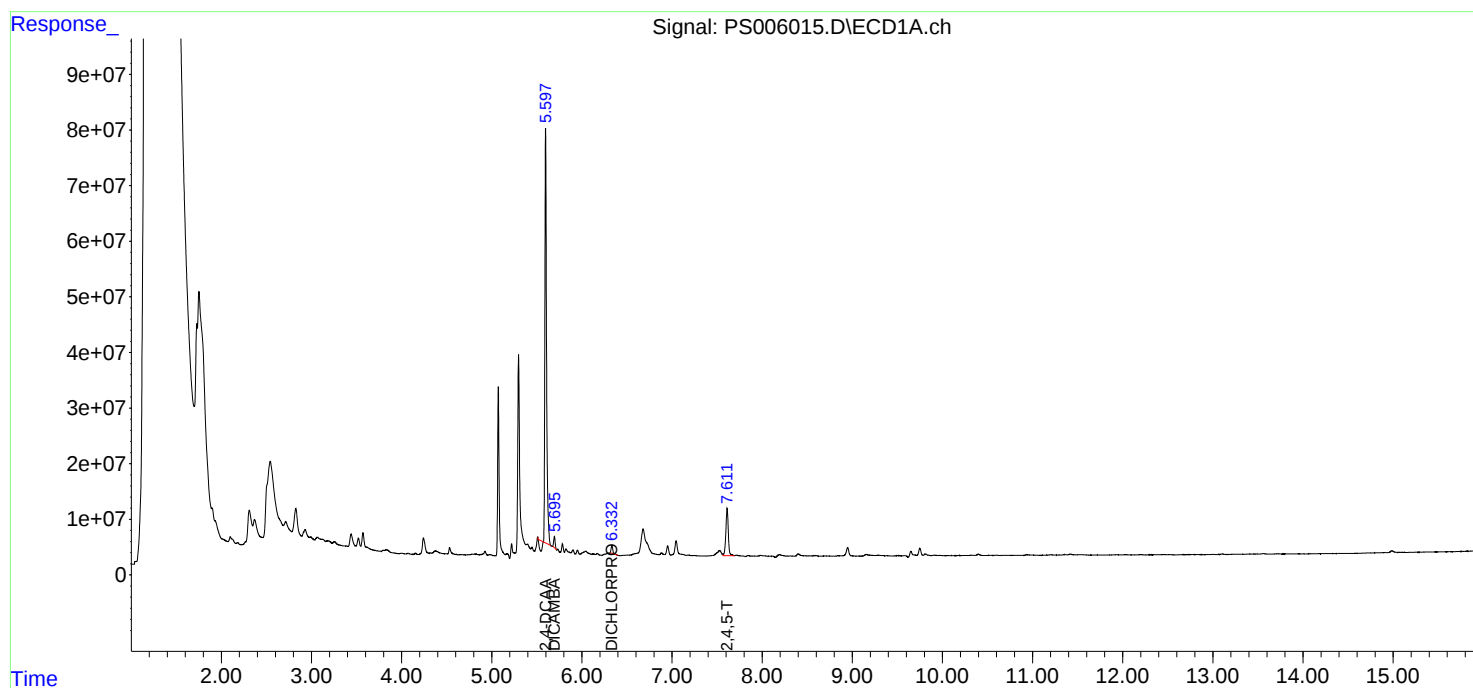


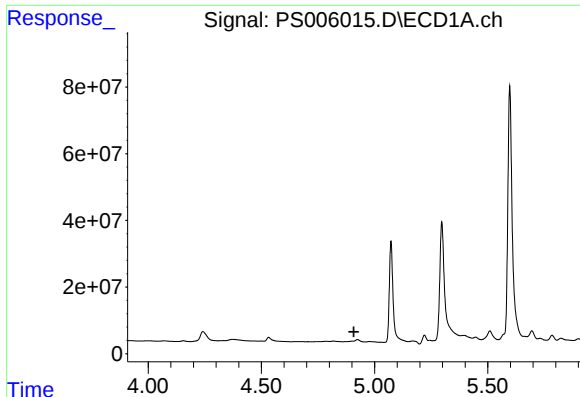

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-25

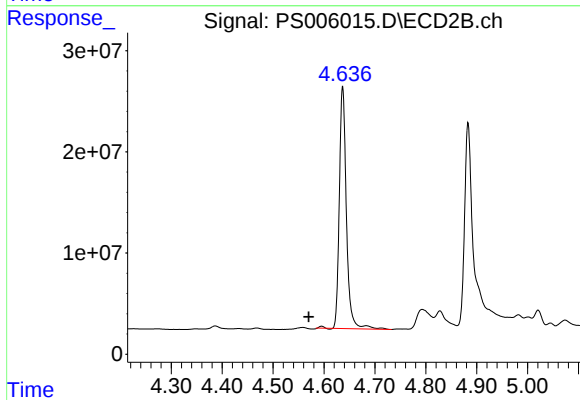


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.637 min
Delta R.T.: 0.067 min
Response: 230684574
Conc: 177.82 ng/ml

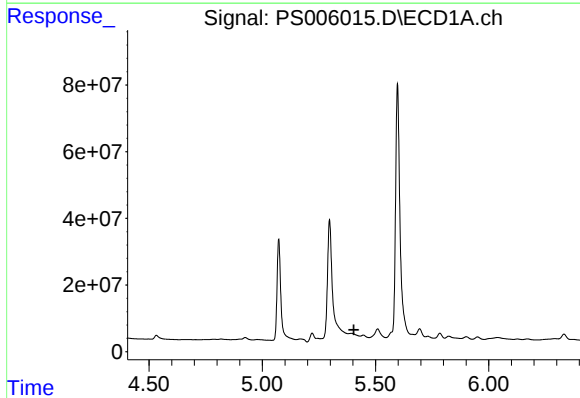


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

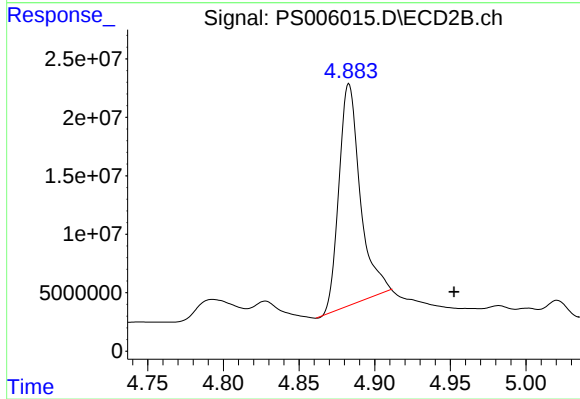

#3 4-Nitrophenol


R.T.: 4.883 min
Delta R.T.: -0.069 min
Response: 187161056
Conc: 377.81 ng/ml

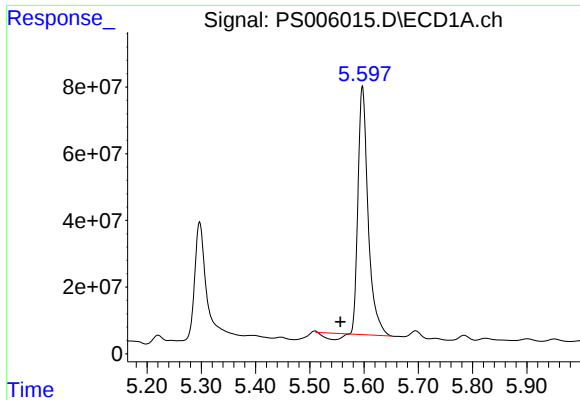

#4 2,4-DCAA


R.T.: 5.597 min
Delta R.T.: 0.041 min
Response: 934562323
Conc: 644.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-25

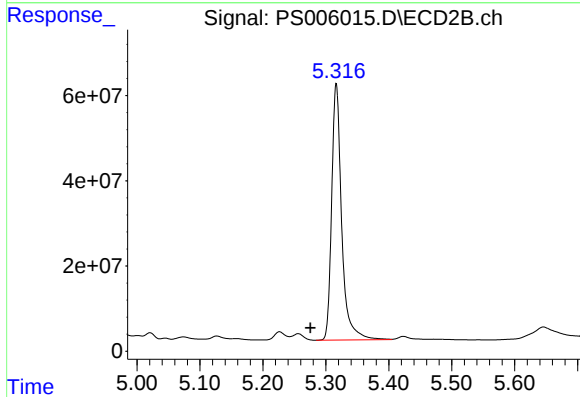


#4 2,4-DCAA

R.T.: 5.317 min
Delta R.T.: 0.041 min
Response: 665669885
Conc: 669.23 ng/ml

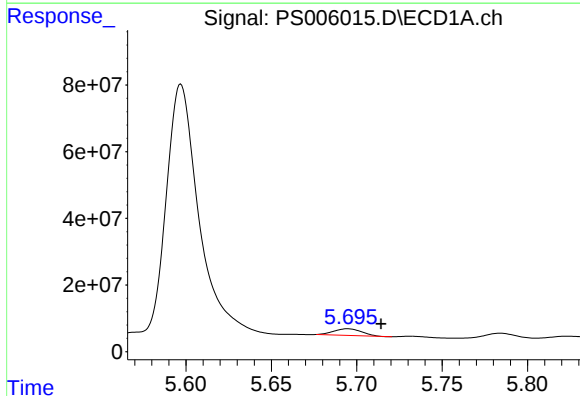


#5 DICAMBA

R.T.: 5.695 min
Delta R.T.: -0.019 min
Response: 22867491
Conc: 3.83 ng/ml

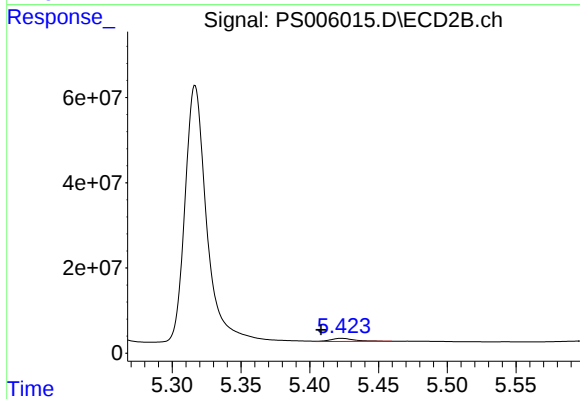

#5 DICAMBA


R.T.: 5.423 min
Delta R.T.: 0.015 min
Response: 8984749
Conc: 2.41 ng/ml

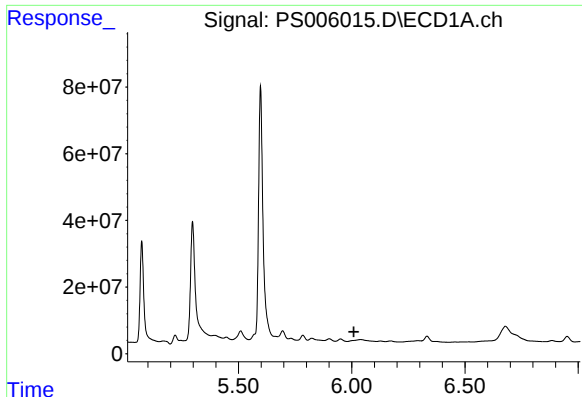

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-25

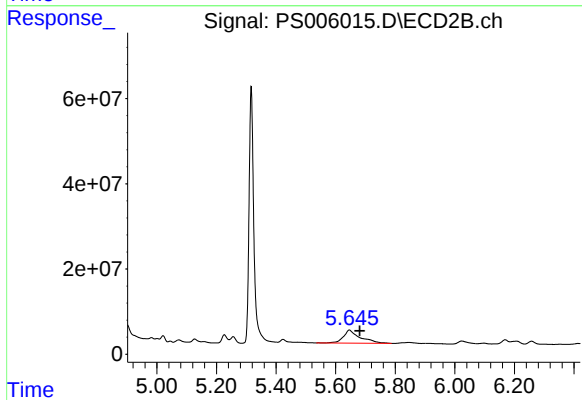


#7 MCPA

R.T.: 5.646 min
Delta R.T.: -0.035 min
Response: 118734206
Conc: 28.21 ug/ml

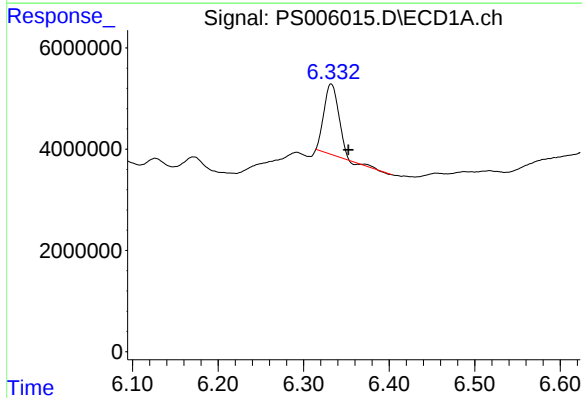


#8 DICHLORPROP

R.T.: 6.332 min
Delta R.T.: -0.020 min
Response: 16772663
Conc: 11.66 ng/ml

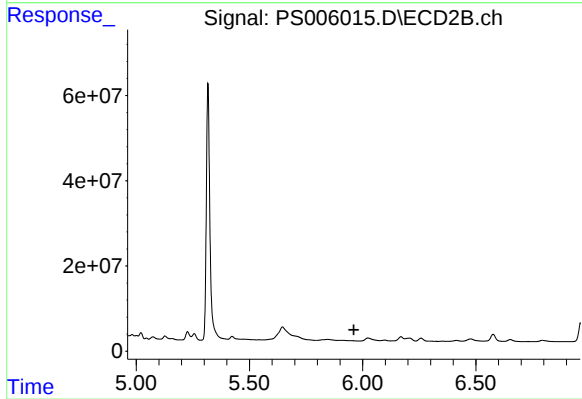

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 5.961 min
Response: 0
Conc: N.D.

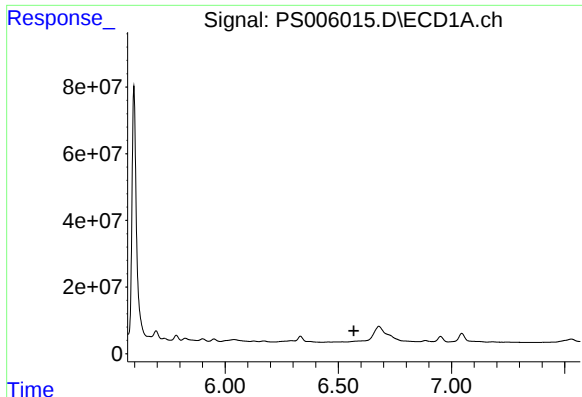

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-25

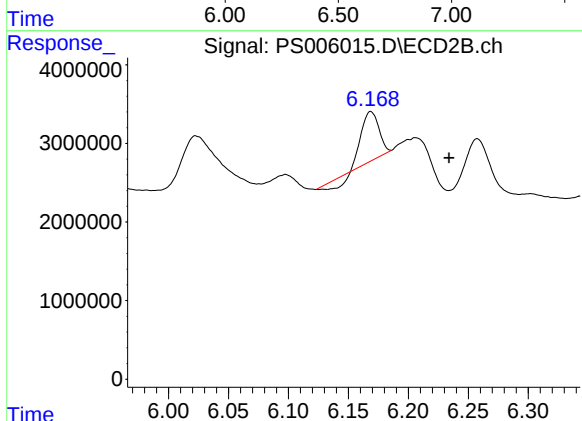


#9 2,4-D

R.T.: 6.169 min
Delta R.T.: -0.065 min
Response: 5268448
Conc: 4.90 ng/ml

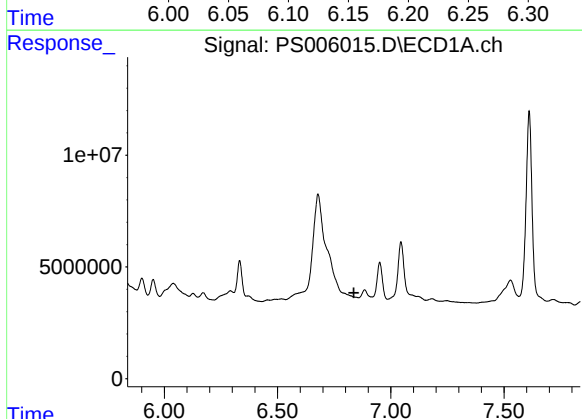


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

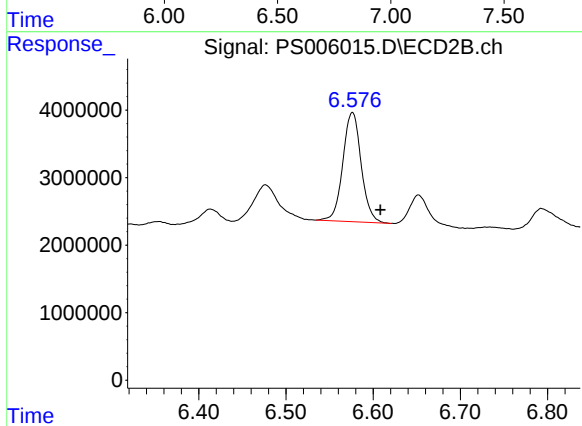

#10 Pentachlorophenol


R.T.: 6.576 min
Delta R.T.: -0.032 min
Response: 23724335
Conc: 1.83 ng/ml

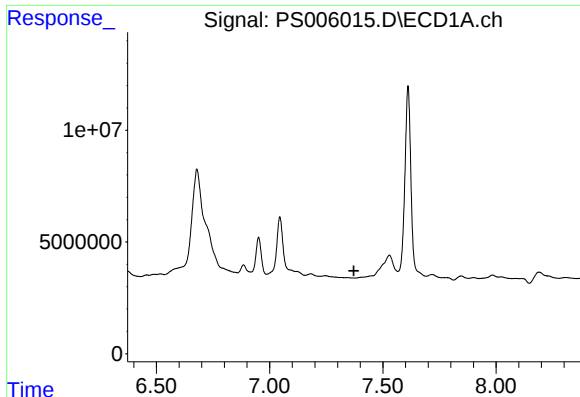

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-25

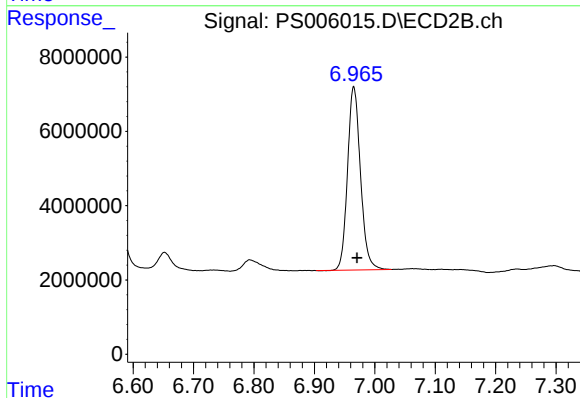


#11 2,4,5-TP (SILVEX)

R.T.: 6.965 min
Delta R.T.: -0.005 min
Response: 73546992
Conc: 14.18 ng/ml

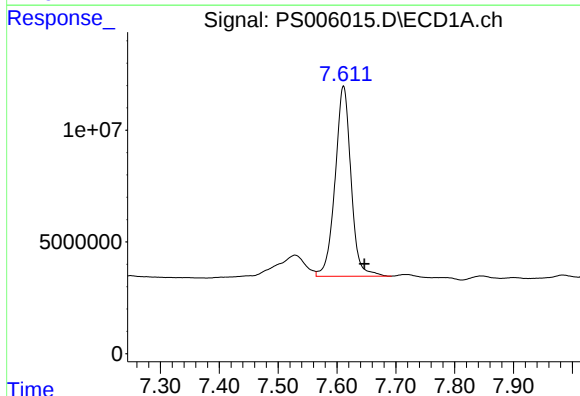

#12 2,4,5-T

R.T.: 7.611 min
Delta R.T.: -0.036 min
Response: 159714366
Conc: 19.13 ng/ml

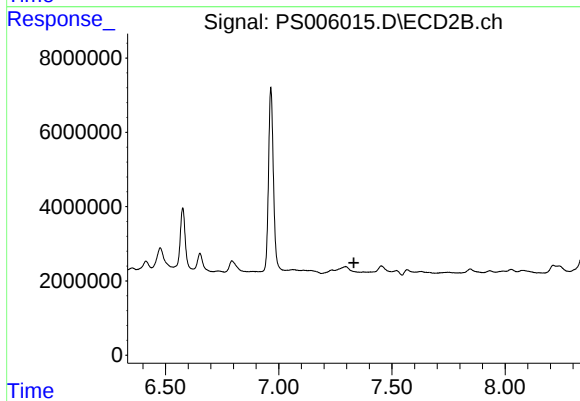

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.