

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 23:16
 Operator : SM\AJ
 Sample : K4245-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-26

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:17:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.559	5.280	1019.8E6	633.6E6	702.916	636.963
Target Compounds							
1) T	Dalapon	2.061	0.000	26990270	0	14.563	N.D. #
2) T	3,5-DICHL...	0.000	4.600	0	167.9E6	N.D.	129.405
3) T	4-Nitroph...	5.354	4.983	12680894	52412056	21.081	105.801 #
5) T	DICAMBA	5.746	0.000	57496326	0	9.627	N.D. #
6) T	MCPD	5.863	0.000	12434320	0	2.684	N.D. #
7) T	MCPA	5.997	0.000	35063831	0	5.373	N.D. #
8) T	DICHLORPROP	6.295	5.983	58328922	20917430	40.561	22.650 #
9) T	2,4-D	0.000	6.221	0	14084884	N.D.	13.111
10) T	Pentachlo...	0.000	6.538	0	22389350	N.D.	1.725
11) T	2,4,5-TP ...	0.000	6.928	0	48433555	N.D.	9.337
15) T	Picloram	0.000	9.106	0	26449850	N.D.	3.521



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 23:16
Operator : SM\AJ
Sample : K4245-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-26

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:17:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

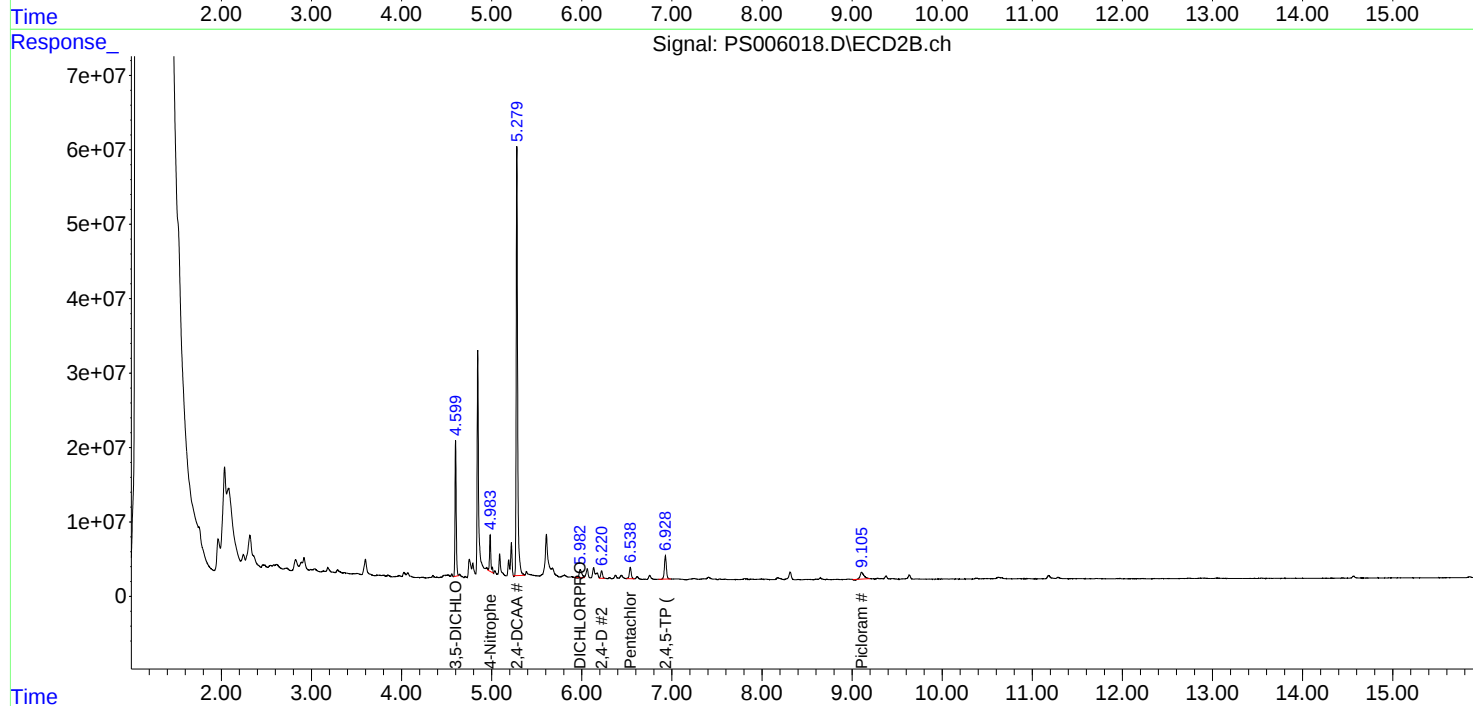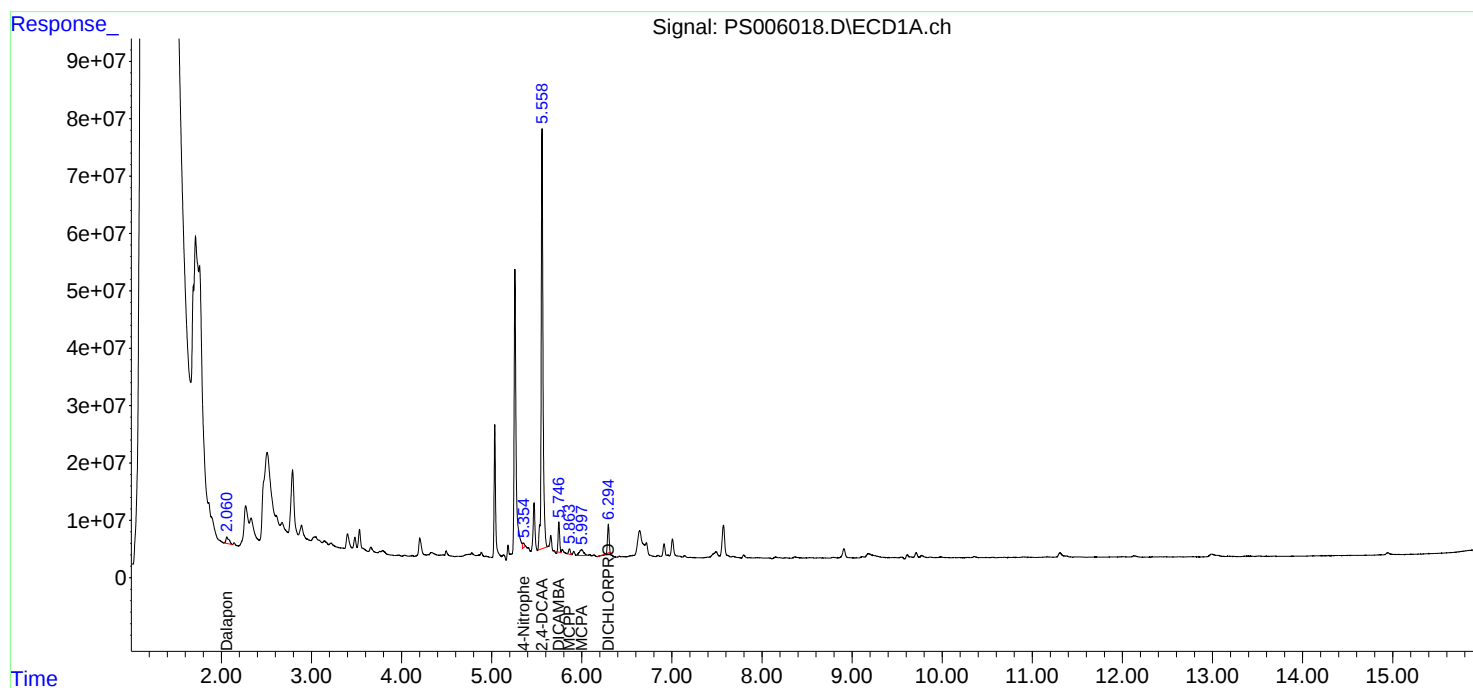


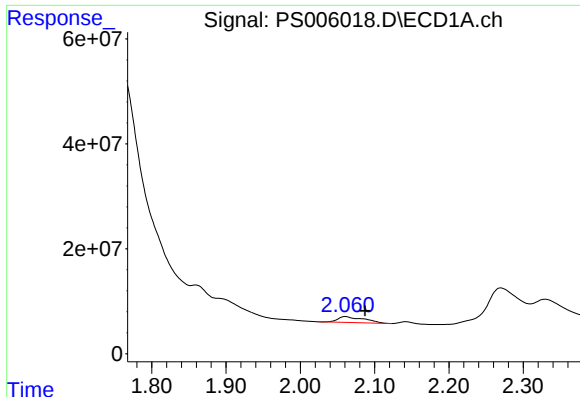

#1 Dalapon


R.T.: 2.061 min
Delta R.T.: -0.026 min
Response: 26990270
Conc: 14.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-26

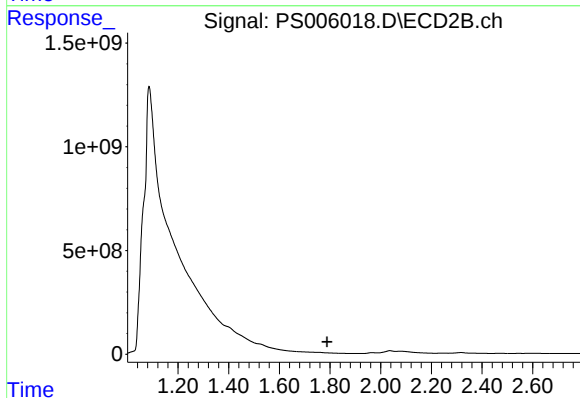


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

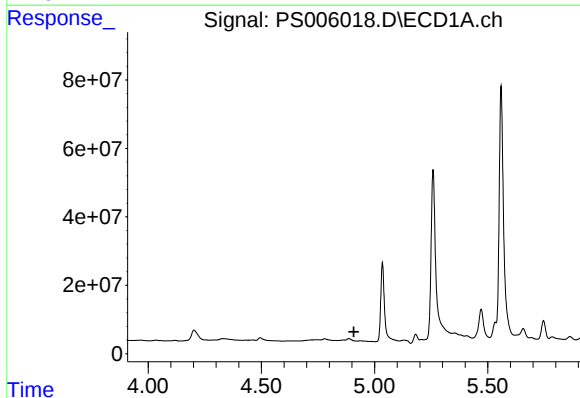


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

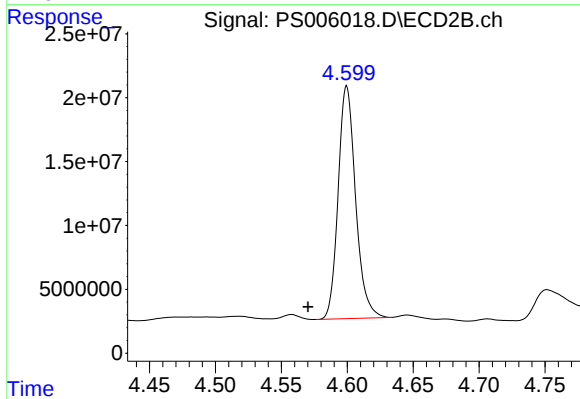

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.600 min
Delta R.T.: 0.029 min
Response: 167879264
Conc: 129.41 ng/ml

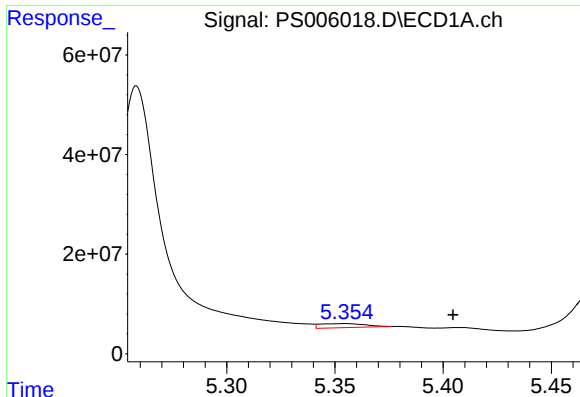

#3 4-Nitrophenol


R.T.: 5.354 min
Delta R.T.: -0.051 min
Response: 12680894
Conc: 21.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-26

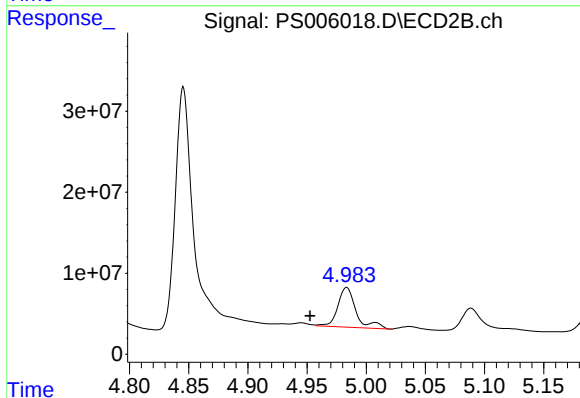


#3 4-Nitrophenol

R.T.: 4.983 min
Delta R.T.: 0.031 min
Response: 52412056
Conc: 105.80 ng/ml

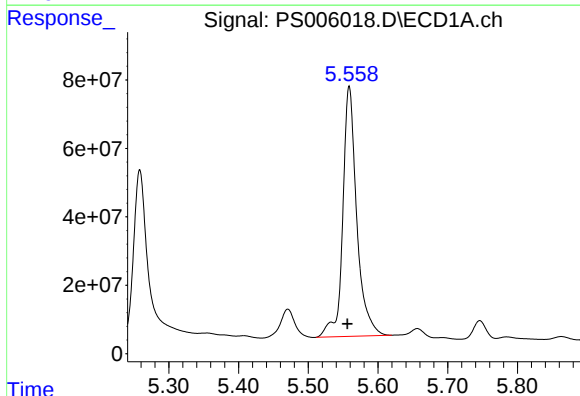


#4 2,4-DCAA

R.T.: 5.559 min
Delta R.T.: 0.003 min
Response: 1019802799
Conc: 702.92 ng/ml

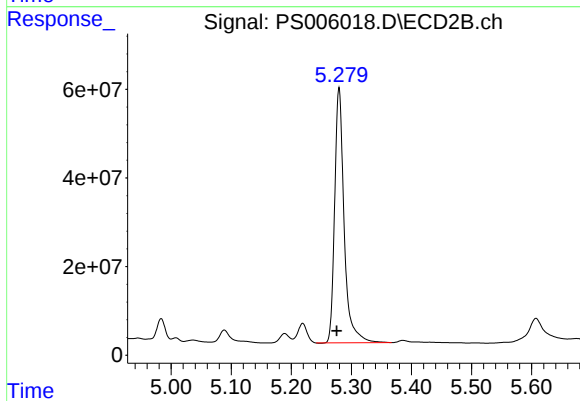

#4 2,4-DCAA


R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 633573646
Conc: 636.96 ng/ml

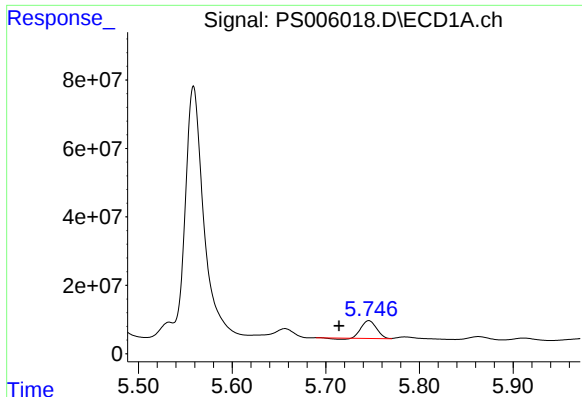

#5 DICAMBA


R.T.: 5.746 min
Delta R.T.: 0.032 min
Response: 57496326
Conc: 9.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-26

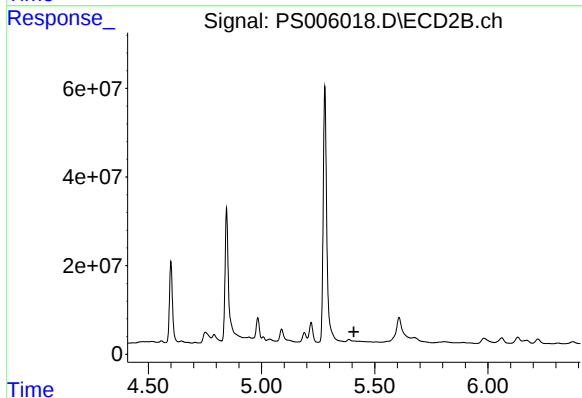


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

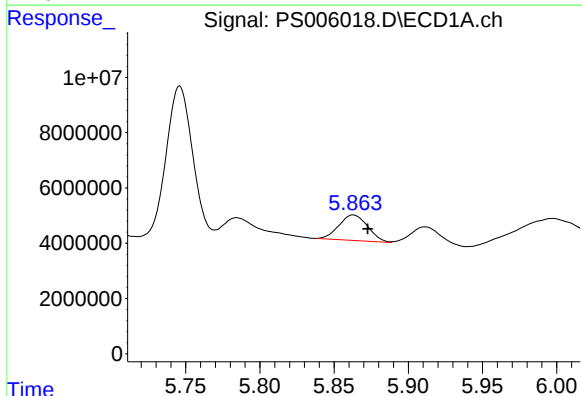


#6 MCP

R.T.: 5.863 min
Delta R.T.: -0.010 min
Response: 12434320
Conc: 2.68 ug/ml

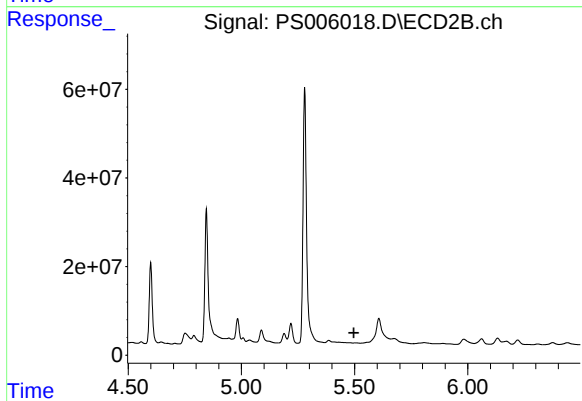

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

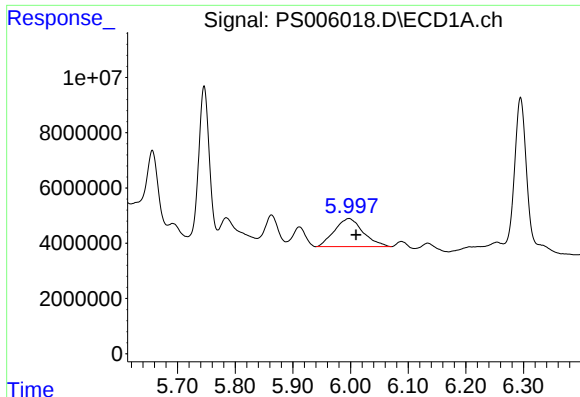

#7 MCPA


R.T.: 5.997 min
Delta R.T.: -0.012 min
Response: 35063831
Conc: 5.37 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-26

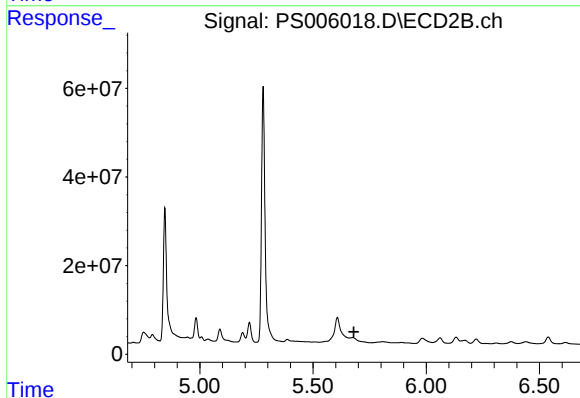


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 5.681 min
Response: 0
Conc: N.D.

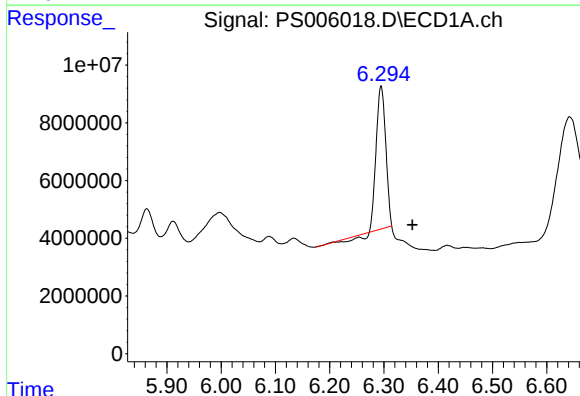


#8 DICHLORPROP

R.T.: 6.295 min
Delta R.T.: -0.057 min
Response: 58328922
Conc: 40.56 ng/ml

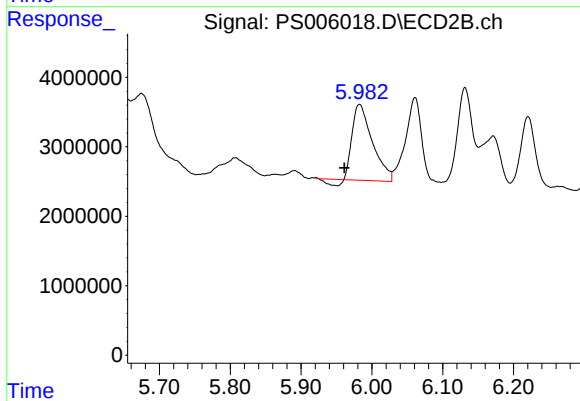

#8 DICHLORPROP


R.T.: 5.983 min
Delta R.T.: 0.021 min
Response: 20917430
Conc: 22.65 ng/ml

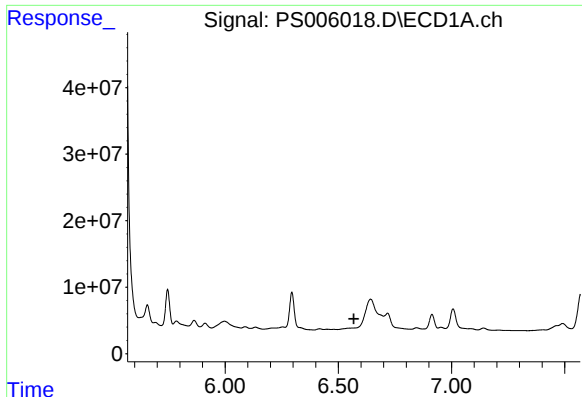

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-26

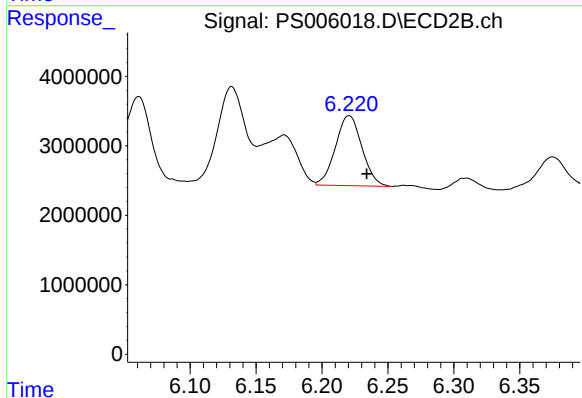


#9 2,4-D

R.T.: 6.221 min
Delta R.T.: -0.013 min
Response: 14084884
Conc: 13.11 ng/ml

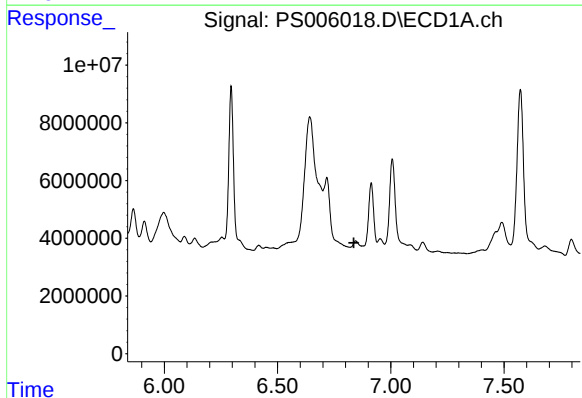


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

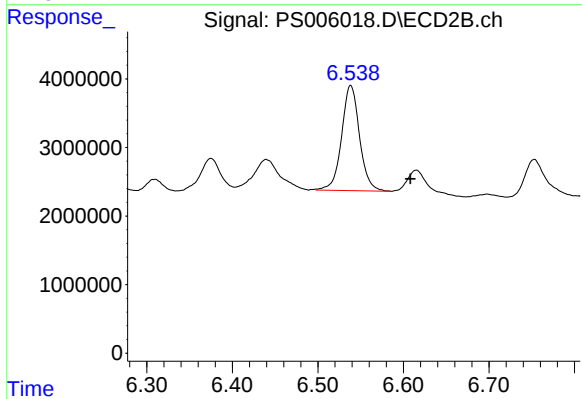

#10 Pentachlorophenol


R.T.: 6.538 min
Delta R.T.: -0.070 min
Response: 22389350
Conc: 1.72 ng/ml

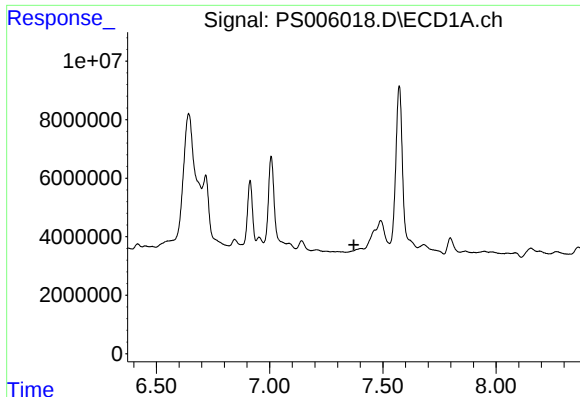

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-26

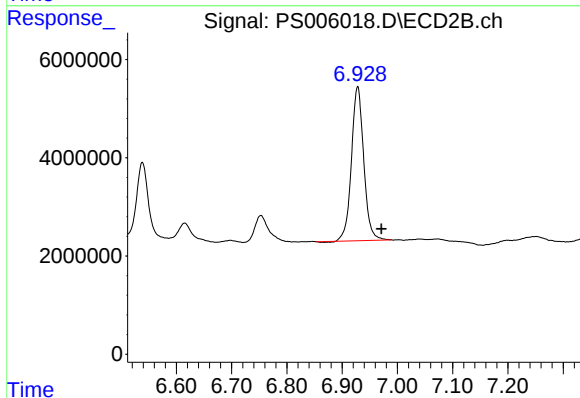


#11 2,4,5-TP (SILVEX)

R.T.: 6.928 min
Delta R.T.: -0.043 min
Response: 48433555
Conc: 9.34 ng/ml

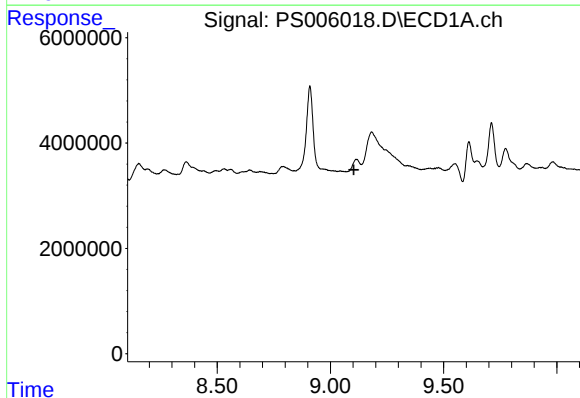

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.104 min
Response: 0
Conc: N.D.

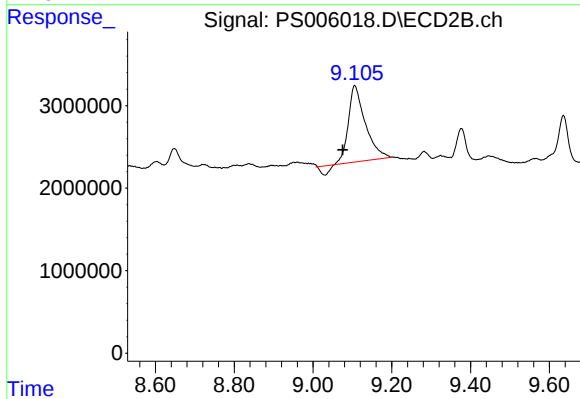

#15 Picloram

R.T.: 9.106 min
Delta R.T.: 0.031 min
Response: 26449850
Conc: 3.52 ng/ml