

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 03:42
 Operator : SM\AJ
 Sample : K4228-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 2S-F1-F4-COMP-(0-1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:26:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.590	5.273	405.6E6	54282848	279.576	54.573 #
Target Compounds							
1) T	Dalapon	0.000	1.764	0	689.8E6	N.D.	547.236
2) T	3,5-DICHL...	0.000	4.529	0	5767347	N.D.	4.446
6) T	MCPD	5.897	0.000	22428348	0	4.841	N.D. #
7) T	MCPA	5.993	5.721	18653732	90054192	2.859	21.395 #
9) T	2,4-D	6.579	6.251	29583078	31495837	19.740	29.318 #
10) T	Pentachlo...	6.871	6.569	28473746	25920158	1.362	1.996 #
12) T	2,4,5-T	7.591	0.000	37306712	0	4.470	N.D. #
13) T	2,4-DB	8.212	0.000	70546885	0	66.811	N.D. #
14) T	DINOSEB	0.000	8.119	0	73453670	N.D.	19.739
15) T	Picloram	0.000	9.135	0	31177742	N.D.	4.150



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 03:42
Operator : SM\AJ
Sample : K4228-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(0-1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:26:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

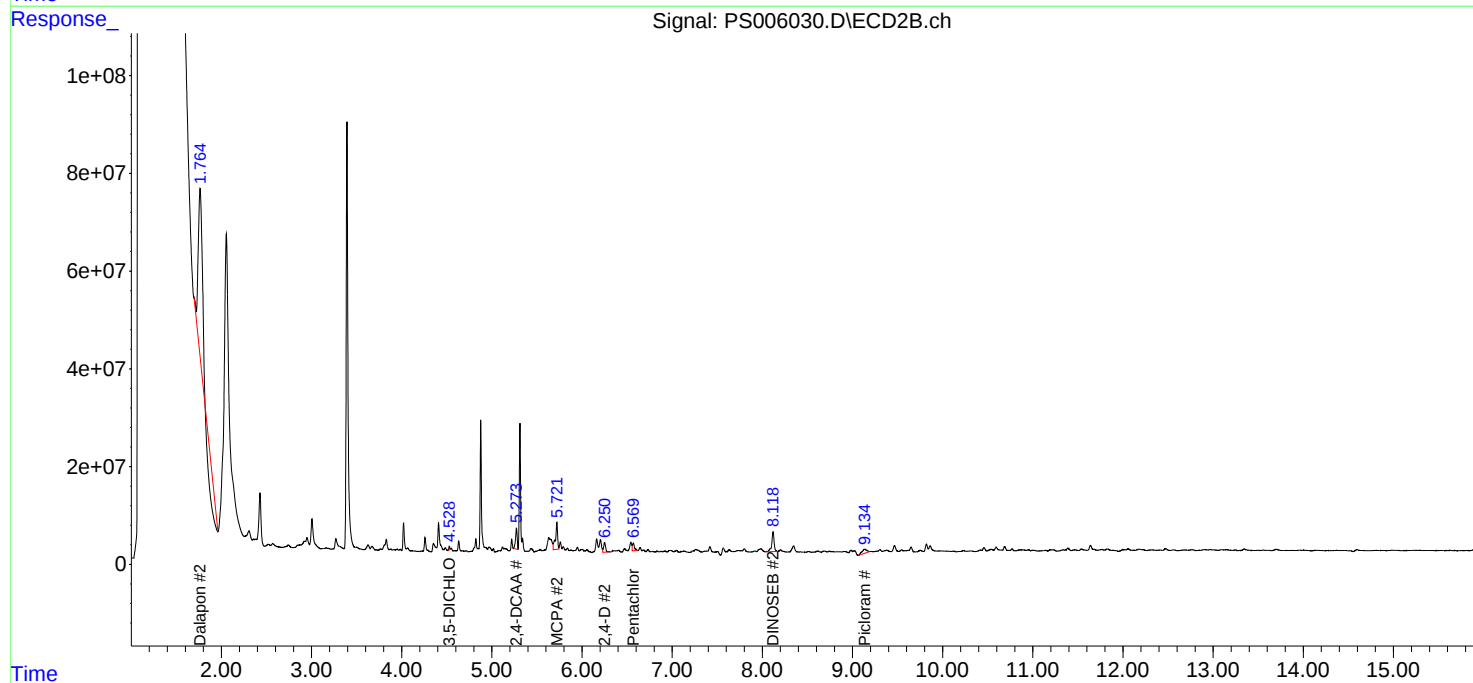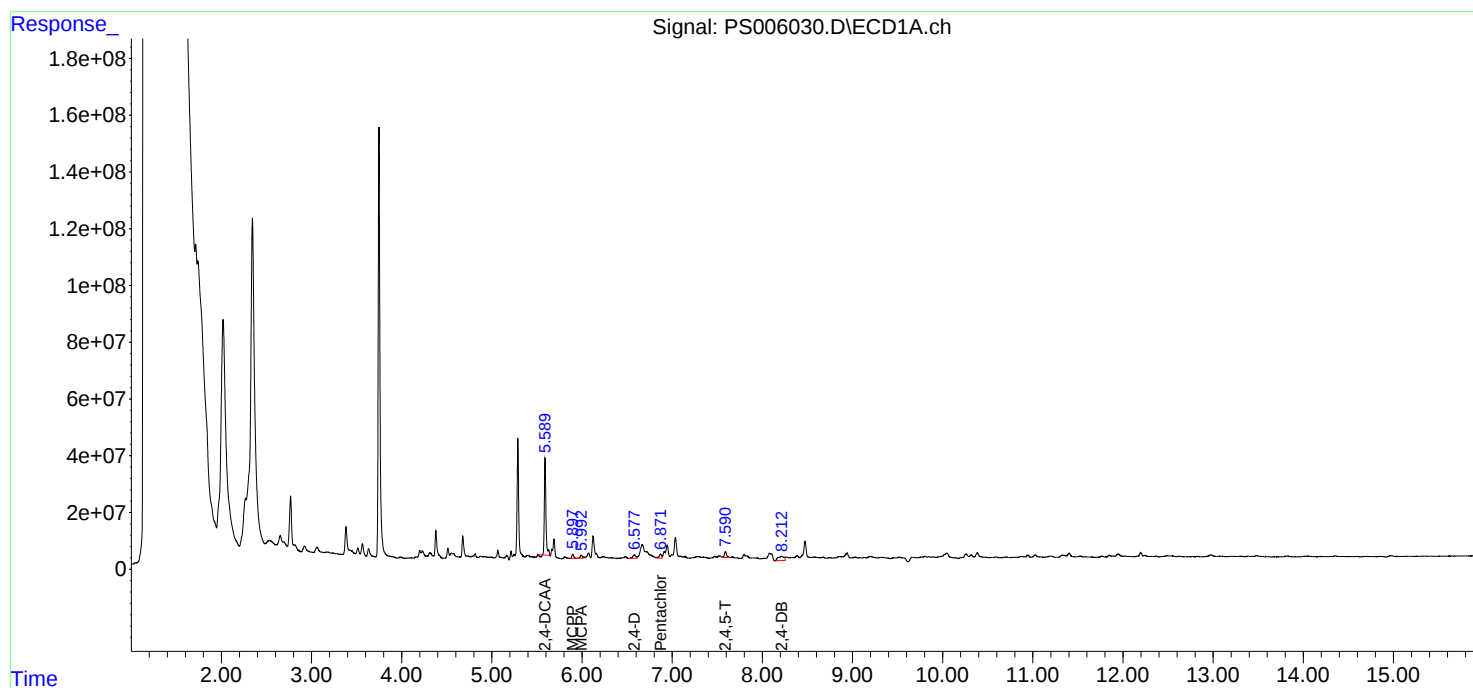


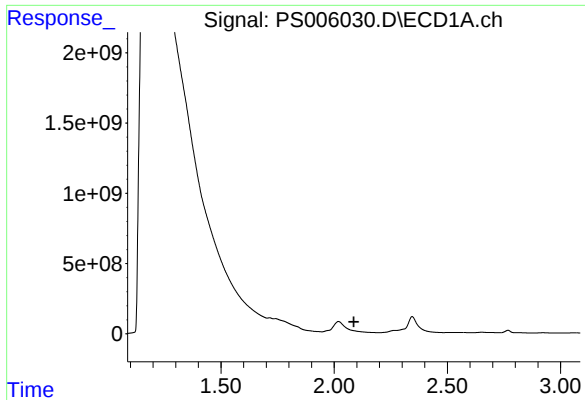

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(0-1)

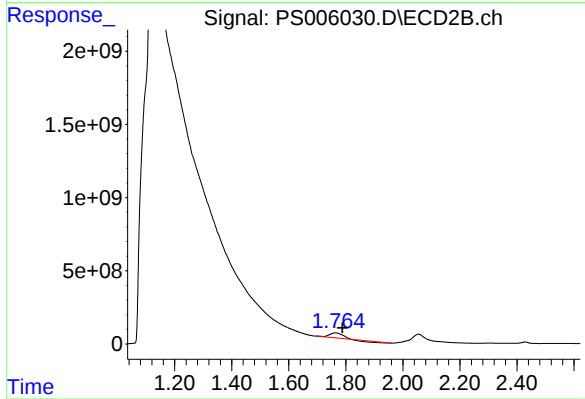


#1 Dalapon

R.T.: 1.764 min
Delta R.T.: -0.024 min
Response: 689833426
Conc: 547.24 ng/ml

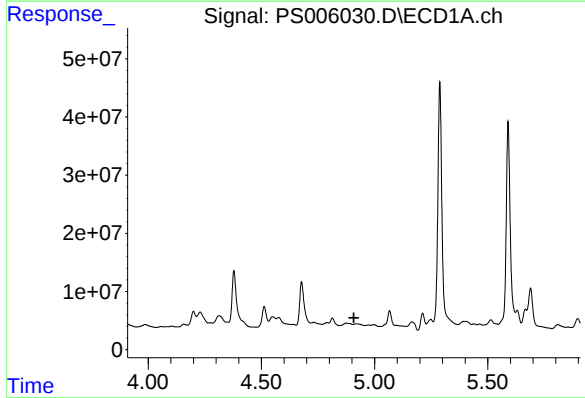


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

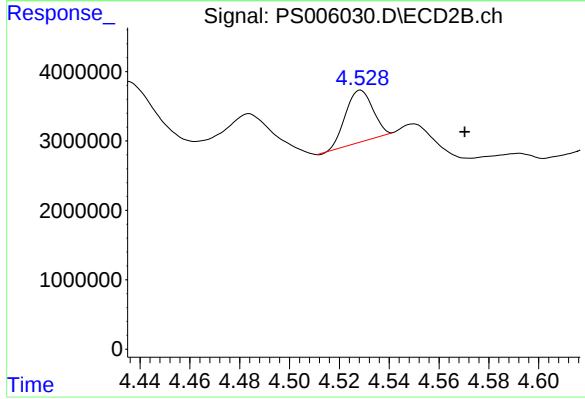

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.529 min
Delta R.T.: -0.042 min
Response: 5767347
Conc: 4.45 ng/ml

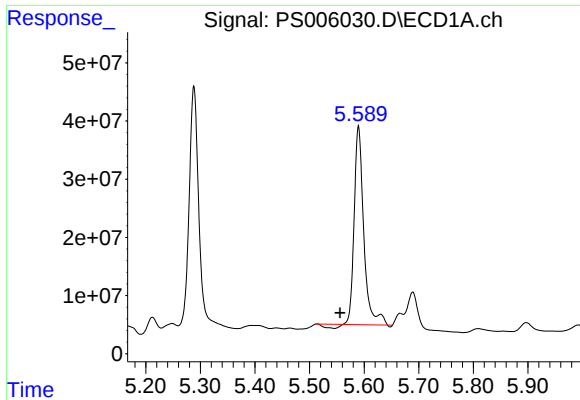

#4 2,4-DCAA


R.T.: 5.590 min
Delta R.T.: 0.034 min
Response: 405613154
Conc: 279.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(0-1)

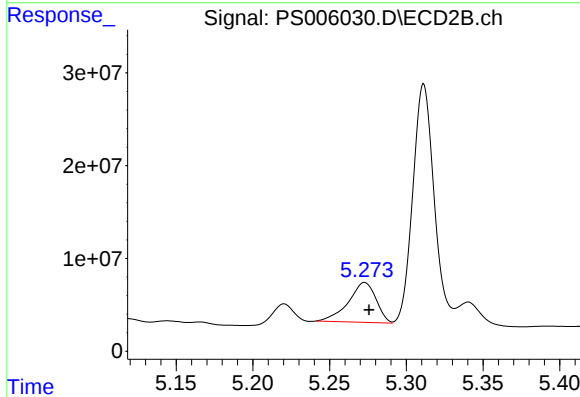


#4 2,4-DCAA

R.T.: 5.273 min
Delta R.T.: -0.003 min
Response: 54282848
Conc: 54.57 ng/ml

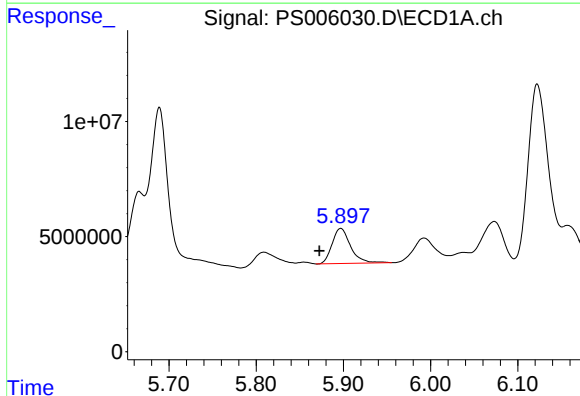


#6 MCP

R.T.: 5.897 min
Delta R.T.: 0.025 min
Response: 22428348
Conc: 4.84 ug/ml

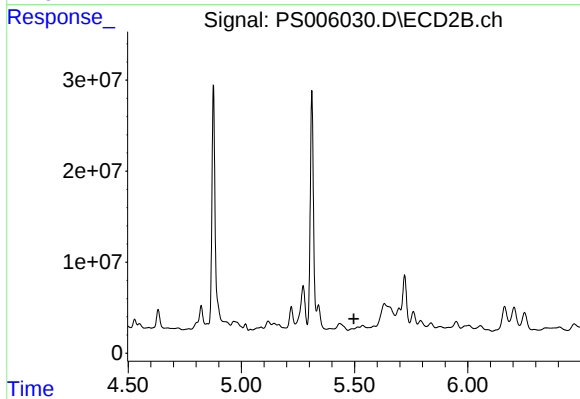

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

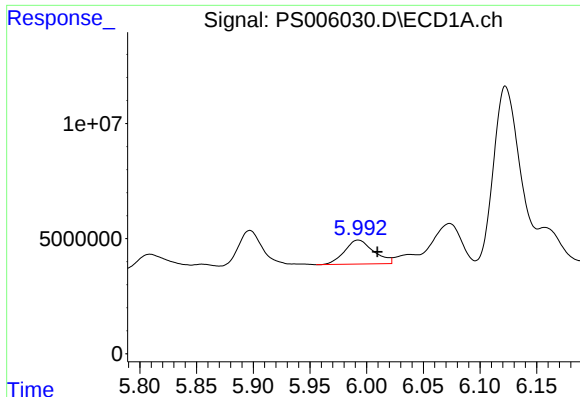

#7 MCPA


R.T.: 5.993 min
Delta R.T.: -0.016 min
Response: 18653732
Conc: 2.86 ug/ml

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(0-1)

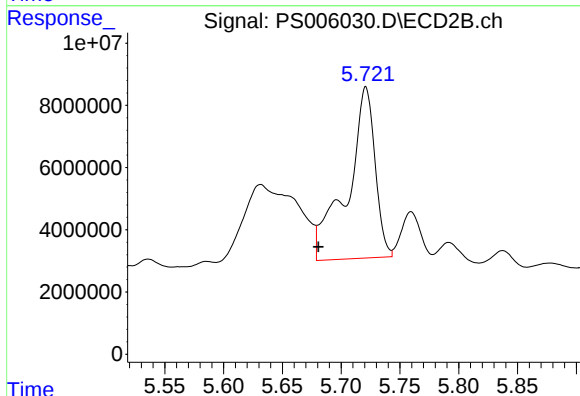


#7 MCPA

R.T.: 5.721 min
Delta R.T.: 0.040 min
Response: 90054192
Conc: 21.40 ug/ml

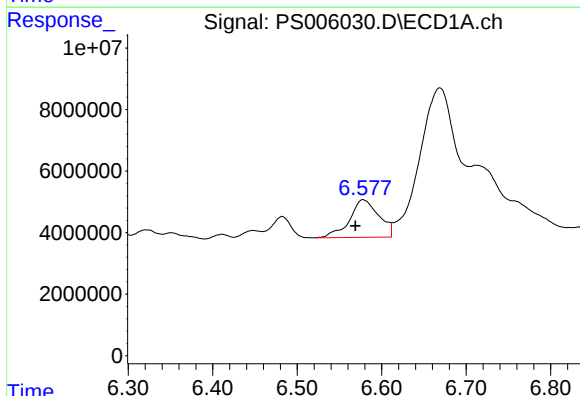


#9 2,4-D

R.T.: 6.579 min
Delta R.T.: 0.010 min
Response: 29583078
Conc: 19.74 ng/ml

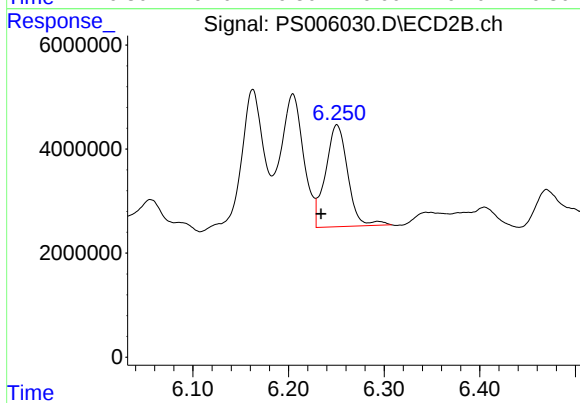

#9 2,4-D


R.T.: 6.251 min
Delta R.T.: 0.017 min
Response: 31495837
Conc: 29.32 ng/ml

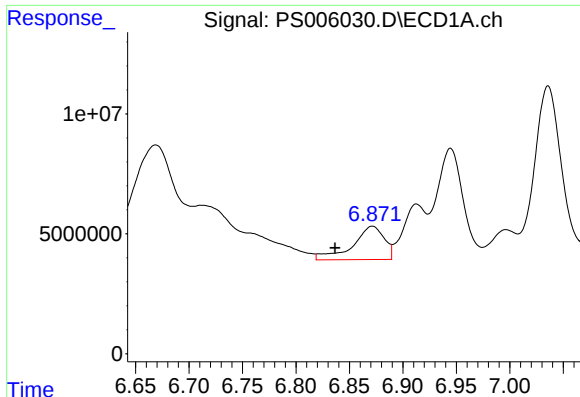

#10 Pentachlorophenol


R.T.: 6.871 min
Delta R.T.: 0.035 min
Response: 28473746
Conc: 1.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(0-1)

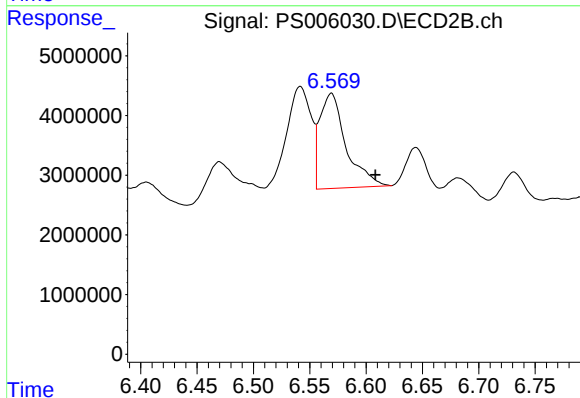


#10 Pentachlorophenol

R.T.: 6.569 min
Delta R.T.: -0.039 min
Response: 25920158
Conc: 2.00 ng/ml

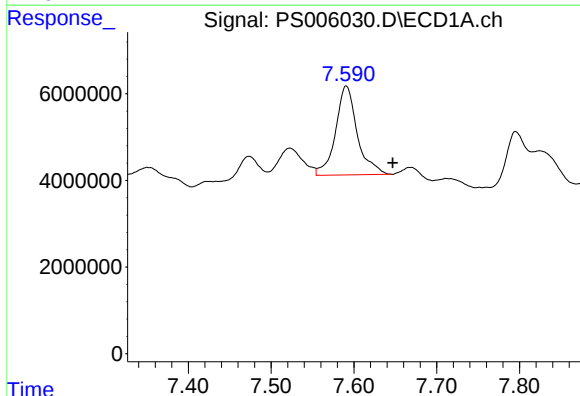


#12 2,4,5-T

R.T.: 7.591 min
Delta R.T.: -0.056 min
Response: 37306712
Conc: 4.47 ng/ml

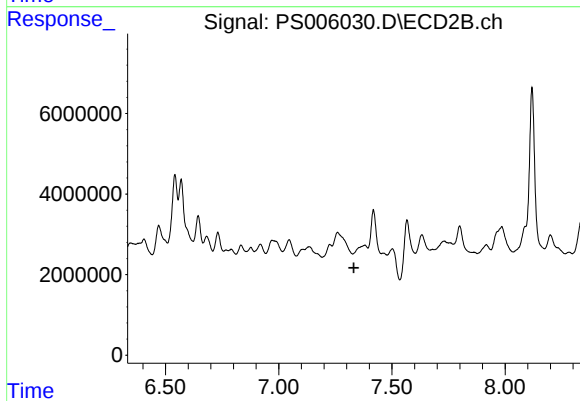

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.

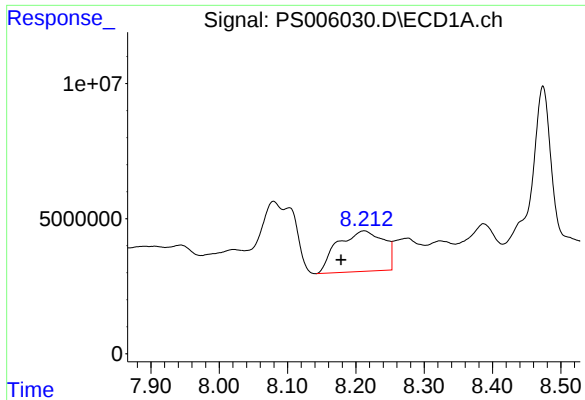

#13 2,4-DB


R.T.: 8.212 min
Delta R.T.: 0.034 min
Response: 70546885
Conc: 66.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(0-1)

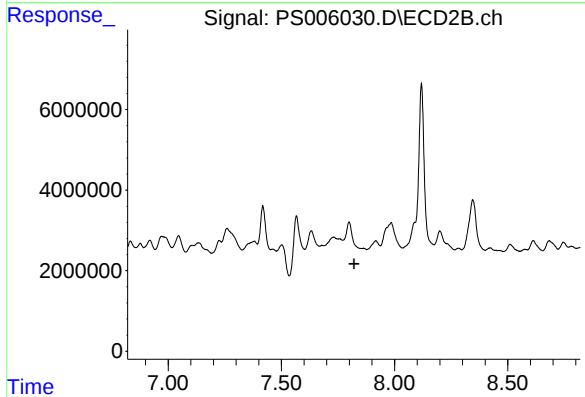


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.821 min
Response: 0
Conc: N.D.

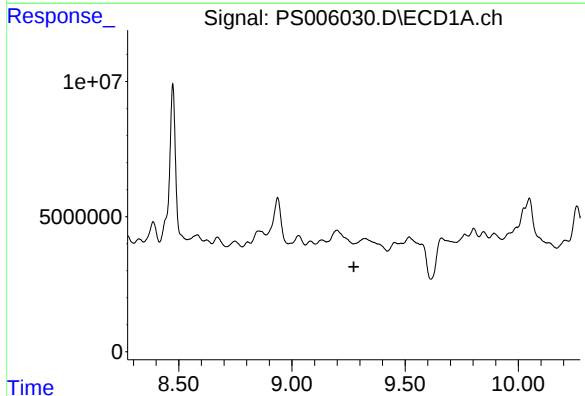


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.273 min
Response: 0
Conc: N.D.

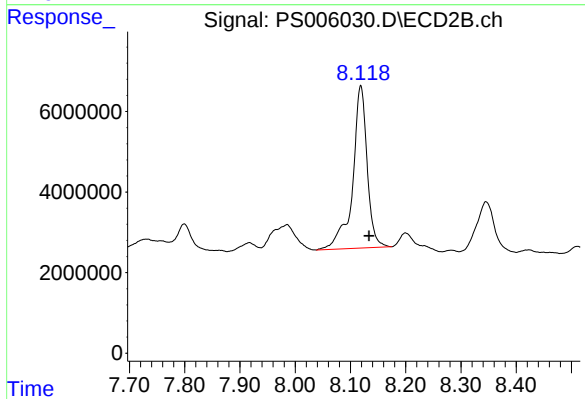

#14 DINOSEB


R.T.: 8.119 min
Delta R.T.: -0.015 min
Response: 73453670
Conc: 19.74 ng/ml

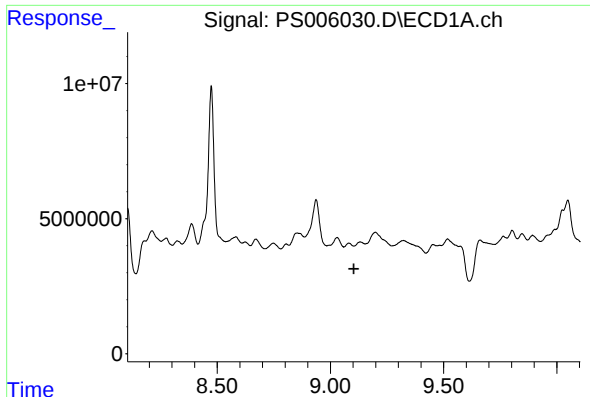

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
2S-F1-F4-COMP-(0-1)

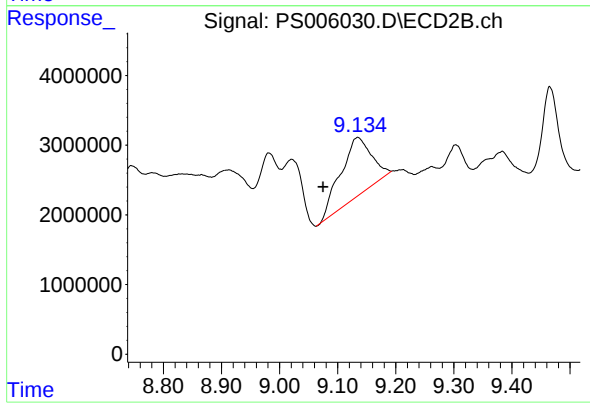

#15 Picloram

R.T.: 9.135 min
Delta R.T.: 0.059 min
Response: 31177742
Conc: 4.15 ng/ml