

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 05:33
 Operator : SM\AJ
 Sample : K4245-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 09:25:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.296	47386636	13369266	32.662	13.441 #
Target Compounds							
2) T	3,5-DICHL...	0.000	4.612	0	29916611	N.D.	23.060
6) T	MCP	5.877	0.000	18503483	0	3.993	N.D. #
7) T	MCPA	5.974	5.677	11795888	35546310	1.808	8.445 #
9) T	2,4-D	6.554	6.231	20389356	19691078	13.605	18.329 #
10) T	Pentachlo...	0.000	6.549	0	27441739	N.D.	2.114



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 05:33
Operator : SM\AJ
Sample : K4245-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 09:25:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

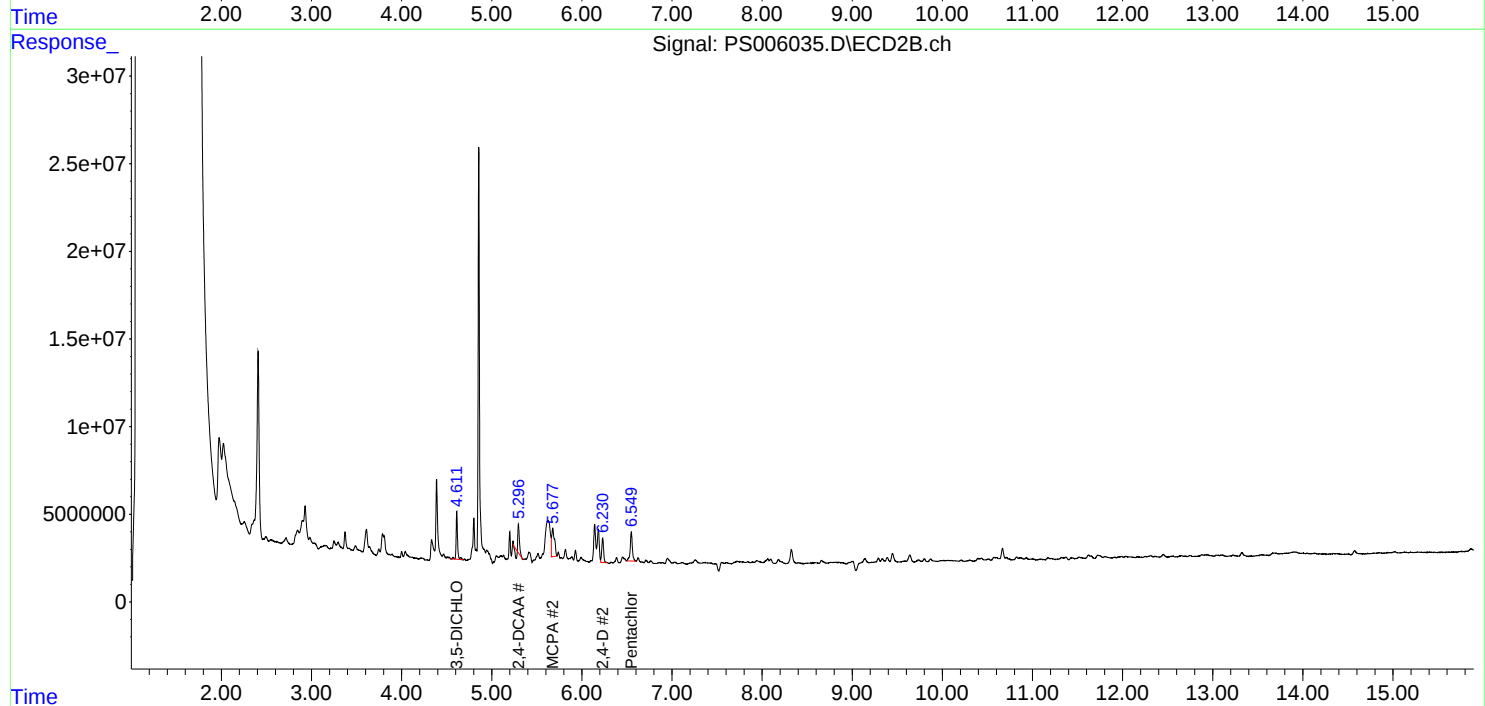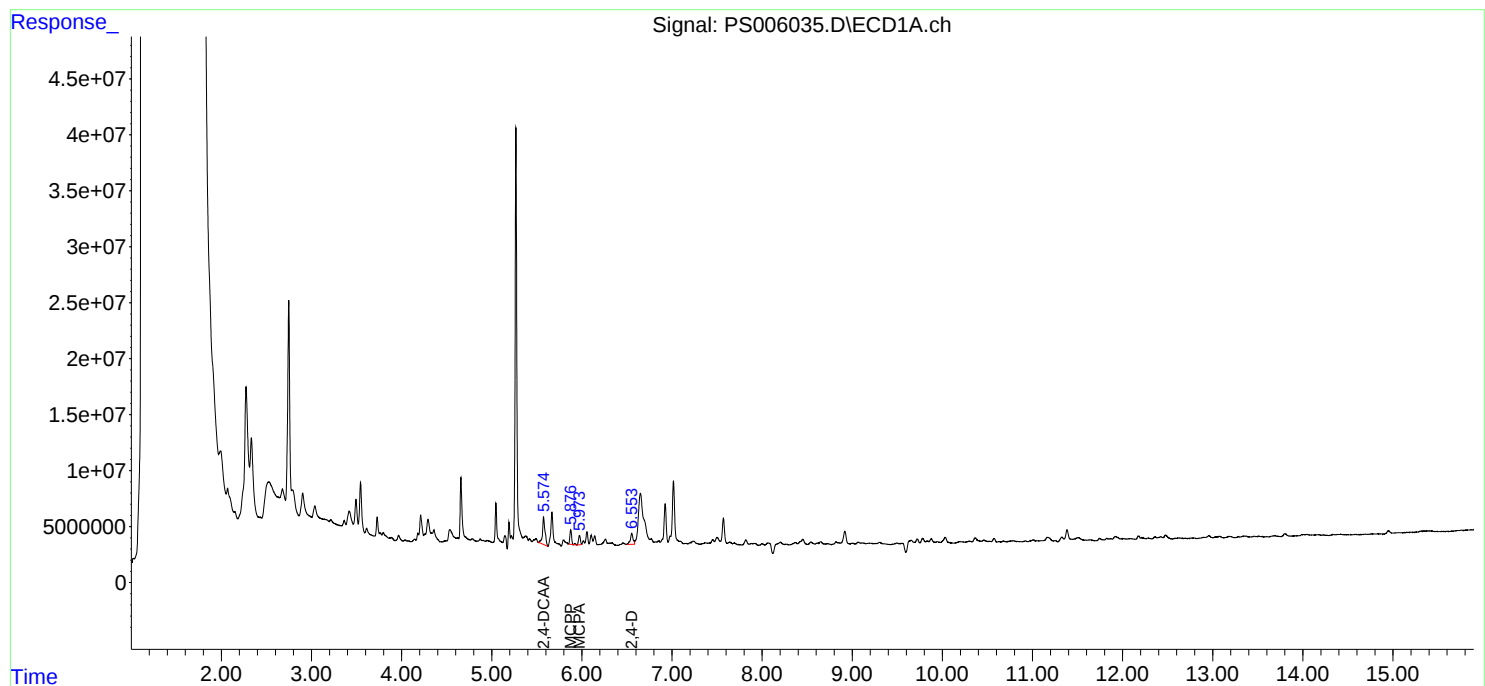


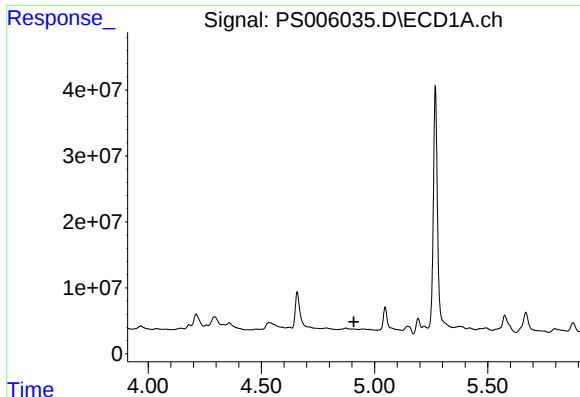

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-25

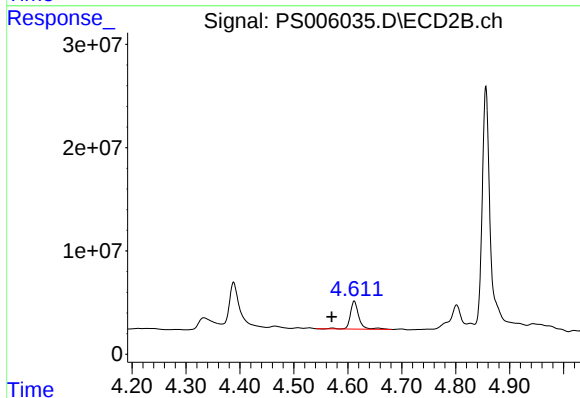


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.612 min
Delta R.T.: 0.042 min
Response: 29916611
Conc: 23.06 ng/ml

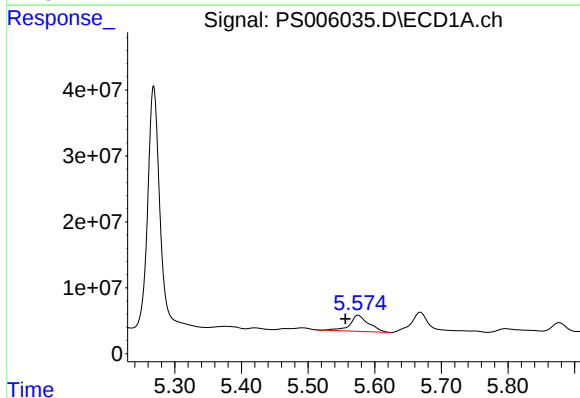


#4 2,4-DCAA

R.T.: 5.576 min
Delta R.T.: 0.020 min
Response: 47386636
Conc: 32.66 ng/ml

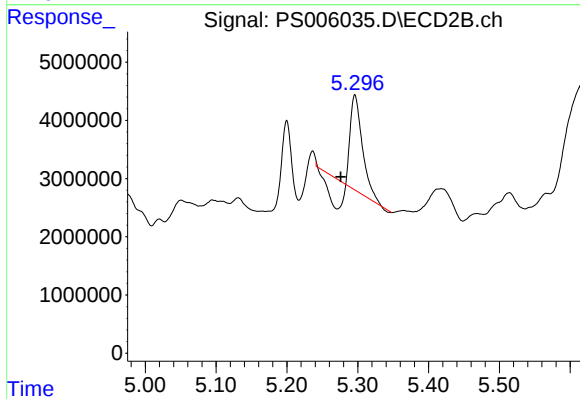

#4 2,4-DCAA


R.T.: 5.296 min
Delta R.T.: 0.021 min
Response: 13369266
Conc: 13.44 ng/ml

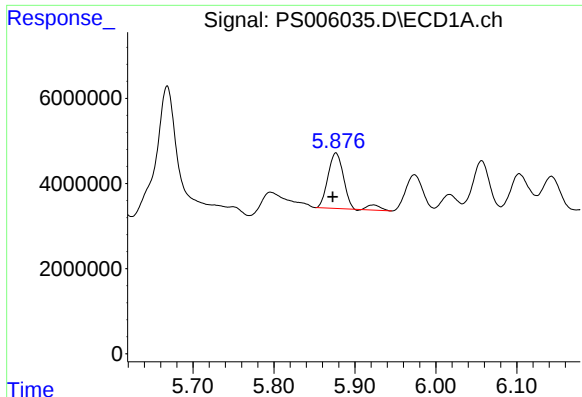

#6 MCPP


R.T.: 5.877 min
Delta R.T.: 0.004 min
Response: 18503483
Conc: 3.99 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-25

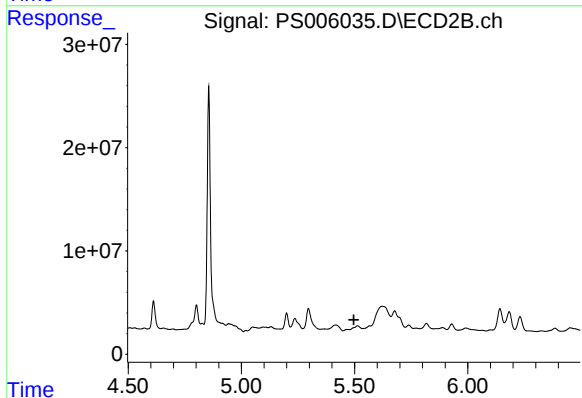


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

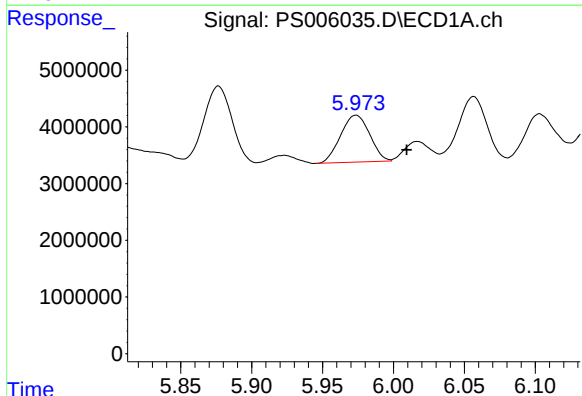


#7 MCPA

R.T.: 5.974 min
Delta R.T.: -0.036 min
Response: 11795888
Conc: 1.81 ug/ml

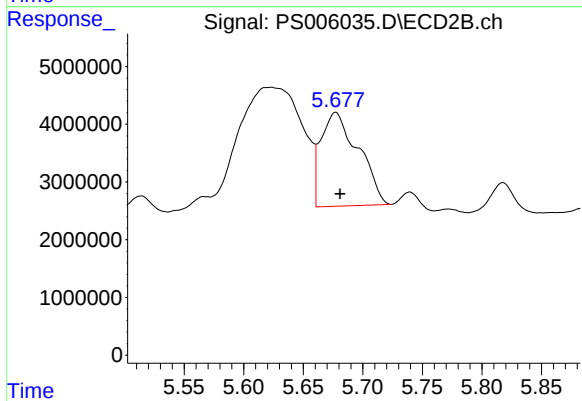

#7 MCPA


R.T.: 5.677 min
Delta R.T.: -0.004 min
Response: 35546310
Conc: 8.45 ug/ml

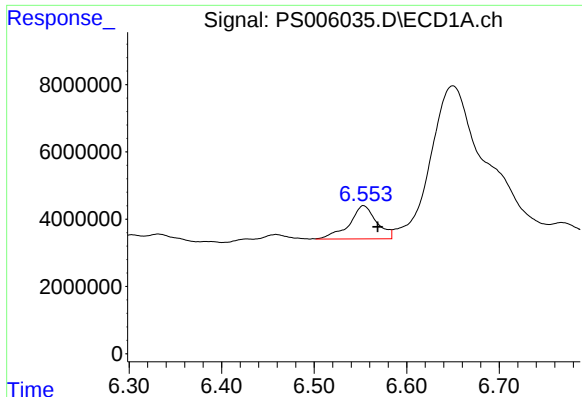

#9 2,4-D


R.T.: 6.554 min
Delta R.T.: -0.015 min
Response: 20389356
Conc: 13.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-25

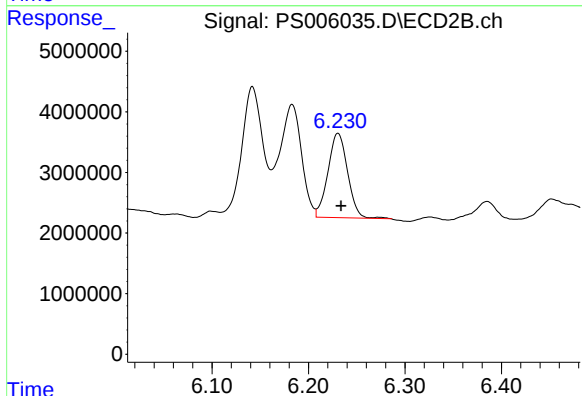


#9 2,4-D

R.T.: 6.231 min
Delta R.T.: -0.003 min
Response: 19691078
Conc: 18.33 ng/ml

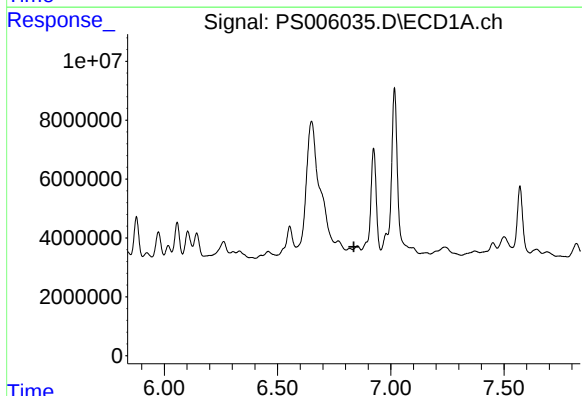

#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

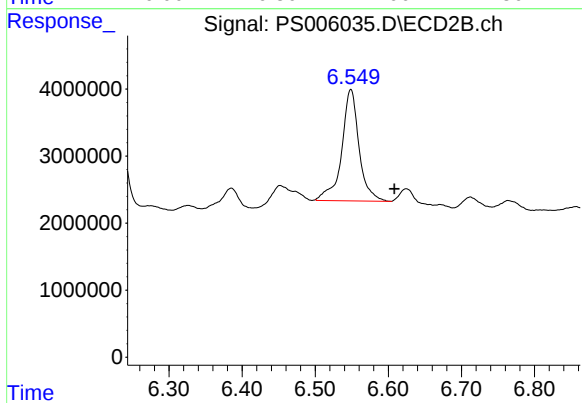

#10 Pentachlorophenol

R.T.: 6.549 min
Delta R.T.: -0.060 min
Response: 27441739
Conc: 2.11 ng/ml