

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
 Data File : PS006037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 06:17
 Operator : SM\AJ
 Sample : K4245-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-27

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 09:25:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.298	41874027	17391726	28.862	17.485 #
Target Compounds							
2) T	3,5-DICHL...	0.000	4.614	0	12326685	N.D.	9.502
5) T	DICAMBA	5.669	0.000	14185608	0	2.375	N.D. #
6) T	MCP	5.878	0.000	18040833	0	3.894	N.D. #
7) T	MCPA	5.974	5.679	12602365	32643950	1.931	7.756 #
9) T	2,4-D	6.555	6.233	18366105	20708211	12.255	19.276 #
10) T	Pentachlo...	0.000	6.551	0	30357208	N.D.	2.338
13) T	2,4-DB	8.205	0.000	38736458	0	36.685	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081219\
Data File : PS006037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 06:17
Operator : SM\AJ
Sample : K4245-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-27

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 09:25:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

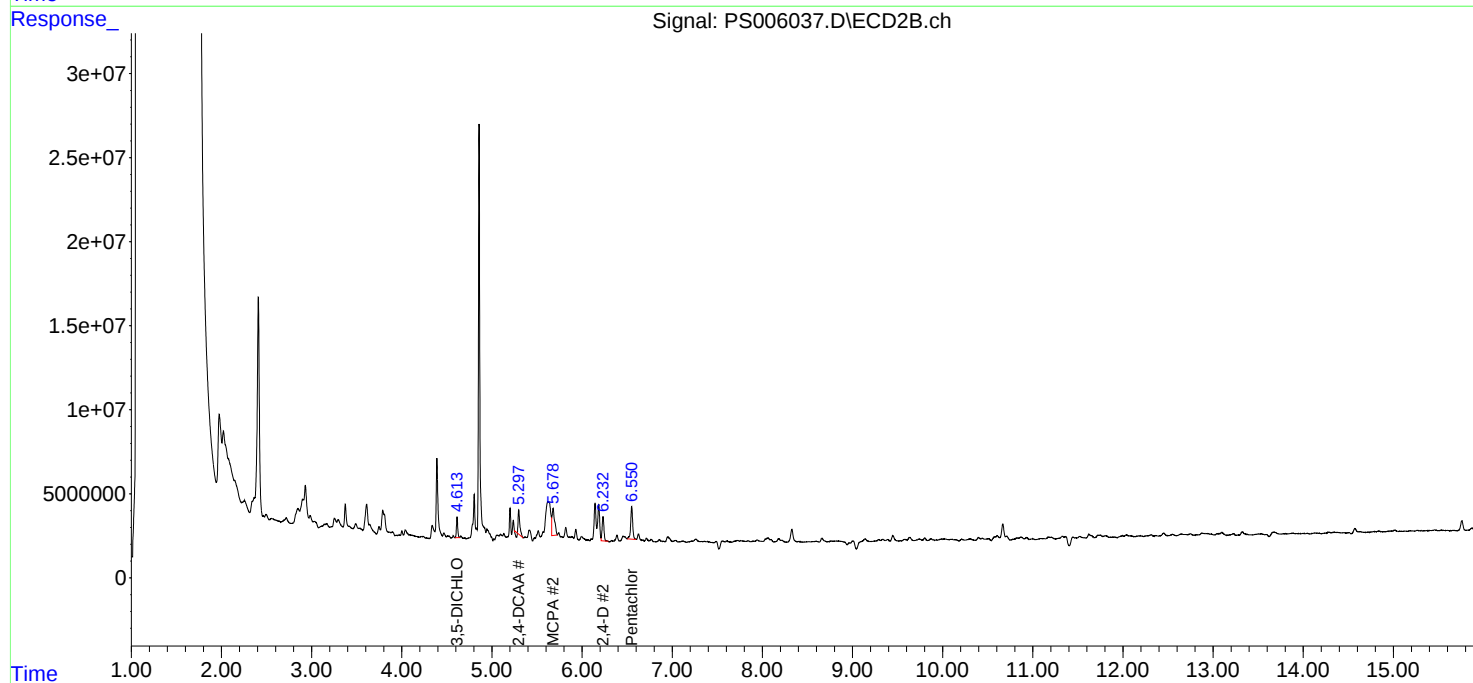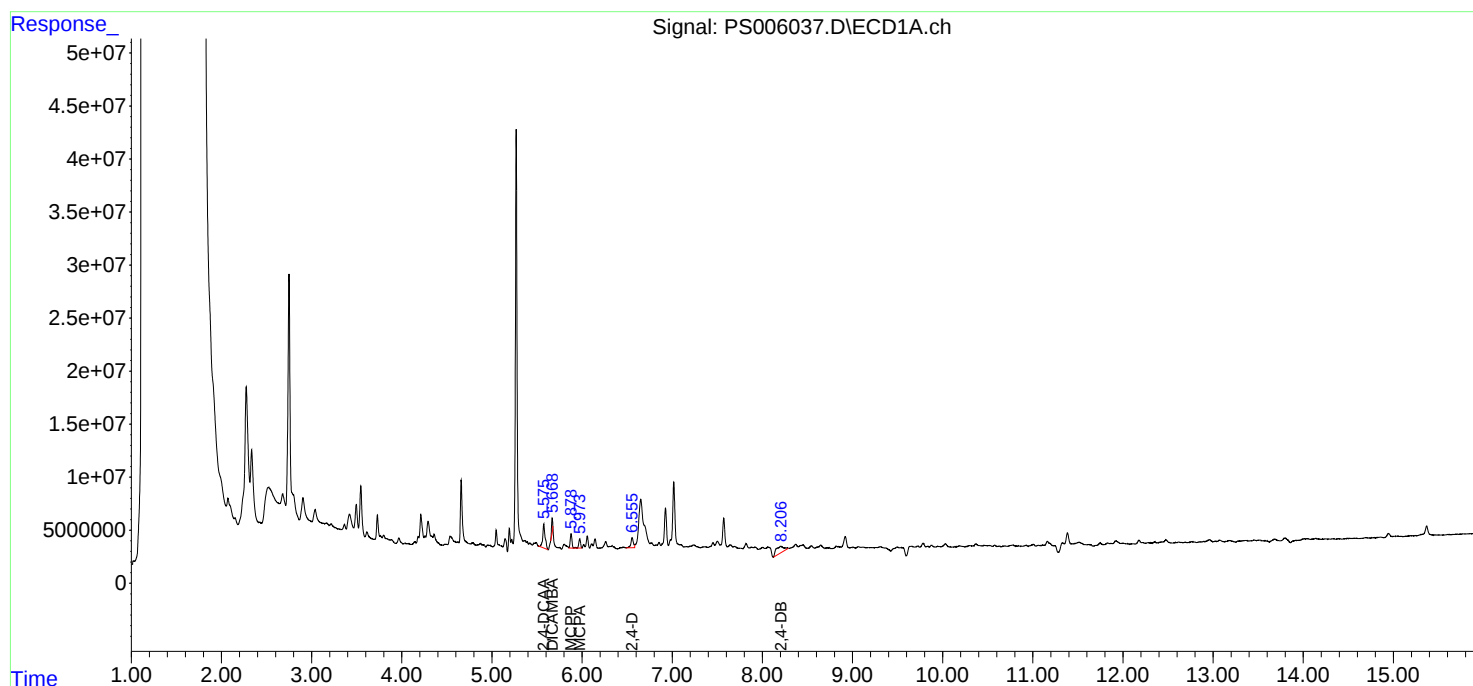


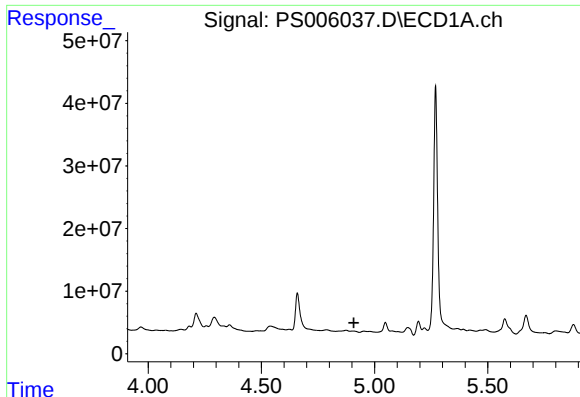

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-27

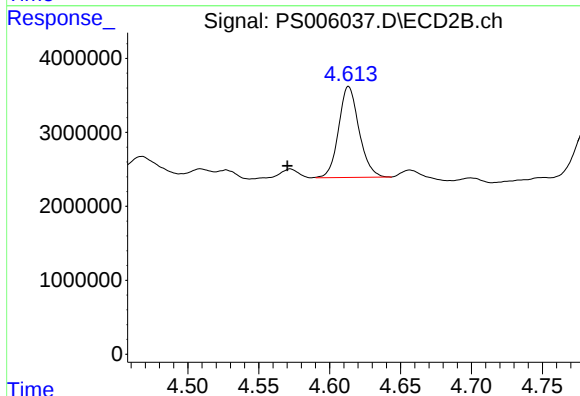


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.614 min
Delta R.T.: 0.043 min
Response: 12326685
Conc: 9.50 ng/ml

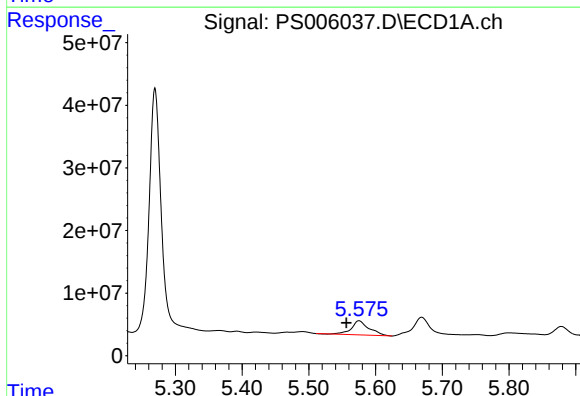


#4 2,4-DCAA

R.T.: 5.575 min
Delta R.T.: 0.019 min
Response: 41874027
Conc: 28.86 ng/ml

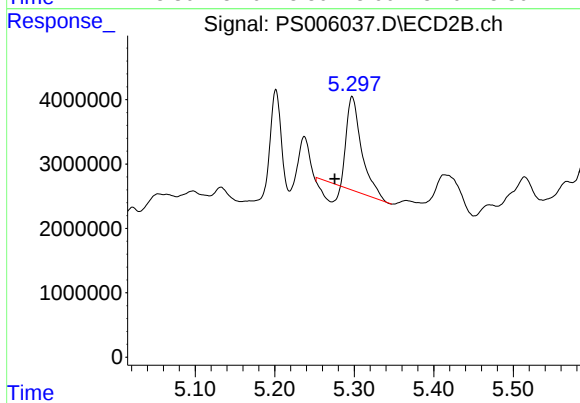

#4 2,4-DCAA


R.T.: 5.298 min
Delta R.T.: 0.022 min
Response: 17391726
Conc: 17.48 ng/ml

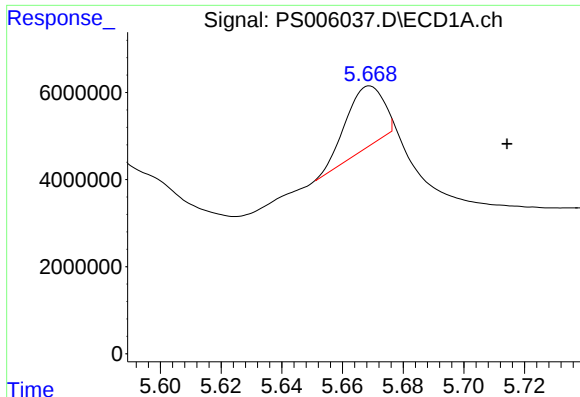

#5 DICAMBA


R.T.: 5.669 min
Delta R.T.: -0.045 min
Response: 14185608
Conc: 2.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-27

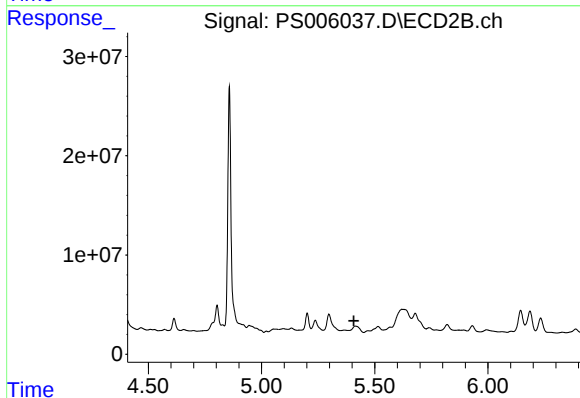


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

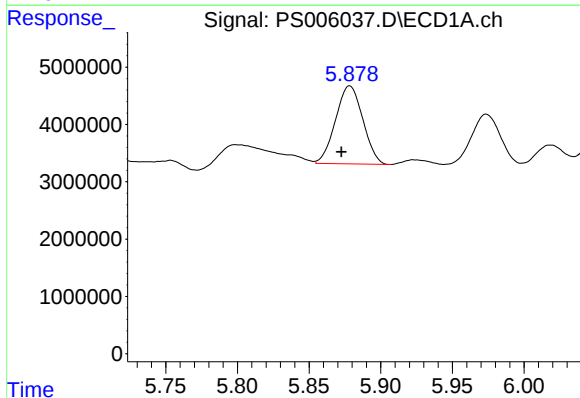


#6 MCP

R.T.: 5.878 min
Delta R.T.: 0.006 min
Response: 18040833
Conc: 3.89 ug/ml

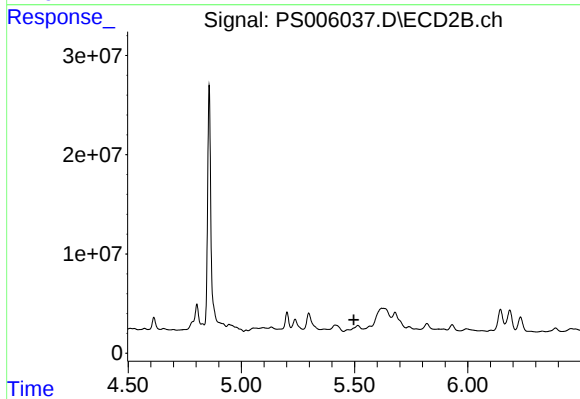

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

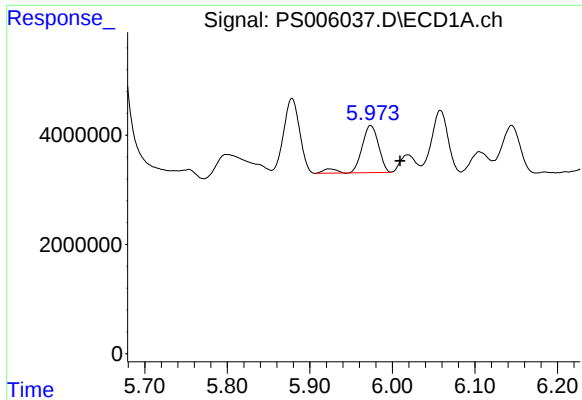

#7 MCPA


R.T.: 5.974 min
Delta R.T.: -0.036 min
Response: 12602365
Conc: 1.93 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-27

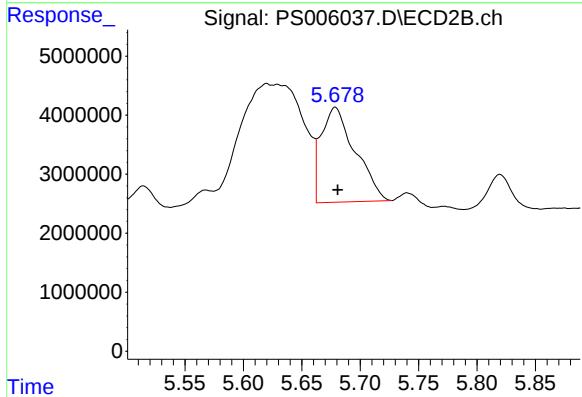


#7 MCPA

R.T.: 5.679 min
Delta R.T.: -0.002 min
Response: 32643950
Conc: 7.76 ug/ml

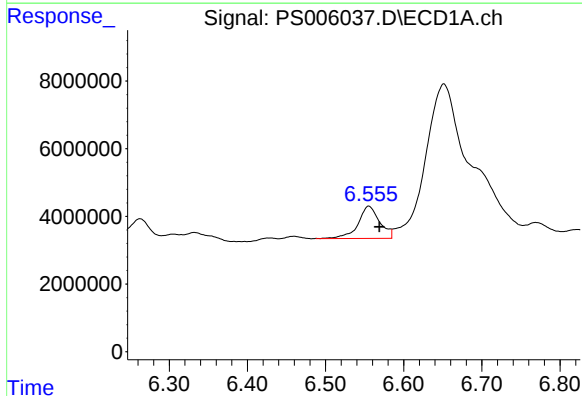


#9 2,4-D

R.T.: 6.555 min
Delta R.T.: -0.013 min
Response: 18366105
Conc: 12.25 ng/ml

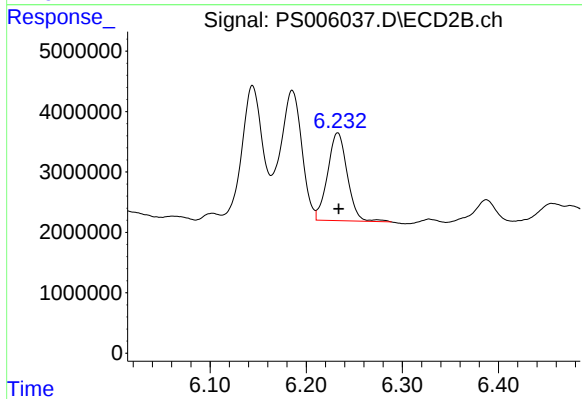

#9 2,4-D


R.T.: 6.233 min
Delta R.T.: -0.001 min
Response: 20708211
Conc: 19.28 ng/ml

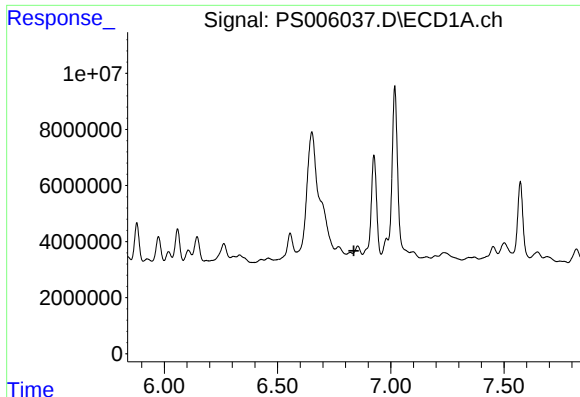

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-27

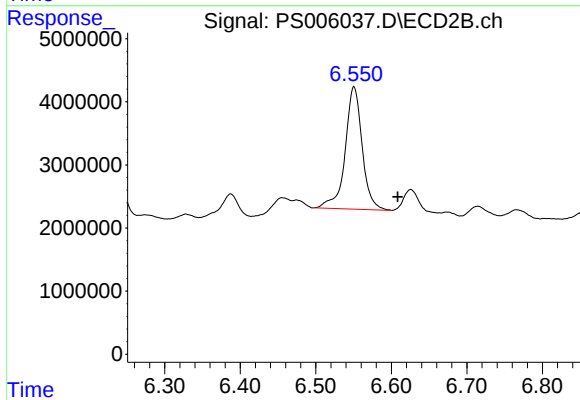


#10 Pentachlorophenol

R.T.: 6.551 min
Delta R.T.: -0.058 min
Response: 30357208
Conc: 2.34 ng/ml

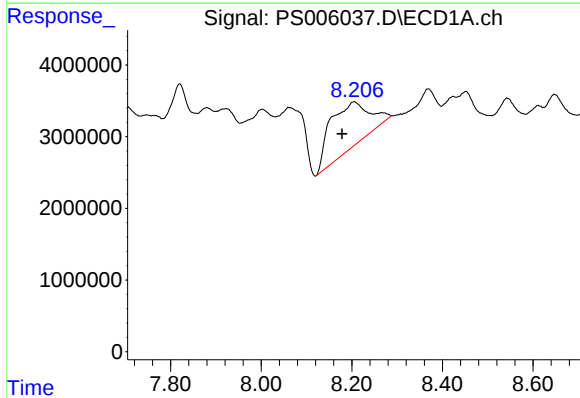

#13 2,4-DB

R.T.: 8.205 min
Delta R.T.: 0.027 min
Response: 38736458
Conc: 36.69 ng/ml

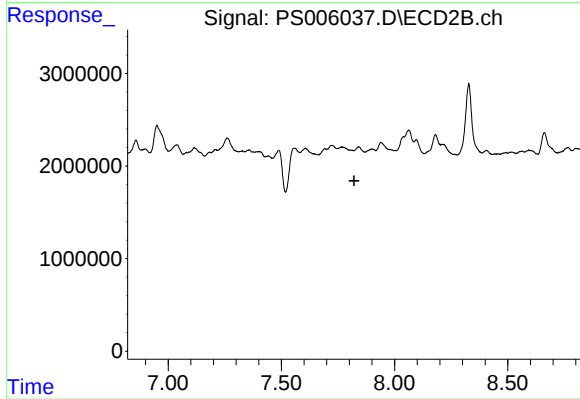

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 7.821 min
Response: 0
Conc: N.D.