

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081221\
 Data File : PS016375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2021 09:34
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:24:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.764	0	2293658	N.D.	4.397
Target Compounds							
1) T	Dalapon	0.000	2.525	0	13660534	N.D.	19.609
5) T	DICAMBA	7.378	6.926	8148822	9633265	1.455	4.421 #
6) T	MCP	0.000	7.064	0	11010944	N.D.	6.373
7) T	MCPA	7.634f	0.000	1570535	0	<MDL	N.D. #
9) T	2,4-D	0.000	7.842	0	2251365	N.D.	3.553
10) T	Pentachlo...	8.607	8.263	15011383	6828298	<MDL	<MDL #
11) T	2,4,5-TP ...	9.159	8.624	12295544	6149093	1.700	2.107
12) T	2,4,5-T	9.446	9.005	23211069	8935131	3.045	3.085
14) T	DINOSEB	11.149	9.834	14754396	4844415	2.798	2.378
15) T	Picloram	10.975	10.815	360.0E6	150.9E6	36.074	37.469
16) T	DCPA	11.417	10.764	21516835	10214785	2.036	2.272



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081221\
Data File : PS016375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2021 09:34
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:24:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

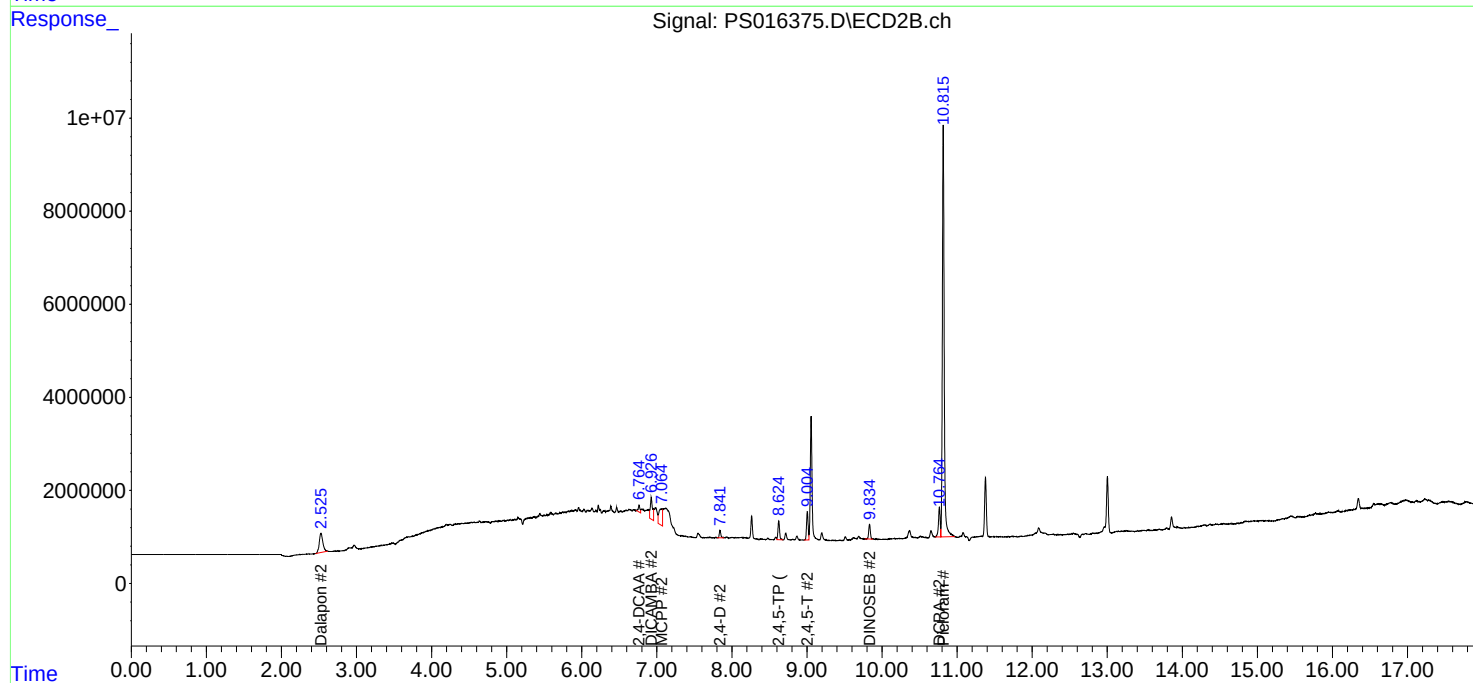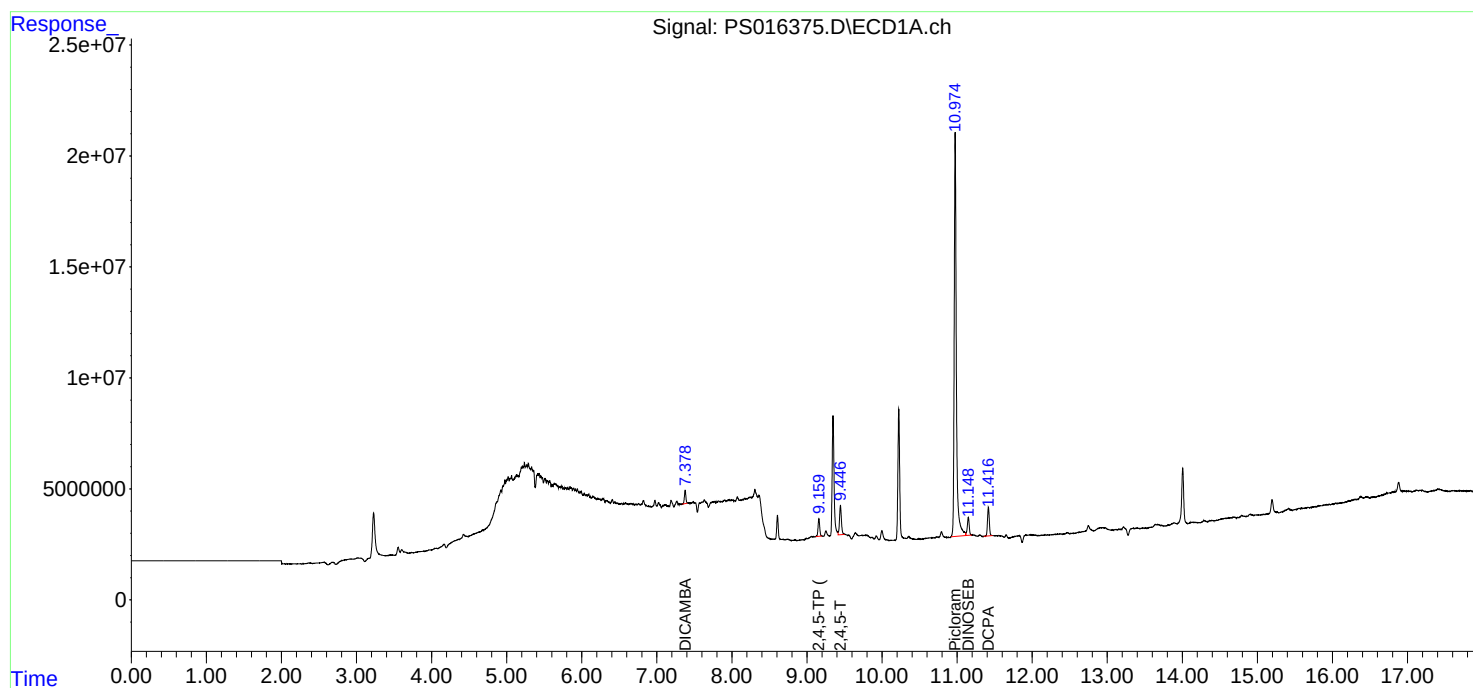


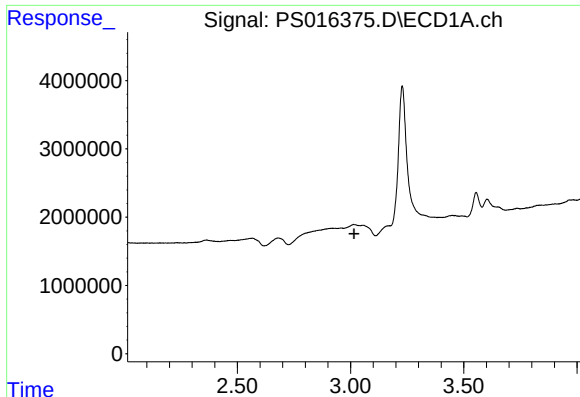

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

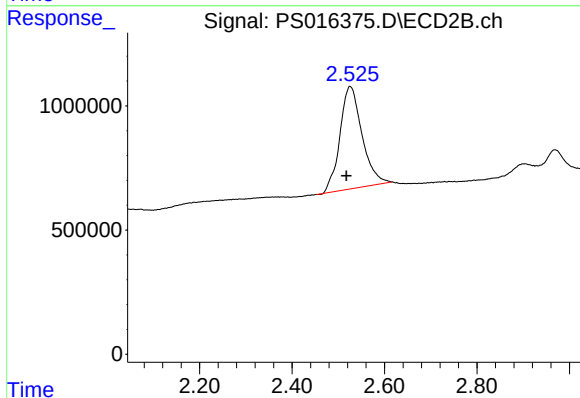


#1 Dalapon

R.T.: 2.525 min
Delta R.T.: 0.008 min
Response: 13660534
Conc: 19.61 ng/ml

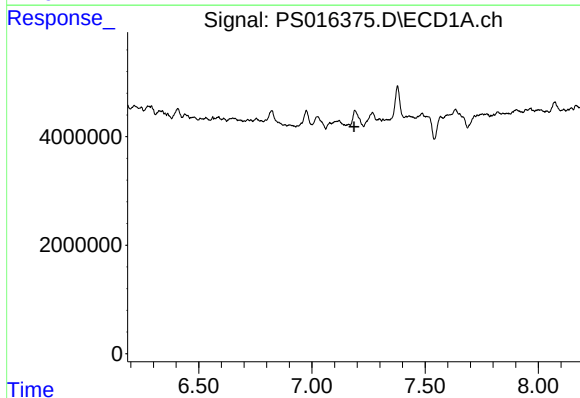


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.186 min
Response: 0
Conc: N.D.

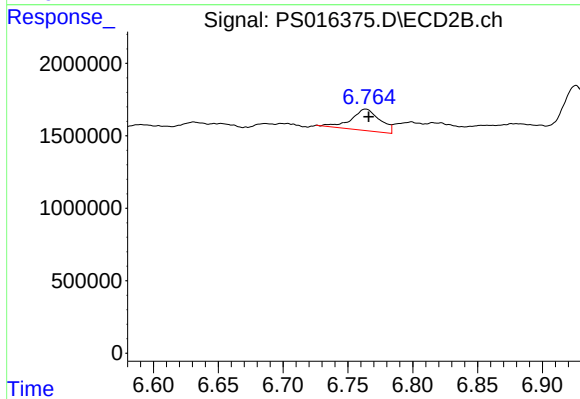

#4 2,4-DCAA


R.T.: 6.764 min
Delta R.T.: -0.002 min
Response: 2293658
Conc: 4.40 ng/ml

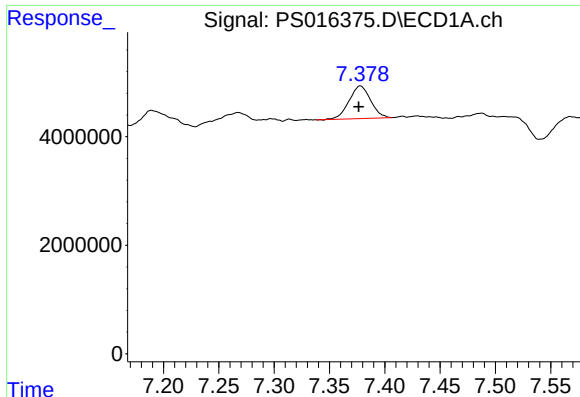

#5 DICAMBA


R.T.: 7.378 min
Delta R.T.: 0.001 min
Response: 8148822
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

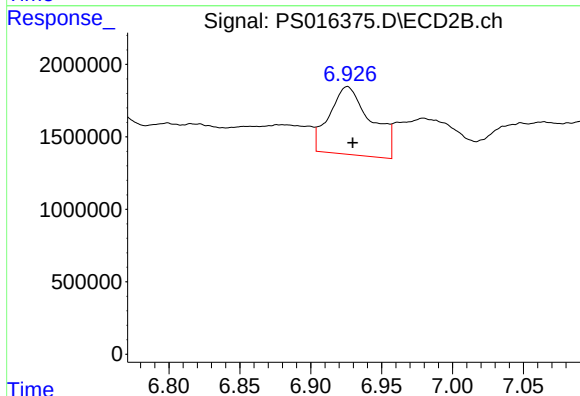


#5 DICAMBA

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 9633265
Conc: 4.42 ng/ml

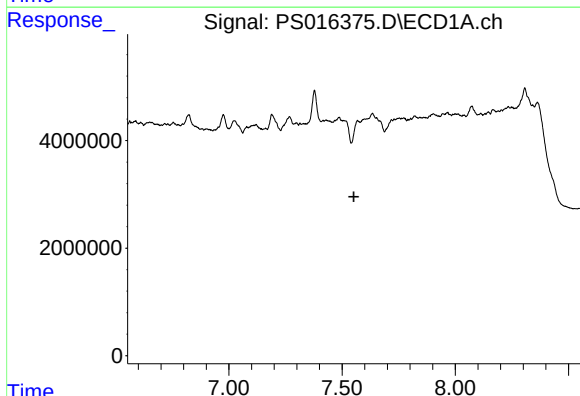


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.552 min
Response: 0
Conc: N.D.

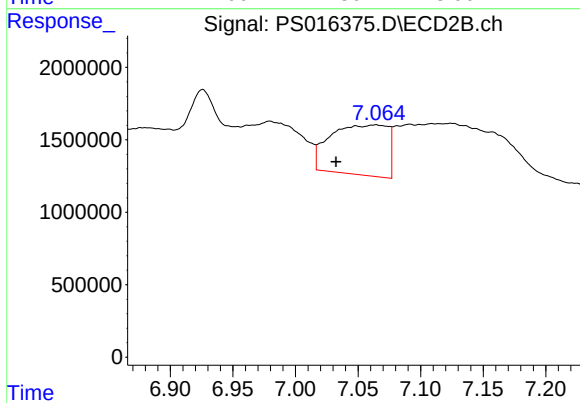

#6 MCPP


R.T.: 7.064 min
Delta R.T.: 0.032 min
Response: 11010944
Conc: 6.37 ug/ml

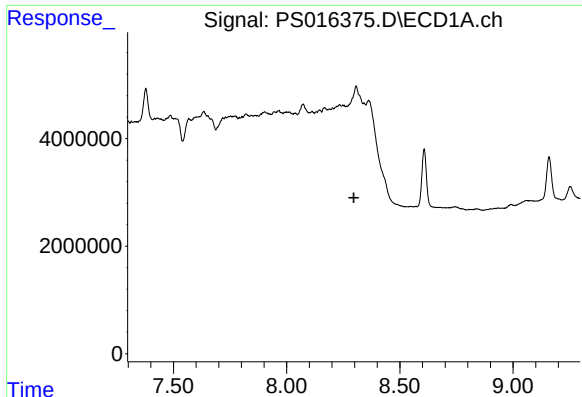

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.297 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

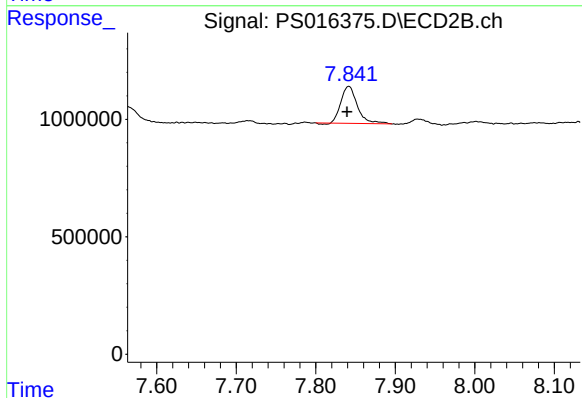


#9 2,4-D

R.T.: 7.842 min
Delta R.T.: 0.002 min
Response: 2251365
Conc: 3.55 ng/ml

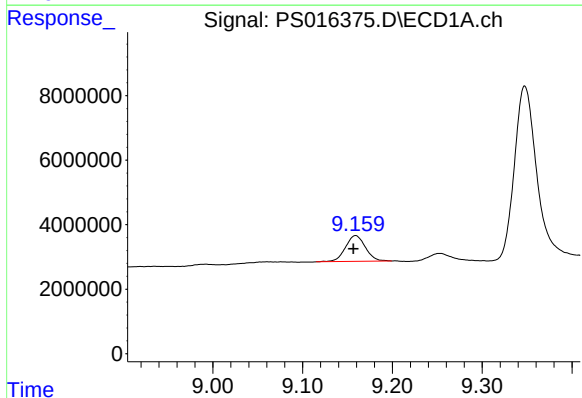


#11 2,4,5-TP (SILVEX)

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 12295544
Conc: 1.70 ng/ml

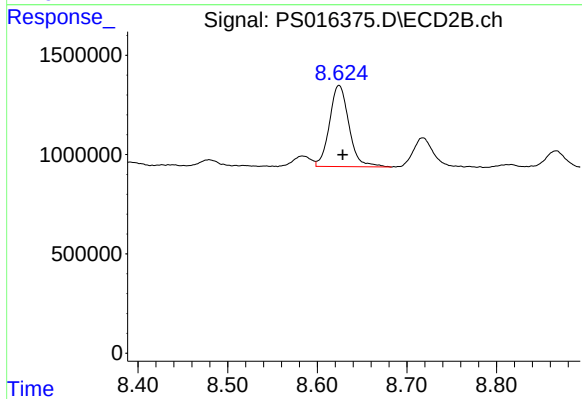

#11 2,4,5-TP (SILVEX)


R.T.: 8.624 min
Delta R.T.: -0.004 min
Response: 6149093
Conc: 2.11 ng/ml

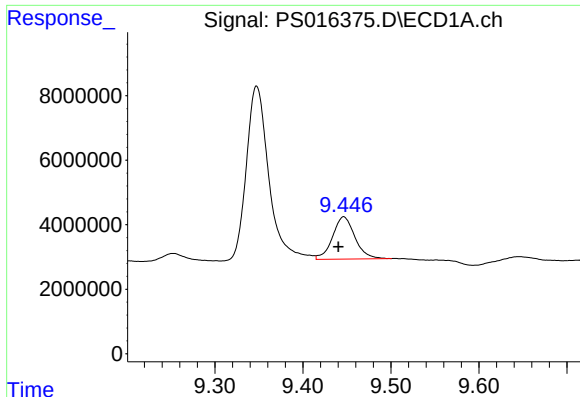

#12 2,4,5-T


R.T.: 9.446 min
Delta R.T.: 0.006 min
Response: 23211069
Conc: 3.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

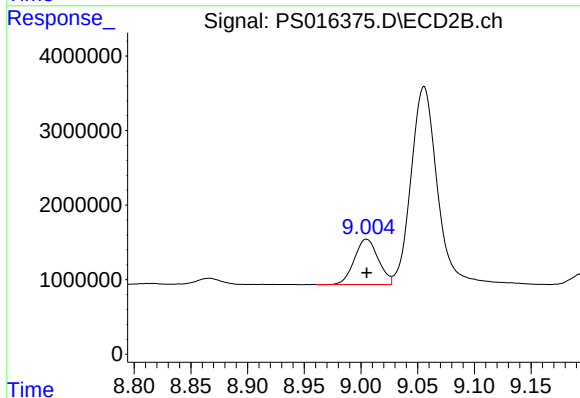


#12 2,4,5-T

R.T.: 9.005 min
Delta R.T.: 0.000 min
Response: 8935131
Conc: 3.08 ng/ml

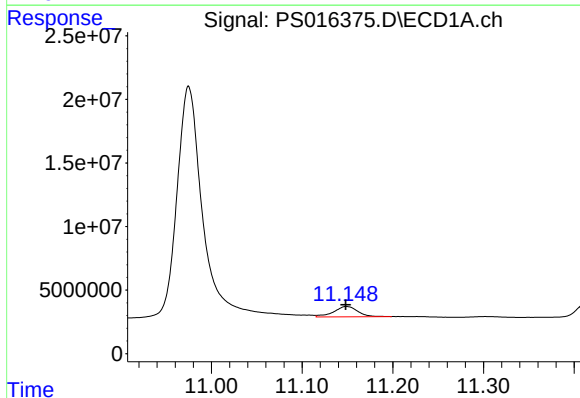


#14 DINOSEB

R.T.: 11.149 min
Delta R.T.: 0.000 min
Response: 14754396
Conc: 2.80 ng/ml

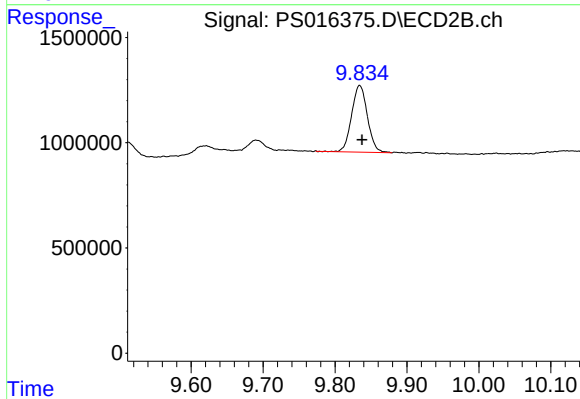

#14 DINOSEB


R.T.: 9.834 min
Delta R.T.: -0.003 min
Response: 4844415
Conc: 2.38 ng/ml

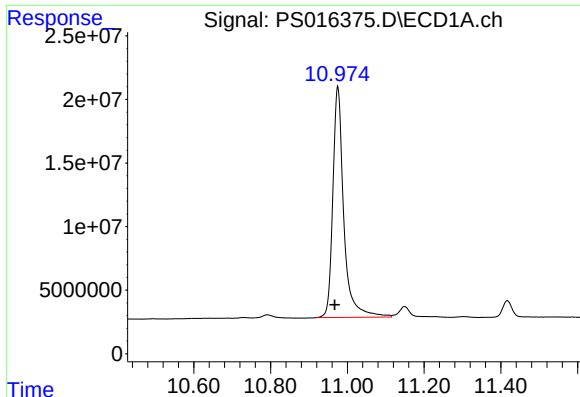

#15 Picloram


R.T.: 10.975 min
Delta R.T.: 0.008 min
Response: 360044259
Conc: 36.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

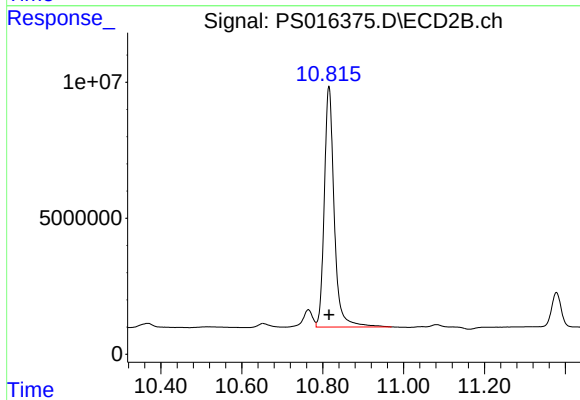


#15 Picloram

R.T.: 10.815 min
Delta R.T.: 0.000 min
Response: 150875624
Conc: 37.47 ng/ml

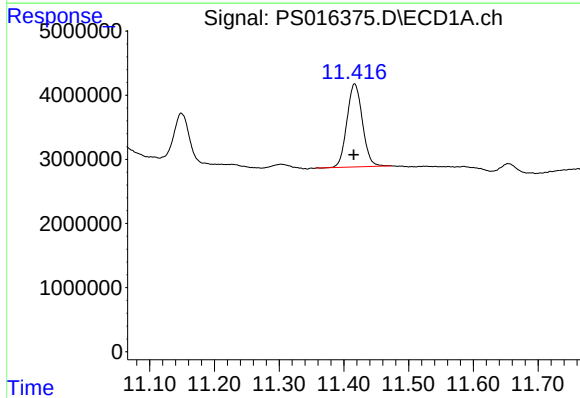

#16 DCPA

R.T.: 11.417 min
Delta R.T.: 0.002 min
Response: 21516835
Conc: 2.04 ng/ml

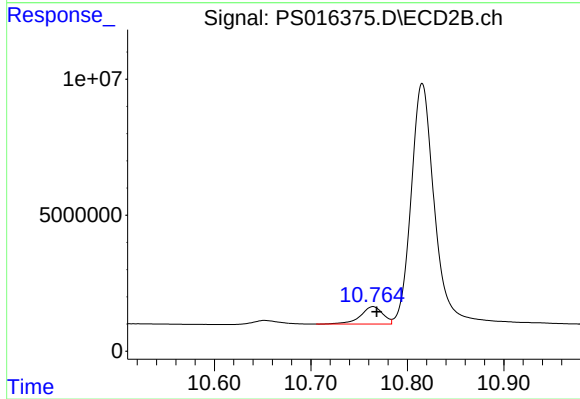

#16 DCPA

R.T.: 10.764 min
Delta R.T.: -0.004 min
Response: 10214785
Conc: 2.27 ng/ml