

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081221\
 Data File : PS016376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2021 09:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:24:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.186	6.764	632.8E6	264.9E6	430.148	507.852
Target Compounds							
5) T	DICAMBA	0.000	6.986f	0	1886391	N.D.	<MDL
6) T	MCP	0.000	6.986f	0	1886391	N.D.	1.092
12) T	2,4,5-T	0.000	9.014	0	2562967	N.D.	<MDL
15) T	Picloram	10.990	10.824	170.6E6	79209813	17.092	19.671
16) T	DCPA	0.000	10.765	0	1801003	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081221\
Data File : PS016376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2021 09:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:24:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

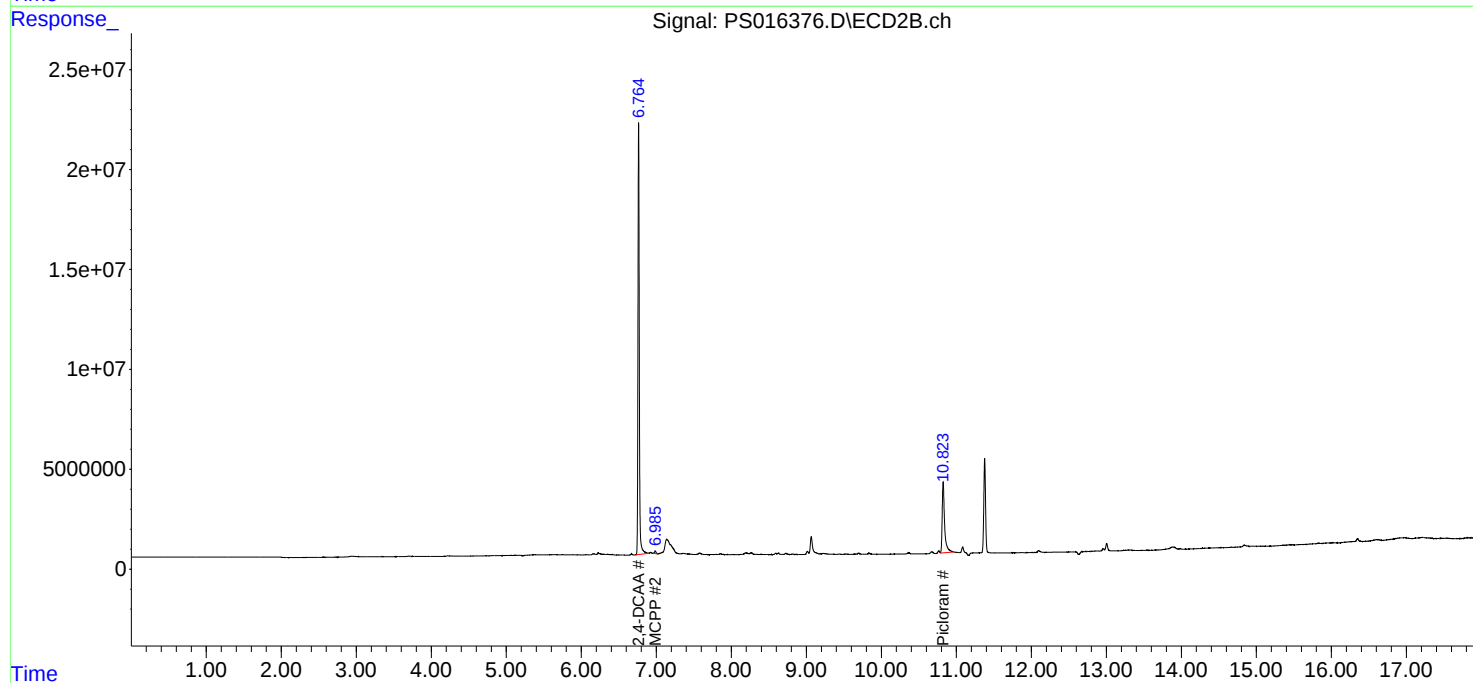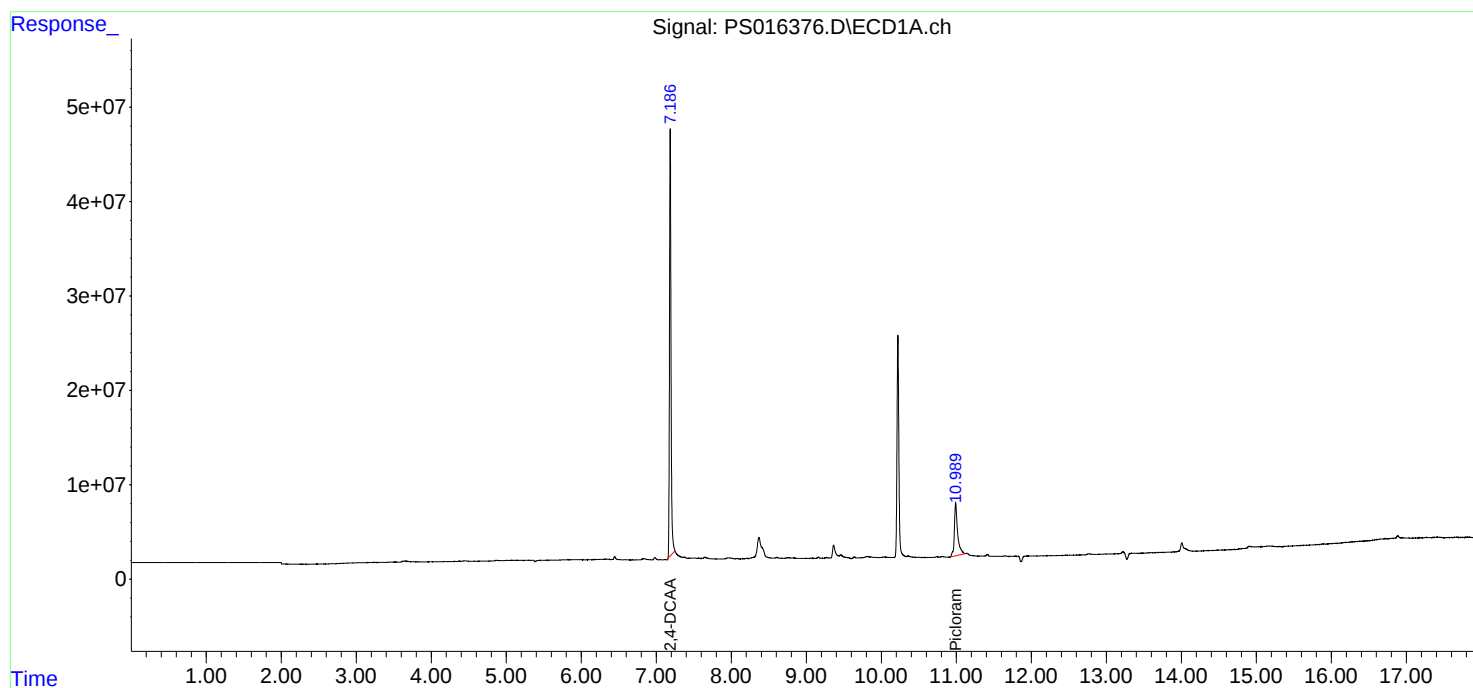


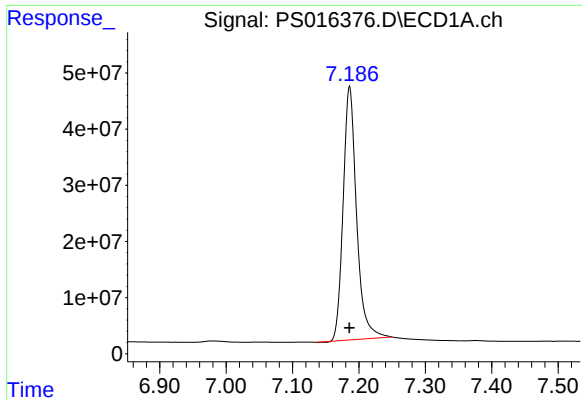

#4 2,4-DCAA


R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 632793374
Conc: 430.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

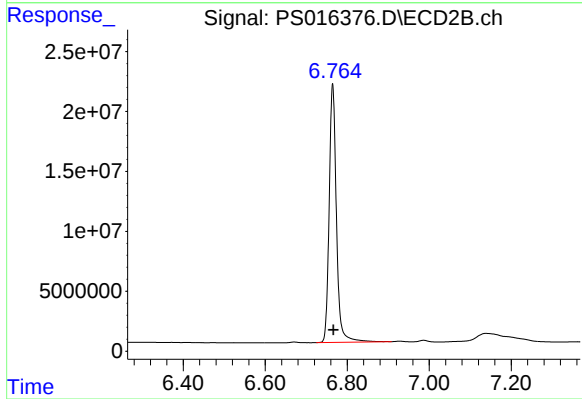


#4 2,4-DCAA

R.T.: 6.764 min
Delta R.T.: -0.001 min
Response: 264908132
Conc: 507.85 ng/ml

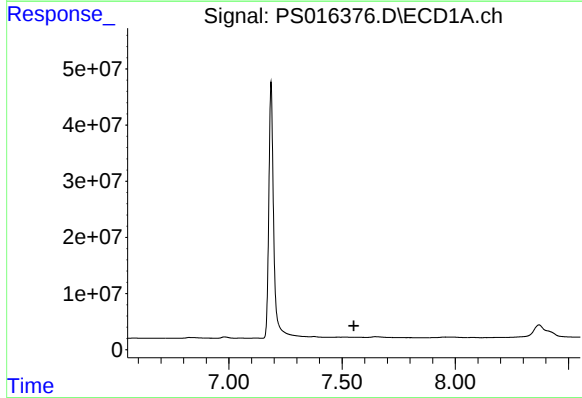


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.552 min
Response: 0
Conc: N.D.

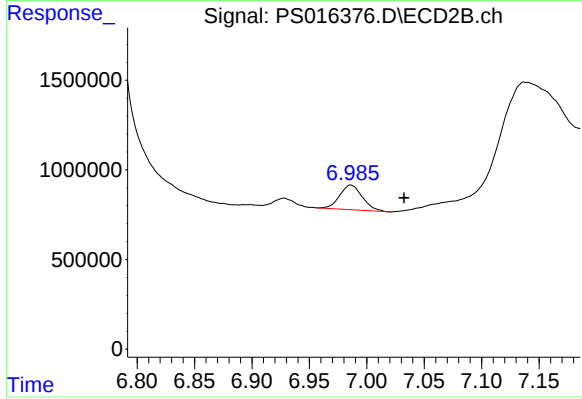

#6 MCP


R.T.: 6.986 min
Delta R.T.: -0.046 min
Response: 1886391
Conc: 1.09 ug/ml

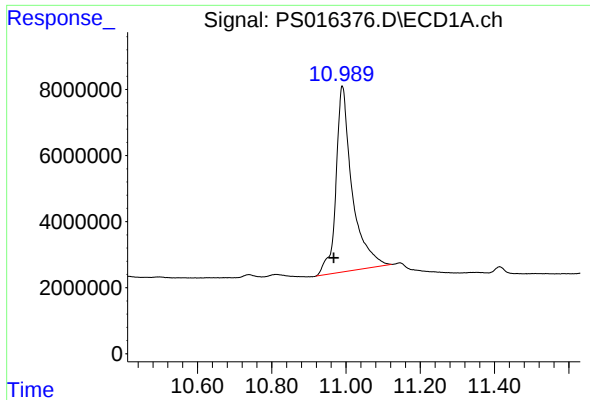

#15 Picloram

R.T.: 10.990 min
Delta R.T.: 0.023 min
Response: 170595251
Conc: 17.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

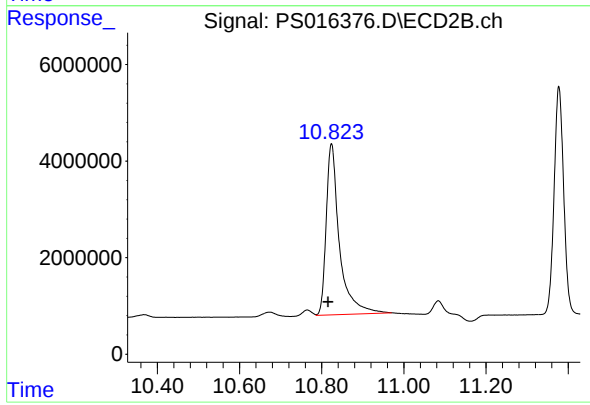

#15 Picloram

R.T.: 10.824 min
Delta R.T.: 0.008 min
Response: 79209813
Conc: 19.67 ng/ml