

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081221\
 Data File : PS016380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2021 12:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:25:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.186	6.765	640.5E6	267.1E6	435.366	512.021
Target Compounds							
5) T	DICAMBA	0.000	6.988f	0	2111649	N.D.	<MDL
6) T	MCPD	0.000	6.988f	0	2111649	N.D.	1.222
8) T	DICHLORPROP	0.000	7.581	0	3271544	N.D.	6.039
15) T	Picloram	10.949	10.834	7464420	3887899	<MDL	<MDL #
16) T	DCPA	0.000	10.834f	0	3887899	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081221\
Data File : PS016380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2021 12:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:25:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

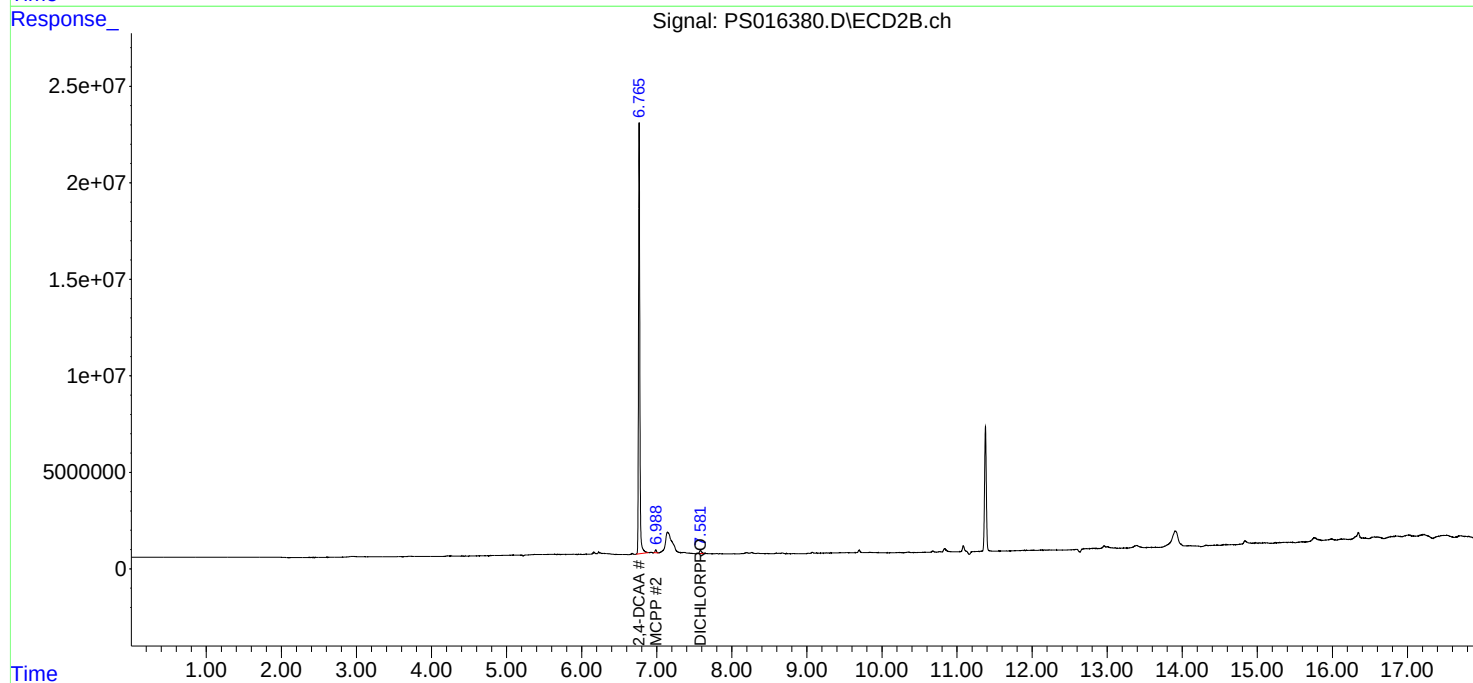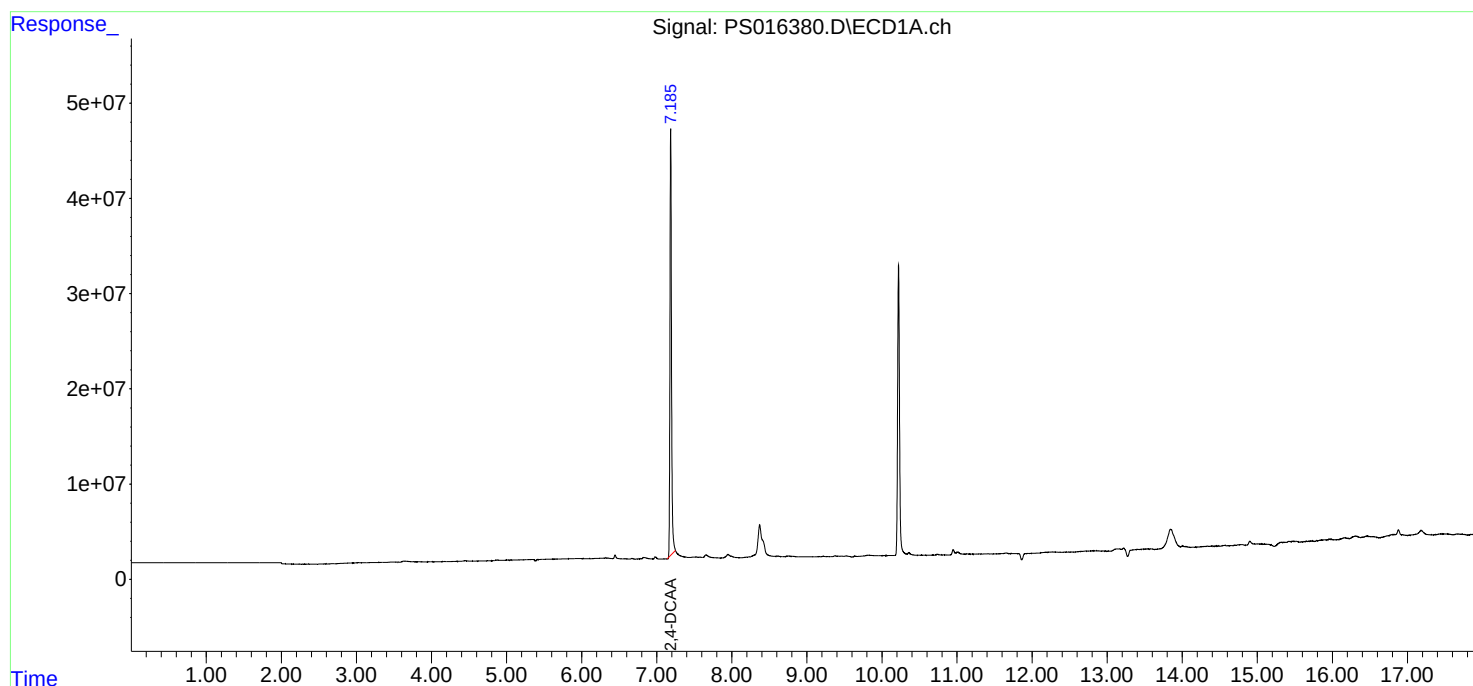


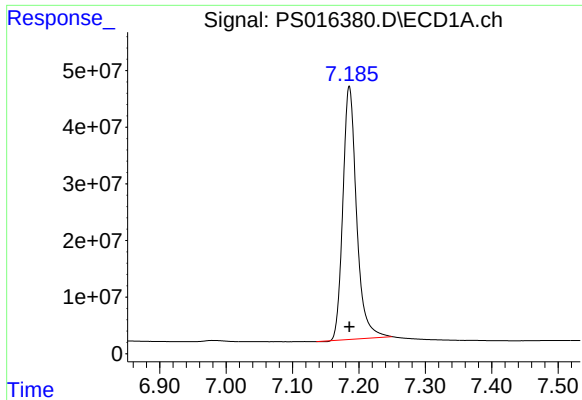

#4 2,4-DCAA


R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 640469623
Conc: 435.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

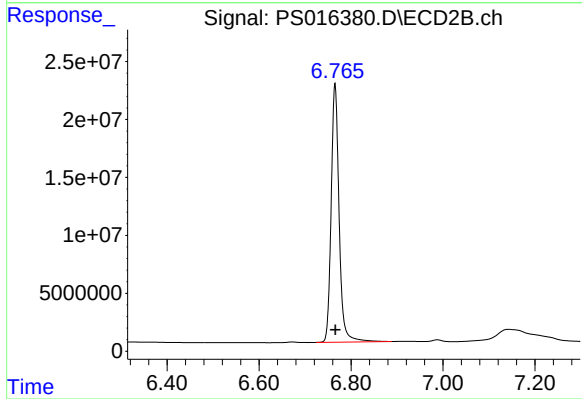


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: 0.000 min
Response: 267082570
Conc: 512.02 ng/ml

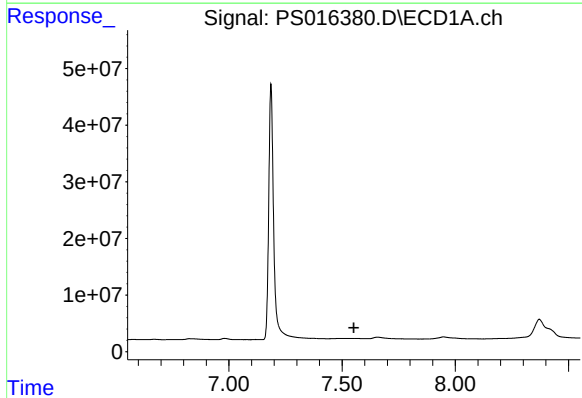


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.552 min
Response: 0
Conc: N.D.

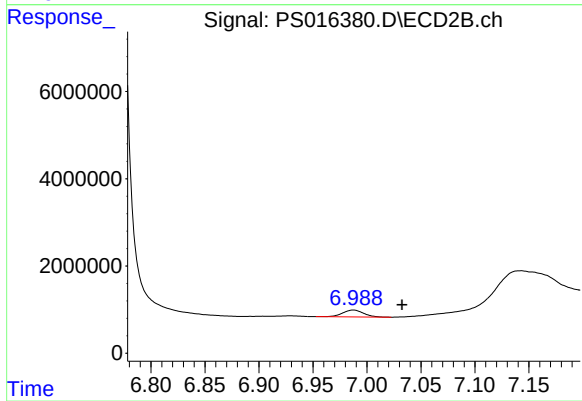

#6 MCP


R.T.: 6.988 min
Delta R.T.: -0.045 min
Response: 2111649
Conc: 1.22 ug/ml

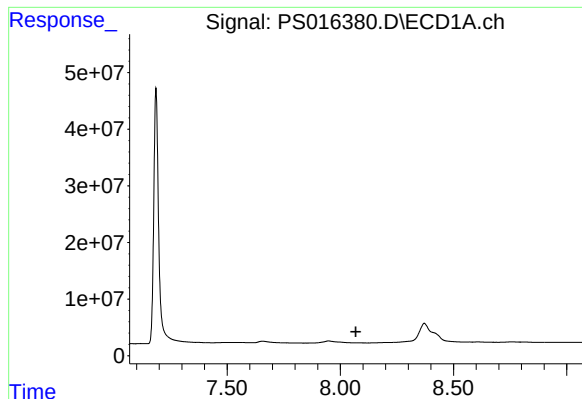

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

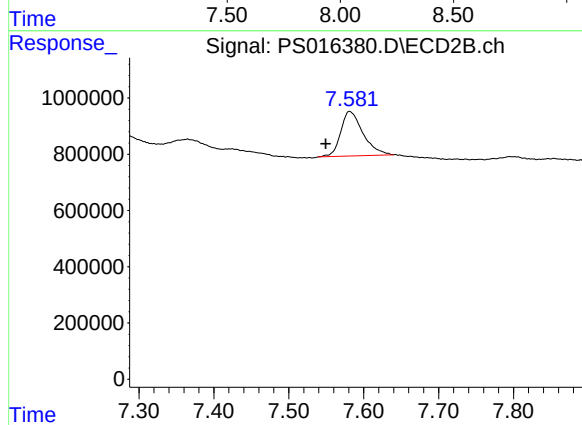

#8 DICHLORPROP

R.T.: 7.581 min
Delta R.T.: 0.032 min
Response: 3271544
Conc: 6.04 ng/ml